

## ACCU-CHEK Instant Meter and mySugr App User Guide

[Home](#) » [ACCU-CHEK](#) » ACCU-CHEK Instant Meter and mySugr App User Guide 

*ACCU-CHEK Instant Meter and mySugr  
App User Guide*

# QUICK REFERENCE GUIDE

WITH MYSUGR®



## ⚠ WARNING

The mySugr Bolus Calculator is intended for the management of insulin dependent diabetes by calculating a bolus insulin dose or carbohydrate intake based on your entered data. The mySugr Bolus Calculator is licenced for people with diabetes over the age of 18 years. The mySugr logbook is licenced for people with diabetes over the age of 16 years.

## ⚠ WARNING

This Quick Reference Guide does not replace the detailed User Manuals for the mySugr App and Accu-Chek Instant blood glucose monitoring system. Be sure to comply with the safety information in the User Manual and in the package insert of the test strip. Consult healthcare professional before changing target range on App.

## Contents


- 1 PAIRING THE ACCU-CHEK INSTANT METER TO THE MYSUGR® APP
- 2 CHANGING THE TARGET RANGE ON YOUR ACCU-CHEK INSTANT METER
- 3 LOG AN ENTRY
- 4 Documents / Resources
- 5 Related Posts

## PAIRING THE ACCU-CHEK INSTANT METER TO THE MYSUGR® APP


1. On the mySugr homepage go to the “connections” option on the bottom right of the screen and select “Accu-Chek Instant” then select the “Connect now” button.



2. Turn the meter off if it's on, then press and hold the bottom button until you see the Bluetooth® symbol on the meter display.

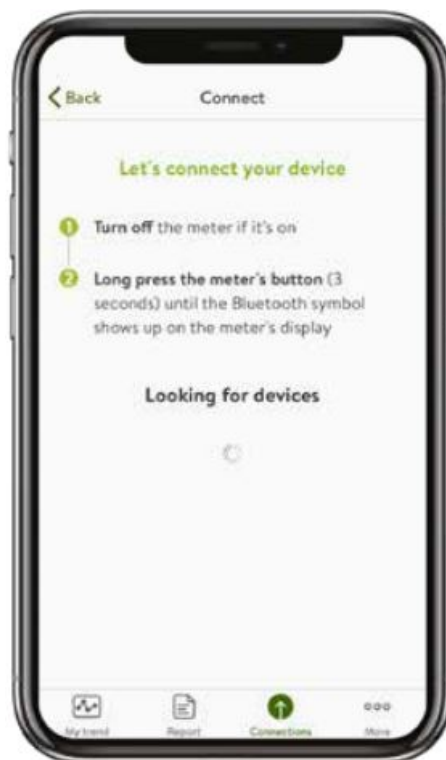

3. You will then see the serial number of the Accu-Chek Instant meter displayed in the mySugr app. Select the meter to confirm pairing.

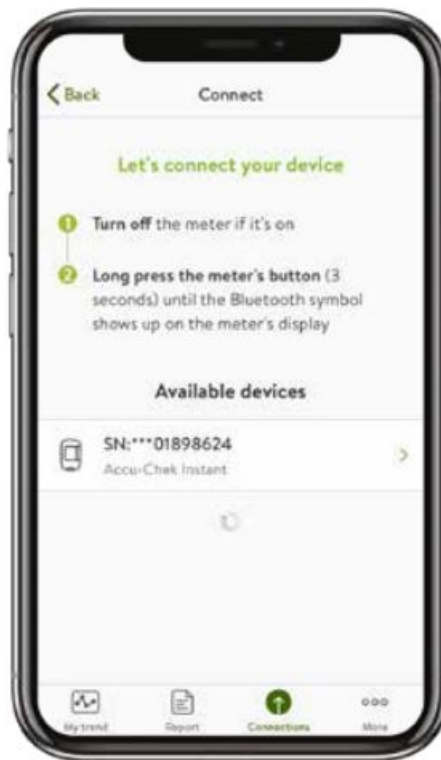

4. Enter the pin number that is on the back of your Accu-Chek Instant meter.



5. After you have entered the Pin select "pair" and the pairing will be completed.



6. You have now successfully paired your Accu-Chek Instant meter to your mySugr app. You will need to perform a blood glucose test in order to unlock mySugr Pro.



Connects with  mySugr




Download the mySugr app to set up your account.

## CHANGING THE TARGET RANGE ON YOUR ACCU-CHEK INSTANT METER

Once your Accu-Chek Instant meter has been paired to the mySugr app, you are able to change the target ranges on your meter via the mySugr app.

**Start by opening the mySugr app.**

To confirm the new target range on the Instant meter, please perform another blood glucose test.

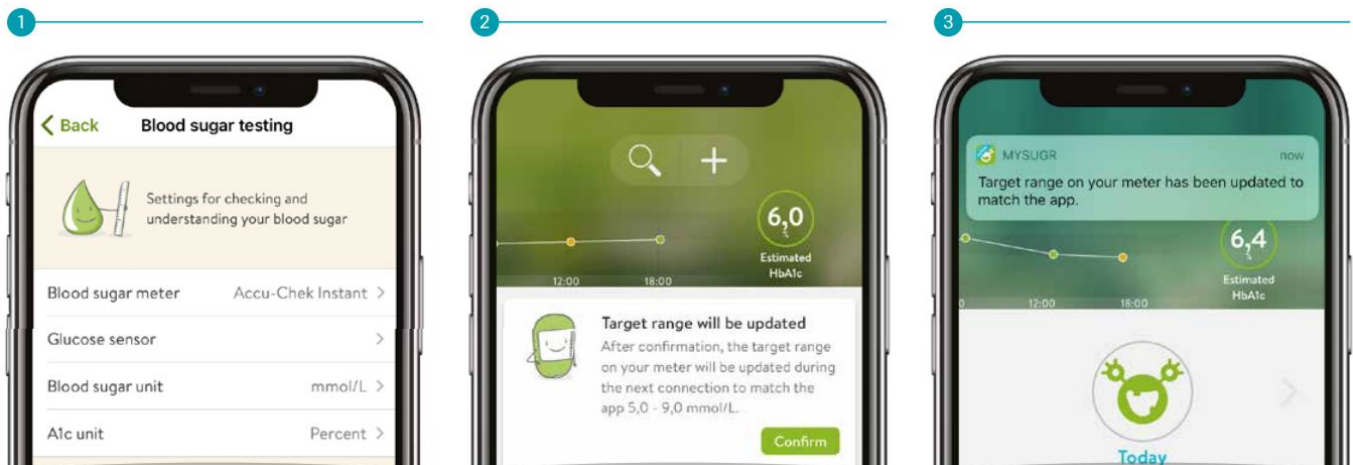


Select “More” on the bottom right of the home screen then select “Profile Settings” then “Blood sugar testing”. Select your “Hyper” “Target range” and “Hypo” and scroll up or down to select the required range.

Once settings have been updated you will receive a confirmation message.

You may also receive a confirmation notification when your meter has been updated to match the target range on the mySugr app.

## LOG AN ENTRY


mySugr Bolus Calculator is licenced for people with diabetes over the age of 18 years. mySugr logbook is licenced for people with diabetes over the age of 16 years.

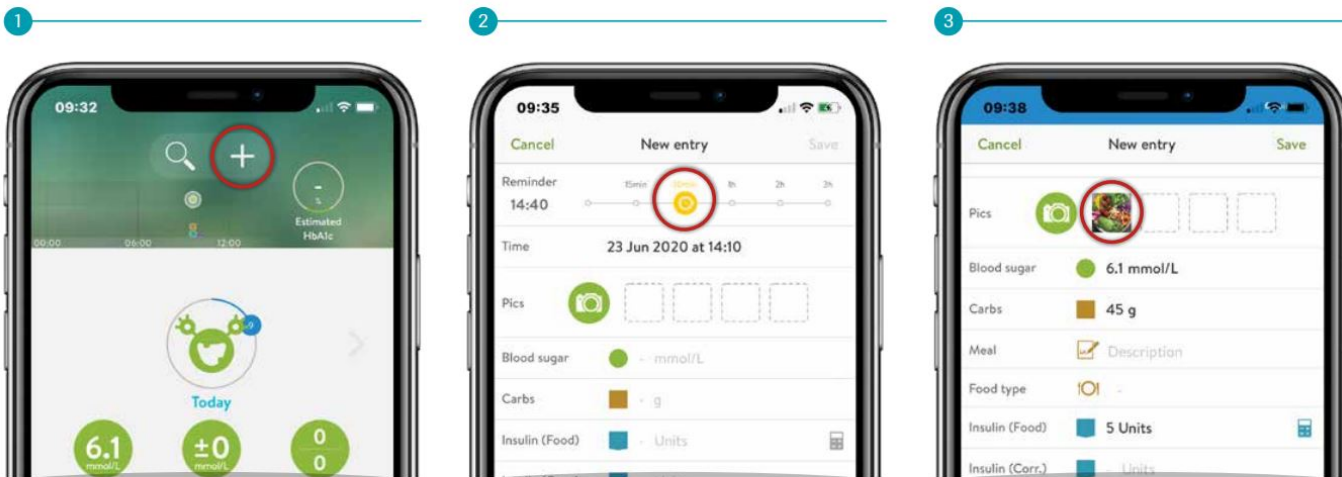

Tap the 'Plus' button on your screen.

Set a reminder.

Take a picture of your food.

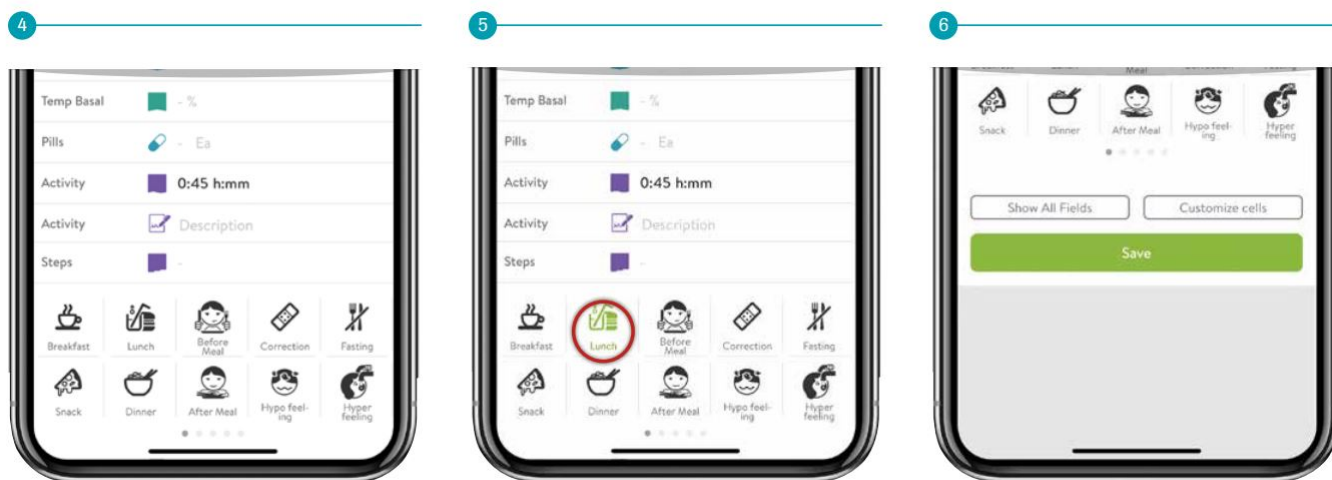

Enter values for your blood glucose, carbs, insulin, pills and activities.

Select the tags you want to save.

Save the entry.

The Bluetooth® word mark and logos are registered trademarks owned by Bluetooth SIG, Inc., and any use of such marks by Roche is under license.


© 2021 Roche Diabetes Care Limited. All rights reserved. ACCU-CHEK, ACCU-CHEK INSTANT and MYSUGR are trademarks of Roche. All other trademarks or brand names are the property of their respective owners.

Roche Diabetes Care Limited, Charles Avenue, Burgess Hill, West Sussex, RH15 9RY, UK. Company Registration Number 9055599

For use in the UK & Ireland only Date of preparation: February 2021 Material Number: 09426507001

[www.accu-check.co.uk](http://www.accu-check.co.uk) [www.accu-check.ie](http://www.accu-check.ie)

## Documents / Resources



**[ACCU-CHEK Instant Meter and mySugr App](#)** [pdf] User Guide  
Instant Meter and mySugr App