



AEMC INSTRUMENTS L430 Simple Logger DC Module User Manual

[Home](#) » [AEMC INSTRUMENTS](#) » AEMC INSTRUMENTS L430 Simple Logger DC Module User Manual 

Contents

- [1 AEMC INSTRUMENTS L430 Simple Logger DC Module](#)
- [2 IMPORTANT NOTICE BEFORE OPERATING](#)
- [3 INTRODUCTION](#)
- [4 PRODUCT FEATURES](#)
- [5 SPECIFICATIONS](#)
- [6 OPERATION](#)
- [7 MAINTENANCE](#)
 - [7.1 Repair and Calibration](#)
- [8 Limited Warranty](#)
- [9 Documents / Resources](#)
 - [9.1 References](#)



AEMC INSTRUMENTS L430 Simple Logger DC Module



Product Information

The product is a Simple Logger DC Module, available in three Bmodels: L320, L410, and L430. It is a data logging device used for recording and monitoring DC signals. The user manual provides detailed information on the product features, specifications, maintenance, and additional instructions for importing files into a spreadsheet and time-extension recording.

Product Features

- Indicators and Buttons
- Inputs and Outputs
- Mounting

Specifications

- Electrical Specifications
- Mechanical Specifications
- Environmental Specifications
- Safety Specifications

Maintenance

- Battery Installation
- Cleaning

Appendix A – Importing .TXT Files into a Spreadsheet

This section provides instructions on how to import .TXT files generated by the Simple Logger into a spreadsheet application like Excel. It includes information on opening the file in Excel and formatting the date and time.

Appendix B -Time-Extension Recording (TXRTM)

This section explains the process of time-extension recording using the Simple Logger. It provides instructions on how to perform this function.

Important Notice Before Operating

Prior to saving a downloaded DC Logger file, it is essential to set a scale for the logger to function correctly. The manual provides two methods for creating scales: with the logger connected and without the logger connected. The predefined scales are saved in the directory for the Simple Logger software.

Product Usage Instructions

To set a scale with the Logger connected:

1. Go to the File menu and select Scaling.
2. Select the appropriate range for the model used.
3. In the scaling window, create a custom scale if needed.
4. Save the scale using the File-Save Command.

To set a scale without the Logger connected:

1. Go to the File menu and select Scaling.
2. Select the appropriate range for the model used.
3. In the scaling window, create a custom scale if needed.
4. Save the scale using the File-Save Command.

Note: A scale can be set prior to or after downloading, but it should be set before saving.

IMPORTANT NOTICE BEFORE OPERATING

A scale must be set prior to saving a downloaded DC Logger file for the logger to function correctly

To create scales with the Logger connected:

The first time a DC logger is used with a fresh install of the Simple Logger software a scale must be set for each different DC logger model. Once a scale is set for a specific model, the software will default to this scale each time that model is connected. To set a scale for the model in use, connect the logger and a Scale menu will appear. Click on Scale and the scaling window for the model used will appear. From the scaling window you may set a custom scale or open a predefined scale from the File-Open menu. The predefined scale is in the directory for the Simple Logger software.

To create scales without the Logger connected:

Go to Scaling from the File menu and select the range for the model used. From the scaling window you may create a custom scale and save it using the File-Save Command. The predefined scales are saved in the directory for the Simple Logger software. A scale may be set prior to or after downloading, but before saving.

INTRODUCTION

WARNING

These safety warnings are provided to ensure the safety of personnel and proper operation of the instrument.

- Read the instruction manual completely and follow all safety information before operating this instrument.
- Use caution on any circuit: Potentially high voltages and currents may be present and may pose a shock hazard.
- Read the specifications section prior to using the data logger.
Never exceed the maximum voltage ratings given.
- Safety is the responsibility of the operator.
- For maintenance, use only original replacement parts.
- NEVER open the back of the instrument while connected to Any circuit or input.
- ALWAYS connect the leads to the logger before inserting the leads to the test voltage
- ALWAYS inspect the instrument and leads prior to use.
Replace any defective parts immediately.
- NEVER use the Simple Logger® Models L320, L410, L430 on electrical conductors rated above 600V Cat. III.

International Electrical Symbols

This symbol signifies that the instrument is protected by double or reinforced insulation. Use only specified replacement parts when servicing the instrument.

This symbol on the instrument indicates a WARNING and that the operator must refer to the user manual for instructions before operating the instrument. In this manual, the symbol preceding instructions indicates that if the instructions are not followed, bodily injury, installation/sample and product damage may result. Risk of electric shock. The voltage at the parts marked with this symbol may be dangerous.

<https://manual-hub.com/>

Simple Logger® Models L320 / L410 / L430 5

Definition of Measurement Categories

- Cat. I: For measurements on circuits not directly connected to the AC supply wall outlet such as protected secondaries, signal level, and limited energy circuits.
- Cat. II: For measurements performed on circuits directly connected to the electrical distribution system.
Examples are measurements on household appliances or portable tools.
- Cat. III: For measurements performed in the building installation at the distribution level such as on hardwired equipment in fixed installation and circuit breakers.
- Cat. IV: For measurements performed at the primary electrical supply (<1000V) such as on primary overcurrent protection devices, ripple control units, or meters.

Receiving Your Shipment

Upon receiving your shipment, make sure that the contents are consistent with the packing list. Notify your distributor of any missing items. If the equipment appears to be damaged, file a claim immediately with the carrier and notify your distributor at once, giving a detailed description of any damage.

Save the damaged packing container to substantiate your claim.

Ordering Information

- Simple Logger® Model L320 – DC Current (4 to 20mA Input).....
Cat. #2113.97
- Simple Logger® Model L410 – DC Voltage (0 to 100mVDC Input).....
Cat. #2114.05
- Simple Logger® Model L430 – DC Voltage (0 to 10VDC Input).....
Cat. #2114.07

All DC Simple Loggers® are supplied with software (CD-ROM), 6 ft DB-9 RS-232 serial cable, 9V Alkaline battery and user manual.

1. Accessories and Replacement Parts


Two 5 ft Voltage Leads with Clips..... Cat. #2118.51

Order Accessories and Replacement Parts Directly Online

Check our Storefront at www.aemc.com for availability


PRODUCT FEATURES

Models L410 and L430:

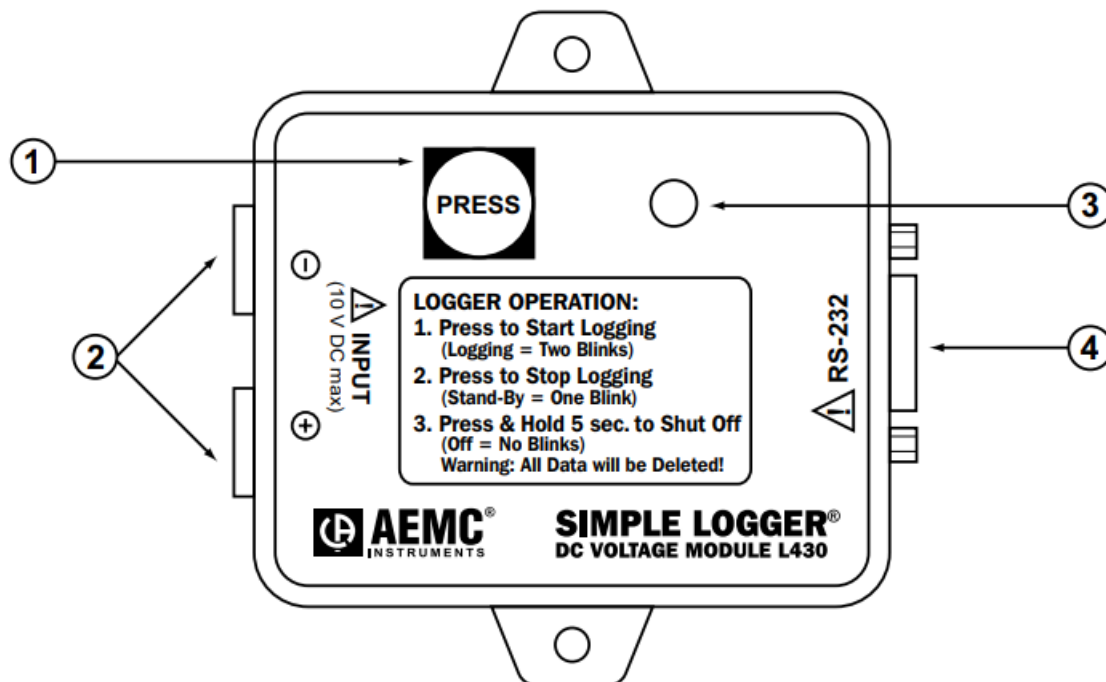

1. Start/Stop Button
2. Input Safety Plugs
3. Red LED Indicator
4. RS-232 Interface

Model L320:

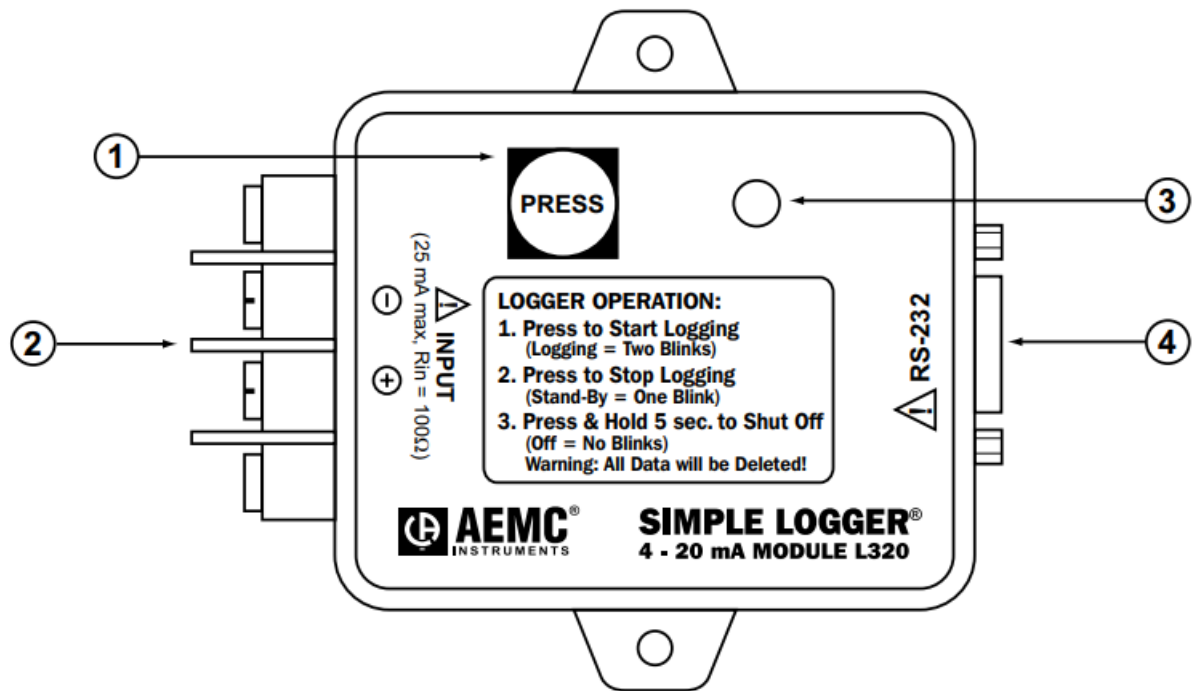

1. Start/Stop Button
2. Input Terminal Strip
3. Red LED Ind
4. RS-232 Interface

Indicators and Buttons

The Simple Logger® has one button and one indicator. Both are located on the front panel. The PRESS button is used to start and stop recordings and to turn the logger on and off.

The Red LED indicates the status of the logger:

- Single Blink: STAND-BY mode
- Double Blink: RECORD mode
- Continuously On: OVERLOAD condition
- No Blinks: OFF mode

Inputs and Outputs

The left side of the Simple Logger® incorporates 4mm safety banana jacks for the Models L410 and L430 and a screw connector for the Model L320.

The right side of the logger has a female 9-pin "D" shell serial connector used for data transmission from the logger to your computer.

Mounting

Your Simple Logger® is equipped with clearance holes in the base plate tabs for mounting. For less permanent mounting, the Velcro® pads (supplied loose) can be attached to the logger and the surface to which the logger will be mounted.

SPECIFICATIONS

Electrical Specifications

- Number of Channels: 1
- Measurement Range: L320: 0 to 25mADC
 - L410: 0 to 100mVDC
 - L430: 0 to 10VDC
- Input Connection: L320: two post screw terminal strip
L410 and L430: recessed safety banana jacks
- Input Impedance: L320: 100Ω
L410 and L430: 1MΩ

L320: 8 Bit (12.5μA min resolution)

Scale Range	Maximum Input	Resolution
100%	25.5mA	0.1mA
50%	12.75mA	0.05mA
25%	6.375mA	0.025mA
12.5%	3.1875mA	0.0125mA

L410: 8 Bit (50μV min resolution)

Scale Range	Maximum Input	Resolution
100%	102mV	0.4mV
50%	51mV	0.2mV
25%	25.5mV	0.1mV
12.5%	12.75mV	0.05mV

L430: 8 Bit (5mV min resolution)

Scale Range	Maximum Input	Resolution
100%	10.2V	40mV
50%	5.1V	20mV
25%	2.55V	10mV
12.5%	1.275V	5mV

Reference condition: 23°C ± 3K, 20 to 70% RH, Frequency 50/60Hz, No AC external magnetic field, DC magnetic field ≤ 40A/m, battery voltage 9V ± 10%.
Accuracy: 1% ± 2cts

- Sample Rate: 4096/hr max; decreases by 50% each time memory is full
- Data Storage: 8192 readings
- Data Storage Technique: TXR™ Time Extension Recording™

- Power: 9V Alkaline NEDA 1604, 6LF22, 6LR61
- Battery Life Recording: Up to 1 year recording @ 77°F (25°C)
- Output: RS-232 via DB9 connector (1200 Baud)

Mechanical Specifications

- Size: 2-7/8 x 2-5/16 x 1-5/8" (73 x 59 x 41mm)
- Weight (with battery): 5 oz (140g)
- Mounting: Base plate mounting holes or Velcro® pads
- Case Material: Polystyrene UL V0

Environmental Specifications

- Operating Temperature: -4 to 158°F (-20 to 70°C)
- Storage Temperature: -4 to 176°F (-20 to 80°C)
- Relative Humidity: 5 to 95% non-condensing

Safety Specifications

Working Voltage: EN 61010, 30V Cat. III

*All specifications are subject to change without notice

OPERATION

Software Installation

Minimum Computer Requirements

- Windows® 98/2000/ME/NT and XP
- Processor – 486 or higher
- 8MB of RAM
- 8MB of hard disk space for application, 400K for each stored file
- One 9-pin serial port; one parallel port for printer support
- CD-ROM drive

1. Insert the Simple Logger® CD into your CD-ROM drive.

If auto-run is enabled, the Setup program will start automatically. If auto-run is not enabled, select Run from the Start menu and type in D:\SETUP (if your CD-ROM drive is drive D. If this is not the case, substitute the appropriate drive letter).

2. The Set-up window will appear.

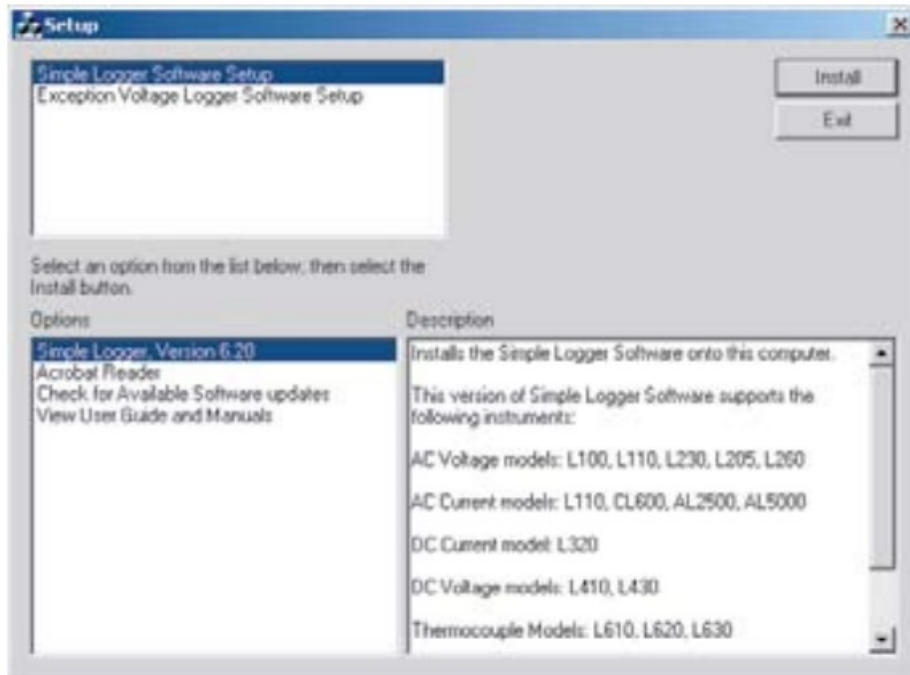


Figure 1

There are a several options to choose from. Some options(*) require an internet connection.

- Simple Logger, Version 6.xx – Installs the Simple Logger® software to the computer.
 - *Acrobat Reader – Links to the Adobe® web site to download the most recent version of Adobe® Acrobat Reader. Acrobat Reader is required for viewing PDF documents supplied on the CD-ROM.
 - *Check for Available Software Updates – Opens the AEMC Software update web site, where updated software versions are available for downloading, if necessary.
 - View User Guide and Manuals – Opens Windows® Explorer for viewing of documentation files.
3. To install the software, select Simple Logger Software Setup in the top section of the Set-up window, then select Simple Logger, Version 6.xx in the Options section.
 4. Click the Install button and follow the on-screen prompts to install the software.

Recording Data

- Connect the logger to the circuit to be tested.
NOTE: Be sure to observe the polarity or you may not get a reading.
- Press the PRESS button on the top of the logger to begin the recording session. The LED indicator will double-blink to indicate that the recording session has started.
- When the desired recording session has finished, press the PRESS button to end the recording. The LED indicator will single-blink to indicate the recording session has ended and the logger is in Stand-by.
- Remove the logger from the circuit under test and transport it to the computer for data downloading. See the User Guide on the CD-ROM for downloading instructions.

Using the Software

Launch the software and connect the RS-232 cable from your compute to the logger.

NOTE: A language will need to be selected upon the first launch.

Select Port from the menu bar and select the Com port (COM 1, 2 3 or 4) you will be using (see your computer manual). Once the software automatically detects the baud rate, the logger will communicate with the computer.

(ID number of the logger and number of points recorded displayed). Select Download to display the graph. (Takes about 90 seconds.) Select File from the menu bar, then Scaling and the Range of your logger.

Scale and Engineering Unit Programming

The Simple Logger® Models L320, L410, and L430 allow the operator to program the values for scale and engineering units from within the software.

This permits the user to display the recorded data on the graph or in the tabular listing directly, in the units appropriate to the measurement, rather than mathematically converting a voltage or a current to the proper scale and value after the graph is displayed.

Scales can be programmed from two locations in the software:

- File menu option: Use this option to create a library of scales to use with DC voltage and DC current loggers. This will allow the user to select a number of predefined scales.
- Scale menu option: Use this option to create scales for loggers connected to the serial port for downloading.

The Simple Logger® software allows the operator to define up to 17 points along the scale for DC current measurement and up to 11 points for DC voltage measurement type loggers.

Any combination of points may be used to create the scale, which allows the user to plot both linear and non-linear data. (See Figures 2 and 3).

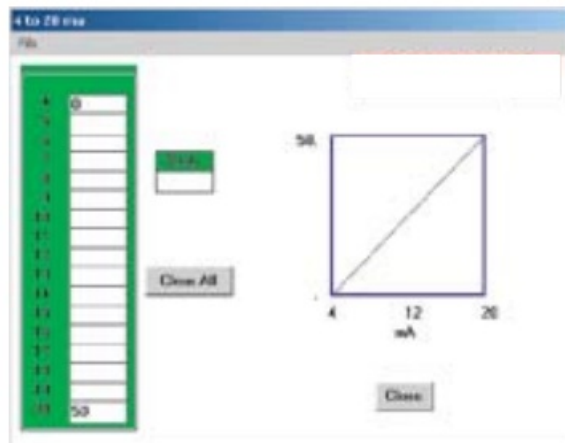


Figure 2

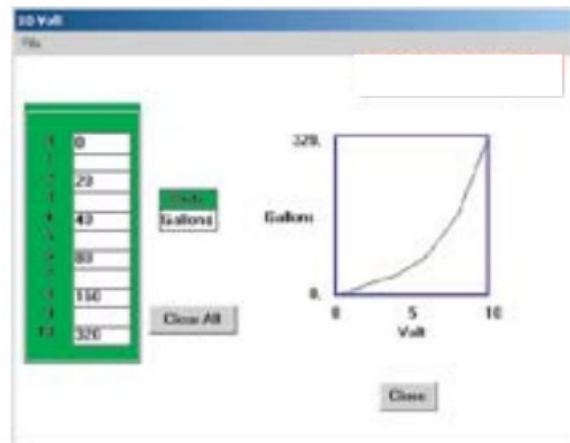


Figure 3

Creating a Library of Scales

- Select File and then Scaling from the main menu.
- Select the type of logger to be scaled from the choices presented.
- A window similar to Figure 4 will appear as soon as you make your selection. This window shows the programmable scale points and the programmable units field. The left screen provides the scale and unit programming, while the right side displays the profile of the programmed scale in relationship to the actual input to the logger.

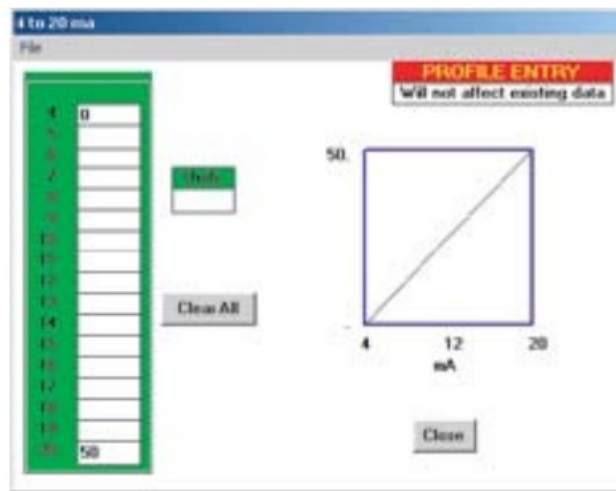


Figure 4

Scale values entered here will not effect the current graph, should one be on the screen. This window is strictly for creating templates to be used at a later date with newly downloaded loggers.

Creating and storing the scales and units here will save you time later on, especially for frequently used scale settings.

Two buttons are available from within this window:

- Clear All button: This will clear all scale numbers entered and any units entered allowing you the opportunity to start over again.
- Close button: Returns to the main menu without saving the data.

Perform the following steps to create a Template:

- Click in any of the blank slots and type in a number (up to 5 characters) to enter a scale value. The minus sign and decimal point can be used as valid characters (e.g. -10.0 would be a valid 5 character number).
As you enter numeric data in the scale slots, the scale profile will appear on the small graph in the right side of the window. Both linear and non-linear profiles are acceptable.
- Once the scale is defined, click in the Units box to program the engineering units to be displayed on the graph. Up to 5 alphanumeric characters may be typed in this box (e.g. PSIG or GPM, etc.).
- After all the data is entered and you are satisfied with the template, click on File at the top left side of the dialog box window.
- Choose one of the available options:
 - Open: Retrieves a previously stored template.
 - Save: Saves the current template you just created for future use.
 - Print: Prints a copy of the scale and unit programming window as seen on the screen.

Creating Scales for Connected Loggers

- Connect the Simple Logger® to the computer's serial port for downloading. See main manual for downloading instructions.
- Once the proper port is selected, data will appear in the update box at the top right hand side of the screen. This is an indication that the software has made connection to the logger. The Scale command will also appear on the task bar if the logger detected allows scale and engineering unit programming.

- A screen similar to Figure 5 will appear. The left side of the screen provides the scale and unit programming, while the right side displays the profile of the programmed scale in relationship to the actual input to the logger.

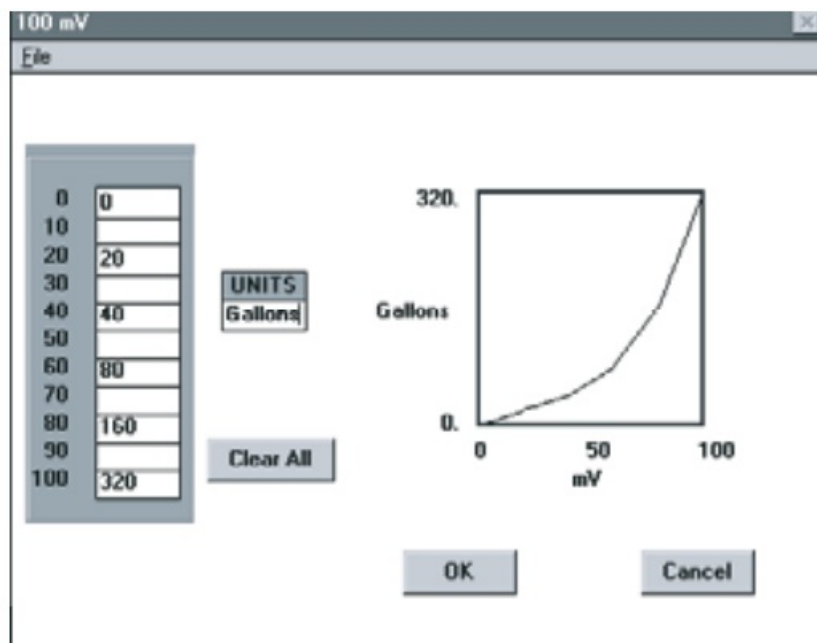


Figure 5

- The operator may set the scale by programming as few as two points, the low end and the high end, or by entering as many points as necessary to define the scale up to 17 points for the 4-20 mA logger and up to 11 points for the DC voltage loggers. The points entered do not have to be linear but should be an accurate representation of the relationship of the DC signal to the scale points.
- To enter a scale value in any of the slots, click on the slot and type in a number up to 5 characters. The minus sign and decimal point may be used as valid characters (e.g. -25.4 would be a valid 5-character number).
- Once the scale is defined, click in the Unit box to program the engineering units to be displayed on the graph. Up to 5 alphanumeric characters may be typed in this box.
- Once you have entered the correct scale and unit data, click on OK to proceed. The screen in Figure 6 will appear giving you the opportunity to save the entered data for future use. Click on Yes to save the data or No to bypass saving the data and use one time only.
- If you click Yes, a dialog box will open similar to Figure 7 where you can type in the name (up to 8 characters) you wish to use for the file.
- Click on OK to save the file and plot the graph with the new scale and unit data or click on Cancel to discard it and return to the scale and unit programming screen.

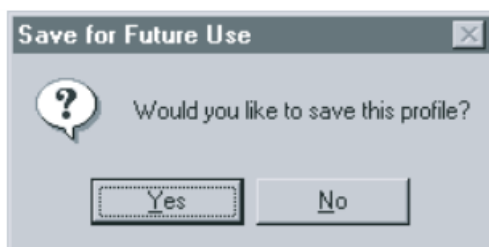


Figure 6

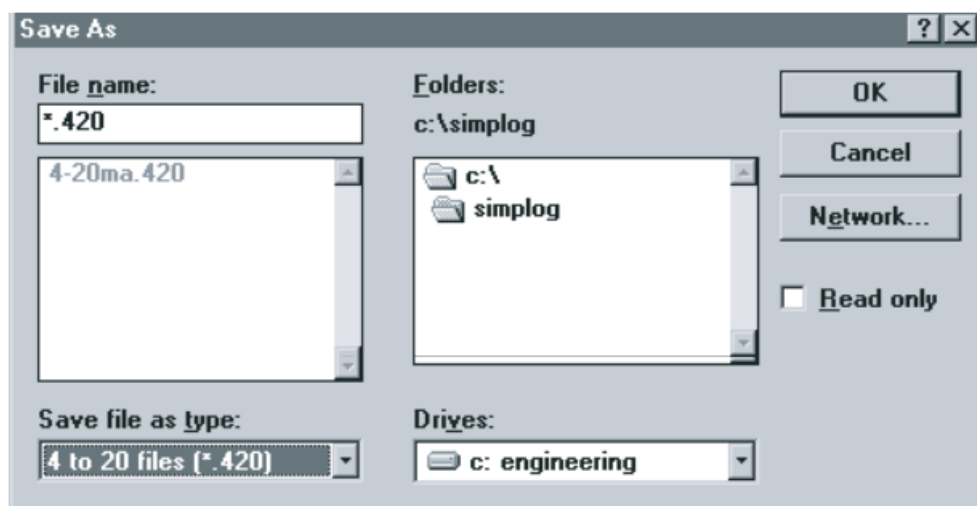


Figure 7

MAINTENANCE

Battery Installation

Under normal conditions, the battery will last up to a year of continuous recording unless the logger is restarted very frequently.

In the OFF mode, the logger puts almost no load on the battery. Use the OFF mode when the logger is not in use. Replace the battery once a year in normal use.

If the logger will be used at temperatures below 32°F (0°C) or is frequently turned on and off, replace the battery every six to nine months.

1. Make sure your logger is turned off (no blinking light) and all inputs are disconnected.
2. Turn the logger upside down. Remove the four Phillips head screws from the base plate, then take off the base plate.
3. Locate the two-wire (red/black) battery connector and attach the 9V battery to it. Make sure that you observe polarity by lining up the battery posts to the proper terminals on the connector.
4. Once the connector is plugged onto the battery, insert the battery into the holding clip on the circuit board.
5. If the unit is not in record mode after installing the new battery, disconnect it and press the button twice then reinstall the battery.
6. Reattach the base plate using the four screws removed in Step 2. Your logger is now recording (LED blinking). Press the PRESS button for five seconds to stop the instrument.

NOTE: For long-term storage, remove the battery to prevent discharge effects.

Cleaning

The body of the logger should be cleaned with a cloth moistened with soapy water. Rinse with a cloth moistened with clean water. Do not use solvent.

APPENDIX A

Importing .TXT Files into a Spreadsheet

Opening a Simple Logger .TXT file in Excel

The following example used with Excel Ver. 7.0 or higher.

1. After opening the Excel program, select “File” from the main menu and then select “Open”.
2. In the dialog box that appears, browse and open the folder where your logger .TXT files are stored. This will be located in C:\Program Files\Simple Logger 6.xx if you accepted the default choice offered by the logger installation program.
3. Next, change the file type to “Text Files” in the field labeled Files of Type. All the .TXT files in the logger directory should now be visible.
4. Double-click on the desired file to open the Text Import Wizard.
5. Review the selections in the first wizard screen and make sure that the following choices are selected:
 - Original Data Type: Delimited
 - Start Import at Row: 1
 - File Origin: Windows (ANSI)
6. Click the “NEXT” button at the bottom of the Wizard dialog box.
The second wizard screen will appear.
7. Click on “Comma” in the Delimiters box. A check mark should appear.
8. Click the “NEXT” button at the bottom of the Wizard dialog box.
The third wizard screen will appear.
9. A view of the actual data to be imported should appear in the lower section of the window. Column 1 should be highlighted. In the Column Data Format window, select “Date”.
10. Next, click on “Finish” to complete the process and import the data.
11. The data will now appear in your spreadsheet in two columns (A and B) and will look similar to that shown in Table A-1.

A	B
8	Arms
35401.49	3.5
35401.49	5
35401.49	9
35401.49	13.5
35401.49	17
35401.49	20
35401.49	23.5
35401.49	27.5
35401.49	31
35401.49	34.5
35401.49	38

Table A-1 – Sample Data Imported into Excel.

Formatting the Date and Time

Column 'A' contains a decimal number that represents both date and time.

Excel can convert this number directly as follows:

1. Click on column 'B' at the top of the column to select the data, then click on "Insert" from the main menu and select "Columns" from the drop-down menu.
2. Next, click on column 'A' at the top of the column to select the data, then click on "Edit" from the main menu and select "Copy" to copy the entire column.
3. Click on cell 1 of column 'B' and then click on "Edit" and select "Paste" to insert a duplicate of column 'A' into column 'B'. This is necessary if you want to show the date and time in two separate columns.
4. Next, click on the top of column 'A', then click on "Format" and select "Cells" from the drop-down menu.
5. In the dialog box that opens, select the "Date" option from the category list on the left. Select the date format you desire and click on "OK" to format the column.
6. Click on the top of column 'B', then click on "Format" and select "Cells" from the drop-down menu.
7. In the dialog box that opens, select the "Time" option from the category list on the left. Select the time format you desire and click on "OK" to format the column.

Table A-2 shows a typical spreadsheet with date, time and value displayed.

It may be necessary to change the column width to see all the data.

A	B	C
12/02/04	11:45 AM	17
12/02/04	11:45 AM	20
12/02/04	11:45 AM	23.5
12/02/04	11:45 AM	27.5
12/02/04	11:45 AM	31
12/02/04	11:45 AM	34.5
12/02/04	11:45 AM	38
12/02/04	11:45 AM	41.5
12/02/04	11:45 AM	45.5
12/02/04	11:46 AM	49
12/02/04	11:46 AM	52

Table A-2 – Shows Date, Time and Value

APPENDIX B

Time-Extension Recording (TXR™)

Time extension recording is an automatic process that updates the sample rate and the number of stored data points based on the length of the recording. The maximum number of stored data points is 8192. When the data logger starts a new recording session, it does so at its fastest sample rate of 4096 points per hour (0.88 seconds per point). The Simple Loggers® can record at this rate for two hours. If the recording session continues beyond two hours, the time extension recording technique becomes active.

Beginning with the sample, after the completion of two hours of recording, the logger continues recording by

selectively overwriting previously stored data. The Simple Logger® also halves its sample rate to 2048/hr (1.76 seconds per point) for the new stored values to be compatible with the previously recorded values. Recording continues for the next two hours at this new rate until the remaining 4096 storage points are filled.

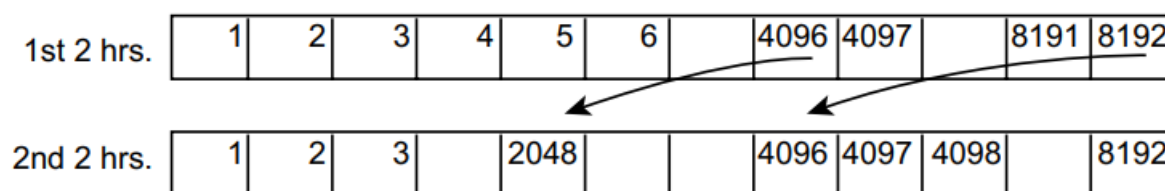


Table B-1 - Time Extension Memory Allocation

The time extension recording process of selectively overwriting previously stored data and halving the sample rate for new stored data continues every time the memory fills up. Table B-2 shows the relationship between recording time and sample rate for the data logger using this technique.

Recording continues in this manner until the battery wears out or recording is stopped. For convenience in data analysis, the recording interval takes on values of fifteen minutes, one-half hour, one hour and so on. Like automatic scaling, time extension recording is practically invisible to the user. For best results, set the logger to standby mode when the measurement is completed, both to avoid including unwanted information in the plot, and to provide maximum resolution for the period of interest.

Sample Rate per hr.	Seconds Per Sample	Total Recording Time (hrs)	Total Recording Time (days)
4096	0.88	2	0.083
2048	1.76	4	0.167
1024	3.52	8	0.333
512	7.04	16	0.667
256	14.08	32	1.333
128	28.16	64	2.667
64	56.32	128	5.333
32	112.64	256	10.667
16	225.28	512	21.333
8	450.56	1024	42.667
4	901.12	2048	85.333
2	1802.24	4096	170.667
1	3604.48	8192	341.333

Repair and Calibration

To ensure that your instrument meets factory specifications, we recommend that it be scheduled back to our factory Service Center at one-year intervals for recalibration, or as required by other standards or internal procedures.

For instrument repair and calibration:

You must contact our Service Center for a Customer Service Authorization Number (CSA#). This will ensure that when your instrument arrives, it will be tracked and processed promptly. Please write the CSA# on the outside of the shipping container. If the instrument is returned for calibration, we need to know if you want a standard calibration, or a calibration traceable to N.I.S.T. (Includes calibration certificate plus recorded calibration data).

Ship To: Chauvin Arnoux®, Inc. d.b.a. AEMC® Instruments
15 Faraday Drive Dover, NH 03820 USA

- Phone: (800) 945-2362 (Ext. 360) (603) 749-6434 (Ext. 360)
- Fax: (603) 742-2346 or (603) 749-6309
- E-mail: repair@aemc.com
- (Or contact your authorized distributor)

Costs for repair, standard calibration, and calibration traceable to N.I.S.T. are available.

NOTE: You must obtain a CSA# before returning any instrument.

Technical and Sales Assistance

If you are experiencing any technical problems, or require any assistance with the proper operation or application of your instrument, please call, mail, fax or e-mail our technical support team:

- Chauvin Arnoux®, Inc. d.b.a. AEMC® Instruments
- 200 Foxborough Boulevard
- Foxborough, MA 02035 USA
- Phone: (800) 343-1391
- (508) 698-2115
- Fax: (508) 698-2118
- E-mail: techsupport@aemc.com
- www.aemc.com
- **NOTE:** Do not ship Instruments to our Foxborough, MA address.

Limited Warranty

The Simple Logger® Model L320/L410/L430 is warranted to the owner for a period of one year from the date of original purchase against defects in manufacture. This limited warranty is given by AEMC® Instruments, not by the distributor from whom it was purchased. This warranty is void if the unit has been tampered with, abused or if the defect is related to service not performed by AEMC® Instruments.

For full and detailed warranty coverage, please read the Warranty Coverage Information, which is attached to the Warranty Registration Card (if enclosed) or is available at www.aemc.com. Please keep the Warranty Coverage Information with your records.

What AEMC® Instruments will do:

If a malfunction occurs within the one-year period, you may return the instrument to us for repair, provided we have your warranty registration information on file or a proof of purchase. AEMC® Instruments will, at its option, repair or replace the faulty material.

REGISTER ONLINE AT: www.aemc.com

Warranty Repairs

What you must do to return an Instrument for Warranty Repair:

First, request a Customer Service Authorization Number (CSA#) by phone or by fax from our Service Department (see address below), then return the instrument along with the signed CSA Form. Please write the CSA# on the outside of the shipping container. Return the instrument, postage or shipment pre-paid to:

Ship To: Chauvin Arnoux®, Inc. d.b.a. AEMC® Instruments
15 Faraday Drive Dover, NH 03820 USA

- **Phone:** (800) 945-2362 (Ext. 360) (603) 749-6434 (Ext. 360)
- **Fax:** (603) 742-2346 or (603) 749-6309
- **E-mail:** repair@aemc.com

Caution: To protect yourself against in-transit loss, we recommend you insure your returned material.

NOTE: You must obtain a CSA# before returning any instrument.

Chauvin Arnoux®, Inc. d.b.a. AEMC® Instruments

15 Faraday Drive


Dover, NH 03820 USA

Phone: (603) 749-6434

Fax: (603) 742-2346

www.aemc.com

Documents / Resources

 <p>L320 L410 L430</p> <p>AEMC</p>	<p>AEMC INSTRUMENTS L430 Simple Logger DC Module [pdf] User Manual L320, L410, L430, L430 Simple Logger DC Module, Simple Logger DC Module, Logger DC Module, DC Module, Module</p>
---	---

References

-  [Get Electrical Testers – Power Analyzers | AEMC Instruments](#)
-  [Search - Manual-Hub.com](#)