



Alecto BC-04 Twin Thermometer Set User Manual

[Home](#) » [Alecto](#) » Alecto BC-04 Twin Thermometer Set User Manual 

Contents

- [1 Alecto BC-04 Twin Thermometer Set](#)
- [2 General](#)
- [3 Temperature](#)
- [4 Cleaning & maintenance:](#)
- [5 Specifications](#)
- [6 Documents / Resources](#)
 - [6.1 References](#)
- [7 Related Posts](#)



Alecto BC-04 Twin Thermometer Set



General

The Alecto TWIN

Thermometer Set allows you to measure the body temperature accurately, quickly and in a simple way. The thermometer set consists of the following 2 thermometers:

- **Model 1, for adults:** for rectal use (between the buttocks), for oral use (in the mouth) or for underneath the armpit
- **Model 2,** pacifier thermometer especially for babies: for oral use (in the mouth) with babies (measurement after 3-5 mins) Before use, read the safety guidelines to prevent endangering your baby. Please retain this manual for future use.

Safety guidelines:

- Never attach a rope or cord to the pacifier thermometer; it might get entangled around your child's neck and cause suffocation.
- Before every use, check the pacifier of the pacifier thermometer for wear and tear and verify that the pacifier is still correctly fastened. Do not longer use a pacifier when loosened or damaged.
- Never use the pacifier thermometer as a regular pacifier.
- Always clean the thermometers before and after use.
- Store the thermometers out of reach of children.
- The thermometer model-1 is suitable only for measuring the temperature of babies underneath the armpit.

Temperature

The temperature of the human body usually falls within the range of 36.5° c to 37.5°C. This temperature depends on a great many factors such as age and the activities directly before measuring the temperature. Additionally, the place where you measure the temperature (between the buttocks, underneath the armpit, in the mouth) and the time of the day influence the temperature (*). When consulting your doctor, always mention how you've measured the temperature.

- Generally, the most accurate way to measure the temperature is rectal use (between the buttocks). An orally (in the mouth) measured temperature is approximately 0.5°C lower than between the buttocks. Furthermore, the temperature measured underneath the armpit is 0.5°C lower than in the mouth. Your temperature in the morning is lower than in the afternoon.

To measure the temperature:

1. Press the power button once and wait until 'X °C' appears with the previous measurement value followed by '37 °C'.
2. Choose which thermometer to use and, based on your choice and the person you're measuring the temperature of, place the thermometer between the buttocks, in the mouth or underneath the armpit.
3. Leave the thermometer in place until you hear beeping tones or until 'X °C' remains constant. You may now read the temperature in the display. Fever alert: above 37.8°C rapid beeps.
4. Press the power button again to switch off the thermometer.
5. Clean and then store the thermometer.

Memory:

The thermometers are provided with a memory for the last measured temperature. As soon as you turn on the

thermometer, at first the last measured temperature will appear in the display together with the letter M. Attention: this display only appears briefly and just once per measurement.

Power supply:

The thermometers are provided with long-life button cell batteries, which last for up to 1000 measurements or 250 hours.


Battery saving function:

In case you forget to switch off the thermometers manually, the thermometers will switch off automatically after 9 minutes.

To replace the thermometer battery:

Model 1:

1. Remove the small screw of the battery cover and push the battery cover of the thermometer.
2. Use a sharp object (not metal) to remove the battery. Insert the new battery with the '+' side downward.
3. Replace the battery cover and tighten the screw again.

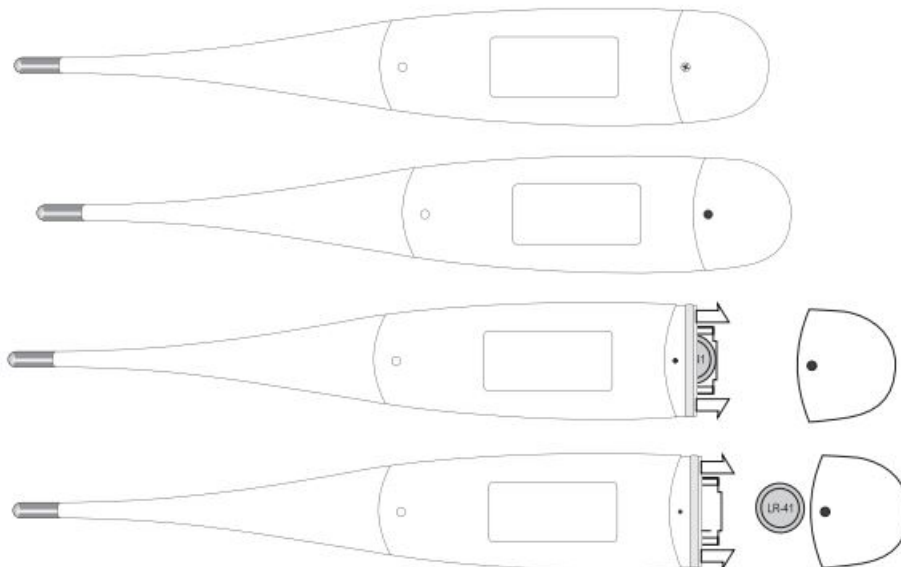

Battery type: 1.5V, LR41 alkaline or equivalent.

Model 2:



■ The battery of this model cannot be replaced. Please return the thermometer to the shop; they'll ensure an environment-friendly disposal.



Cleaning & maintenance:

- After each use, clean the thermometer with a soft, moist cloth or wash it in water.
- Never boil the thermometers, clean them in a dishwasher, place them in a microwave or high-frequency steriliser oven or clean them with chemical cleaning products.

- Don't drop the thermometers and never expose them to vibrations or high temperatures.
- Don't store the thermometers in direct sunlight or near heating equipment. Tip for hygiene: for rectal use (between the buttocks), you may purchase hygienic sleeves from your pharmacist that you can slide over the thermometer (model 1).

DECLARATION OF CONFORMITY



- Hereby, Hesdo declares that the Alecto BC-04 is in compliance with directive 93/42/EEG. The full text of the EU declaration of conformity is available at the following internet address: <http://DOC.hesdo.com/BC-04.pdf>
- Don't simply dispose of empty or exhausted batteries; bring them to your local collection point for Small Chemical Waste.
- Battery-LO indication:  or  (flashing)

Specifications

- **Measuring range:**
 - 32,0 °C ~42,9°C
- **Measuring time:**
 - soother 3~5 min.
 - clinical 10 sec.
- **Accuracy:**
 - $\pm 0,1^{\circ}\text{C}$ for 35~42°C
 - $\pm 0,2^{\circ}\text{C}$ for remaining range at an ambient of 22°C
- **Battery:**
 - LR41 1,5V DC
- **Battery life:**
 - ± 250 hours or
 - 1000 times
- **Weight:**
 - soother 16gr.
 - clinical 10,2gr.

Imported by: Hesdo bv. Aziëlaan 12 5232 BA 's-Hertogenbosch The Netherlands



Manufacturer


Manufacturer TM03 + TM09AS: Cotronic Technology Ltd, Floor4-6, Block 7, West of ZhouShi Road, XiXiang

Street, BaoAn Zone,
Shenzhen, Guangdong, China. Cotronic Technology Ltd Floor 4-6, Block 7, west of ZhouShi road XiXiang Street
BaoAn Zone, ShenZhen, GuangDong China



Well Kang Limited, The Black Church, St. Mary’s Place, Bublin 7, Ireland wellkang Ltd, Enterprise Hub, NW
Business Complex,1 Beraghmore Road, Derry,BT48 8SE, Northern Ireland, UK

Documents / Resources

| | |
|-----------------------------------------------------------------------------------|----------------------------------------------------------------------------------------------------------------------------------------|
|  | <p>Alecto BC-04 Twin Thermometer Set [pdf] User Manual BC-04, Twin Thermometer Set, BC-04 Twin Thermometer Set</p> |
|-----------------------------------------------------------------------------------|----------------------------------------------------------------------------------------------------------------------------------------|

References

- [A Alecto.nl | alectonl](#)