Saved from manuals.plus.
Open the live page for links to other documents and user manuals.

Drive Medical BLS20FBD-SF

Drive Medical Blue Streak Lightweight Wheelchair User Manual

Model: BLS20FBD-SF

Introduction

This manual provides essential instructions for the safe and effective use, setup, and maintenance of your Drive Medical Blue Streak Lightweight Wheelchair. Designed for dependable, comfortable mobility, this wheelchair features a durable steel frame, smooth-rolling wheels, and a compact folding design for easy transport and storage.

Please read this manual thoroughly before operating the wheelchair and retain it for future reference.

Safety Information

General Safety Guidelines

- Always engage the wheel locks before transferring in or out of the wheelchair.
- Ensure all components are securely fastened before each use.
- Do not exceed the maximum weight capacity of 300 pounds.
- Avoid using the wheelchair on uneven or excessively sloped surfaces without assistance.
- Regularly inspect the wheelchair for any signs of wear or damage.

Legal Disclaimer

It is solely the buyer's responsibility to choose the correct item. Please note our policies are set by the manufacturers we represent. No return will be accepted after 14 calendar days from the purchase date and without a valid RMA#. Returns are subject to a 15% restock fee plus the cost of outbound & inbound shipping costs. Any return request after the 14 day period will be decided on a case by case basis depending on the product & circumstances & is subject to a restocking fee up to 60%.

Setup Instructions

1. **Unfolding the Wheelchair:** Place the folded wheelchair on a flat, stable surface. Grasp the seat rails and push outwards until the wheelchair is fully open and the seat is flat. Ensure the frame locks into place.



Image: The Drive Medical Blue Streak Lightweight Wheelchair, fully unfolded and ready for use.

2. **Attaching Footrests:** Align the footrest hangers with the receiving brackets on the front of the wheelchair frame. Push down firmly until they click into place. The swing-away footrests can be adjusted or removed as needed for transfers.



Image: Detailed view of the swing-away footrests, highlighting their functionality for easy transfers.

3. **Adjusting Flip-Back Desk Arms:** The desk arms can be flipped back to allow closer access to tables or desks. To do so, locate the release lever near the armrest pivot point and lift the armrest upwards and backward.



Image: User comfortably positioned at a table, showcasing the convenience of the flip-back desk arms.

Setup Video Guide

Your browser does not support the video tag.

Video: A comprehensive guide demonstrating the unboxing, setup, and initial use of the Drive Medical Blue Streak Wheelchair.

Operating Instructions

1. **Engaging Wheel Locks:** To secure the wheelchair, push the lever on each wheel lock forward until it engages with the tire. Ensure both locks are fully engaged before attempting transfers or when stationary.



Image: Detailed view of the push-to-lock wheel mechanism, illustrating how to secure the wheelchair.

2. **Self-Propelling:** Grasp the handrims on the large rear wheels and push forward to move. Use both hands for steering and propulsion. For assistance, a caregiver can use the push handles located at the back of the chair.



Image: A user being assisted by a caregiver, highlighting the wheelchair's maneuverability.

3. **Folding for Transport/Storage:** To fold the wheelchair, first remove the footrests. Then, pull up on the center of the seat upholstery until the sides of the wheelchair begin to collapse inward. Continue pulling until fully folded.



Image: The wheelchair in its folded state, demonstrating how it fits into a vehicle for transport.

Operation Video Guide

Your browser does not support the video tag.

Video: Demonstrating the comfortable and easy maneuverability of the Drive Medical Blue Streak Wheelchair.

Maintenance

- **Cleaning:** The breathable and easy-to-clean nylon fabric seat and backrest can be wiped down with a damp cloth and mild soap. Avoid abrasive cleaners.

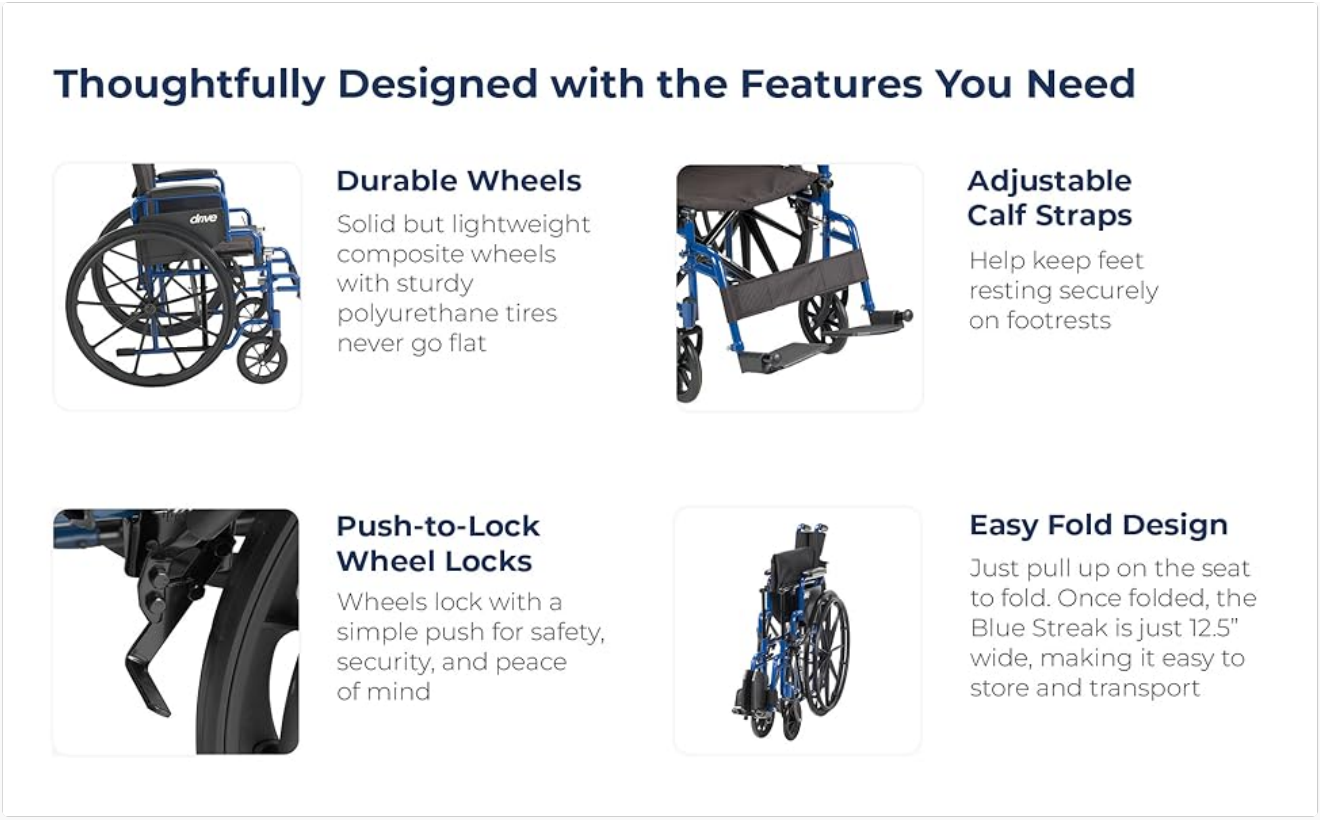


Image: Cleaning the durable nylon upholstery of the wheelchair.

- **Wheel Inspection:** Periodically check the solid, maintenance-free tires for debris and ensure they roll smoothly.
- **Hardware:** Inspect all nuts, bolts, and fasteners regularly to ensure they are tight. Do not overtighten.

Specifications

Feature	Detail
Brand	Drive Medical
Model Number	BLS20FBD-SF
Color	Blue
Item Weight	41.3 pounds
Product Dimensions (D x W x H)	12.5"D x 26"W x 36"H
Seat Width	20 inches
Seat Height	20 inches
Seat Depth	16 inches
Maximum Weight Recommendation	300 pounds
Frame Material	Alloy Steel
Wheel Type	Solid
Brake Style	Push-to-Lock
Included Components	Wheelchair with Flip Back Desk Arms, 20 in Seat and Swing-Away Footrests



Image: Key dimensions and weight capacity of the wheelchair.

Warranty Information

The Drive Medical Blue Streak Lightweight Wheelchair comes with a**3 Year Limited Warranty**. Please refer to the warranty documentation included with your product for full details on coverage and terms. Keep your proof of purchase for warranty claims.

Support

For additional support, troubleshooting, or to view other Drive Medical products, please visit the official Drive Medical store or website:

Drive Medical Store: Visit the Drive Medical Store on Amazon

Official Website: DriveMedical.com

© 2023 Drive Medical. All rights reserved.

Ask a question about this manual

Ask about setup, troubleshooting, compatibility, parts, safety, or missing instructions. Manuals+ will review the question and use this page's manual context to help answer it.

Name

Anonymous

Email

you@example.com

After a successful submission, we securely hash the supplied account or form email before sending it to Microsoft Advertising for conversion attribution. Privacy details.

Question

Example: How do I reset this device or fix this error?

Details

Model number, symptoms, what you tried, or the section of the manual you are using.

Submit question

Open the live page

https://manuals.plus/asin/B008KMKUGO

More documents and user manuals: **https://manuals.plus/**