Saved from manuals.plus.
Open the live page for links to other documents and user manuals.

Braun IRT6500US

Braun ThermoScan 5 Ear Thermometer User Manual

Model: IRT6500US

1. Overview

The Braun ThermoScan 5 Ear Thermometer provides clinically validated accuracy, making it a trusted tool for monitoring body temperature. Utilizing infrared technology, it delivers rapid temperature results. Its design incorporates a pre-warmed tip for enhanced accuracy and comfort, along with the ExacTemp Stability Indicator that confirms correct positioning in the ear through a light and an audible beep. The device also features a memory function to recall the last nine temperature readings.





Figure 1: Braun ThermoScan 5 Ear Thermometer with digital display.

2. Key Features

- **ExacTemp Stability Indicator:** A light and beep confirm stable positioning for accurate readings.
- **Pre-warmed Tip:** Ensures accurate results by minimizing the cooling effect of the probe.
- **Memory Function:** Stores the last nine temperature measurements for easy tracking.
- **Disposable Hygiene Caps:** Includes 21 caps to maintain hygiene and prevent cross-contamination.
- **Fast Readings:** Provides temperature results in seconds.

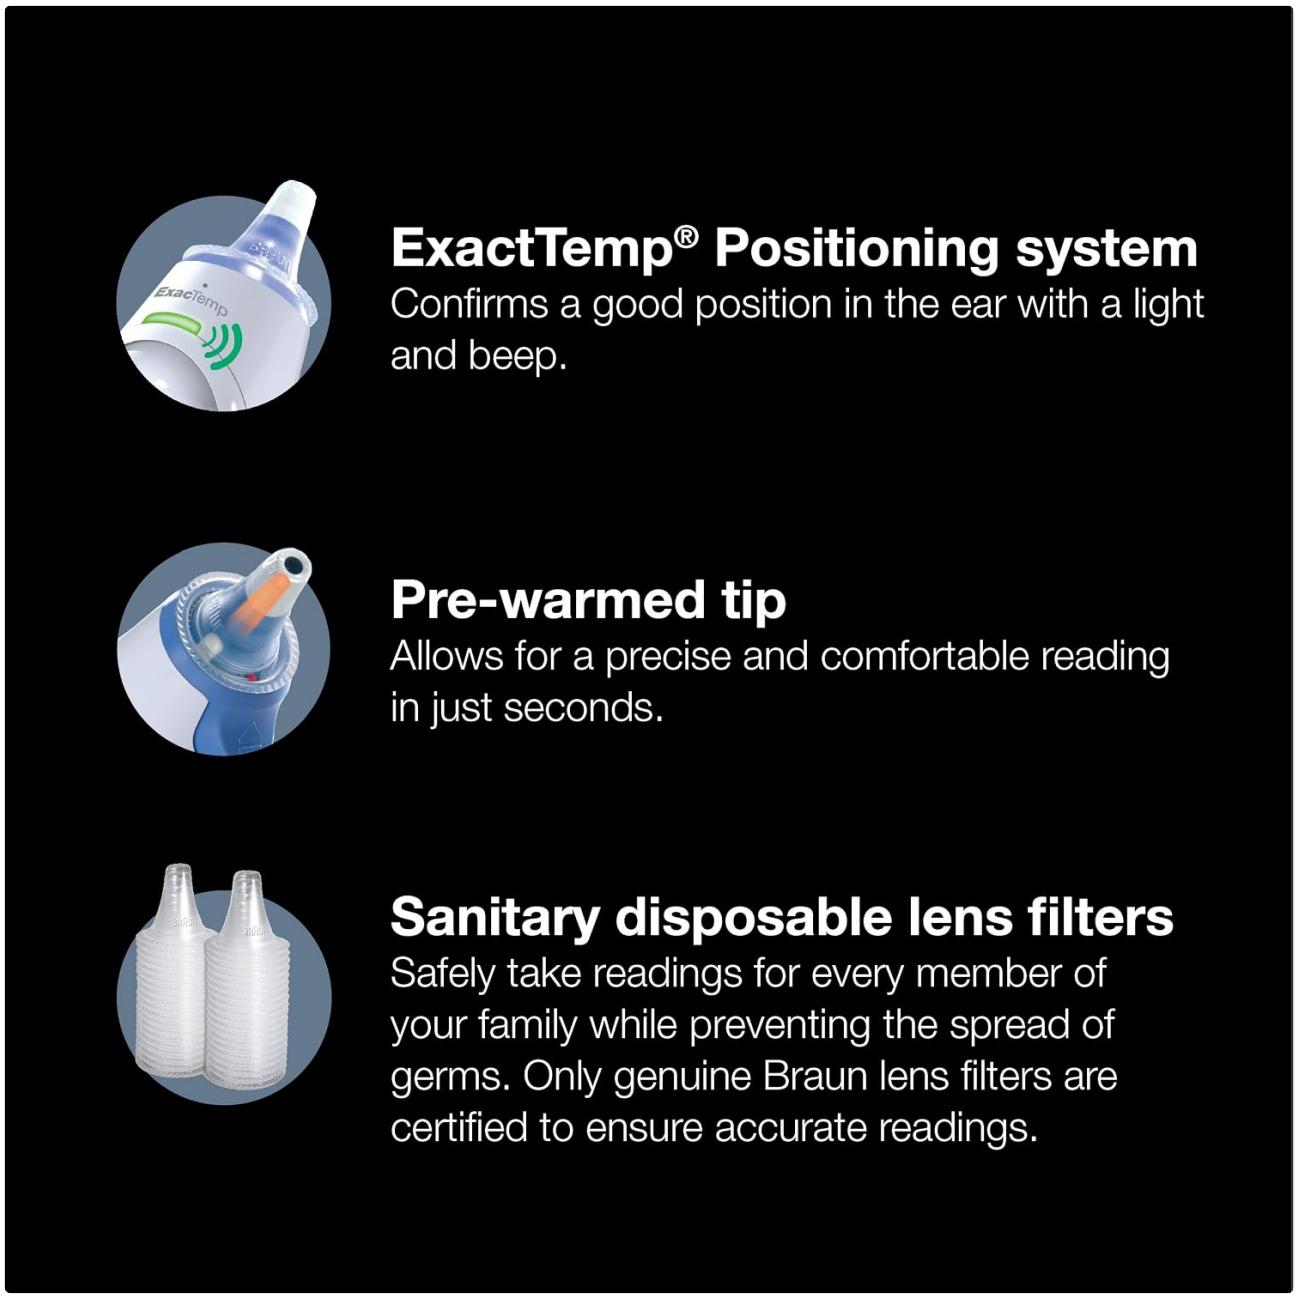


Figure 2: Illustration of ExacTemp Positioning, Pre-warmed Tip, and Sanitary Lens Filters.

3. Package Contents

Your Braun ThermoScan 5 Ear Thermometer package should contain the following items:

- Braun ThermoScan 5 Ear Thermometer
- Protective Cradle/Cap for storage
- 21 x Disposable Hygiene Caps
- 2 x AA Alkaline Batteries (included)



Figure 3: All items included in the product package.

4. Setup

4.1. Installing Batteries

The thermometer requires 2 AA batteries. To install or replace them, slide open the battery compartment cover located at the bottom of the device. Insert the batteries, ensuring correct polarity (+/-), then close the cover securely.

4.2. Attaching a Hygiene Cap

Before each measurement, attach a new, clean disposable hygiene cap to the thermometer tip. Push the tip firmly into the cap until it clicks into place. The thermometer will not function without a hygiene cap properly attached.

4.3. Changing Temperature Units (Fahrenheit/Celsius)

The Braun ThermoScan 5 can display temperatures in either Fahrenheit (°F) or Celsius (°C). Refer to the full user manual for specific instructions on how to switch between these units, as the method may vary slightly by model version.



Figure 4: Labeled components of the thermometer.

5. Operating Instructions

Follow these steps to take an accurate temperature reading:

1. Ensure a new, clean hygiene cap is securely attached to the thermometer tip.
2. Press the Power button () to turn on the thermometer. Wait for the display to show 'READY' or three lines, indicating it's prepared for measurement.
3. Gently insert the probe tip into the ear canal. For accurate readings, ensure the probe is positioned correctly. The ExacTemp Stability Indicator will help confirm proper placement.
4. Press the Temperature button (thermometer icon) and hold it down.
5. Release the button once you hear a long beep and the ExacTemp light confirms stable positioning. The temperature reading will be displayed on the screen.
6. After measurement, press the Lens Release button to eject the used hygiene cap into a waste bin.



Figure 5: Proper use of the thermometer for temperature measurement.

6. Maintenance and Care

6.1. Cleaning

To clean the thermometer, wipe the exterior surfaces with a soft, dry cloth. For the probe tip, use an alcohol swab or cotton swab moistened with alcohol. Ensure no liquid enters the thermometer casing. Do not immerse the thermometer in water or any cleaning solution.

6.2. Hygiene Caps

Always use a new, clean Braun disposable hygiene cap for each measurement to ensure hygiene and accuracy. Replace the cap after every use to prevent the spread of germs and maintain optimal performance.

6.3. Storage

Store the thermometer in its protective cradle/cap in a dry place, away from direct sunlight and extreme

temperatures. Remove batteries if the device will not be used for an extended period.

7. Troubleshooting

If you encounter issues with your Braun ThermoScan 5, consider the following common solutions:

- **No Power/Display Issues:** Check if the batteries are correctly inserted and have sufficient charge. Replace batteries if necessary.
- **Inaccurate Readings:** Ensure a new, clean hygiene cap is used. Verify the probe is inserted correctly and stably in the ear canal (listen for the ExacTemp beep). Avoid taking measurements immediately after bathing or intense physical activity.
- **Error Messages:** Refer to the full user manual for specific error code explanations and solutions.

If problems persist, contact Braun customer support for further assistance.

8. Specifications

Model Number	IRT6500US
Product Dimensions	1.5 x 1.88 x 5.85 inches
Weight	6.24 ounces
Power Source	Battery Powered (2 AA batteries)
Display Type	Digital
Manufacturer	Braun
Recommended Age	1 month and up
Care Instructions	Wipe Clean

9. Warranty and Support

For detailed warranty information and customer support, please refer to the official Braun website or the full user manual provided with your product. You can also access the digital user guide here.

© 2023 Braun. All rights reserved.

Ask a question about this manual

Ask about setup, troubleshooting, compatibility, parts, safety, or missing instructions. Manuals+ will review the question and use this page's manual context to help answer it.

Name

Anonymous

Email

you@example.com

After a successful submission, we securely hash the supplied account or form email before sending it to Microsoft Advertising for conversion attribution. Privacy details.

Question

Example: How do I reset this device or fix this error?

Details

Model number, symptoms, what you tried, or the section of the manual you are using.

Submit question

Open the live page

https://manuals.plus/asin/B00MUK6M82

More documents and user manuals: **https://manuals.plus/**