Saved from manuals.plus.
Open the live page for links to other documents and user manuals.

Braun IRT3030

Braun ThermoScan 3 Ear Thermometer User Manual

Model: IRT3030

Introduction

The Braun ThermoScan 3 Ear Thermometer is designed to provide fast, accurate, and reliable temperature measurements. It is suitable for use by the whole family, including infants and adults. This manual provides essential information on how to set up, operate, maintain, and troubleshoot your device to ensure optimal performance and accurate readings.



Image: The Braun ThermoScan 3 Ear Thermometer shown alongside a stack of disposable lens filters, highlighting the product and its essential accessories.

Key features include 1-second measurement, an audio fever indicator, and a memory function that recalls the last temperature taken. For hygienic use and accurate results, always use a new disposable lens filter for each measurement.

Setup

1. Battery Installation

Your Braun ThermoScan 3 requires 1 AAA battery, which is included. To install or replace the battery:

1. Locate the battery compartment cover on the device.
2. Slide the cover off.
3. Insert the AAA battery, ensuring the correct polarity (+ and -) as indicated inside the compartment.
4. Slide the battery compartment cover back into place until it clicks securely.

2. Attaching a New Lens Filter

For accurate readings and hygienic use, a new disposable lens filter must be attached before each measurement.

1. Ensure the thermometer is off.
2. Gently push the thermometer probe into a new disposable lens filter until it clicks into place.
3. Do not attempt to take a reading without a lens filter attached, as this can affect accuracy and hygiene.



Image: A close-up of the Braun ThermoScan 3 thermometer with a disposable lens filter correctly attached to its probe, ready for use.

Operating Instructions

Taking a Temperature Reading

1. Ensure a new, clean disposable lens filter is securely attached to the probe.
2. Press the power button to turn on the thermometer. The display will show the last measured temperature for a few seconds.
3. Gently insert the probe tip into the ear canal, ensuring it is pointing towards the eardrum. For children, gently pull the earlobe back to straighten the ear canal.
4. Press the measurement button. A beep will sound, indicating the measurement is complete (approximately 1 second).

5. Remove the thermometer from the ear and read the temperature displayed on the screen.



Image: An adult's hand gently inserting the Braun ThermoScan 3 thermometer into a child's ear, demonstrating proper usage for temperature measurement.

Audio Temperature Indicator

The ThermoScan 3 provides audio cues to help interpret temperature readings:

- **1 Beep:** Indicates a normal temperature (approximately 98.6°F / 37.0°C).
- **2 Beeps:** Indicates a slightly elevated temperature (approximately 99.5°F / 37.5°C).
- **4 Beeps:** Indicates a fever (approximately 101.5°F / 38.6°C or higher).

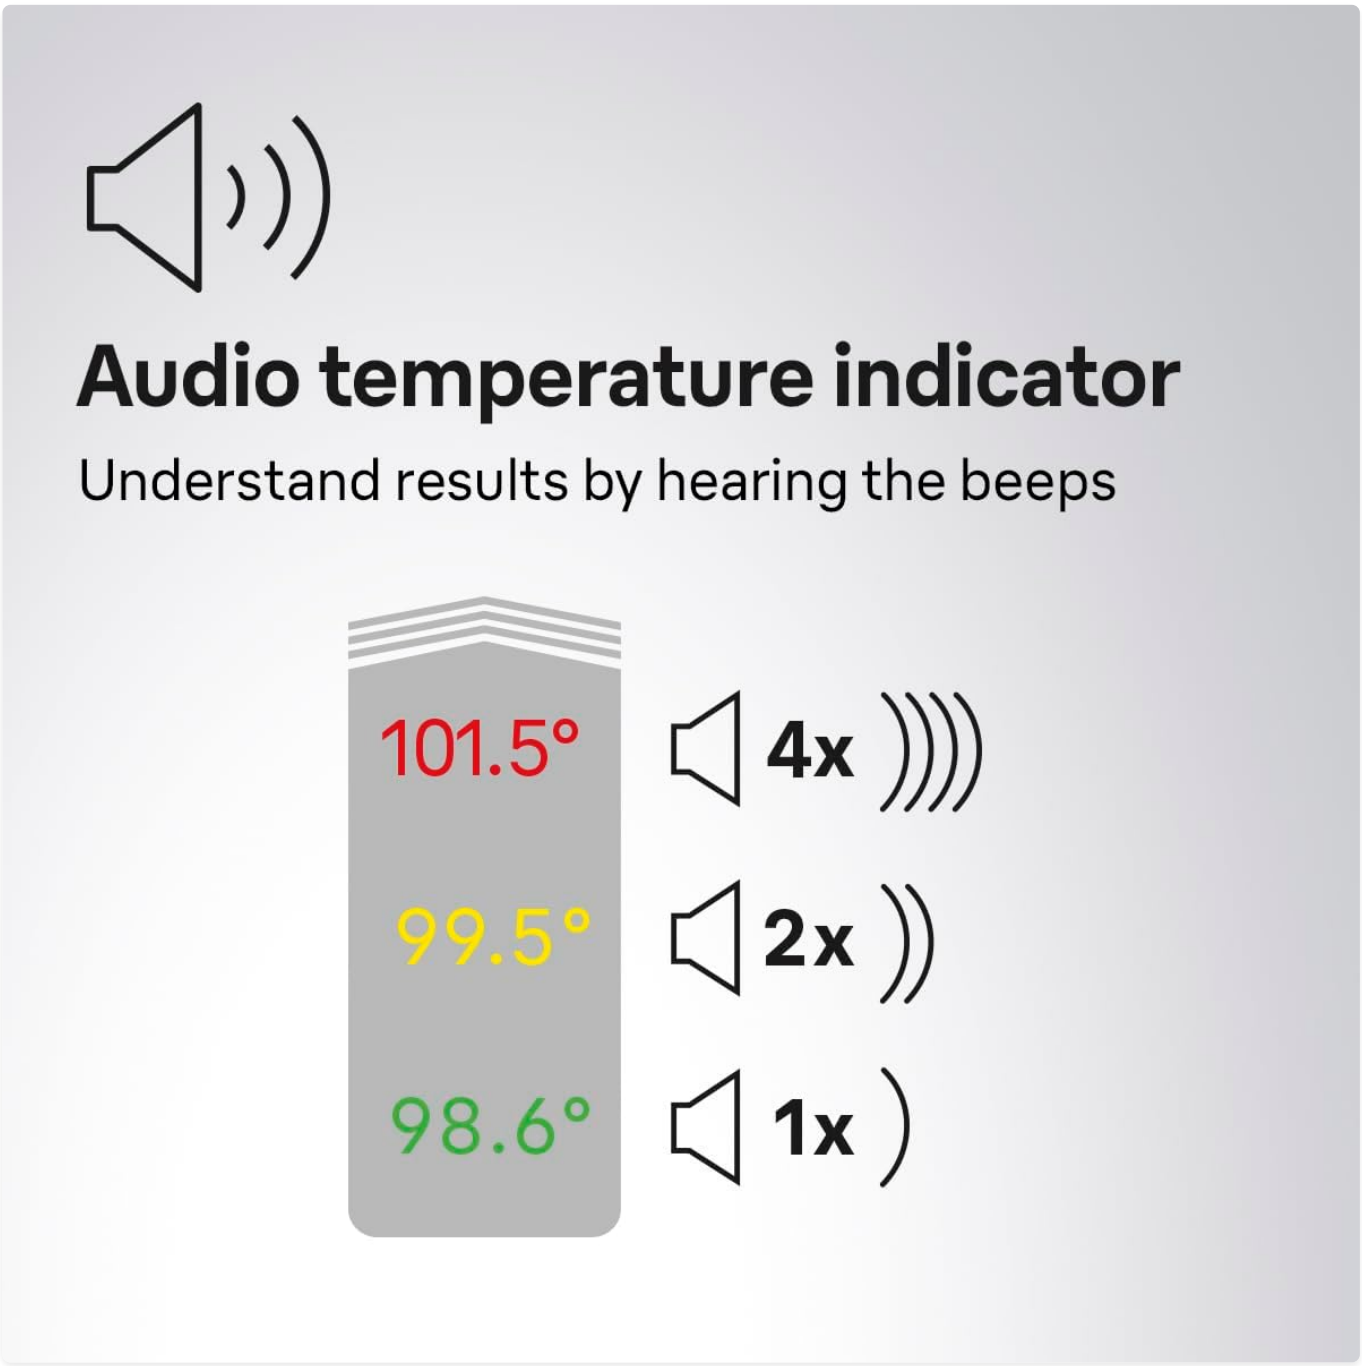


Image: A visual representation of the audio temperature indicator, showing different temperature ranges (green, yellow, red) corresponding to 1, 2, or 4 beeps, indicating normal, elevated, or fever temperatures.

Memory Function

The thermometer automatically recalls the last temperature taken. This reading will be displayed briefly when the device is powered on.

Maintenance

Cleaning the Thermometer

To ensure hygiene and proper functioning, clean your thermometer regularly:

- Use a soft, dry cloth to clean the thermometer display and exterior.
- Do not use abrasive cleaners or submerge the thermometer in water or any other liquid.
- The probe tip should only be cleaned by replacing the disposable lens filter. Do not clean the probe directly with liquids or cloths.

Storage

Store the thermometer and disposable lens filters in a dry location, free from dust and contamination, and away from direct sunlight. Keep out of reach of children.

Replacing Disposable Lens Filters

Always replace the disposable lens filter after each use to ensure hygiene, prevent cross-contamination, and maintain measurement accuracy. Used filters should be discarded responsibly.

Troubleshooting

Problem	Possible Cause	Solution
Thermometer does not turn on.	Dead or incorrectly installed battery.	Check battery polarity or replace with a new AAA battery.
Inaccurate or inconsistent readings.	Used or dirty lens filter; improper probe placement; earwax obstruction.	Always use a new lens filter. Ensure probe is correctly inserted and pointing towards the eardrum. Check for earwax.
Display shows "POS" or similar positioning error.	Probe not correctly positioned in the ear canal.	Re-insert the probe, ensuring it is snug and pointing towards the eardrum.

Specifications

Feature	Detail
Model Number	IRT3030
Product Dimensions	3.9 x 1.5 x 7.9 inches
Weight	4.66 ounces
Batteries	1 AAA battery (included)
Measurement Time	1 second
Display Type	Digital
Special Features	Fast Reading System, Audio Fever Indicator
Color	White
Material	Plastic

Warranty and Support

For information regarding product warranty, please refer to the warranty card included with your product packaging or visit the official Braun Healthcare website. For additional support, frequently asked questions, or to download the full user guide, please visit the manufacturer's support page.
A digital version of the user guide is available here:Braun ThermoScan 3 User Guide (PDF)
Please note that protection plans mentioned on product listings are typically extended service agreements and not the standard manufacturer's warranty.

Official Product Videos

No official product videos from the seller were found in the provided product information.

© 2023 Braun. All rights reserved.

Ask a question about this manual

Ask about setup, troubleshooting, compatibility, parts, safety, or missing instructions. Manuals+ will review the question and use this page's manual context to help answer it.

Name

Anonymous

Email

you@example.com

After a successful submission, we securely hash the supplied account or form email before sending it to Microsoft Advertising for conversion attribution. Privacy details.

Question

Example: How do I reset this device or fix this error?

Details

Model number, symptoms, what you tried, or the section of the manual you are using.

Submit question

Open the live page

https://manuals.plus/asin/B01MA1S4SM

More documents and user manuals: **https://manuals.plus/**