Beurer IH 60

Beurer IH 60 Portable Nebulizer Instruction Manual

Model: IH 60 (602.06)

Introduction

The Beurer IH 60 Nebulizer is a compact and silent inhaler designed for the treatment of upper and lower respiratory tracts. Utilizing compressed air technology, it effectively nebulizes liquid medication into fine particles, allowing active ingredients to penetrate deeply into the respiratory system. Its portable design and rechargeable battery make it ideal for use at home or while traveling. This manual provides essential information for the safe and effective operation and maintenance of your device.

Package Contents

Before first use, please ensure all components are present in the package:

- Nebulizer unit
- Mouthpiece
- Nosepiece
- Adult mask
- Children's mask
- Compressed air hose
- Mains adapter
- Filter
- Storage bag
- Transport bag



Image: The Beurer IH 60 Nebulizer unit displayed with all included accessories, such as masks, mouthpiece, nosepiece, air hose, and carrying cases.

Important Safety Information

Please read this entire instruction manual carefully before using the Beurer IH 60 Nebulizer. Keep this manual for future reference. Consult your doctor or pharmacist for any questions regarding medication or treatment plans. This device is intended for personal use and should not be shared without proper disinfection. Do not use the device near flammable gases or vapors.

Setup Instructions

1. Charging the Device

The Beurer IH 60 features a rechargeable lithium-ion battery. Before initial use, fully charge the device using the provided mains adapter. Connect the adapter to the nebulizer and a power outlet. The charging indicator lights will show the charging status.

2. Assembling the Nebulizer

1. Ensure all parts are clean and disinfected before assembly.
2. Connect the compressed air hose to the air outlet on the nebulizer unit and to the medication container.
3. Attach the desired accessory (mouthpiece, nosepiece, adult mask, or children's mask) to the medication container.



Image: A detailed view of the Beurer IH 60 Nebulizer, illustrating the connection points for the air hose and medication container, highlighting its compressed air technology.

Operating Instructions

1. Preparing for Inhalation

1. Open the medication container and pour the prescribed amount of medication into it. Do not overfill.
2. Close the medication container securely.

2. Starting Inhalation

1. Press the power button on the nebulizer unit to turn it on. The device will begin to produce a fine mist.
2. Position the mouthpiece, nosepiece, or mask comfortably on your face.

3. During Inhalation

Breathe calmly and deeply through the chosen accessory. Continue until the medication is fully nebulized, which typically takes a short duration due to the efficient nebulization rate of approximately 0.25 ml/min. The device is designed for quiet operation, enhancing user comfort.



Image: A woman demonstrating the use of the Beurer IH 60 Nebulizer, holding the mask comfortably over her face during an inhalation session.



Image: A man relaxing on a sofa, illustrating the quiet and comfortable experience of using the Beurer IH 60 Nebulizer for respiratory therapy.

Care and Maintenance

1. Cleaning the Nebulizer

After each use, disassemble the medication container and accessories. Wash them thoroughly with warm water and a mild detergent. Rinse well and allow to air dry completely. The nebulizer unit itself should be wiped with a damp cloth. The device and its accessories can be disinfected to ensure hygiene.

2. Filter Replacement

The air filter should be checked regularly and replaced when it appears discolored or after approximately 100-120 operating hours, or as indicated in the full user manual. Using a clean filter ensures optimal performance and hygiene.

Troubleshooting

Problem	Possible Cause	Solution
Device does not turn on or charge.	Low battery; faulty connection; device malfunction.	Ensure the device is fully charged. Check the mains adapter connection. If issues persist, contact customer support.
No mist or weak mist production.	Insufficient medication; clogged air filter; improper assembly.	Ensure correct medication level. Replace the air filter if dirty. Reassemble components correctly.
Accessories (mask/mouthpiece) do not stay attached securely.	Improper attachment; worn out accessory.	Ensure accessories are firmly clicked into place. Replace if worn or damaged.

Technical Specifications

- **Model:** IH 60 (602.06)
- **Dimensions (L x W x H):** 11 x 4.7 x 6.2 cm
- **Weight:** 222 grams
- **Nebulization Rate:** Approximately 0.25 ml/min
- **Particle Size (MMAD):** 4.1 µm
- **Technology:** Compressed Air Technology (DC compressor)
- **Battery:** 1 Lithium-ion (included)
- **Power Supply:** Mains adapter
- **Country of Origin:** China

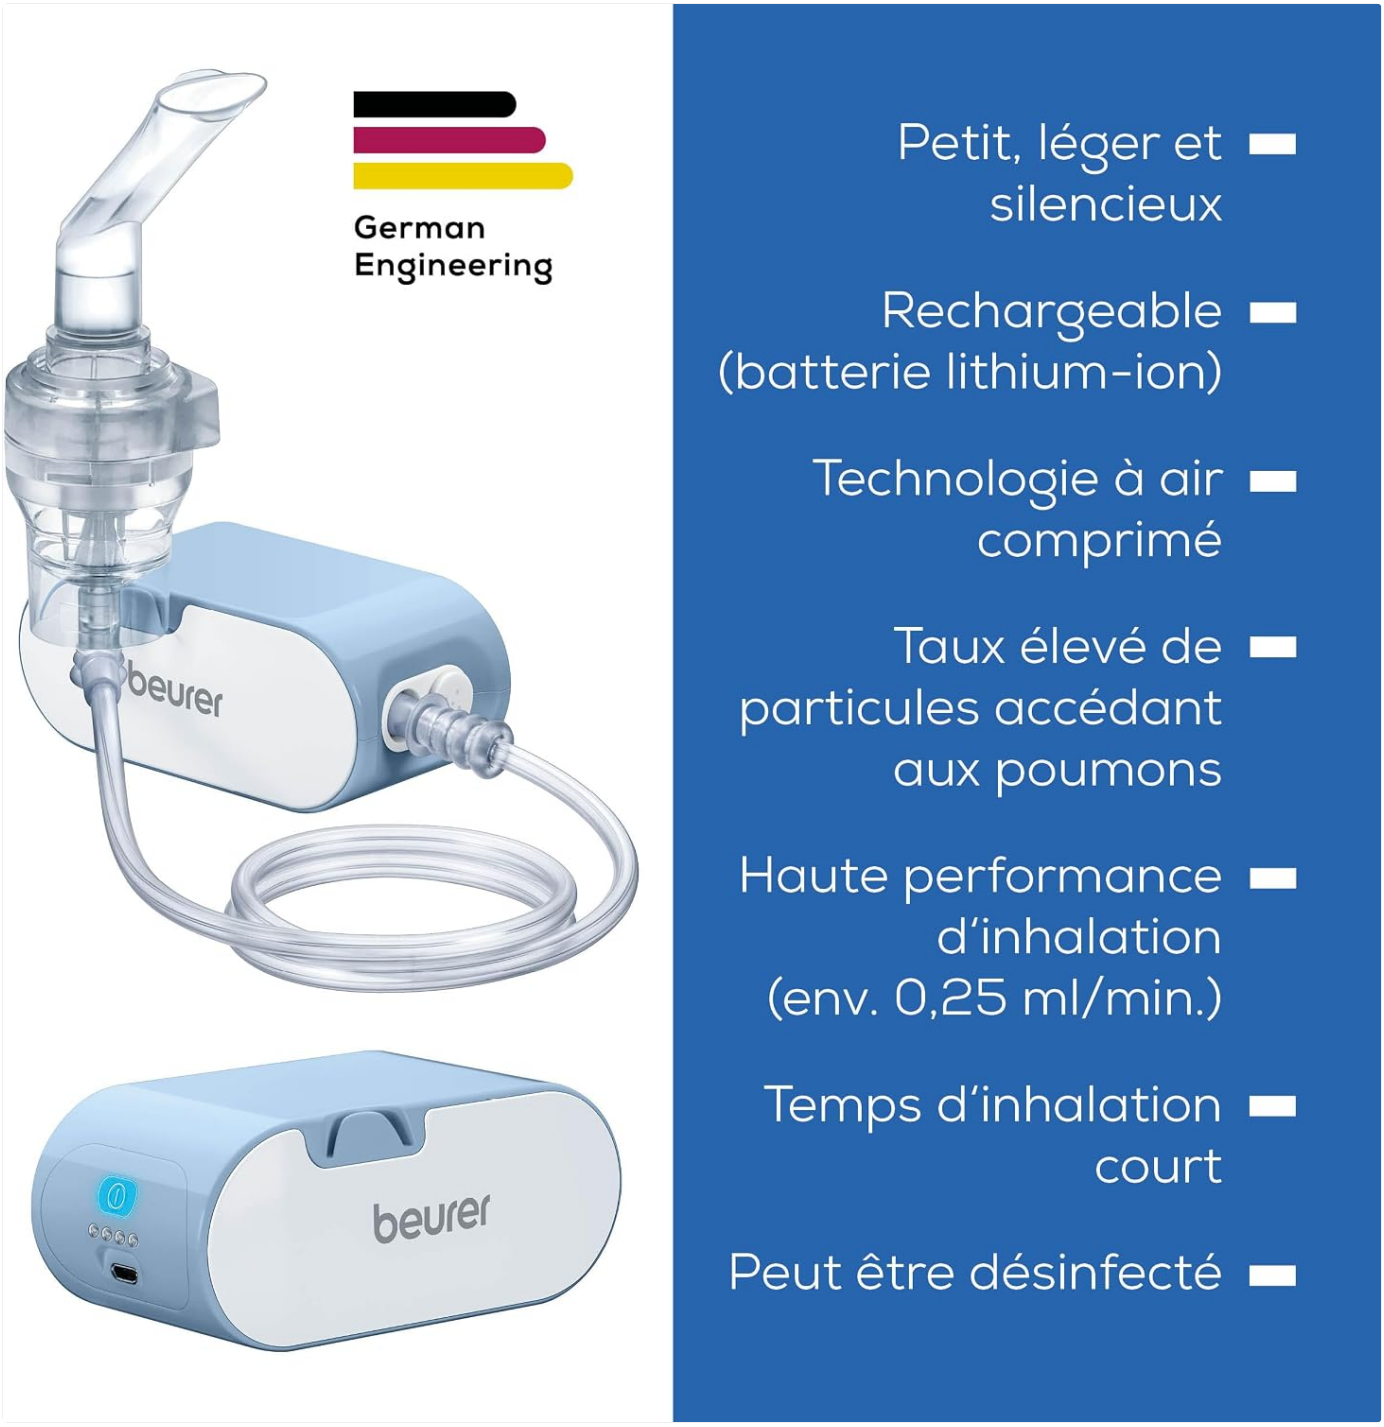


Image: An infographic summarizing the key features of the Beurer IH 60 Nebulizer, including its compact size, rechargeable battery, compressed air technology, and high nebulization performance.

Warranty and Customer Support

Beurer products are manufactured to the highest quality standards. In the event of a defect, please refer to your purchase documentation for warranty details. For technical assistance, spare parts, or further inquiries, please contact Beurer customer support. Contact information can typically be found on the official Beurer website or within the product packaging.

Ask a question about this manual

Ask about setup, troubleshooting, compatibility, parts, safety, or missing instructions. Manuals+ will review the question and use this page's manual context to help answer it.

Name

Anonymous

Email

you@example.com

After a successful submission, we securely hash the supplied account or form email before sending it to Microsoft Advertising for conversion attribution. Privacy details.

Question

Example: How do I reset this device or fix this error?

Details

Model number, symptoms, what you tried, or the section of the manual you are using.

Submit question