GLO Science FETEGT173

GLO Science GLO Brilliant Advanced White Smile Teeth Whitening Device Kit Instruction Manual

Introduction

This manual provides detailed instructions for the safe and effective use of your GLO Science GLO Brilliant Advanced White Smile Teeth Whitening Device Kit. Please read all instructions carefully before initial use and retain this manual for future reference.

Product Components

The GLO Brilliant Advanced White Smile Teeth Whitening Device Kit includes the following components:

- GLO Brilliant Warming Mouthpiece
- GLO Control and Lanyard with heat indicator light
- USB Charging Cable
- GLO Vegan Lip Care
- Teeth Whitening GLO Vials (Mint Flavor)



Image: Overview of the GLO Science GLO Brilliant Advanced White Smile Teeth Whitening Device Kit components, including the mouthpiece, control, charging cable, lip care, and whitening vials.



Image: Detailed view of the kit contents, showing the GLO Control, GLO Brilliant Warming Mouthpiece, USB Charging Cable, GLO Vegan Lip Care, and five Teeth Whitening GLO Vials.

Safety Information

Keep out of reach of children. Avoid contact with skin and eyes. If ingested, seek medical help immediately. Store in a cool, dry place and use as directed.

Ingredients

GLO VIALS INGREDIENTS: 6% Hydrogen Peroxide, Mint Flavor. Net Wt. 5 x 2.9 ml (0.1 oz). Distilled Water, Polyethylene Glycol, Hydrogen Peroxide, Potassium Nitrate, Glycerin, Edetate Disodium, Sodium Saccharin, Sodium Fluoride, Sodium Hydroxide, Flavor.
GLO® VEGAN LIP CARE INGREDIENTS: Ricinus Communis (Castor) Seed Oil, Myrica Cerifera (Bayberry) Wax, Helianthus Annuus (Sunflower) Seed Wax, Mentha Piperita (Peppermint) Oil, Butyrospermum Parkii (Shea) Nut Butter *, Menthol, Medium Chain Triglyceride, Tocopherol, Triolein, Copernicia Cerifera (Carnauba) Wax *, Glyceryl Dioleate, Ceramide Np, Monoammonium Glycyrrhizinate, Natural Flavor, Ethyl, Alcohol.

Setup

1. Open the product packaging and ensure all components are present.
2. Before first use, fully charge the GLO Brilliant Advanced Teeth Whitening Control using the provided USB charging cable. The indicator light will show charging status.
3. Apply the GLO Vegan Lip Care to your lips to protect them during the whitening process.
4. Twist off the cap of a GLO Whitening Vial and apply a thin layer of the whitening gel directly to your teeth, avoiding the gums.
5. Insert the GLO Brilliant Warming Mouthpiece into your mouth.
6. Connect the mouthpiece to the GLO Control.

Operating Instructions

Follow these steps for an effective whitening session:

1. After setup, press the button on the GLO Control to initiate an 8-minute whitening session. The mouthpiece will illuminate and warm up.
2. Keep the mouthpiece in your mouth for the full 8-minute duration.
3. Once the session concludes, the device will automatically turn off.
4. For optimal results, immediately repeat the application of gel and another 8-minute session up to three more times.
5. Repeat this entire process for 5 consecutive days for one full treatment cycle.



Image: A visual guide demonstrating the five steps for using the GLO Brilliant device: Apply Lip Care, Apply Whitening Gel to Teeth, Insert Illuminated Mouthpiece, Complete 8-Minute Session, and Immediately Repeat 3 More Times.

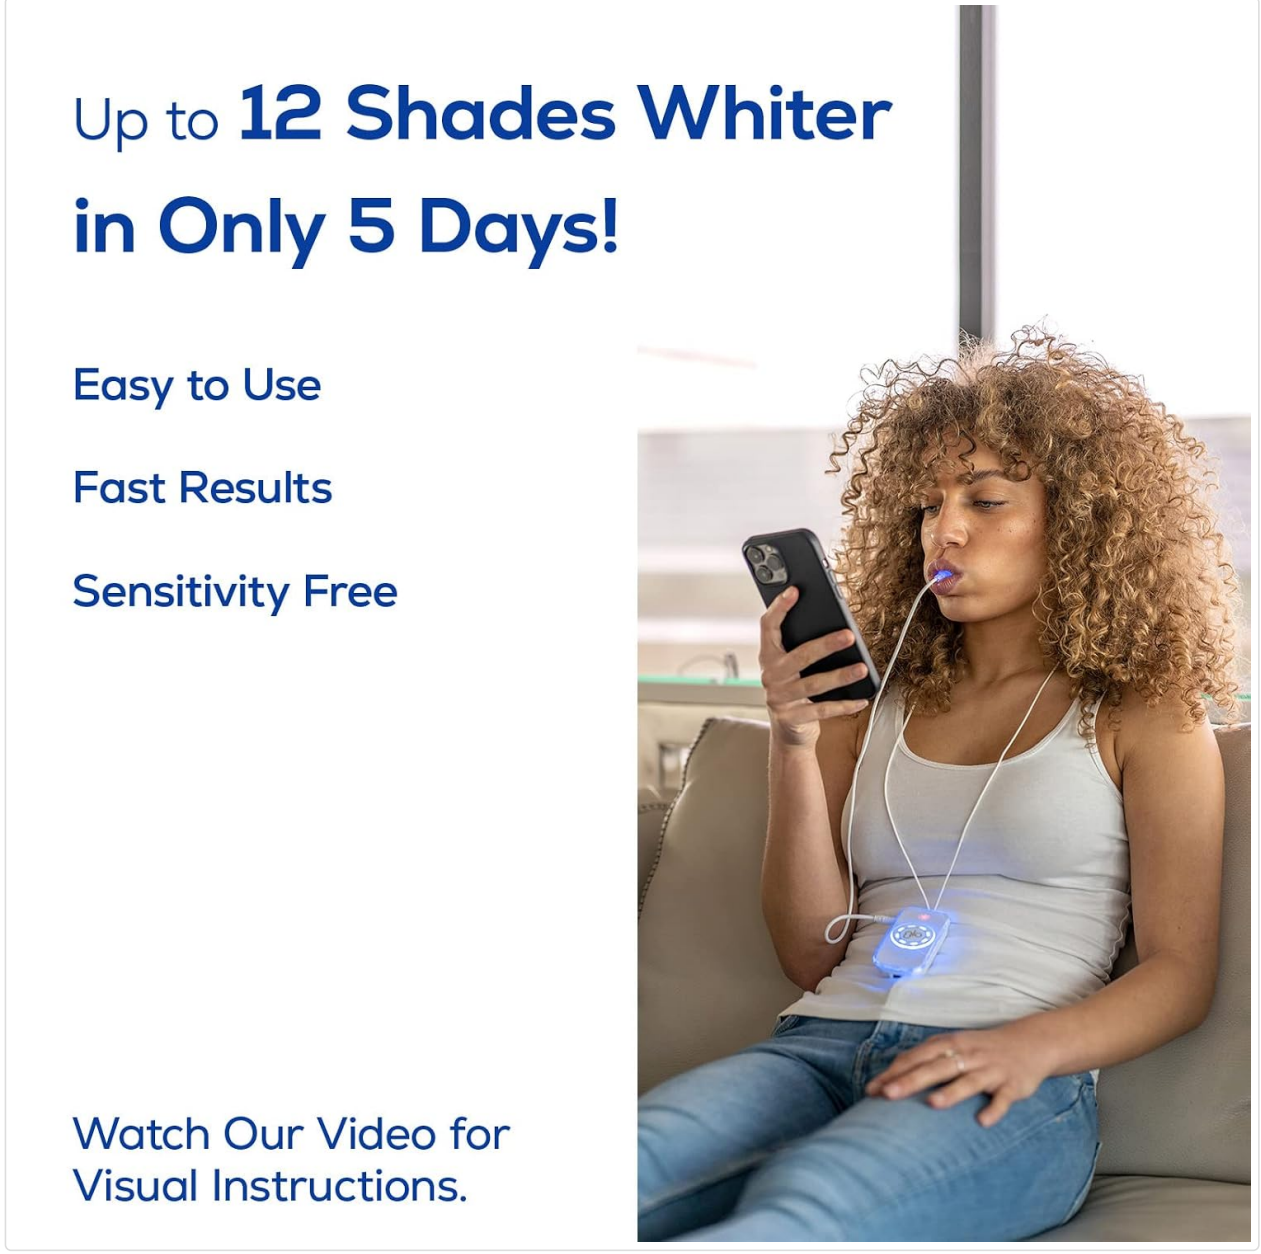


Image: A person using the GLO Brilliant Advanced White Smile device, with the mouthpiece inserted and the control unit hanging around their neck, illustrating typical use.

The patented warming mouthpiece technology accelerates the whitening process. For more information on this technology, refer to the diagram below:



Image: A diagram explaining the advanced continuous warming mouthpiece technology, highlighting how it safely and quickly catalyzes hydrogen peroxide for more effective and efficient teeth whitening.

Maintenance

- **Cleaning the Mouthpiece:** After each use, rinse the mouthpiece thoroughly with water. Do not submerge the GLO Control unit in water.
- **Charging:** Recharge the GLO Control unit as needed. A full charge typically provides power for multiple whitening sessions.
- **Storage:** Store the device and vials in a cool, dry place away from direct sunlight.

Troubleshooting

- **Device Not Turning On:** Ensure the GLO Control unit is fully charged. Connect it to the USB charging cable and allow sufficient time to charge.
- **Reduced Battery Life:** Battery performance can vary over time. Ensure the device is fully charged before each use. If battery life significantly diminishes, contact customer support.
- **Gum Sensitivity or Irritation:** If you experience gum sensitivity, ensure that the whitening gel is applied only to the teeth and not to the gums. Reduce the frequency of use or consult a dental professional if irritation persists.
- **No Whitening Results:** Ensure consistent use as directed (5 consecutive days for a full treatment). Verify that the mouthpiece is properly connected and illuminating during sessions.

Specifications

Feature	Detail
Product Dimensions	22 x 16 x 16 inches; 1 ounces

Item Model Number	FETEGT173
UPC	850030314079
Brand	GLO Science
Product Benefits	A brighter smile up to 12 shades whiter in 5 days, without sensitivity.
Item Form	Gel
Number of Items	1
Material Type Free	Bisphenol A Free, Diethanolamine Free, Mineral Oil Free, Phthalate Free, Triclosan Free, Sugar Free, Sulfate Free
GTIN	850030314079

Warranty Information

The GLO Science GLO Brilliant Advanced White Smile Teeth Whitening Device Kit typically includes a 1-year limited warranty from the date of purchase. Please refer to the warranty card included in your product packaging or visit the official GLO Science website for complete warranty terms and conditions.

Customer Support

For further assistance, product inquiries, or technical support, please visit the official GLO Science website or contact their customer service department. You can find more information and products at the GLO Science Store on Amazon.