Saved from manuals.plus.
Open the live page for links to other documents and user manuals.

Hurchen Lift Transfer Chair

Hurchen Patient Lift Transfer Chair Instruction Manual

Model: Lift Transfer Chair

1. Introduction

This manual provides essential information for the safe and effective use of your Hurchen Patient Lift Transfer Chair. Please read all instructions carefully before assembly and operation. Proper use ensures the safety and comfort of the user and caregiver.

Safety Information

- Maximum weight capacity: 275 lbs. Do not exceed this limit.
- Ensure all locking mechanisms are engaged before transferring a patient.
- Always use the seat belt to secure the patient during transfer.
- The patient should be able to sit upright independently or with minimal assistance for safe use.
- Exercise caution when moving the chair over uneven surfaces.
- Regularly inspect all components for wear or damage. Do not use if damaged.



Figure 1: The Hurchen Patient Lift Transfer Chair in operation, assisting a user from a bed.

2. Components Overview

The Hurchen Patient Lift Transfer Chair is designed with several key components for functionality and safety:

- **Main Frame:** Constructed from thickened painted steel pipes for durability and stability.
- **Detachable Backrest:** Made with PU foam molding technology for optimal back support.
- **Wheels:** Four silent, non-slip 360° rotating wheels, all equipped with brakes for secure positioning.

- **Armrests:** Soft armrests for user comfort.
- **Foot Pads:** Rubber foot pads with anti-slip texture for enhanced safety.
- **Seat Cushions:** Includes two types: a newly upgraded hard seat cushion (PE board and sponge-filled) and a soft toilet seat cushion with an open design.
- **Seat Belt:** Adjustable length with metal buckles for patient stability.
- **Lifting Crank:** Manual crank for adjusting the chair's height.
- **Adjustable Base:** Allows for width adjustment to navigate various spaces.



Figure 2: The two included seat cushions: a hard cushion for general use and a soft toilet seat cushion with an open design.

3. Setup and Assembly

The Hurchen Patient Lift Transfer Chair is designed for easy installation and disassembly without the need for specialized tools. Follow these steps for assembly:

1. Unpack all components and verify against the parts list.
2. Attach the wheels to the base frame. Ensure the two wheels with brakes are installed at the front.
3. Secure the main vertical support to the base.
4. Install the armrests by aligning them with the designated holes and inserting the fixing pins.

5. Attach the seat cushion by securing the four buckles to the armrest frame.
6. Insert the backrest into the corresponding holes on the armrest frame.
7. Ensure all pins and fasteners are securely in place before use.

Assembly Video

Your browser does not support the video tag.

Video 1: Detailed installation guide for the Hurchen Patient Lift Transfer Chair, demonstrating step-by-step assembly.

Additional Assembly Video

Your browser does not support the video tag.

Video 2: Visual instructions on how to install the patient lift chair, covering key assembly points.

4. Operating Instructions

The Hurchen Patient Lift Transfer Chair simplifies patient transfers, reducing caregiver strain and enhancing patient dignity. It can be used as a patient transfer device, wheelchair, bedside commode, or shower chair.

Transferring a Patient

1. Position the chair close to the patient. Ensure the patient is able to sit upright or can be assisted to an upright position.
2. Adjust the chair's height using the lifting crank to match the height of the bed, sofa, or other surface. The height can be adjusted between 33.5 to 45 inches.
3. Adjust the base width using the rocker to fit around furniture or through doorways (width adjustable between 22.8 to 29.5 inches).
4. Engage all wheel brakes to prevent movement.
5. Assist the patient to place their feet on the foot pads and hold onto the armrests.
6. Fasten the seat belt securely around the patient.
7. Disengage the wheel brakes and carefully move the chair to the desired location.
8. Once in position, engage the wheel brakes, adjust height as needed, and unfasten the seat belt to allow the patient to transfer.



Figure 3: The lifting crank allows for easy height adjustment to suit various patient needs and transfer scenarios.



Figure 4: The adjustable base width allows the chair to navigate various environments and fit around different furniture types.

Operational Videos

Your browser does not support the video tag.

Video 3: Demonstration of the deluxe model patient lift in various home settings, showcasing its functionality.

Your browser does not support the video tag.

Video 4: Illustrates the patient lift aid for home use, including transfer to a shower or as a wheelchair.

Your browser does not support the video tag.

Video 5: An operation video demonstrating the patient lift for home use, highlighting ease of movement.

Your browser does not support the video tag.

Video 6: Shows various applicable scenarios for patient lifts, demonstrating versatility in different environments.

Your browser does not support the video tag.

Video 7: Features the patient lift functioning as a wheelchair, highlighting its mobility.

Car Transfer

The chair's lightweight, detachable, and compact design allows for easy storage and transport, making it suitable for car transfers. It can be placed in a car trunk without occupying excessive space.

Your browser does not support the video tag.

Video 8: Demonstrates the patient lift transfer chair being used as a portable car lift aid, showing ease of use for vehicle transfers.

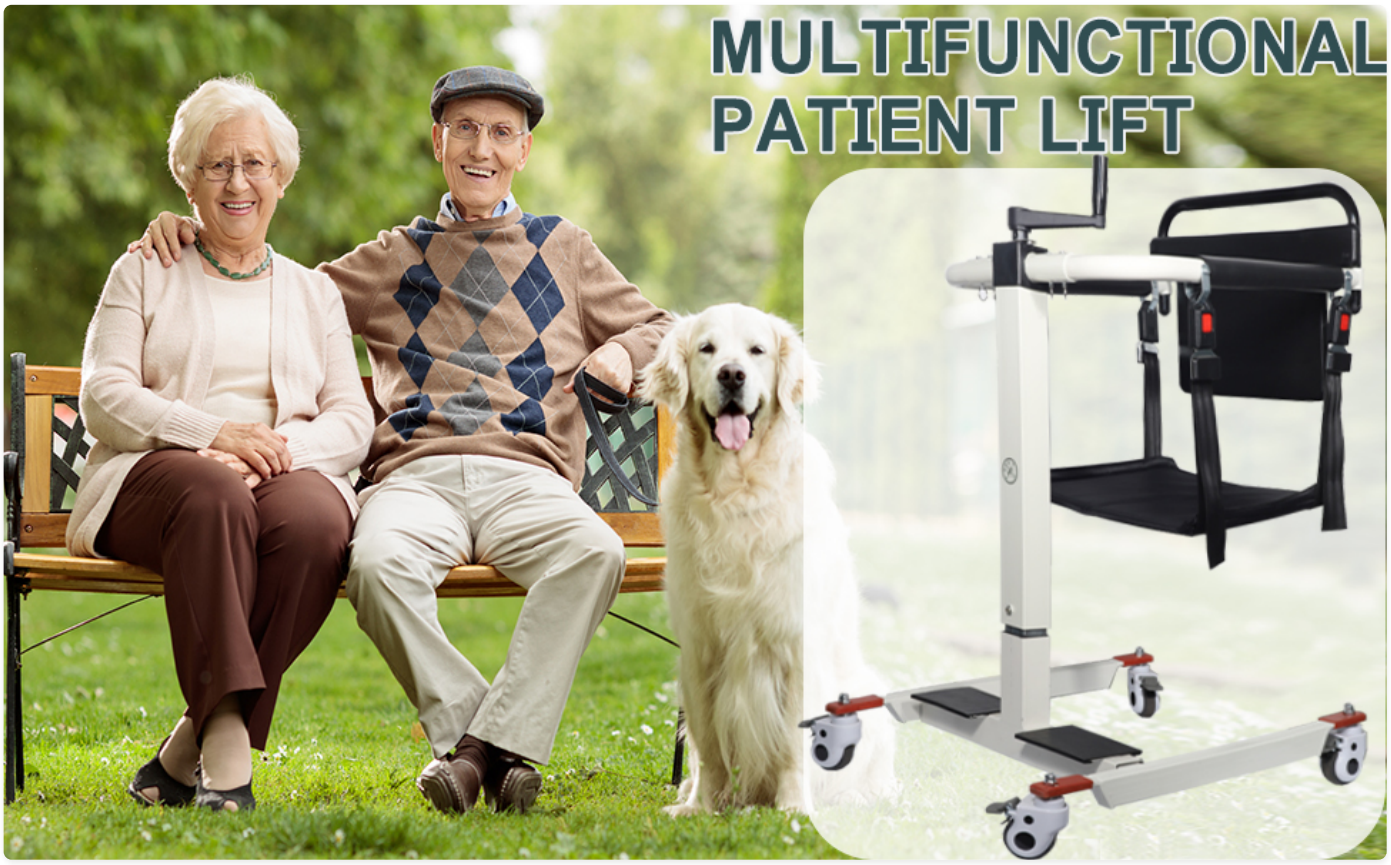


Figure 5: The transfer chair can be easily disassembled and stored in a car trunk for convenient transportation.

5. Maintenance

To ensure the longevity and safe operation of your Hurchen Patient Lift Transfer Chair, regular maintenance is recommended:

- **Cleaning:** Wipe down the frame and components with a damp cloth and mild detergent. Avoid abrasive cleaners.
- **Inspection:** Periodically check all screws, bolts, and pins to ensure they are tight and secure.
- **Wheel Care:** Keep the wheels free of debris and ensure they rotate smoothly. Test the brakes regularly.
- **Cushion Care:** Clean seat cushions as needed according to their material.

6. Troubleshooting

If you encounter any issues with your Hurchen Patient Lift Transfer Chair, refer to the following common solutions:

- **Chair not moving smoothly:** Check for debris in the wheels. Ensure brakes are fully disengaged.
- **Difficulty adjusting height:** Ensure the lifting crank is properly engaged and free of obstructions.
- **Instability during transfer:** Verify all locking pins are secured and the seat belt is properly fastened. Ensure the base width is appropriate for the transfer.
- **Unusual noises:** Inspect all moving parts for loose connections or wear. Contact customer support if the issue persists.

7. Specifications

Feature	Specification

Product Dimensions	29.5"D x 20.4"W x 24.5"H
Item Weight	46.3 Pounds (21 Kilograms)
Maximum Load Capacity	275 lbs
Adjustable Height Range	33.5 to 45 inches
Adjustable Width Range	22.8 to 29.5 inches
Material	Thickened painted steel pipes, PU foam
Model Number	Lift Transfer Chair

8. Warranty and Support

Hurchen is committed to customer satisfaction. Your Patient Lift Transfer Chair comes with the following:

- **One-Year Warranty:** Covers manufacturing defects and major component failures.
- **30-Day Return Guarantee:** For your peace of mind.
- **Free Component Replacement:** During the warranty period, damaged parts such as seat cushions, casters, seat belt buckles, or screws will be replaced free of charge.
- **Customer Support:** Our professional team is available to assist you with any questions or concerns. Please refer to your purchase documentation for contact information.

© 2026 Hurchen. All rights reserved.

Ask a question about this manual

Ask about setup, troubleshooting, compatibility, parts, safety, or missing instructions. Manuals+ will review the question and use this page's manual context to help answer it.

Name

Anonymous

Email

you@example.com

After a successful submission, we securely hash the supplied account or form email before sending it to Microsoft Advertising for conversion attribution. Privacy details.

Question

Example: How do I reset this device or fix this error?

Details

Model number, symptoms, what you tried, or the section of the manual you are using.

Submit question

Open the live page

https://manuals.plus/asin/B0C13BH3L1

More documents and user manuals: **https://manuals.plus/**