Saved from manuals.plus.
Open the live page for links to other documents and user manuals.

YUYTE yuytekepx12a0zc

YUYTE Vaginal Test Strips Instruction Manual

Model: yuytekepx12a0zc

1. Introduction

The YUYTE Vaginal Test Strips are designed for quick and intuitive detection of vaginal pH levels, aiding in the assessment of vaginal health. These disposable strips provide accurate results to help monitor and maintain intimate health.

Each package contains 100 test strips, offering a convenient supply for regular monitoring. The strips are formulated to resist VC interference, ensuring reliable readings.



Image: YUYTE Vaginal Test Strips packaging and individual strips, showing the product bottle and several loose strips.

This manual provides detailed instructions on how to use, maintain, and understand the results from your YUYTE Vaginal Test Strips.

2. Purpose of Use

These test strips are intended for self-assessment of vaginal pH levels. Monitoring vaginal pH can help identify potential imbalances that may lead to discomfort or indicate a need for further medical consultation. The product is suitable for use when experiencing symptoms such as itching, unusual odor, or pain, as well as for general daily health monitoring.



Image: This image illustrates common situations when the vaginal test strips can be used, including symptoms like itching, peculiar smell, pain, and for routine daily health checks.

3. Setup and Preparation

Before using the test strips, ensure you have a clean, well-lit area. No complex setup is required for this product.

3.1 Unpacking

- Carefully open the product packaging.
- Remove the sealed bottle containing the 100 test strips.
- Ensure the bottle is intact and sealed before first use.



Image: The bottle of YUYTE Vaginal Test Strips, opened to show the individual strips stored inside, with a blurred background of a person holding their abdomen.

3.2 Important Pre-Test Considerations

- Avoid sexual activity within 24 hours prior to testing.
- Do not wash private parts or bathe immediately before testing.
- Do not use vaginal douches or other vaginal products before testing.
- This product is not suitable for individuals with diabetes, during menstruation, or for pregnant women.

4. Operating Instructions

Follow these steps to accurately use the YUYTE Vaginal Test Strips:

1. **Prepare the Strip:** Open the sealed bottle and carefully remove one test strip. Close the bottle immediately to protect the remaining strips from moisture.
2. **Collect Sample:** Using a clean cotton swab, collect a sample of female vaginal secretion.
3. **Apply Sample:** Apply the collected secretion onto the reactive pad of the test strip. Ensure the pad is adequately

moistened.

4. **Wait:** Allow 30 seconds for the reaction to occur. Keep the strip in a normal light and temperature environment.
5. **Read Results:** Compare the color change on the test strip's reactive pad with the color chart provided on the product packaging.

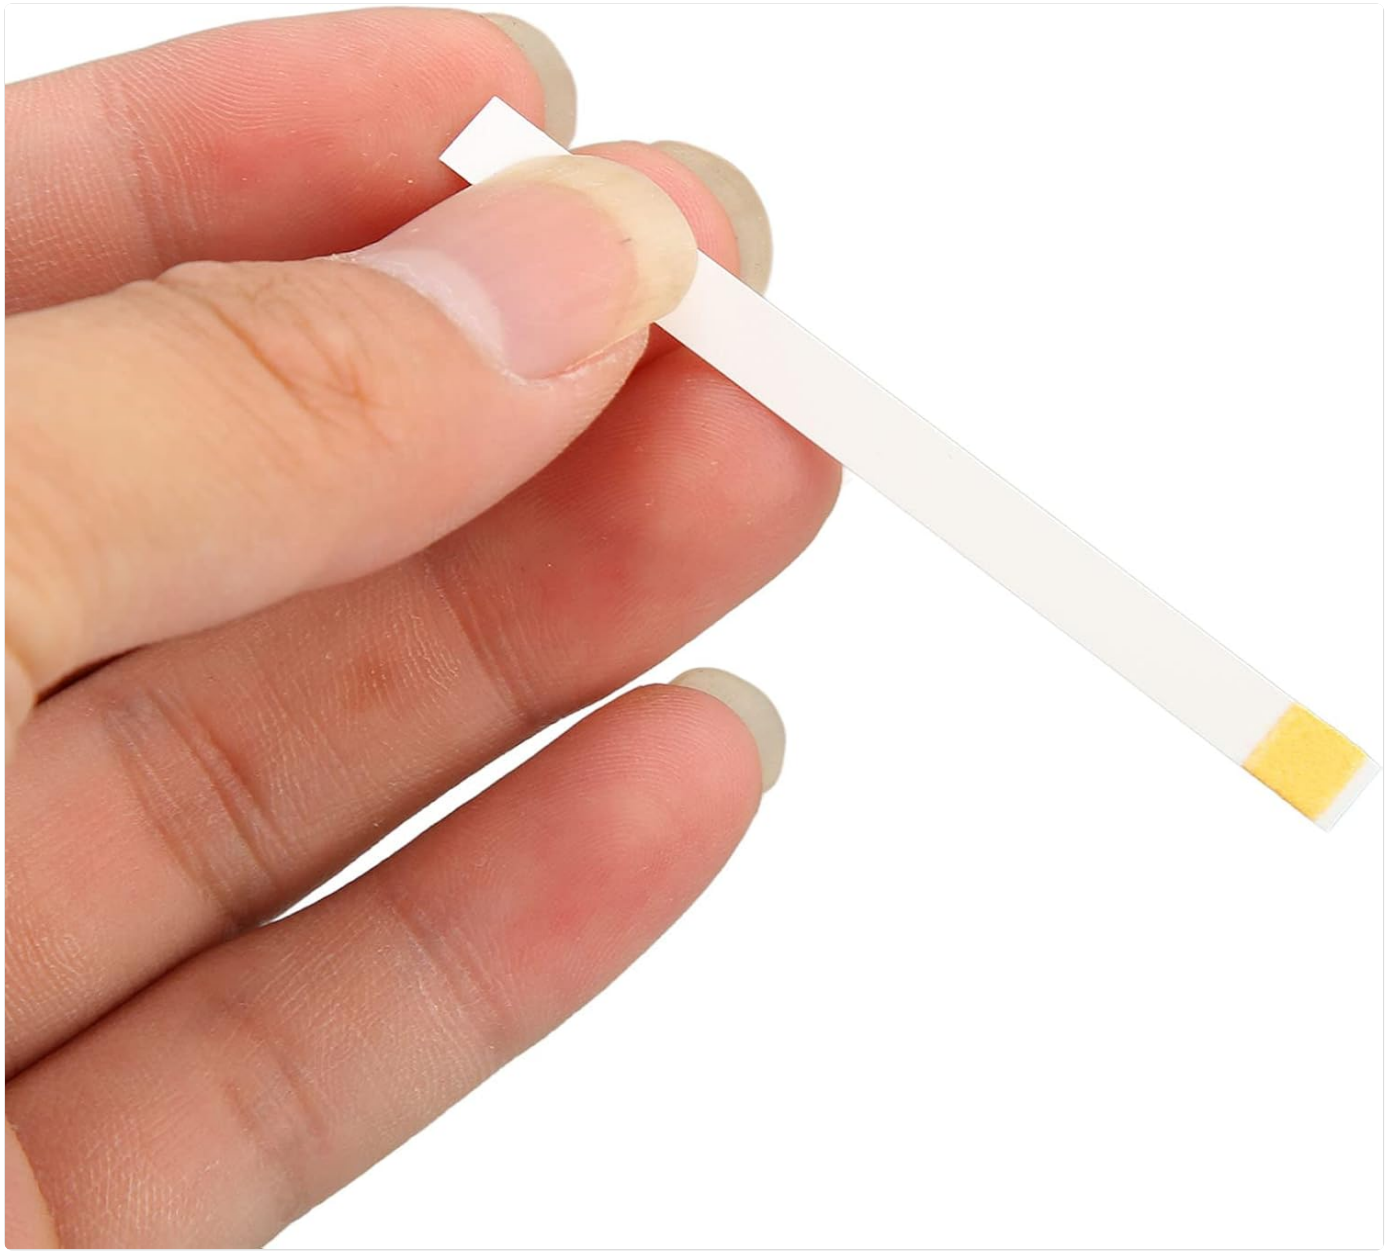


Image: A close-up view of a hand holding a single YUYTE Vaginal Test Strip, showing the reactive pad at the tip.

4.1 Interpreting Results

The test strips measure pH levels within the range of 4.0, 5.0, 6.0, 6.5, 7.0, and 8.0. Refer to the color chart on the bottle for specific interpretations. A normal vaginal pH typically falls between 3.8 and 4.5. Deviations from this range may indicate an imbalance.



Image: The YUYTE Vaginal Test Strips packaging, highlighting the pH testing range (4.0, 5.0, 6.0, 6.5, 7.0, 8.0) on the label.

5. Maintenance and Storage

Proper storage ensures the longevity and accuracy of your test strips.

- **Storage:** Keep the test strips sealed in their original bottle. Store them away from direct light and moisture.
- **Shelf Life:** The shelf life of the sealed product is 2 years. Once opened, use the strips as soon as possible for optimal accuracy.
- **Disposal:** Each strip is for single use only and cannot be reused. Dispose of used strips responsibly according to local regulations.



Image: An open bottle of YUYTE Vaginal Test Strips, illustrating how the strips are stored and dispensed.

6. Troubleshooting

If you encounter unexpected results or issues, consider the following:

- **Abnormal pH Reading:** If the initial pH reading is abnormal, it is recommended to perform the test several more times on different occasions. If the results consistently show an abnormal pH, consult a healthcare professional.
- **No Color Change/Faint Color:** Ensure sufficient sample was applied to the reactive pad. Verify the strip has not expired and was stored correctly.
- **Interference:** The test strips are designed to be resistant to VC interference. However, other substances or improper sample collection might affect results. Ensure all pre-test considerations (Section 3.2) were followed.

7. Product Specifications

Feature	Detail
Item Type	Vaginal Test Strips
Material	Paper
Test Range	4.0, 5.0, 6.0, 6.5, 7.0, 8.0
Test Sample	Female secretion
VC Disturbance Resistance	Yes
Shelf Life	2 years (sealed)
Quantity	100 pieces

Feature	Detail
Model Number	yuytekepx12a0zc
Manufacturer	YUYTE

8. Warranty and Support

Information regarding product warranty and customer support was not available in the provided product data. For any inquiries or support needs, please refer to the seller or manufacturer's contact information provided at the point of purchase or on the product packaging.

© 2023 YUYTE. All rights reserved.

Ask a question about this manual

Ask about setup, troubleshooting, compatibility, parts, safety, or missing instructions. Manuals+ will review the question and use this page's manual context to help answer it.

Name

Anonymous

Email

you@example.com

After a successful submission, we securely hash the supplied account or form email before sending it to Microsoft Advertising for conversion attribution. Privacy details.

Question

Example: How do I reset this device or fix this error?

Details

Model number, symptoms, what you tried, or the section of the manual you are using.

Submit question

Open the live page

https://manuals.plus/asin/B0C6YGMT3G

More documents and user manuals: **https://manuals.plus/**