PELEGON RTS1

PELEGON Raised Toilet Seat With Handles (400lb) - Instruction Manual

Model: RTS1 | Brand: PELEGON

Introduction

Thank you for choosing the PELEGON Raised Toilet Seat With Handles. This product is designed to provide enhanced stability, comfort, and support for individuals requiring assistance with toilet use, including those recovering from knee or hip surgery, or elderly and disabled users. Please read this manual thoroughly before assembly and use to ensure safe and proper operation.

Important Safety Information

- Always ensure all components are securely fastened before each use.
- Do not exceed the maximum weight capacity of 400 lbs (181 kg).
- Regularly inspect the product for any signs of wear, damage, or loose parts. Discontinue use if any issues are found.
- Ensure the non-slip rubber tips are clean and free from debris to maintain stability.
- Consult a healthcare professional for guidance on proper use, especially after surgery or for specific medical conditions.
- This product is intended for use as a raised toilet seat, bedside commode, or shower chair. Do not use for purposes other than those specified.

Setup and Assembly

The PELEGON Raised Toilet Seat is designed for tool-free assembly. Follow these steps for proper setup:

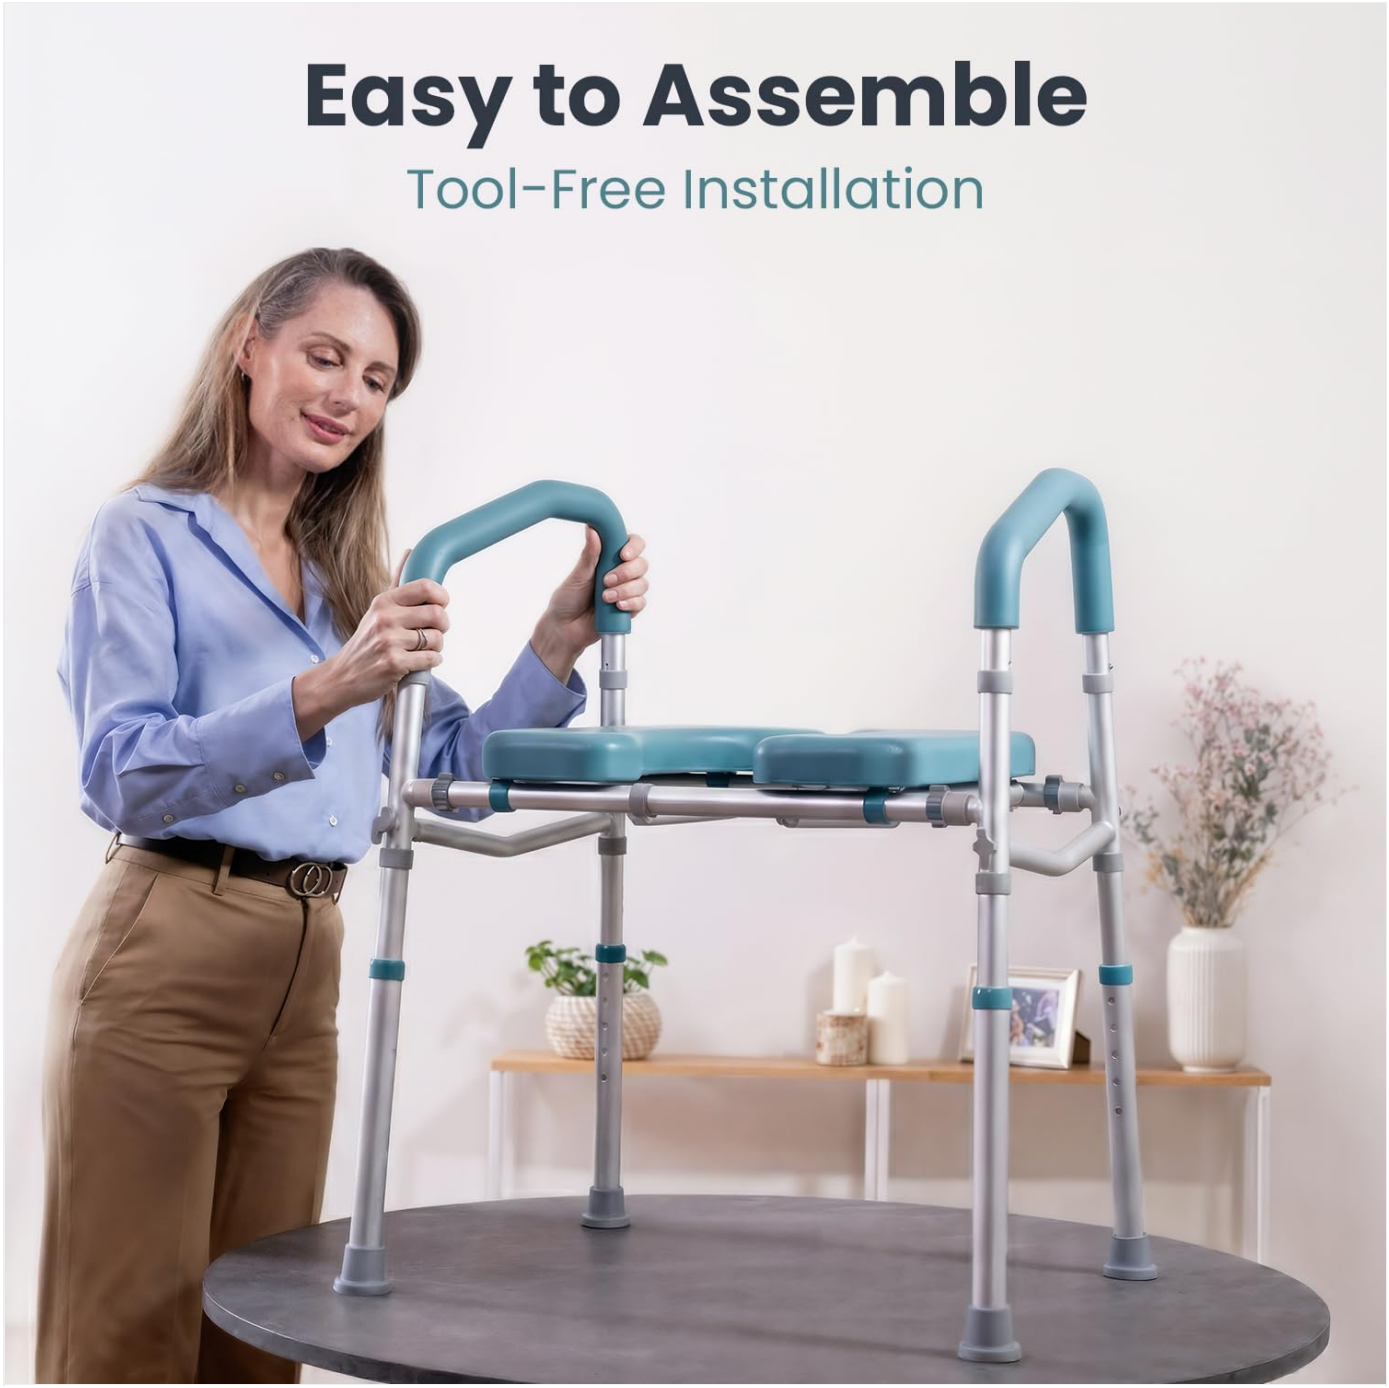


Figure 1: Tool-Free Assembly. The product is designed for easy, tool-free installation, allowing for quick setup.

1. **Unpack Components:** Carefully remove all parts from the packaging. Verify that all components are present: main frame, padded seat, and handles.
2. **Attach Legs:** Insert the legs into the designated slots on the main frame. Ensure the spring pins snap into place, securing each leg.
3. **Attach Handles:** Slide the padded handles into the frame. Adjust the height of the handles to a comfortable and supportive level, ensuring the locking pins are fully engaged.
4. **Attach Seat:** Place the padded seat onto the frame. Ensure it is properly aligned and secured.
5. **Adjust Height:** The seat height is adjustable from 16 inches (minimum) to 22 inches (maximum). Press the push-buttons on each leg and slide the leg up or down to the desired height. Ensure all four legs are set to the same height and the push-buttons are fully engaged in the adjustment holes.
6. **Adjust Width:** The leg width can be adjusted from 21 inches to 26 inches, and seat width from 20.5 inches to 24.5 inches to fit various toilet sizes. Ensure the frame is stable and centered over the toilet.



Figure 2: Adjustable Seat Height and Width. This diagram shows the minimum and maximum adjustable dimensions for seat height and leg width, allowing customization for user comfort and toilet compatibility.

Operating Instructions

The PELEGON Raised Toilet Seat can be used in three primary configurations:

1. As a Raised Toilet Seat

- Position the unit directly over your existing toilet. Ensure the legs are stable and the non-slip rubber tips are firmly on the floor.
- Use the padded handles for support when sitting down or standing up.
- The raised height reduces the distance needed to lower or raise, providing relief for knees and hips.



Figure 3: Enhanced Stability for Use. The design provides stability, which is beneficial for individuals recovering from knee or hip surgery, or those needing extra support.

2. As a Bedside Commode

- For bedside use, ensure the detachable pail is securely placed beneath the seat opening.
- Position the commode near the bed for easy access.
- Empty and clean the pail regularly as described in the Maintenance section.

3. As a Shower Chair

- The waterproof padded seat allows for use in the shower.
- Ensure the non-slip rubber tips are clean and the floor surface is not excessively slippery.
- Use the handles for support when sitting and standing in the shower.

Maintenance and Cleaning

Regular cleaning and maintenance will prolong the life of your PELEGON Raised Toilet Seat.

- **Cleaning the Frame:** Wipe the frame with a damp cloth and mild soap. Rinse thoroughly and dry immediately to prevent corrosion.
- **Cleaning the Padded Seat:** The ergonomic padded seat is waterproof and easy to clean. Use a mild disinfectant or soap and water. Wipe clean and dry.
- **Cleaning the Pail (for commode use):** Empty the pail after each use. Wash with warm water and a disinfectant cleaner. Rinse thoroughly and dry before reinserting.
- **Inspection:** Periodically check all bolts, screws, and pins to ensure they are tight and secure. Inspect the rubber tips for wear and tear; replace if damaged.



Figure 4: Ergonomic Padded Seat. The seat is designed to be waterproof and easy to clean, ensuring hygiene and durability.

Troubleshooting

Problem	Possible Cause	Solution

Problem	Possible Cause	Solution
Unit feels unstable or wobbly.	Legs not adjusted to the same height; locking pins not fully engaged; rubber tips worn or dirty; uneven floor surface.	Ensure all legs are at the same height and pins are engaged. Clean rubber tips. Place unit on a flat, even surface. Inspect and replace worn rubber tips.
Difficulty adjusting leg height.	Push-buttons are stuck or obstructed.	Ensure push-buttons are fully depressed. Check for any debris obstructing the mechanism. Apply light pressure while adjusting.
Pail does not fit securely (commode use).	Pail is not correctly aligned or inserted.	Ensure the pail is oriented correctly and pushed firmly into its designated slot beneath the seat.

Specifications

- **Model Number:** RTS1
- **Brand:** PELEGON
- **Maximum Weight Capacity:** 400 lbs (181 kg)
- **Product Dimensions:** 41.1 x 58.6 x 99.21 cm (L x W x H)
- **Product Weight:** 3.81 kg
- **Adjustable Seat Height:** 16 inches (min) to 22 inches (max)
- **Adjustable Leg Width:** 21 inches (min) to 26 inches (max)
- **Adjustable Seat Width:** 20.5 inches (min) to 24.5 inches (max)
- **Features:** Triple-duty design (raised toilet seat, bedside commode, shower chair), padded handles, non-slip rubber tips, tool-free assembly.



Figure 5: Enhanced Safety Features. The product includes padded handles for comfort and grip, non-slip rubber tips for stability, and is lab-tested to support up to 400 lbs.

Warranty and Support

For warranty information or technical support, please contact PELEGON customer service. Refer to your purchase documentation for specific warranty terms and contact details.

Manufacturer: PELEGON

Date First Available: December 7, 2023

Ask a question about this manual

Ask about setup, troubleshooting, compatibility, parts, safety, or missing instructions. Manuals+ will review the question and use this page's manual context to help answer it.

Name

Anonymous

Email

you@example.com

After a successful submission, we securely hash the supplied account or form email before sending it to Microsoft Advertising for conversion attribution. Privacy details.

Question

Example: How do I reset this device or fix this error?

Details

Model number, symptoms, what you tried, or the section of the manual you are using.

Submit question