Saved from manuals.plus.
Open the live page for links to other documents and user manuals.

Equipmed 4in1 Patient Lift Transfer Chair

EQUIPMED 4in1 Patient Lift Transfer Chair User Manual

Model: 4in1 Patient Lift Transfer Chair

Product Overview

The EQUIPMED 4in1 Patient Lift Transfer Chair is designed to assist with the safe and easy transfer of individuals with limited mobility. This versatile chair functions as a patient lift, transfer chair, shower chair, and commode, making it ideal for various care environments including clinics, hospitals, and home care.



Figure 1: The EQUIPMED 4in1 Patient Lift Transfer Chair, showcasing its robust design and integrated features for patient transfer and care.

Key features include a robust 2mm double thickened steel frame with a 120kg capacity, a hydraulic height adjustment system, a 180-degree split seat for easy transfers, and quiet castor wheels for smooth maneuvering.

Safety Information

ALWAYS READ THE LABEL AND FOLLOW THE DIRECTIONS FOR USE.

- Ensure all brakes are engaged before transferring a patient or when the chair is stationary.

- Always use the integrated safety belt to secure the patient during transfers.
- Do not exceed the maximum user load of 120kg.
- Ensure the floor is dry and clear of obstructions before moving the chair.
- Regularly inspect the chair for any signs of wear or damage. Do not use if damaged.



Figure 2: The double safety design, highlighting the secure latch and safety belt for patient security during transfers.

Setup and Assembly

The EQUIPMED Patient Lift Transfer Chair requires minimal assembly. Upon unboxing, ensure all components listed in the "In the Box" section are present.

Unpacking and Initial Inspection:

1. Carefully remove all components from the packaging.
2. Inspect all parts for any shipping damage. Contact your supplier immediately if any damage is found.

3. Verify that all listed components are included.

Assembly Steps:

While specific assembly steps are minimal, ensure the commode bucket is correctly placed if using the commode function, and the seat pad is securely attached.

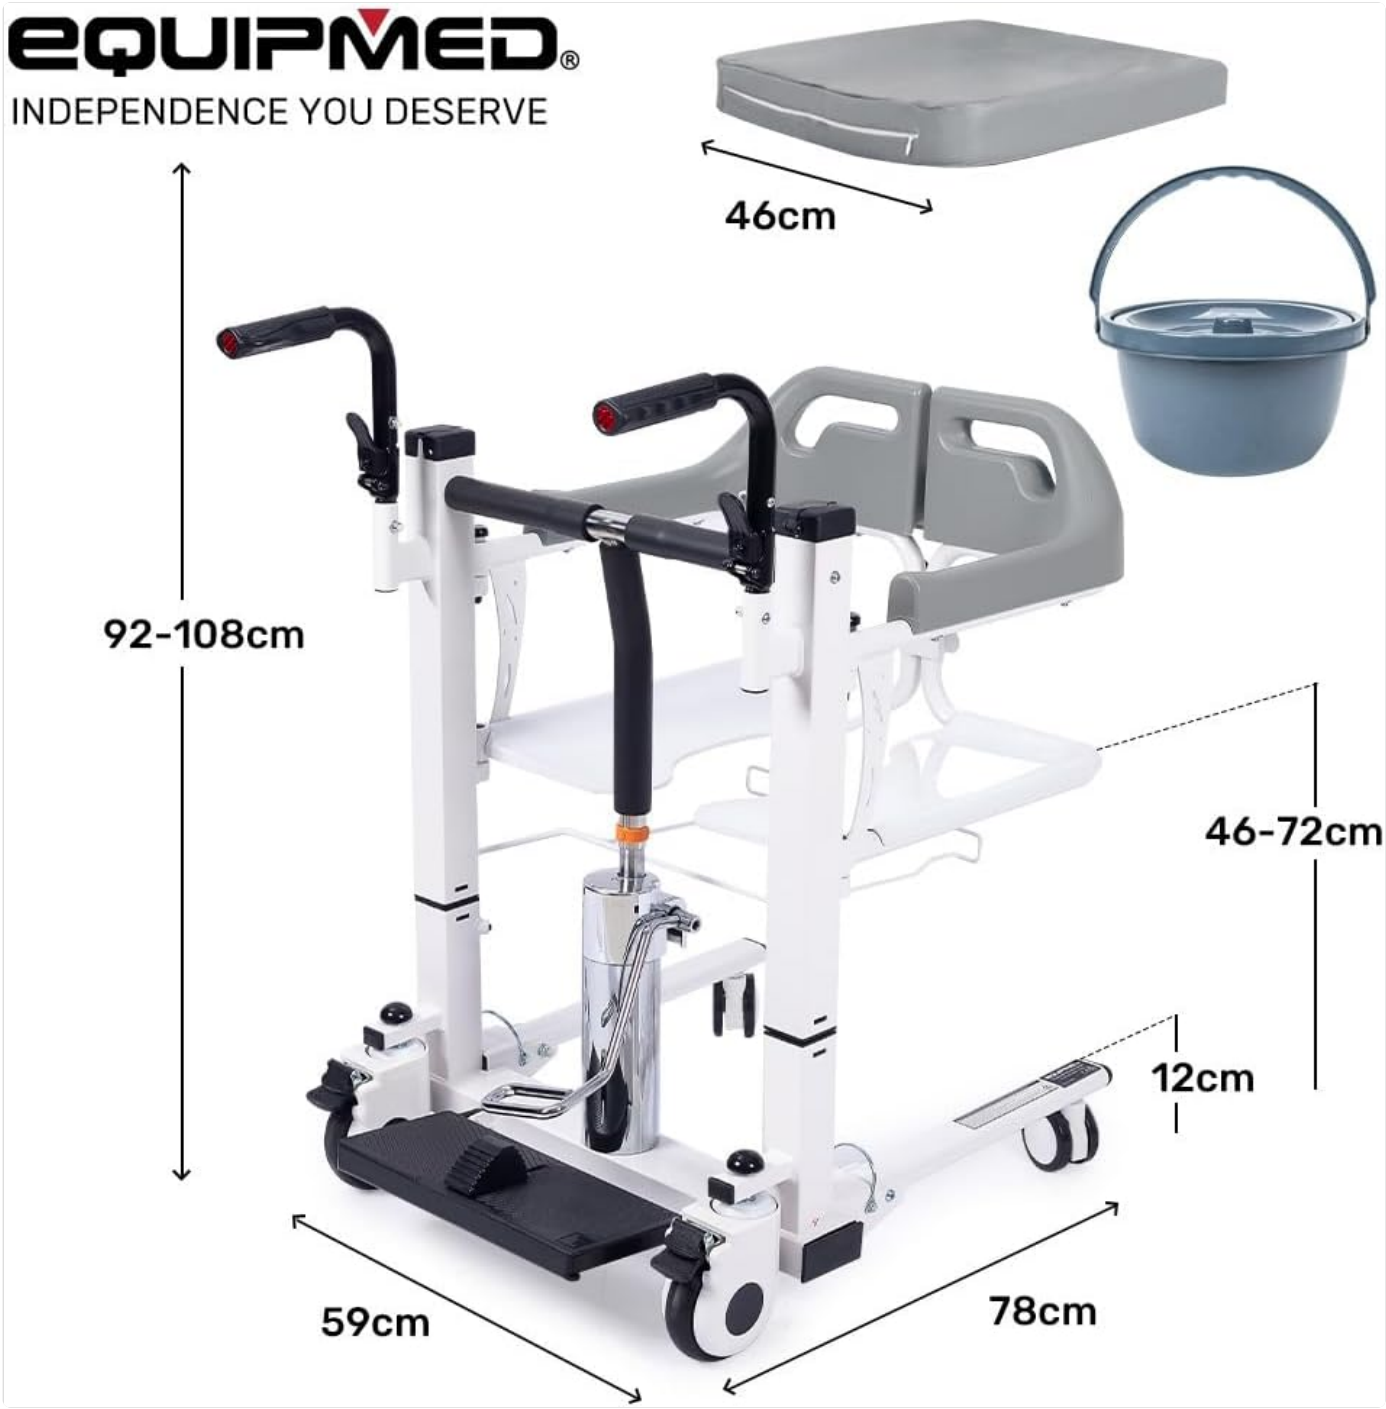


Figure 3: Overview of the chair's components and dimensions, including the commode bucket and seat pad.

Operating Instructions

Patient Transfer (180° Split Seat):

1. Position the chair close to the bed, wheelchair, or lounge from which the patient will be transferred.
2. Engage the brakes on all wheels to ensure stability.
3. Open the 180-degree split seat by releasing the secure latch.

4. Carefully slide the open chair under the patient, ensuring they are centered and comfortable.
5. Close the split seat, ensuring the latch is securely double-locked.
6. Fasten the integrated safety belt around the patient.
7. Disengage the brakes and gently move the chair to the desired location.



Figure 4: Demonstrating simple transfers between a bed and the patient lift chair using the split seat feature.



Figure 5: Close-up view of the 180-degree split seat, designed to easily slide under a passenger for transfers.

Hydraulic Height Adjustment:

The chair features an easy-to-depress hydraulic foot lever for height adjustment.

- To raise the chair: Repeatedly press the hydraulic foot lever with your foot. The chair will smoothly ascend.
- To lower the chair: Shift the safety block on the hydraulic mechanism and then press the foot lever. The chair will descend.



Figure 6: Illustration of the easy hydraulic lifting mechanism, showing the foot lever for height adjustment.

Using as a Commode or Over Toilet Chair:

- **Commode Function:** Ensure the removable commode bucket is placed securely beneath the seat. The smooth seat pan allows for easy use.
- **Over Toilet Function:** Position the chair directly over a standard toilet. Adjust the height using the hydraulic lift to clear the toilet bowl. Ensure the chair is stable and brakes are engaged before use.



Figure 7: The patient lift chair positioned as a convenient over-toilet chair, also showing the removable commode bucket.

Maneuvering and Braking:

The chair is equipped with quiet 5-inch front castor wheels and 3-inch rear 360-degree castor wheels for easy maneuvering.

- **Moving the Chair:** Disengage all foot-activated park brakes. Gently push or pull the chair using the handles.
- **Engaging Brakes:** Press down on the foot levers located on each wheel to engage the brakes. Ensure all four wheels are locked for maximum stability.
- **Releasing Brakes:** Lift the foot levers on each wheel to release the brakes.



Figure 8: Detail of the 5-inch front and 3-inch rear castor wheels, highlighting the foot-activated park brakes for easy maneuvering and stability.

Maintenance and Care

- **Cleaning:** The removable soft vinyl covered seat pad is easy to clean. Wipe down all surfaces of the chair with a damp cloth and mild disinfectant regularly. Avoid abrasive cleaners.
- **Inspection:** Periodically check all bolts, screws, and moving parts to ensure they are secure and functioning correctly. Tighten any loose fasteners.
- **Hydraulic System:** The hydraulic system is largely maintenance-free. If you notice any issues with lifting or lowering, consult a qualified technician.
- **Wheels:** Keep the wheels free of hair, lint, and debris to ensure smooth operation.



Figure 9: The ergonomically contoured padded backrest and the washable seat cover, emphasizing ease of cleaning and comfort.

Troubleshooting

Problem	Possible Cause	Solution
Chair does not lift or lowers slowly.	Low hydraulic fluid or air in the system; mechanical obstruction.	Ensure no obstructions. If issue persists, contact customer support for professional service.
Wheels are difficult to move.	Brakes engaged; debris in wheels; damaged castor.	Check and release all brakes. Clean any debris from wheels. If damaged, contact support for replacement parts.
Split seat does not close securely.	Latch mechanism obstructed or damaged.	Check for any obstructions in the latch area. Ensure the seat halves align correctly. If damaged, do not use and contact support.

Specifications

Attribute	Detail
Brand	Equipmed
Type	Hydraulic Patient Lift Transfer Chair
Colour	White
Seat Width	46cm
Seat Depth	40cm
Max User Load	120kg
Frame Material	2mm double thickened steel
Recommended User Height	135cm - 198cm
Rear Wheels	3” 360° castor wheels w/ brakes
Front Wheels	5" castor wheels w/ brakes
Seat Height Range	46 - 72cm
Height of Base	12cm
Product Dimensions (W x L x H)	78 x 59 x 92-108cm
Product Weight	37kg
ARTG	472191

Warranty and Support

For warranty information, please refer to the documentation provided at the time of purchase or contact Equipmed customer support directly. Keep your proof of purchase for any warranty claims.

If you require technical assistance, replacement parts, or have any questions regarding the operation or maintenance of your EQUIPMED Patient Lift Transfer Chair, please contact Equipmed customer service through their official website or the contact details provided with your product.

Manufacturer: Equipmed

© 2024 Equipmed. All rights reserved.

Ask a question about this manual

Ask about setup, troubleshooting, compatibility, parts, safety, or missing instructions. Manuals+ will review the question and use this page’s manual context to help answer it.

Name

Anonymous

Email

you@example.com

After a successful submission, we securely hash the supplied account or form email before sending it to Microsoft Advertising for conversion attribution. Privacy details.

Question

Example: How do I reset this device or fix this error?

Details

Model number, symptoms, what you tried, or the section of the manual you are using.

Submit question

Open the live page

https://manuals.plus/asin/B0D542R6PP

More documents and user manuals: **https://manuals.plus/**