LifePro B0D59YQMB8

LifePro Vibration Red & Infrared Knee Brace and Portable Red Light Therapy Device User Manual

Model: B0D59YQMB8

1. Introduction

This manual provides essential information for the safe and effective use of your LifePro Vibration Red & Infrared Knee Brace and Portable Red Light Therapy Device. This bundle is designed to offer comprehensive pain relief and recovery through a combination of red light therapy, near-infrared light therapy, and vibration massage.



Figure 1.1: The LifePro Red Light Therapy Bundle, including the knee brace and the portable red light therapy device, along with their packaging.

1.1 Safety Information

Please read all safety instructions before using the device. Failure to follow these instructions may result in injury or damage to the product.

- Consult with a healthcare professional before use if you have any pre-existing medical conditions, are pregnant, or have

implanted medical devices.

- Do not use on open wounds, broken skin, or areas with active infections.
- Avoid direct eye exposure to the light. Protective eyewear is recommended.
- Do not exceed recommended session times (20-30 minutes per session) to prevent skin irritation or discomfort.
- If you experience excessive heat, redness, or discomfort, discontinue use immediately.
- Keep out of reach of children.
- Do not immerse the devices in water or use them in wet environments.
- Use only the provided charging cables and adapters.

2. Product Components

The LifePro Red Light Therapy Bundle includes the following items:

- LifePro Vibration Red & Infrared Knee Brace
- Portable Red Light Therapy Device (LumiCare Lamp)
- USB Charging Cable(s)
- Storage Case for Portable Device
- User Manual (this document)



Figure 2.1: The LifePro Red Light Therapy Knee Brace, shown with its retail packaging.

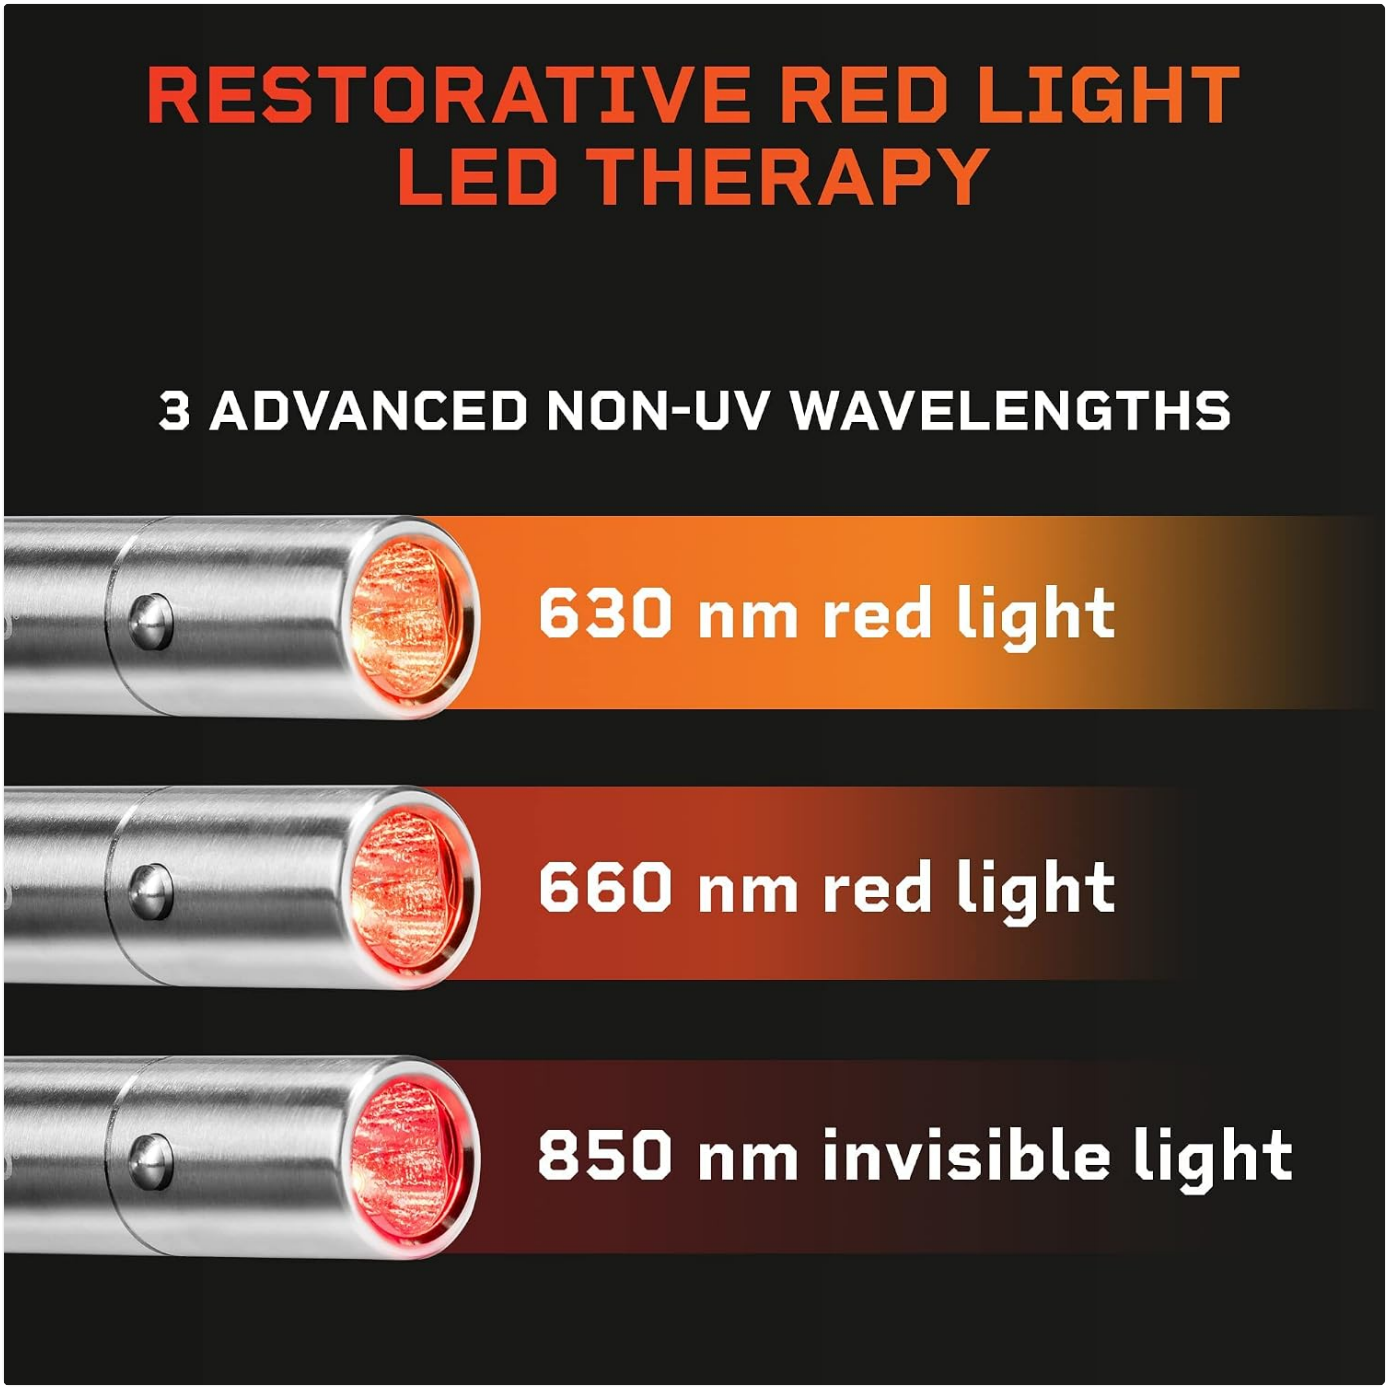


Figure 2.2: The LifePro Portable Red Light Therapy Device, presented with its zippered carrying case.

3. Setup

3.1 Charging the Devices

Before first use, fully charge both the Knee Brace and the Portable Red Light Therapy Device.

- Connect the provided USB charging cable to the charging port on each device.
- Plug the other end of the USB cable into a compatible USB power adapter (not included) or a computer USB port.
- The indicator light will show charging status (refer to device-specific indicators for full charge).

3.2 Preparing the Knee Brace

- Ensure the knee brace is clean and dry before application.
- Unfold the brace and identify the light panel section.

- Position the brace around your knee, ensuring the light panel is centered over the area you wish to treat.
- Secure the brace using the adjustable straps for a comfortable yet snug fit. Do not overtighten.

4. Operating Instructions

4.1 LifePro Vibration Red & Infrared Knee Brace



Figure 4.1: A user demonstrating the application of the LifePro Knee Brace, highlighting the 660nm Red Light and 850nm Near-Infrared Light modes, along with 5 vibration levels.

1. **Power On:** Press and hold the power button on the control panel of the knee brace to turn it on.
2. **Select Light Mode:**
    - **660 nm Red Light:** Primarily for pain relief and circulation improvement.
    - **850 nm Near-Infrared Light:** Designed for deep muscle and tissue repair.
    - **Combined Mode:** Activates both red and near-infrared lights simultaneously for comprehensive therapy.

Press the mode button to cycle through these options.

3. **Adjust Vibration:** The knee brace features 5 vibration levels, including a pulse mode. Press the vibration button to adjust the intensity or activate the pulse setting.
4. **Session Duration:** Recommended session time is 20-30 minutes. The device may have an automatic shut-off feature after a set duration.
5. **Power Off:** Press and hold the power button to turn off the device after your session.



Figure 4.2: Detailed view of the knee brace in use, emphasizing the recommended session time limit of 20-30 minutes and explaining that skin redness is a normal response to therapeutic heat.

Note on Skin Redness: It is normal to experience some skin redness after a session. This is a therapeutic heat response from the LEDs and not an indication of burning. If discomfort occurs, adjust the light intensity or discontinue use.

4.2 Portable Red Light Therapy Device



Figure 4.3: A user applying the portable red light therapy device to her neck, illustrating its benefits for skin rejuvenation, inflammation reduction, improved circulation, and mood promotion.

1. **Power On:** Press the power button on the device to turn it on. The light will illuminate.
2. **Application:** Hold the device directly over the desired treatment area (e.g., back, shoulders, joints). Maintain a distance of 1-3 inches from the skin.
3. **Session Duration:** Recommended session time is 20-30 minutes per area.
4. **Power Off:** Press the power button again to turn off the device.

5. Maintenance

5.1 Cleaning

- Ensure both devices are powered off and unplugged before cleaning.
- Wipe the surfaces of the devices with a soft, damp cloth.

- Do not use abrasive cleaners, solvents, or harsh chemicals.
- Allow devices to air dry completely before storing or next use.

5.2 Storage

- Store the devices in a cool, dry place away from direct sunlight and extreme temperatures.
- Use the provided storage case for the portable device to protect it from dust and damage.

6. Troubleshooting

Problem	Possible Cause	Solution
Device does not turn on.	Battery is low or depleted.	Charge the device fully using the provided USB cable.
Light output seems weak.	Battery is low. / Device is dirty.	Recharge the device. / Clean the light panel with a soft cloth.
Excessive heat or discomfort.	Session duration too long. / Device too close to skin.	Reduce session time. / Ensure proper distance (1-3 inches for portable device). Discontinue use if discomfort persists.
Vibration not working (Knee Brace).	Vibration mode not activated. / Battery low.	Press the vibration button to cycle through modes. / Charge the device.

7. Specifications

- **Product Name:** LifePro Vibration Red & Infrared Knee Brace and Portable Red Light Therapy Device
- **Model:** B0D59YQMB8
- **Brand:** LifePro
- **Wavelengths:**
  - 660 nm (Red Light)
  - 850 nm (Near-Infrared Light)
  - (Portable device may also include 630 nm, as per image)
- **Power Source:** Rechargeable Battery (USB Charging)
- **Recommended Session Time:** 20-30 minutes per session/area
- **Date First Available:** May 27, 2024



Figure 7.1: Illustration of the three advanced non-UV wavelengths used in the portable device: 630 nm red light, 660 nm red light, and 850 nm invisible light.

8. Warranty and Support

LifePro products are designed for durability and performance. For warranty information, product support, or any questions regarding your device, please contact LifePro customer service.
You can typically find contact details on the official LifePro website or through the retailer where you purchased the product.
Website: Visit the LifePro Store on Amazon

Ask a question about this manual

Ask about setup, troubleshooting, compatibility, parts, safety, or missing instructions. Manuals+ will review the question and use this page's manual context to help answer it.

Name

Anonymous

Email

you@example.com

After a successful submission, we securely hash the supplied account or form email before sending it to Microsoft Advertising for conversion attribution. Privacy details.

Question

Example: How do I reset this device or fix this error?

Details

Model number, symptoms, what you tried, or the section of the manual you are using.

Submit question