NANSIKE B0DGXL3GYW

NANSIKE Under Eye Red Light Therapy Glasses User Manual

Overview Safety Information Product Components Setup Operation Maintenance Troubleshooting Specifications Warranty & Support

1. Product Overview

The NANSIKE Under Eye Red Light Therapy Glasses are designed to provide targeted red light therapy and massage to the delicate skin around the eyes. This device aims to promote collagen regeneration, reduce the appearance of dark circles, eye bags, and fine lines, and alleviate eye fatigue. Its lightweight and ergonomic design allows for comfortable use during various activities.



Image: The NANSIKE Under Eye Red Light Therapy Glasses being worn, illustrating the red light emitted around the eye area.



Image: Visual comparison demonstrating the reduction of eye bags, dark circles, and fine lines with consistent use.



Image: Graphical representation of key benefits including firming, lifting, fading fine lines, relaxing eye muscles, improving nutrition, brightening the eye area, and enhancing circulation.

2. Important Safety Information

- **For external use only.** Do not use internally.
- Always remove makeup and thoroughly clean the skin around your eyes before each use.
- Apply a water-based eye cream, gel, or other water-based skincare product to the under-eye area before activating the massage function. Insufficient humidity or lack of contact with the conductive patches will prevent the massage function from activating.
- Do not use if you have any pre-existing eye conditions, skin sensitivities, or are pregnant without consulting a healthcare professional.
- Keep out of reach of children.
- Clean the device after each use as per maintenance instructions.

3. Product Components

Your NANSIKE Under Eye Red Light Therapy Glasses package includes the following items:

- NANSIKE Under Eye Red Light Therapy Glasses
- USB Charging Cable
- User Manual
- Eyeglass Retaining Cords (adjustable straps)
- Gel Pads (for optimal contact and conductivity)



Image: All components included in the NANSIKE Under Eye Red Light Therapy Glasses package, laid out on a wooden surface.

4. Setup and First Use

1. **Charge the Device:** Before first use, ensure the device is fully charged. Connect the provided USB charging cable to the charging port on the glasses and to a suitable USB power source. A full charge takes approximately 30 minutes

and provides 90-120 minutes of use.

2. **Prepare Your Skin:** Remove all makeup and thoroughly clean the skin around your eyes.
3. **Apply Skincare Product:** Apply a water-based eye cream, gel, or other water-based skincare product to the under-eye area. This is crucial for activating the massage function and ensuring proper conductivity.
4. **Attach Retaining Cords (Optional):** If desired, attach the eyeglass retaining cords to the arms of the glasses for a more secure and perfect fit to the skin. Adjust the straps for comfort.



Image: Close-up of the adjustable straps and the importance of a snug fit for effective treatment.



Image: Step-by-step visual guide for preparing the skin, applying product, and wearing the NANSIKE glasses.

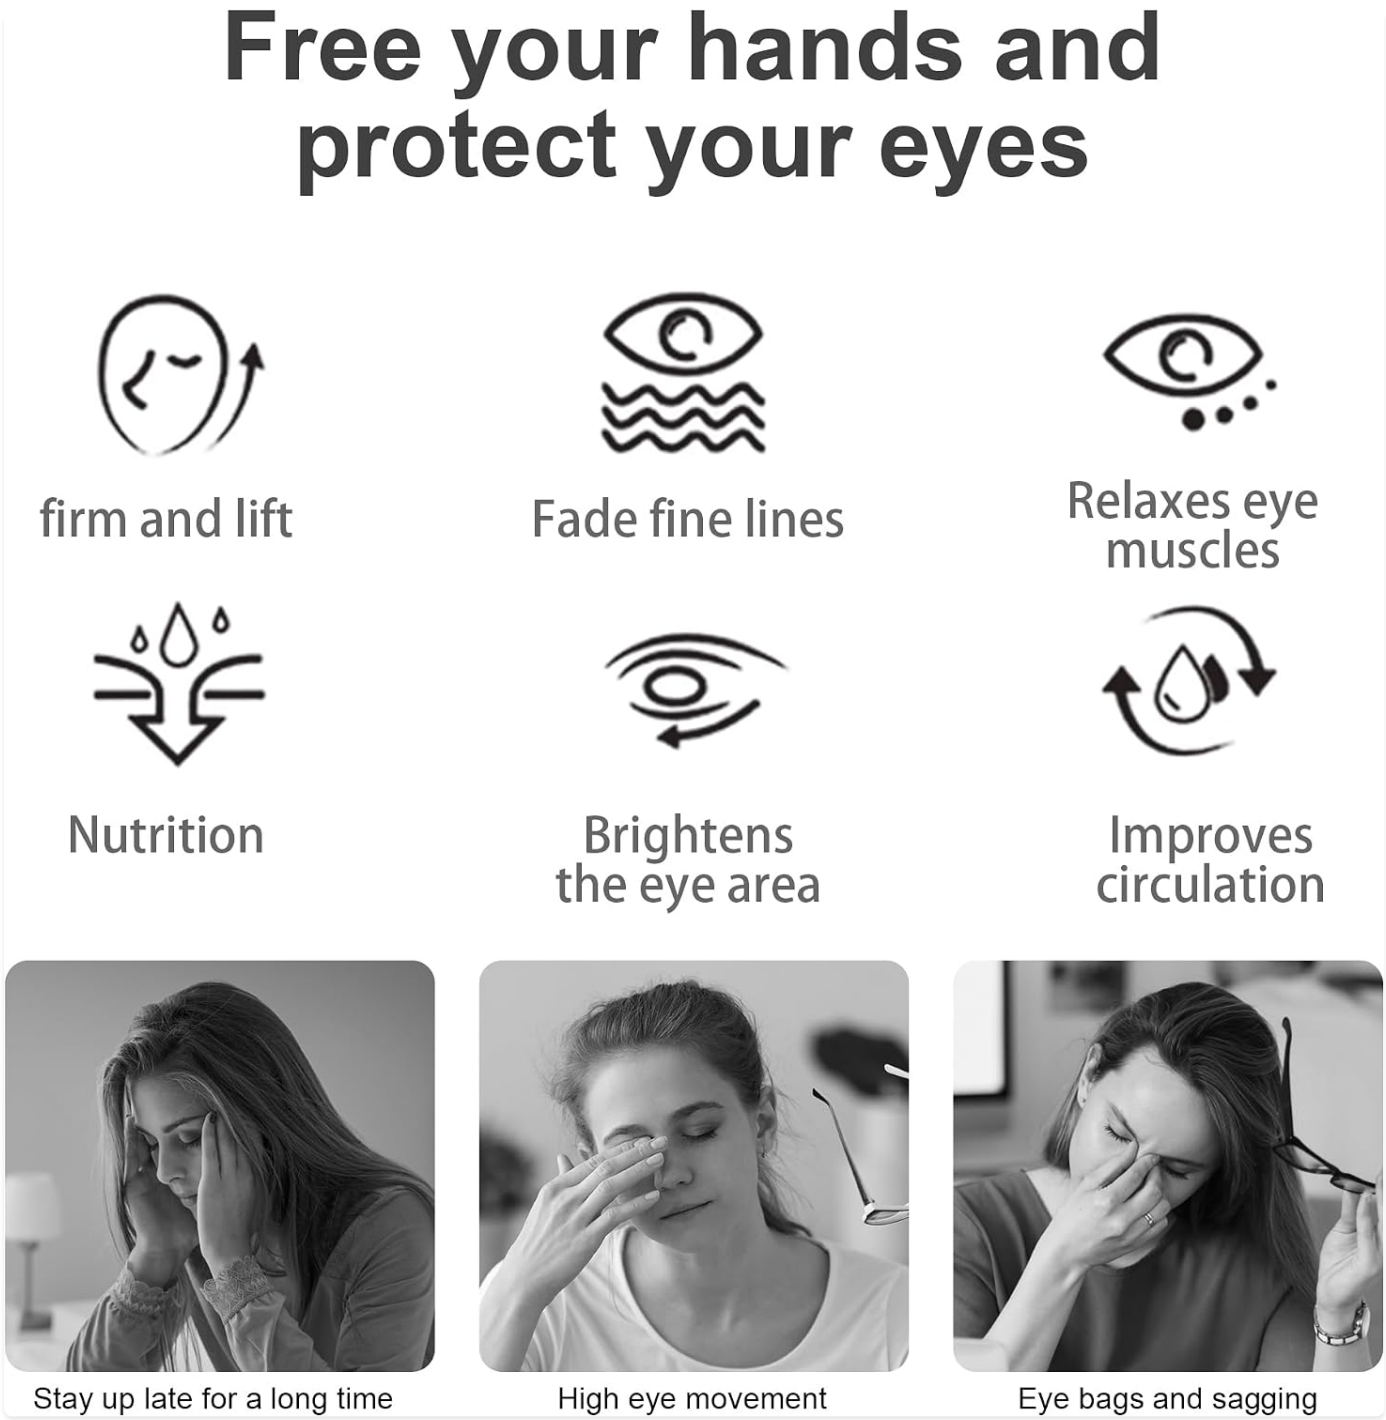


Image: Illustrated guide showing the sequence of steps for using the eye massager, from preparation to the 10-minute session.

5. Operating Instructions

1. **Power On:** Press and hold the power button (usually marked with a power symbol) to turn on the device. The red lights will illuminate.
2. **Select Mode:** The device features different modes and 3-speed intensity levels. Press the 'Mode' button to cycle through available modes (e.g., red light therapy, massage, or combined). Use the '+' and '-' buttons to adjust the intensity of the massage function.
3. **Wear the Glasses:** Place the glasses comfortably over your eyes, ensuring the conductive patches make good contact with your under-eye skin.
4. **Treatment Duration:** Each treatment session is automatically timed for 10 minutes. The device will shut down automatically after 10 minutes. You can switch modes and adjust intensity within this 10-minute period without affecting the timer.
5. **Frequency of Use:** For optimal results, use the device for 10 minutes a day, a couple of times a week.

Your browser does not support the video tag.

Video: Official demonstration of the NANSIKE Under Eye Red Light Therapy Glasses, showing how to use the device for under-eye care.



Image: Detailed view of the red light repair technology, microcurrent technology, and 3-speed adjustment buttons on the device.



Image: Illustration of the intelligent timing feature, indicating a 10-minute work timer and automatic shutdown, with charging time details.



Image: Close-up showing the microcurrent and red light repair technologies integrated into the glasses, along with the 3-speed adjustment controls.

6. Care and Maintenance

To ensure the longevity and hygiene of your NANSIKE Under Eye Red Light Therapy Glasses:

- **Cleaning:** Clean the device thoroughly after each use. Use a soft, damp cloth to wipe down the surfaces, especially the areas that come into contact with your skin. Do not use abrasive cleaners or immerse the device in water.
- **Storage:** Store the glasses in a cool, dry place, away from direct sunlight and extreme temperatures.

7. Troubleshooting

If you encounter issues with your NANSIKE Under Eye Red Light Therapy Glasses, please refer to the following common solutions:

Problem	Possible Cause	Solution
Massage function not activating.	Insufficient humidity or conductive patches not touching the skin.	Ensure you have applied a water-based eye cream or gel to the under-eye area. Adjust the glasses to ensure good contact between the conductive patches and your skin.
Device not turning on.	Low battery or device not charged.	Charge the device fully using the provided USB cable. Ensure the charging cable is securely connected.
Red lights not visible.	Device not powered on or in a different mode.	Press and hold the power button to turn on. Cycle through modes using the 'Mode' button to ensure red light therapy is active.

8. Product Specifications

- **Brand:** NANSIKE
- **Model:** B0DGXL3GYW
- **Package Dimensions:** 6.61 x 2.99 x 2.52 inches
- **Item Weight:** 0.18 Kilograms (6.38 ounces)
- **Batteries:** 1 A battery required (included)
- **Charging Time:** Approximately 30 minutes
- **Usage Time:** 90-120 minutes per full charge
- **Material:** Plastic
- **Frame Type:** Full Rim
- **Lens Coating:** Uncoated
- **Special Features:** Lightweight
- **Care Instructions:** Clean after each use

9. Warranty and Customer Support

For information regarding warranty coverage, returns, or technical support, please refer to the official NANSIKE website or contact their customer service directly. Keep your purchase receipt for warranty claims.

Ask a question about this manual

Ask about setup, troubleshooting, compatibility, parts, safety, or missing instructions. Manuals+ will review the question and use this page's manual context to help answer it.

Name

Anonymous

Email

you@example.com

After a successful submission, we securely hash the supplied account or form email before sending it to Microsoft Advertising for

conversion attribution. Privacy details.

Question

Example: How do I reset this device or fix this error?

Details

Model number, symptoms, what you tried, or the section of the manual you are using.

Submit question