KingPavonini U13

KingPavonini Wireless TENS Unit Muscle Stimulator Model U13 User Manual

Model: U13

Introduction

The KingPavonini Wireless TENS Unit Muscle Stimulator Model U13 is a versatile 3-in-1 device combining TENS (Transcutaneous Electrical Nerve Stimulation), EMS (Electrical Muscle Stimulation), and Massage functions. It is designed to provide targeted pain relief, promote muscle recovery, and ease everyday soreness across various body areas such as the neck, back, shoulders, legs, knees, and joints. Its wireless, pocket-sized design offers freedom of movement, making it suitable for use at home, work, or while traveling. Each unit features 6 modes and 30 intensity levels, with dual-channel control for customized therapy.

Package Contents

Upon unboxing your KingPavonini Wireless TENS Unit, please verify that all the following items are included:



Figure 1: Package Contents. This image displays all items included in the KingPavonini Wireless TENS Unit Muscle Stimulator Model U13 package.

- Wireless TENS Unit ×2
- Charging & Storage Case ×1
- Gel Electrode Pads ×4 (3.23" x 1.86")
- USB-C Charging Cable ×1
- User Manual ×1 (This document)
- Quick Start Guide ×1
- Premium Gift Box ×1

Product Overview

The KingPavonini U13 offers a comprehensive solution for pain management and muscle stimulation with its advanced features.

3-in-1 Functionality



Figure 2: 3-in-1 Functionality. The device combines TENS for pain relief, EMS for muscle activation, and Massage for deep tissue massage.

- **TENS (Transcutaneous Electrical Nerve Stimulation):** Provides targeted pain relief and recovery.
- **EMS (Electrical Muscle Stimulation):** Aids in muscle activation and strengthening.
- **Massage:** Offers deep tissue massage for relaxation and soreness relief.

Wireless and Portable Design



Figure 3: Wireless Design. Enjoy complete freedom of movement with the wireless design, free from tangled cords.

The compact, pocket-sized design allows for discreet and convenient use anywhere. The charging case also serves as a remote control and storage unit.



Figure 4: Pocket-Sized Power. The small, sleek design is made for easy portability.

Dual-Channel Control and Modes

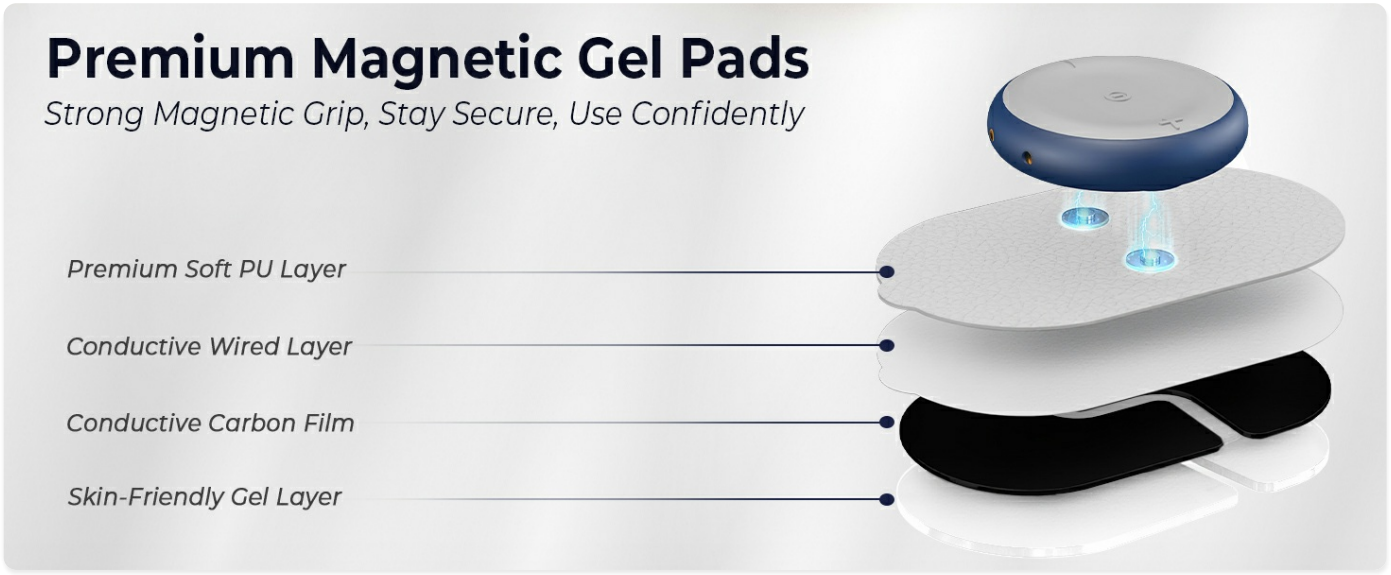


Figure 5: A/B Channel, Independent Control. Adjust each channel independently on the main unit for targeted relief.

Each of the two independent wireless units offers 6 modes and 30 intensity levels. You can fine-tune different modes and intensities for targeted relief on multiple areas simultaneously, or sync both units via the charging case for even recovery.



Figure 6: 2-Way Control. The device offers both button control on the unit and remote control via the charging case.

- **Modes:** Auto, Relax, Beat, Scraping, Knead, Press.
- **Intensity:** 30 adjustable levels.
- **Timer:** 10-60 minutes (adjustable via remote), 15 minutes (fixed via unit button).

Magnetic Gel Pads



Figure 7: Magnetic Gel Pads. The pads feature a multi-layer design for strong adhesion and comfort.

The included magnetic gel pads (3.23" x 1.86") are made with latex-free gel and PU leather, ensuring a soft, breathable, and skin-friendly feel. They are washable and reusable up to 50 times, maintaining strong adhesion after cleaning. The secure magnetic design keeps them firmly in place during use.

Setup

1. **Charge the Device:** Before first use, fully charge the TENS units and the charging case using the provided USB-C cable. The charging case indicates battery status. A full charge provides up to 720 minutes (12 hours) total runtime, with each unit running for approximately 2 hours per charge.



Figure 8: Charging the Device. The charging case provides power and storage for the TENS units.

2. **Prepare the Skin:** Ensure the skin area where the pads will be applied is clean, dry, and free of lotions or oils. This helps maintain optimal adhesion and conductivity.
3. **Attach Gel Pads:** Remove the protective film from the gel electrode pads. Magnetically attach a main TENS unit to each pad.
4. **Apply to Skin:** Place the gel pads with attached TENS units firmly onto the desired treatment area. Ensure good contact with the skin.

Operating Instructions

The KingPavonini U13 can be controlled directly via buttons on the TENS units or remotely using the charging case.

Quick Start Guide (Visual)



Figure 9: How to Use. A visual guide to operating your TENS unit.

Using the TENS Unit Buttons:

1. **Power On:** Long press the power button (center button) on the TENS unit until the indicator light turns on.
2. **Select Mode:** Short press the 'M' button to cycle through the 6 available modes (Auto, Relax, Beat, Scraping, Knead, Press).
3. **Adjust Intensity:** Use the '+' and '-' buttons to increase or decrease the intensity level (1-30). Start with the lowest intensity and gradually increase to a comfortable level.
4. **Timer:** The unit will operate for a fixed 15-minute cycle when controlled directly.
5. **Power Off:** Long press the power button on the TENS unit to turn it off.

Using the Charging Case (Remote Control):

1. **Power On:** Long press the 'M' button on the charging case to power on the connected TENS units.
2. **Select Mode:** Short press the 'M' button on the charging case to cycle through the 6 available modes.
3. **Adjust Intensity:** Use the '+' and '-' buttons on the charging case to increase or decrease the intensity level (1-30). This adjusts both units simultaneously or independently if set up for A/B channel control.
4. **Set Timer:** Short press the 'T' button on the charging case to adjust the treatment timer from 10 to 60 minutes.
5. **Independent Channel Control:** The charging case allows for independent adjustment of each TENS unit. Refer to the quick start guide or full manual for detailed instructions on switching between A/B channel control.
6. **Power Off:** The units will automatically power off after the set timer expires. You can also long press the 'M' button on the charging case to turn them off.
7. **Remote Restart:** If a unit powers off, it can be remotely restarted via the charging case within 15 minutes of power-off.

Maintenance

- **Cleaning Gel Pads:** The gel pads are washable and reusable. Gently clean the adhesive surface with a damp cloth or mild soap and water. Allow them to air dry completely before reattaching the protective film. Proper cleaning extends pad life up to 50 uses.
- **Storing the Device:** After each use, place the TENS units back into the charging and storage case. This keeps them organized, protected, and charged for the next use. Store the device in a cool, dry place away from direct sunlight.
- **Charging:** Recharge the device regularly to ensure it's ready for use. Avoid completely draining the battery for extended periods.

Troubleshooting

Problem	Possible Cause	Solution
No sensation or weak sensation	• Unit not powered on. • Intensity too low. • Pads not making good skin contact. • Pads are dry or worn out. • Battery low.	• Ensure unit is powered on (long press power button). • Increase intensity using '+' button. • Press pads firmly onto skin. Clean skin area. • Clean pads or replace with new ones. • Charge the device.
Pads not sticking well	• Skin is oily or dirty. • Pads are dirty or worn out.	• Clean and dry skin thoroughly before application. • Clean pads with water and air dry. Replace if adhesion is permanently lost.
Device not charging	• Charging cable not properly connected. • Faulty cable or power adapter.	• Ensure USB-C cable is securely connected to both the case and a power source. • Try a different USB-C cable or power adapter.
Remote control not working	• TENS units are out of range or powered off. • Charging case battery low.	• Ensure TENS units are powered on and within close proximity to the charging case. • Charge the charging case.

Specifications

Model Number	U13

Functions	TENS, EMS, Massage (3-in-1)
Channels	Dual Channel (2 independent units)
Modes	6 (Auto, Relax, Beat, Scraping, Knead, Press)
Intensity Levels	30
Timer Settings	10-60 minutes (adjustable via remote), 15 minutes (fixed via unit button)
Battery Type	Lithium Ion (3 included)
Unit Runtime	Approx. 2 hours per unit per charge
Total Runtime (with charging case)	Up to 12 hours (720 minutes)
Pad Dimensions	3.23" x 1.86"
Pad Reusability	Up to 50 times (with proper cleaning)
Product Dimensions	4.21 x 3.03 x 5.1 inches
Weight	10.86 ounces
Manufacturer	KingPavonini

Safety Information

Important: Consult with a healthcare professional before using this device, especially if you have pre-existing medical conditions, are pregnant, have a pacemaker, or any other implanted medical device. Do not use on broken skin, over cancerous lesions, or near the heart or brain.
Statements regarding dietary supplements and medical devices have not been evaluated by the FDA and are not intended to diagnose, treat, cure, or prevent any disease or health condition. This device is intended for personal use as a muscle stimulator and for temporary relief of pain associated with sore and aching muscles due to strain from exercise or normal household and work activities.

Warranty and Support

KingPavonini is committed to providing high-quality products and customer satisfaction. Your KingPavonini Wireless TENS Unit Muscle Stimulator Model U13 is backed by long-term customer service. If you encounter any issues or have questions regarding the operation, maintenance, or performance of your device, please contact KingPavonini customer support through the retailer where you purchased the product or visit the official KingPavonini website for assistance. Please retain your purchase receipt as proof of purchase for any warranty claims.

Instructional Videos

For a visual guide on setting up and using your KingPavonini Wireless TENS Unit, please refer to the following instructional videos:

Wireless TENS Unit Review & Demonstration

Your browser does not support the video tag.

This video provides a comprehensive review and demonstration of the KingPavonini Wireless TENS Unit, covering its features and how it works. (Source: Product Demo Lab)

Detailed Look at TENS Unit Operation

Your browser does not support the video tag.

This video offers a closer look at the functionality and operation of the KingPavonini TENS Unit, demonstrating how to use its various settings. (Source: Searching For Treasures)

Unboxing and Initial Setup

Your browser does not support the video tag.

An unboxing and initial setup guide for the KingPavonini Wireless Muscle Stimulator. (Source: Taza)

© 2026 KingPavonini. All rights reserved.

Ask a question about this manual

Ask about setup, troubleshooting, compatibility, parts, safety, or missing instructions. Manuals+ will review the question and use this page's manual context to help answer it.

Name

Anonymous

Email

you@example.com

After a successful submission, we securely hash the supplied account or form email before sending it to Microsoft Advertising for conversion attribution. Privacy details.

Question

Example: How do I reset this device or fix this error?

Details

Model number, symptoms, what you tried, or the section of the manual you are using.

Submit question