


ASTM Standard for Quantifying Cell Viability



ASTM Standard for Quantifying Cell Viability Instructions


[Home](#) » [ASTM](#) » ASTM Standard for Quantifying Cell Viability Instructions 

Contents

- [1 ASTM Standard for Quantifying Cell Viability](#)
- [2 Standard Recognition Summary \(SRS\)](#)
- [3 Documents / Resources](#)
 - [3.1 References](#)
- [4 Related Posts](#)



ASTM Standard for Quantifying Cell Viability

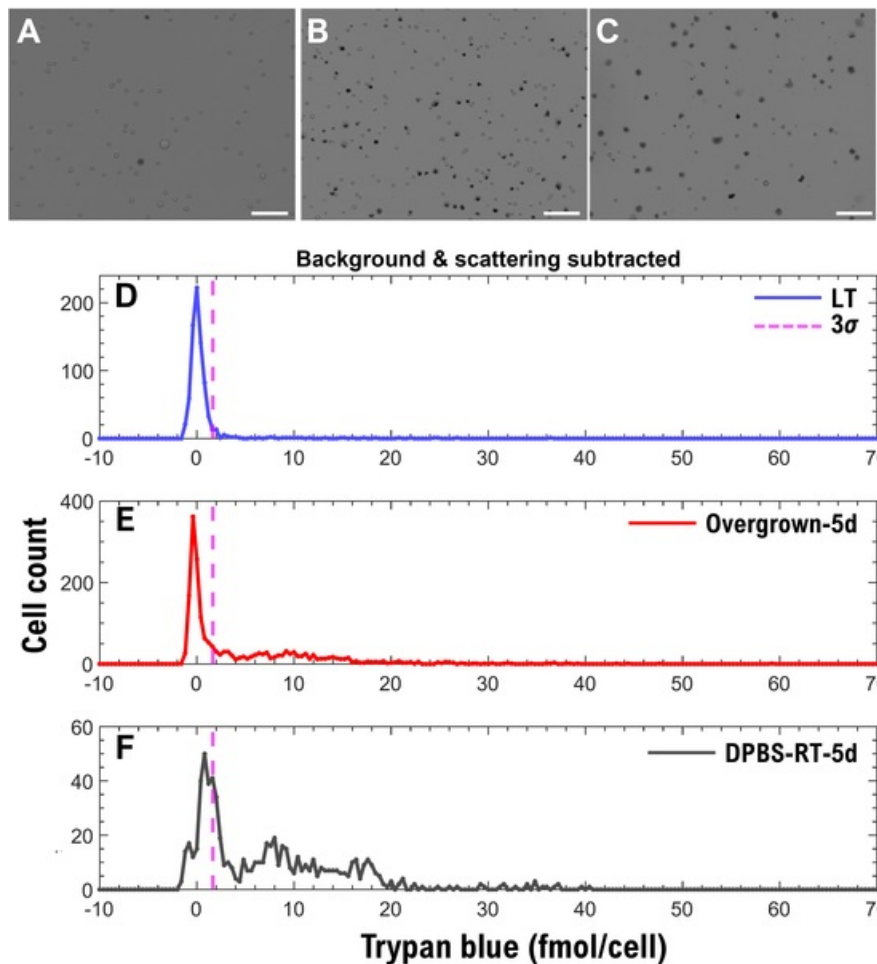

Standard Recognition Summary (SRS)

- **Recognition Number:** 004
- **SDO Name/Designation:** ASTM F2739
- **Date of Recognition:** 06/14/2023
- **Year of Publication:** 2019
- **Title:** Standard Guide for Quantifying Cell Viability and Related Attributes within Biomaterial Scaffolds
- **Scope:**
 1. This guide is a resource of cell viability test methods that can be used to assess the number and distribution of viable and non-viable cells within porous and non-porous, hard or soft biomaterial scaffolds, such as those used in tissue-engineered medical products (TEMPs).
 2. In addition to providing a compendium of available techniques, this guide describes materials-specific interactions with the cell assays that can interfere with accurate cell viability analysis and includes guidance on how to avoid or account for, or both, scaffold material/cell viability assay interactions.
 3. These methods can be used for 3-D scaffolds containing cells that have been cultured in vitro or for scaffold/cell constructs that are retrieved after implantation in living organisms.
 4. This guide does not propose acceptance criteria based on the application of cell viability test methods.
 5. The values stated in SI units are to be regarded as standard. No other units of measurement are included in this standard.
 6. This standard does not purport to address all of the safety concerns, if any, associated with its use. It is the responsibility of the user of this standard to establish appropriate safety, health, and environmental practices and determine the applicability of regulatory limitations prior to use.
 7. This international standard was developed in accordance with internationally recognized principles on


standardization established in the Decision on Principles for the Development of International Standards, Guides and Recommendations issued by the World Trade Organization Technical Barriers to Trade (TBT) Committee.

- **Extent of Recognition:** Partial Recognition.
- **Section not recognized:** 5.8.
- **Rational for Recognition:** This standard references ASTM F748, which conflicts with ISO 10993-1, for which FDA has published a guidance. Until ASTM 748 and ISO 10993 are reviewed by this program, the standard should be recognized except for the reference to ASTM F748.
- **Standard Development Organization:** <https://www.astm.org/>

Please note that this standard may also be recognized under the Center for Devices and Radiological Health's (CDRH) Recognized Consensus Standards Database for Medical Device, found here:

<https://www.accessdata.fda.gov/scripts/cdrh/cfdocs/cfStandards/search.cfm>.

Documents / Resources

	<p>ASTM Standard for Quantifying Cell Viability [pdf] Instructions Standard for Quantifying Cell Viability, Standard, for Quantifying Cell Viability, Quantifying Cell Viability, Cell Viability, Viability</p>
--	---

References

- [User Manual](#)

[Manuals+](#), [Privacy Policy](#)

This website is an independent publication and is neither affiliated with nor endorsed by any of the trademark owners. The "Bluetooth®" word mark and logos are registered trademarks owned by Bluetooth SIG, Inc. The "Wi-Fi®" word mark and logos are registered trademarks owned by the Wi-Fi Alliance. Any use of these marks on this website does not imply any affiliation with or endorsement.