



AtriCure CSK-6130 SUBTLE Cannula with Guide Instructions

[Home](#) » [AtriCure](#) » AtriCure CSK-6130 SUBTLE Cannula with Guide Instructions 

AtriCure CSK-6130 SUBTLE Cannula with



Contents

- 1 PRODUCT DESCRIPTION
- 2 PRODUCT FEATURES
- 3 INDICATIONS
- 4 CONTRAINDICATIONS
- 5 PRECAUTIONS
- 6 POTENTIAL COMPLICATIONS OF THE USE OF THE CANNULA WITH GUIDE
- 7 REQUIRED EQUIPMENT AND SUPPLIES PROVIDED BY HOSPITAL
- 8 RECOMMENDED EQUIPMENT
- 9 CANNULA SET UP
- 10 See Figure 2. Proximal End of Cannula with Guide
- 11 CANNULA DEPLOYMENT AND MANIPULATION
- 12 Cannula with Guide in Guidewire Deployment Position
- 13 AT COMPLETION OF PROCEDURE
- 14 TROUBLESHOOTING
- 15 ABBREVIATIONS
- 16 WARRANTY INFORMATION
- 17 DISCLAIMER
- 18 SYMBOLS GLOSSARY
- 19 Customer Service
- 20 Documents / Resources
- 21 Related Posts

PRODUCT DESCRIPTION


The Cannula with Guide (CSK-6130 & CSK-6140) is provided sterile, for single-use only. This product may be used in conjunction with the following devices provided separately:

[1] nContact Guided Coagulation System, sterile, single-use (under separate IFU)
The Cannula is manufactured PVC free and is not made with natural rubber latex.

PRODUCT FEATURES

See Figure 1. Cannula with Guide Key Features

FIGURE 1

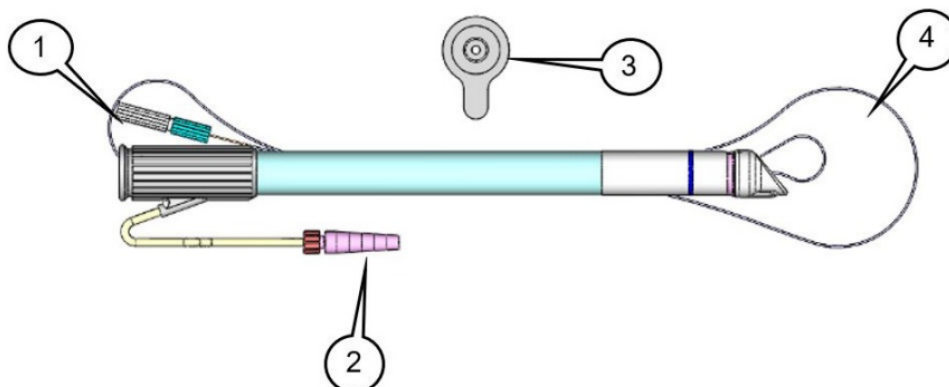

(1) Torquer; (2) Vacuum Port; (3) Cannula Cap; (4) Guidewire (0.026" Diameter)

INDICATIONS

The Cannula with Guide is indicated for endoscopic use to provide cardiothoracic surgical access for AtriCure instrumentation

CONTRAINDICATIONS

There are no known contraindications.



The cannula is provided sterile and is intended for single use only. Do not reprocess or reuse. Reuse can cause patient injury and/or the communication of infectious disease(s) from one patient to another. Inspect the device packaging prior to use. If any breach of the packaging is found, the sterility of the product cannot be assured, and the product should not be used.

Care should be taken when manipulating the guidewire, scope, and any over-the-wire devices.

Excessive forces may damage the cannula and/or guidewire or cause unintended tissue damage.

Inspect the cannula and guidewire prior to use. Ensure cannula distal end and guidewire are smooth with no sharp edges.

Sharp edge can cause potential patient harm. If sharp edge is found, device should not be used.

Care should be taken when inserting or removing the Cannula with Guide. Applying excess force could cause potential patient harm. To reduce friction during insertion, lubricate the cannula with sterile saline.

Care should be taken when manipulating the cannula or guidewire. Always ensure no tissue is caught by the guidewire and brought into the Cannula with Guide lumen as this may cause altered hemodynamics or unintended tissue damage. Avoid excessive pulling on the torquer. Excessive pulling on torquer may damage the cannula and/or guidewire or cause patient injury.



1. Endoscopic procedures should be performed only by physicians with adequate training with endoscopic techniques.
2. Avoid over-rotating the cannula with Guide. Over-rotation can cause the vacuum tubing of the cannula to kink, reducing the cannula suction, thus causing reduced visibility.
3. Avoid over-inserting the Cannula with Guide into patient body. Over insertion may reduce cannula suction.

POTENTIAL COMPLICATIONS OF THE USE OF THE CANNULA WITH GUIDE

- [1] Blunt trauma to adjacent organs
- [2] Infection
- [3] Pericardial effusion
- [4] Vessel injury
- [5] Tissue perforation
- [6] Hemodynamic instabilities
- [7] Arrhythmias
- [8] Thromboembolic complication
- [9] Hernia
- [10] Pneumothorax

REQUIRED EQUIPMENT AND SUPPLIES PROVIDED BY HOSPITAL

1. Vacuum Tubing Set (Sterile).

RECOMMENDED EQUIPMENT

1. 35 cm or 45 cm, 5 mm, and/or 10 mm Scope, depending on Cannula use.
2. 1000 mL 0.9% Normal Saline or Sterile Water.
3. nContact Guided Coagulation Device – Refer to Instructions for Use for the nContact Guided Coagulation Device when being used with the nContact Cannula with Guide.

CANNULA SET UP

1. Inspect all pouches, cartons, and packaging to ensure there has been no package damage, which may result in product contamination. If package damage is discovered, do not use – replace the product.
 - a) Outside the sterile field, remove the pouched cannula from carton.
 - b) Using sterile techniques remove cannula and tray from the pouch and place near patient.
 - c) Remove cannula, cap, and stopcock from tray




WARNING: When removing cannula from packaging, care should be taken to ensure guidewire and cannula cap remain inside sterile field to reduce risk of infection.
de sterile field to reduce risk of infection.

2. Prior to inserting the cannula into body cavity, examine the cannula functionality to ensure no damage during shipping occurred.
3. Examine cannula to ensure distal end and guidewire are not damaged and are smooth with no sharp edges. If cannula is damaged or has sharp edges, do not use – replace the product.
4. Examine cannula to ensure proximal end (Fig. 2) has no damage. If cannula is damaged, do not use – replace the product.
5. If perfusion through the vacuum lumen is preferred, then attach a stopcock as shown in Fig 2. A stopcock is supplied with the 30 cm cannula. Connect perfusion tubing to perfusion port in Figure 2. Insert IV tubing into bag of 0.9% normal saline or sterile water.

See Figure 2. Proximal End of Cannula with Guide

- (1) Cannula Cap;
- (2) Cannula Grip;
- (3) Vacuum Port;
- (4) Stop


FIGURE 2

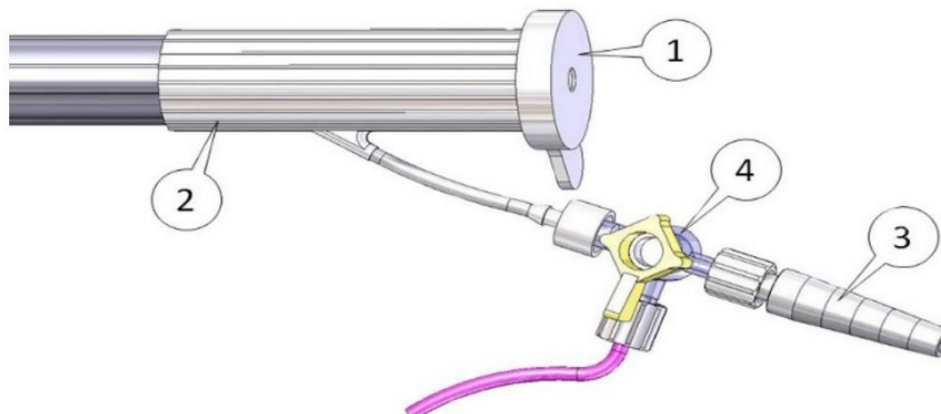

CANNULA DEPLOYMENT AND MANIPULATION

1. Remove torquer from the end of guidewire and thread guidewire through available hole in the center of the cannula cap (**Fig. 3**). Replace torquer over proximal end of guidewire once guidewire is threaded through cap.

FIGURE 3

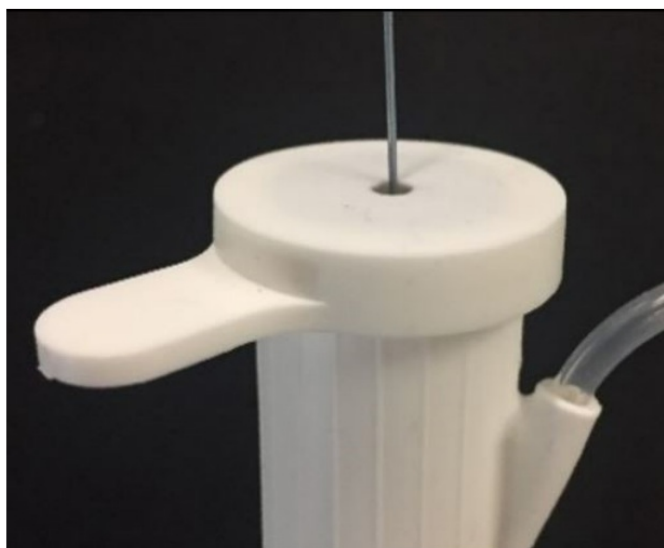

⚠ CAUTION: Failure to place guidewire through hole in center of cap (puncturing cap or placing outside cap entirely) may reduce cap functionality.

⚠ CAUTION: Failure to replace torquer exposes the sharp proximal end of the guidewire.

2. Push cap onto end of cannula handle.

See Figure 3. Cannula with Guide, (Cap and Guidewire)

⚠ CAUTION: Ensure cannula cap is fully attached to the cannula handle – failure to fully attach cap may reduce functionality of the cannula cap.


3. Lubricate exterior of the Cannula with sterile water.

4. Fully retract the guidewire into the lumen of the Cannula with Guide (Fig. 4) prior to insertion into the body

Figure4

Cannula with Guide in Guidewire Deployment Position

FIGURE 4

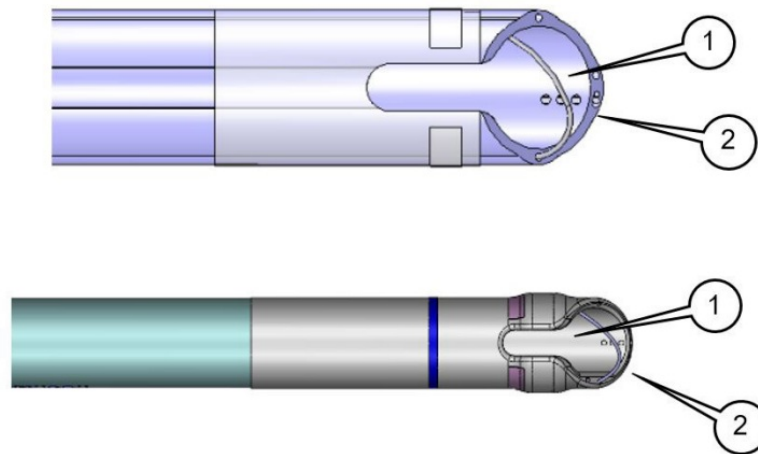

(1) Guidewire; (2) Distal End of Cannula

WARNING: Insertion or removal of the Cannula with Guide while guidewire is extended may cause potential patient harm.

Always fully retract the guidewire into the Cannula with Guide lumen.

5. Before inserting instruments, lubricate cannula lumen by injecting approximately 20 cc sterile water or saline through hole in center of cannula cap.
6. Insert scope into hole in cannula cap as required for visualization. A blue line is on the outside of the cannula to be used as a reference position for the laparoscope (for CSK-6130 only).
7. If resistance is felt as the scope is being inserted, pull back on the scope to readjust its position. Once the position has been adjusted re-insert the scope into the cannula.
8. Insert the Cannula with Guide into the body as desired to create space and visibility. A blue marker line is indicated on the distal end of the cannula, which may be used to facilitate orientation.



CAUTION: Do not manipulate cannula by grasping the tab of the cannula cap. Doing so may loosen or remove cannula cap from cannula causing reduced functionality.

9. Use the guidewire to aid in visualization and in the positioning and manipulation of over-the-wire devices for operative or diagnostic procedures.
10. To use an over-the-wire device, remove the cannula cap from the cannula. Follow device instructions for use for set-up/ manipulation of the over-the-wire device.



WARNING: Cannula cap and torquer should be removed prior to insertion and removal of any over-the-wire devices. Failure to remove cap prior to insertion may result in damage to the cannula cap and/or the over-the-wire devices preventing application of the intended therapy.

11. Connect one end of the vacuum tubing to vacuum port (Fig. 2, #3), and the other to the vacuum trap. Set vacuum pressure to -200 mmHg to remove fluid. Suction saline to improve visibility.

CAUTION: Do not exceed a vacuum pressure of -550 mmHg.

12. Retract surgical instruments from the cannula lumen.
13. Retract the guidewire into the cannula lumen.
14. Remove the Cannula with Guide from the body.



CAUTION: Do not modify cannula – modification could produce sharp edges.



WARNING: Care should be taken when handling surgical instruments near the distal end of the cannula – do not clamp the distal end of the guidewire with surgical instruments or allow surgical instruments to stay outside the cannula ID during manipulation.



CAUTION: To avoid interruption of vacuum or perfusion flow, ensure tubing is not clamped or kinked during coagulation of tissue.



CAUTION: Large blood clots and tissue particles may clog vacuum lumen and impair suction to Cannula with Guide.

AT COMPLETION OF PROCEDURE

Remove cannula from tissue, disconnect all tubes, and discard cannula and tubing sets following local governing ordinances and recycling plans for disposal or recycling of device components.

TROUBLESHOOTING

Symptom	Action
Not able to draw vacuum	<ul style="list-style-type: none">• Check vacuum connections.• Ensure vacuum regulator is set to -200 mmHg.• Examine cannula vacuum lumen for clots.• If clogged, flush vacuum lumen with sterile water.• If problem persists, replace cann
Unable to advance instruments within cannula lumen.	<ul style="list-style-type: none">• Lubricate lumen with sterile water.• Ensure instruments are correct size.

ABBREVIATIONS

- **IFU:** Instructions for Use
- **LBL:** Label

WARRANTY INFORMATION

AtriCure warrants that reasonable care has been used in the design and manufacture of this instrument. This warranty is in lieu of and excludes all other warranties not expressly set forth herein, whether expressed or implied by operation of law or otherwise, including, but not limited to, any implied warranties of merchantability or fitness for a particular use. AtriCure's sole obligation under this warranty is limited to the repair or replacement of this instrument. AtriCure neither assumes, nor authorizes any other person to assume for it, any other or additional liability or responsibility in connection with this instrument. Handling, storage, cleaning and sterilization of this instrument as well as other factors relating to the patient, diagnosis, treatment, surgical procedures, and other matters beyond AtriCure's control directly affect the instrument and the result obtained from its use. AtriCure assumes no liability with respect to instruments deliberately mis-used or those reused, reprocessed or resterilized and makes no warranties expressed or implied, including but not limited to merchantability or fitness for intended use, with respect to such mis-used or reused instruments. AtriCure shall not be liable for any incidental or

















consequential loss, damage, or expense directly or indirectly arising from the deliberate mis-use or re-use of this instrument.

DISCLAIMER

Users assume responsibility for approving the acceptable condition of this product before it is used, and for ensuring that the product is only used in the manner described in these instructions for use, including, but not limited to, ensuring that the product is not re-used.

Under no circumstances will AtriCure, Inc. be responsible for any incidental, special or consequential loss, damage, or expense, which is the result of the deliberate misuse or re-use of this product, including any loss, damage, or expense which is related to personal injury or damage to property.

SYMBOLS GLOSSARY

	Caution		Do not re-sterilize		CE Mark and Identification number of Notified Body\
	Sterilized Using Irradiation		Transit Humidity Limit		Authorized Representative in the European Community
	Single Use Only		Not made with natural rubber latex or dry natural rubber		Consult Instructions for Use
	Use by Date		Lot Number		Manufacturer
	Caution: Federal		Catalog Number		Do Not Use if Package is Damaged
	Transit Temperature Limit				

Customer Service

Manufacturer AtriCure Incorporated 7555 Innovation Way Mason, Ohio 45040 USA

Customer Service:

1-866-349-2342 (toll free)

+1 513-755-4100

(phone)

European Representative:

AtriCure Europe B.V.

De entree 260

1101 EE Amsterdam

NL

+31 20 7005560

ear@atricure.com



Documents / Resources



[AtriCure CSK-6130 SUBTLE Cannula with Guide](#) [pdf] Instructions

CSK-6130 SUBTLE Cannula with Guide, CSK-6130, SUBTLE Cannula with Guide, Cannula with Guide

[Manuals+](#)