

B HLMANN IBDoc Calprotectin Application User Guide


[Home](#) » [B HLMANN](#) » B HLMANN IBDoc Calprotectin Application User Guide 

Contents

- [1 B HLMANN IBDoc Calprotectin Application](#)
- [2 Product Information](#)
- [3 Product Usage Instructions](#)
- [4 Using Instructions](#)
- [5 Contact](#)
- [6 Documents / Resources](#)
 - [6.1 References](#)



B HLMANN IBDoc Calprotectin Application

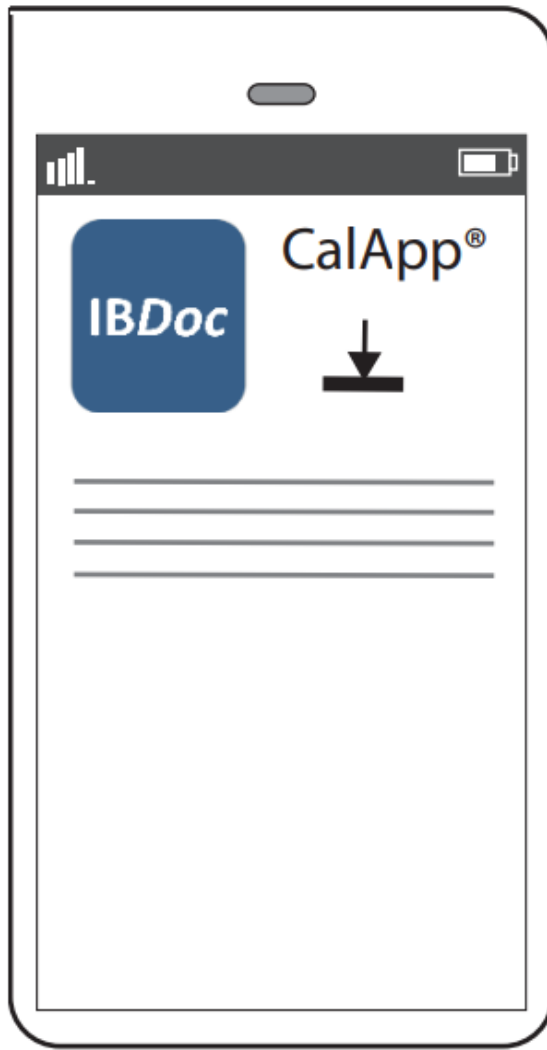

Product Information

- **Product Name:** Quantum Blue Calprotectin TC Testcassette
- **Product Code:** BR-ECFAL-TCB-LFCALUS-TC
- **Lot Number:** 3004
- **Manufacturer:** Buhlmann Laboratories
- **Contact Information:**
 - **Phone:** +41 61 487 12 12
 - **Fax Orders:** +41 61 487 12 99
 - **Email:** info@buhlmannlabs.ch
 - **Website:** www.buhlmannlabs.ch


Product Usage Instructions





1. Ensure you have downloaded the complete user manual from the website www.ibdoc.net.
2. Open the product packaging and take out the Quantum Blue Calprotectin TC Testcassette.
3. Verify the lot number on the test cassette. It should match the lot number mentioned in the user manual (Lot Number: 3004).
4. Read the complete user manual for detailed instructions on performing the test.
5. Prepare the sample according to the instructions provided in the user manual.






6. Place the test cassette on a flat surface.
7. Add the prepared sample to the sample well of the test cassette.
8. Wait for 10 seconds.
9. Press the “Click!” button on the test cassette to initiate the test.
10. Observe the test results after the specified time mentioned in the user manual (e.g., 10 seconds).
11. Record the test results and refer to the interpretation guidelines in the user manual to determine the calprotectin levels.
12. If required, save any additional notes or observations using the “Save” function on the device.
13. Dispose of the used test cassette following proper waste disposal guidelines.

Please note that these instructions are a brief summary. For complete and accurate usage instructions, refer to the user manual downloaded from www.ibdoc.net.


Using Instructions

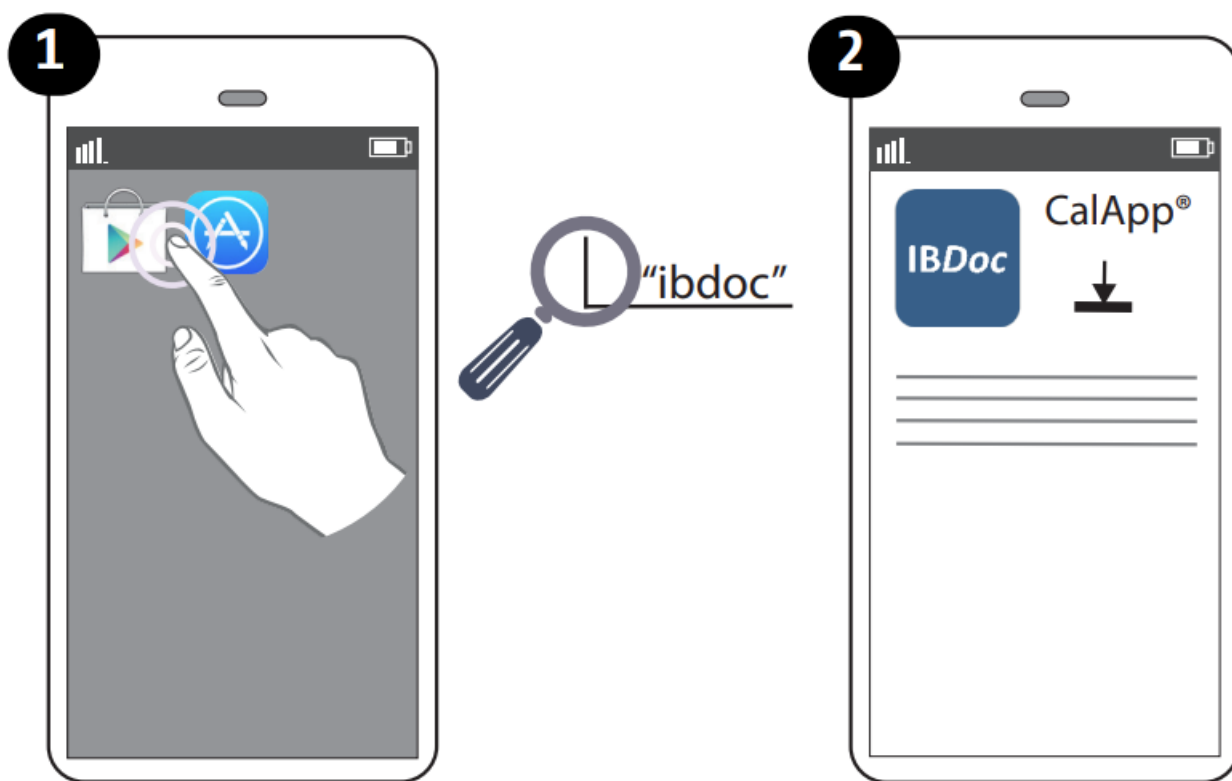

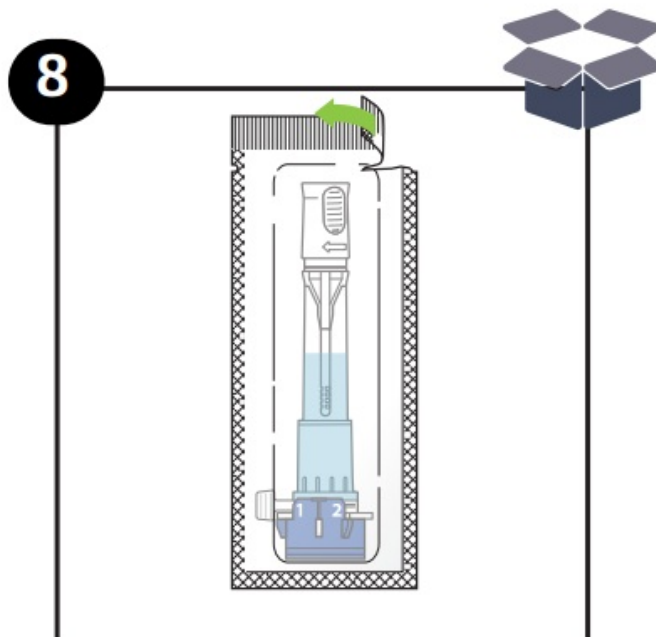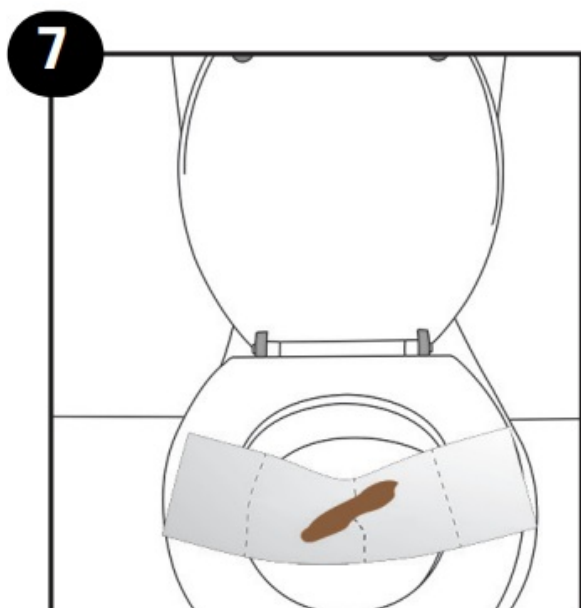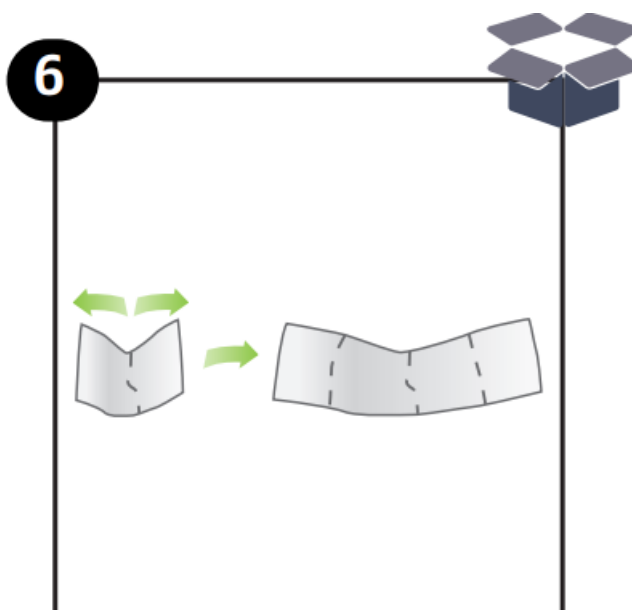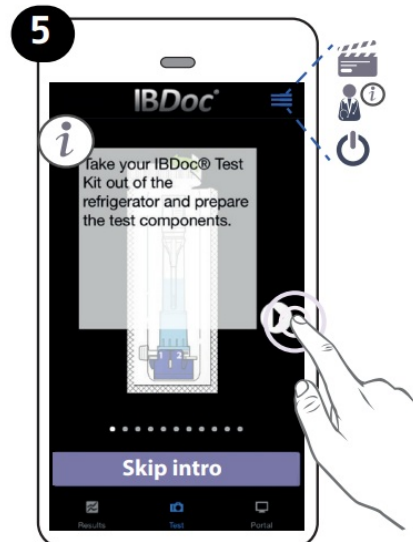


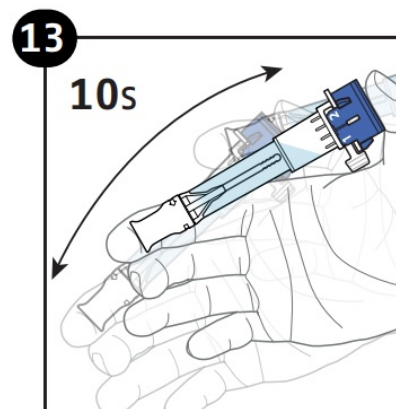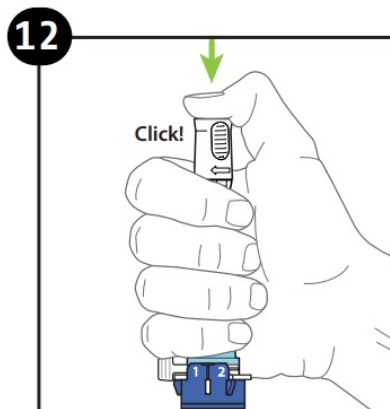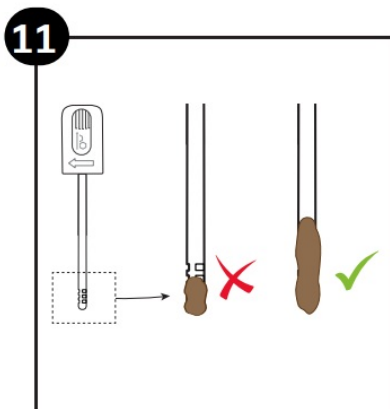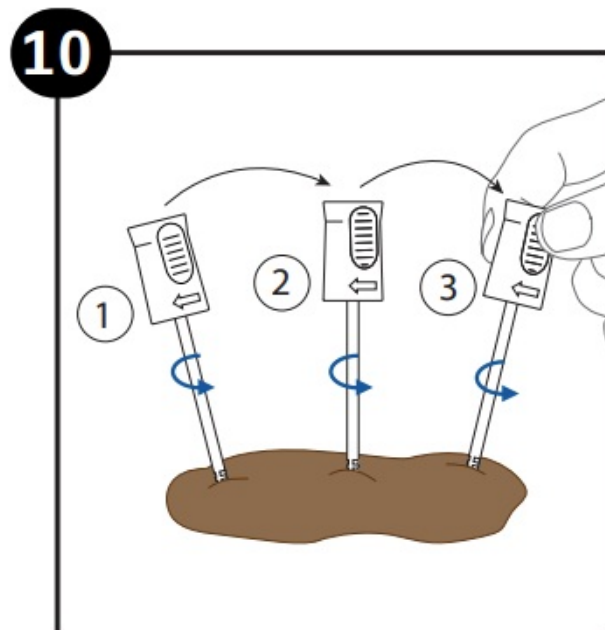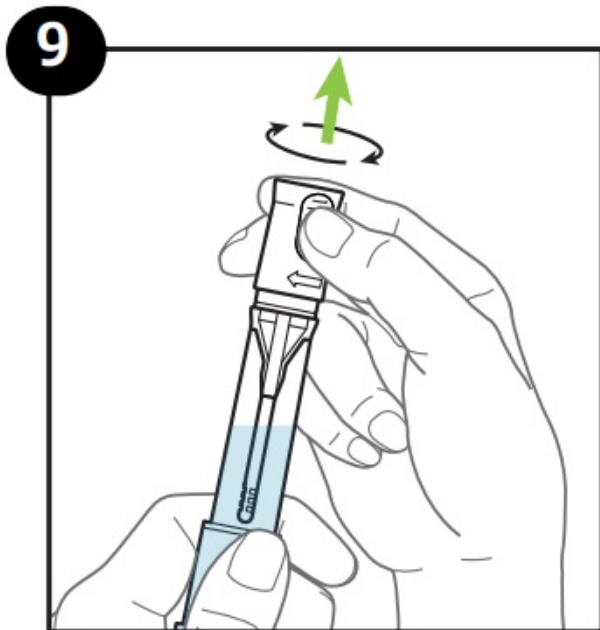


14

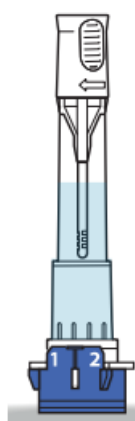


**MIN 2H
MAX 24H**




15

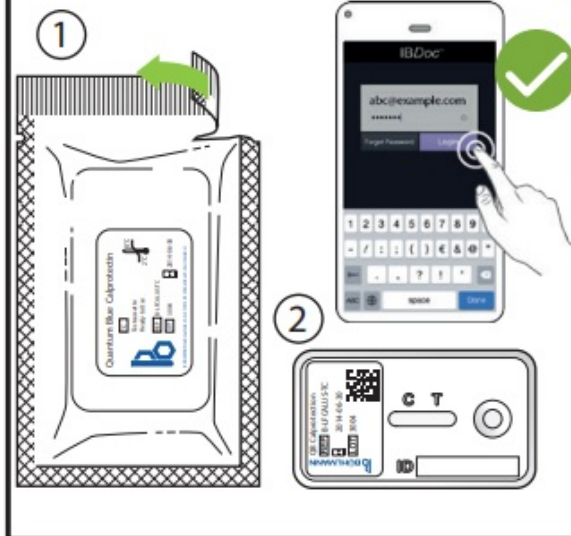


16

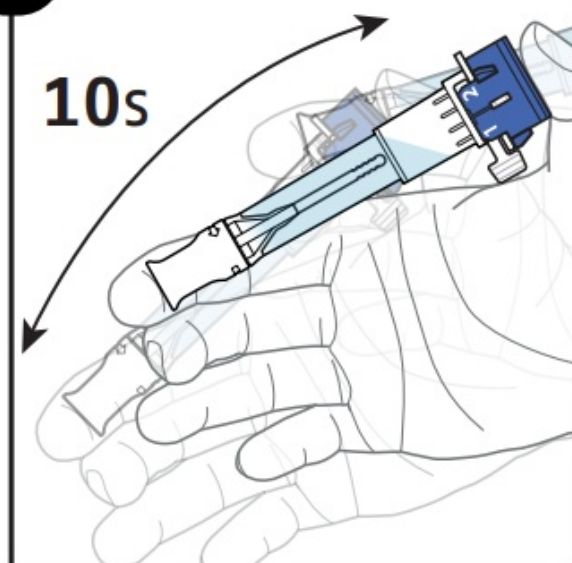


17

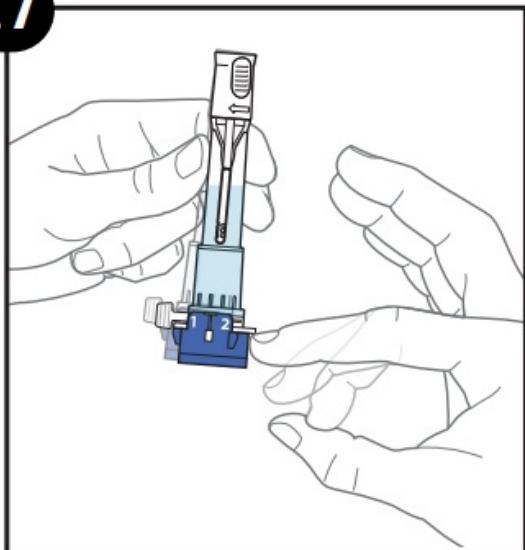



18

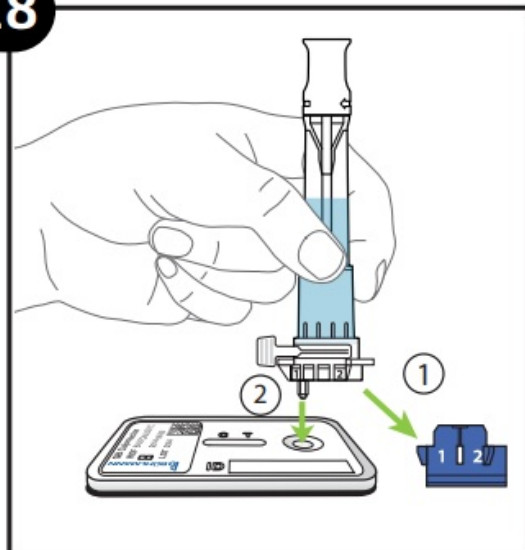


19







20

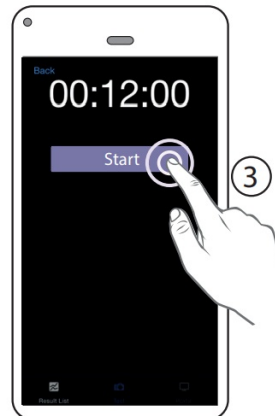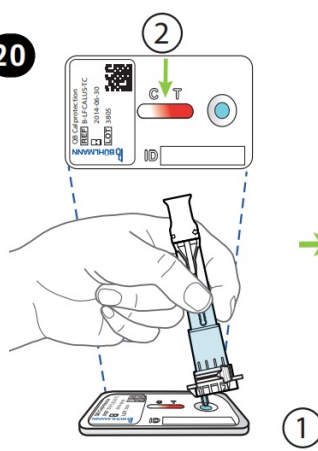

21

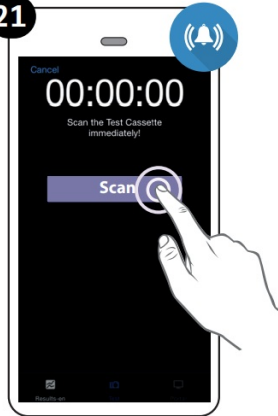

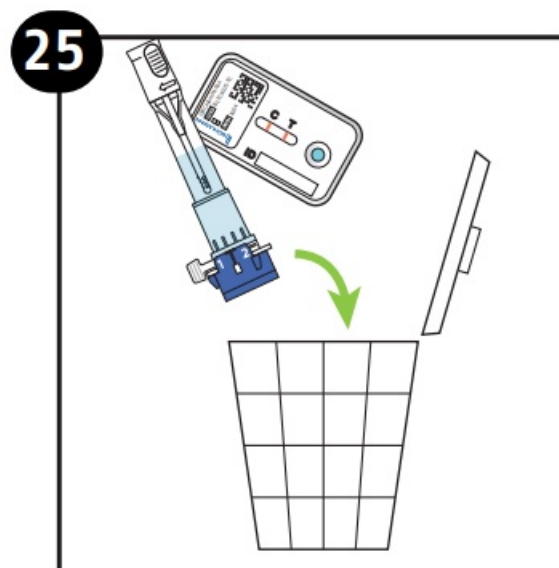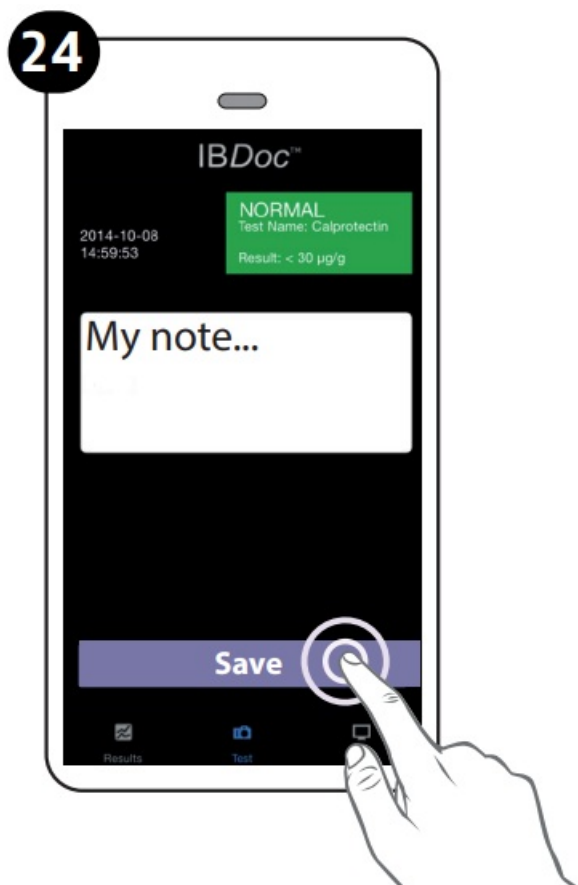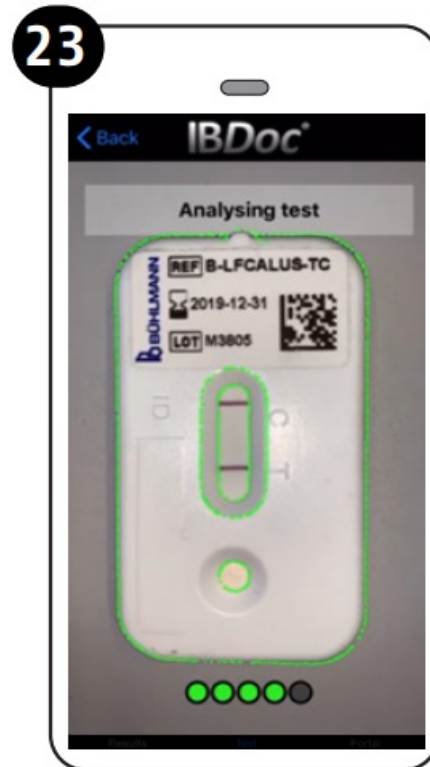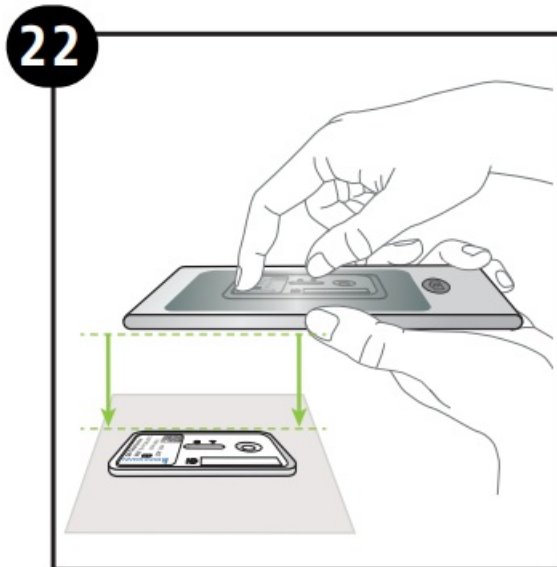

Warning



- The full instruction for use can be downloaded on www.ibdoc.net.

Contact

BÜHLMANN Laboratories AG


- Baselstrasse 55
- 4124 Schönenbuch/Basel Switzerland
- **Phone:** +41 61 487 12 12
- **Fax orders:** +41 61 487 12 99
- info@buhlmannlabs.ch
- www.buhlmannlabs.ch

Scan



CALEX®, IBDoc® and CalApp® are a registered trademarks of BÜHLMANN in many countries.

Documents / Resources

	B HLMANN IBDoc Calprotectin Application [pdf] User Guide IBDoc Calprotectin Application, IBDoc Calprotectin, Application
---	---

References

-  [IBDoc® by BÜHLMANN | Monitor IBD | Calprotectin Home Test](#)
-  buhlmannlabs.ch
-  [IBDoc® by BÜHLMANN | Monitor IBD | Calprotectin Home Test](#)