



Creative EHL-1A Dynamic ECG Recorder User Manual


[Home](#) » [Creative](#) » Creative EHL-1A Dynamic ECG Recorder User Manual 

Contents

- 1 Creative EHL-1A Dynamic ECG Recorder
- 2 Specifications
- 3 Product Information
- 4 Product Usage Instructions
- 5 Frequently Asked Questions (FAQ)
- 6 The basics
- 7 Introduction
- 8 Using Instructions
 - 8.1 Measuring process
 - 8.2 Installation the App
 - 8.3 Using the App
 - 8.4 Data view
- 9 Maintenance
- 10 Accessories
- 11 Specifications
- 12 FCC Warning:
- 13 Electromagnetic compatibility
- 14 ABOUT COMPANY
- 15 Documents / Resources
 - 15.1 References
- 16 Related Posts

Creative

Creative EHL-1A Dynamic ECG Recorder

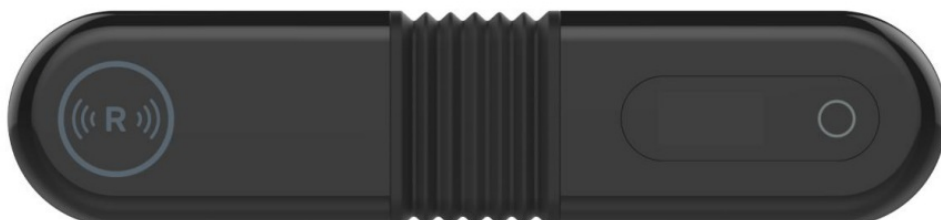

Specifications

- **Product Name:** Dynamic ECG recorder
- **Models:** EHL-1A, EHL-1B, EPatch-A, EPatch-B
- **Enclosure Color:** Black, White
- **Measurement data:** 1-10

Product Information

Intended Use

The Dynamic ECG recorder is designed for monitoring and recording electrocardiogram data for diagnostic purposes.

About EHL-1A, EHL-1B, EPatch-A, EPatch-B

- **Right sign:** Wear with the R side on the right hand side.
- **Display screen:** Shows power, heart rate, charging status, and other information.
- **Power interface contacts:** Connect charging cables.
- **Electrode buckle:** Connect chest straps, disposable ECG electrodes, or charging cables.

Symbols

- **Type BF-Applied Part:** Indicates the type of applied part.
- **IP22:** Protection against water and access to hazardous parts.
- **SN:** Serial number identification.
- **Rx only:** For prescription use only.

Product Structure and Composition

The product includes the Dynamic ECG recorder main unit, OTG adapter, charging cable, and optional chest strap and disposable ECG electrode.

Product Usage Instructions

Before Use

Prior to taking measurements, ensure the following:

- Use only specified cables and accessories.
- This device does not have an audible alarm function.
- Avoid ungrounded equipment near the patient for accurate readings.

Frequently Asked Questions (FAQ)

- **Can this device be used by individuals with pacemakers?**

No, it is not recommended to use this device if you have a pacemaker.

- **What should I do if the device is exposed to water?**

If the device comes into contact with water, immediately disconnect it from any power source and do not

attempt to use it. Contact customer support for assistance.

The basics

This manual contains the instructions necessary to operate the product safely and in accordance with its function and intended use. Observance of this manual is a prerequisite for proper product performance and correct operation and ensures patient and operator safety.

Safety

Warnings and Cautionary Advices

- Before using this equipment, please read this manual carefully and fully understand the warnings and risks.
- This device is not intended to replace the medical diagnosis of a professional doctor.
- The measurement results of this device are for reference only and cannot be directly used as a basis for clinical treatment.
- We do not recommend the use of this device if you have a pacemaker or other implantable device in your body. Please follow the doctor's advice if necessary.
- This device cannot be used with a defibrillator or X-ray (γ-ray) or infrared radiation
- This device cannot be used during MRI CT Diathermy Electrocautery RFID or nuclear magnetic resonance (MRI) procedures.
- The device may present a risk of projectile injury due to the presence of ferromagnetic materials that can be attracted by the MR magnet core.
- Thermal injury and burns may occur due to the metal components of the device that can heat during MR scanning.
- The device may generate artifacts in the MR image.
- The device may not function properly due to the strong magnetic and radiofrequency fields generated by the MR scanner.
- This device cannot be used in an aircraft environment.
- This equipment must not be used in a flammable environment (eg oxygen-rich environment).
- This device is not intended for use by infants weighing less than 10 kg.
- Do not swim or submerge the device in the water. Do not immerse the device in water or other liquids.
- Do not use acetone or other volatile solutions to clean the device.
- Do not strongly collide or crush the device. If the casing is broken, stop using it.
- This device cannot be placed in a pressure vessel or gas sterilization equipment.
- Do not disassemble the device at will, otherwise it may cause machine malfunction or affect the normal operation of the device.
- Keep this device out of the reach of children or pets.
- This device should not be used on people with sensitive skin or allergies.
- This equipment cannot be placed in the following environments: direct sunlight, high temperature, high humidity, close to water or fire sources, and high electromagnetic influence.
- Users should try to avoid sweating. The sweat will affect the contact between the electrodes and the skin, affecting the quality of the measurement.
- Users should inspect loosened electrodes, that can degrade performance or cause other problems
- Do not participate in violent or extensive physical activity in order to make appropriate measurements.
- The measurement results of this device cannot distinguish all diseases. If your body feels unwell, you should

consult your doctor immediately, in addition to the measurement results of this device.

- Do not self-diagnose and take medication based on the measurements of this device without consulting your doctor. In particular, do not take new medications without prior permission.
- This device is not a substitute for professional heart or other organ function measurement equipment. Medical ECG measurement requires more professional and complete measurements.
- This device cannot be used to diagnose a disease directly. Please consult your doctor.
- We recommend that you record your ECG curve and the results of the measurements and provide them to your doctor if necessary.
- Waste (including the equipment itself is scrapped) is disposed of in accordance with relevant laws and regulations.
- When the ambient temperature is 20 °C, the minimum and maximum storage temperature from the product to ready for use is 2H the time required .
- The patient is the expected user.
- Do not pile up the long tubing at the head of the bed, as it may wrap around the head or neck of the patient during sleep.
- Li batteries capacity will decrease after charge discharge for 300 times.
- The electrodes (Applied parts) should not contact other conductive parts including earth.
- The product should not be maintained while in use.
- The product is for prescription use.
- Federal (U.S.) Law restricts this device to sale by or on the order of a physician.

Introduction

Product

Name: Dynamic ECG recorder

Model: EHL-1A,EHL-b,EPatch-A,EPatch-B

Model	Enclosure Color	Measurement data
EHL-1A	Black	1
EHL-1B	Black	10
EPatch-A	White	1
EPatch-B	White	10

Intended Use

The Dynamic ECG recorder is intended to capture, record, and store continuous electrocardiogram (ECG) information for long-term monitoring (up to 7 days) at home or in healthcare environment. It is indicated for use on adult patients 18 years or older who may be asymptomatic or who may suffer from transient symptoms such as palpitations, shortness of breath, dizziness, light-headedness, pre-syncope, syncope, fatigue, or anxiety. The ECG metrics include single-lead information which is provided for review by technicians or clinicians to render a diagnosis based on clinical judgment and experience.

Contraindications:


The product is not intended for use in patients with cardiac pacemakers or other implantable devices.

- The product is NOT intended for use during external defibrillation procedures; such use may cause the

defibrillator's discharge pulse to be ineffective for the patient.

- The product is NOT to be used in a magnetic resonance imaging (MRI) environment. The device must be removed from the patient's skin before any MRI procedure.
- The device is NOT intended for use on patients with unhealed surgical incisions/dressings on the thoracic regions.
- The product is NOT intended for use on patients with skin or soft tissue damage in the area where the product is placed (such as burns, irritation, infections, wounds, etc.).

About EHL-1A,EHL-1B,EPatch-A,EPatch-B

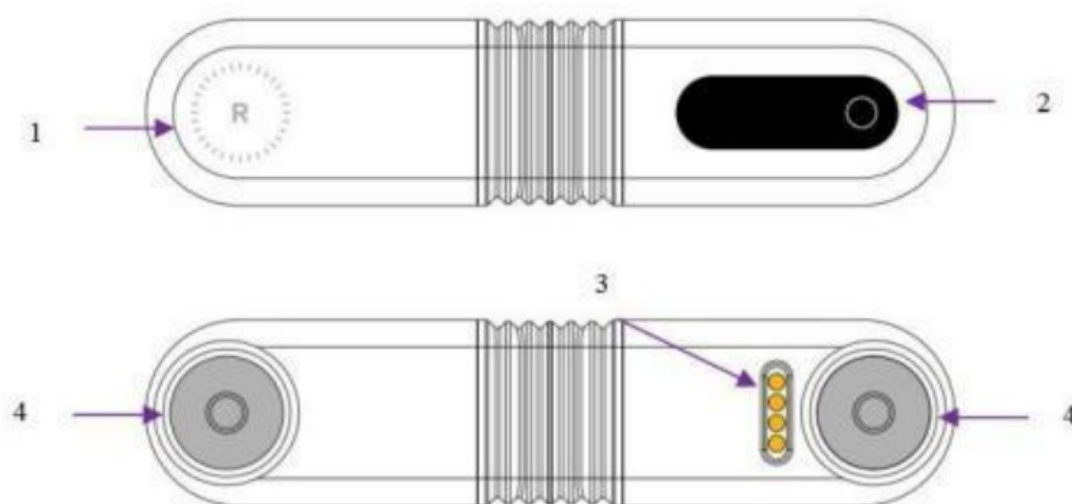

1. Right sign

When wearing, the side marked “R” should be on the right hand side of the wearer.

2. Display screen

The display displays the device's power, heart rate, charging status and other information.









3. Power interface contacts

Used to connect charging cables.

4. Electrode buckle

Used to connect chest straps, disposable ECG electrodes or charging cables.

Symbols

Symbol	Significance
	Type BF-Applied Part
	Manufacturer
	Authorized representative in the European Community
	Caution , Incorrect use may cause personal injury and damages of goods. Refer to instruction manual.
IP22	Protected against spraying water and against access to hazardous parts with a tool, per IEC 60529.
	Follow Instructions for Use.
	Non-ionizing radiation
SN	Serial number
	Indicate separate collection for electrical and electronic equipment (WEEE).
Rx only	Prescription Use
	MRI unsafe. Presents hazards in all MR environments as product contains strongly ferromagnetic materials.

Product structure and composition

This product is mainly composed of Dynamic ECG recorder main unit, OTG adapter, charging cable and Chest strap (optional). Disposable ECG electrode(optional).

Using Instructions

Before use

Warnings and Cautionary Advices

Before taking measurements, please pay attention to the following points to ensure the accuracy of the measurement data.

- Use only the cables and accessories specified in this manual.
- This device has no alarm function and therefore does not generate an audible alarm for the result of the measurement.
- Ungrounded equipment next to the patient and interference from electrosurgery can cause waveform instability.

Open box to check

- Please check the box carefully before unpacking. If you find any damage, please contact the carrier or the company immediately

- If the package is complete, unpack the package in the correct way and carefully remove the device and other components from the box. Check the device for any mechanical damage and complete items.
- If you have any questions, please contact us immediately.

Warnings and Cautionary Advices

- Please save the box and packing materials for future transportation or storage.
- When handling packaging materials, you must follow local regulations or the hospital's waste disposal system and place the packaging materials out of reach of children.
- The device may be contaminated by microorganisms during storage, transportation and use. Please confirm that the packaging is in good condition before use.
- The date of manufacture and the date of use of the product are listed on the label.

Boot

When the device is shipped from the factory, it is completely inactive by default. The device should be charged to activate the device before it is used for the first time.

Measuring process

1. Measurement methods

1. ECG electrode wearing method:

Remove the packaging of the single-use ECG electrode, install the ECG electrode on the device through the electrode buckle, and wear the Dynamic ECG recorder with the ECG electrode on the chest as shown in the figure.

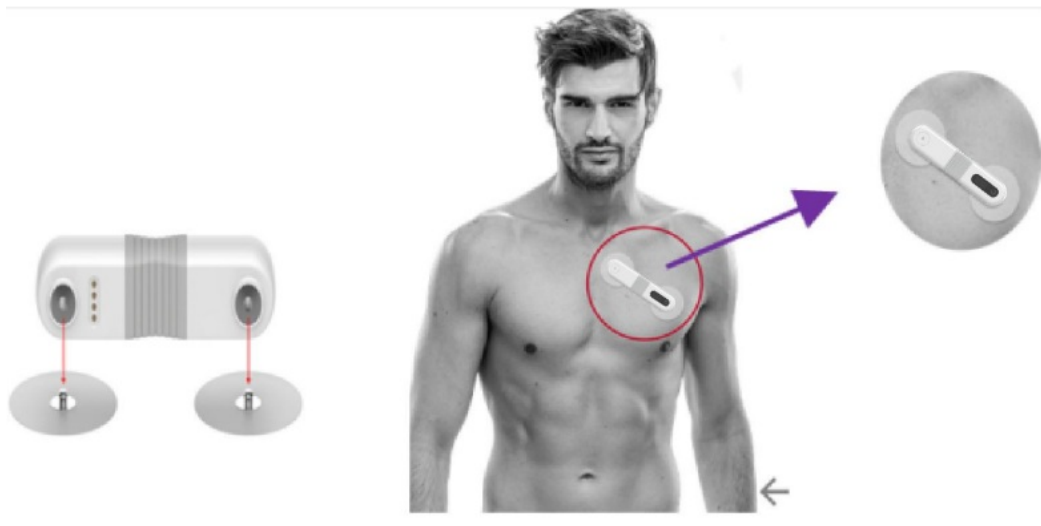


Figure 2

2. Chest Strap measurement method:

Attach the main unit to the strap and then wear the Chest strap with the main unit attached to the precordium (The marked with the English letter "R" is on the right hand side of the wearer.) as shown below.

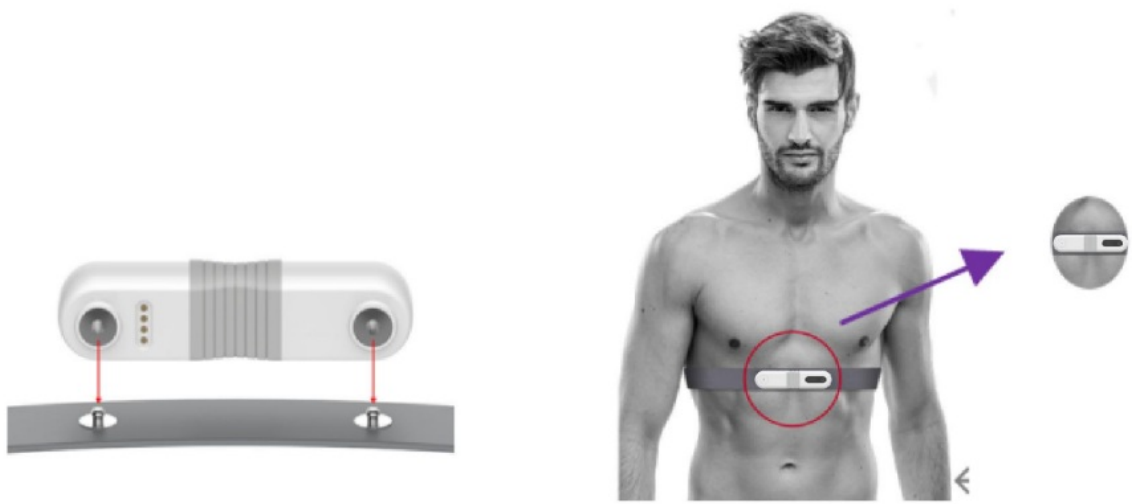


Figure 3

Precautions:

- Before use, please check whether the single-use ECG electrode is within the validity period.
- The ECG electrode must be in direct contact with the skin.
- Before wearing, if necessary, remove the hair on the electrode part, then clean the skin with clean water, and dry it before attaching the ECG electrode
- When using the Chest strap measurement method, if necessary, remove the hair from the electrode part, then clean the skin with water, and then apply the electrode after drying.
- Do not speak and remain still during the measurement. Any movement will affect the measurement results.
- Please sit when measuring possible.

2. Measuring step

1. After selecting a measurement method, the device detects that the ECG signal is automatically turned on, The display displays the ECG waveform with heart rate ,the device starts to measure.
2. The duration of a measurement is 5 minutes to 168 hours. If you want to end the measurement, please remove the Disposable ECG electrodes or unfasten the chest strap to remove the device. After 1 minute, the device completes data storage.
3. When the test is less than 5 minutes, there is no data to save, and more than 5 minutes will be saved. When the continuous measurement time is 168 hours, the measurement will be ended and the data will be saved.

Installation the App

Download the App

- **App name:** ViHealth Mobile
- **App Version:** V1.0.0
- **iOS:** App Store
- **Android:** Google Play




Install the App

Install the app on an Apple product or Android-powered device, including smart phones and tablets.

Using the App

Preparing to Start


1. Make sure that Bluetooth is enabled on your smart device and run ViHealth.
2. Follow the screen guide to sign in or sign up. You can also choose the guest mode.
3. Tap the detected monitor icon “ER1” in the ViHealth app
4. Click the device icon Tap the detected monitor icon “ER1” in the ViHealth app, then hold and touch the electrodes on the monitor to start pairing.

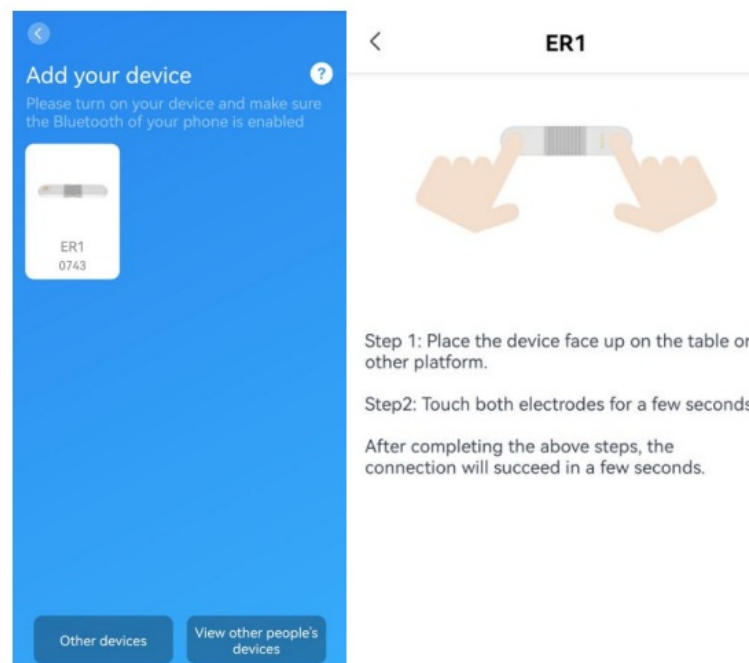

Data view


You can review history measurement results on the History screen. Tap the desired recording to view detailed information. There are two different types of records:

- Heart rate recording, which is transmitted from the monitor.
- ECG recording, which is generated after real-time ECG recording.

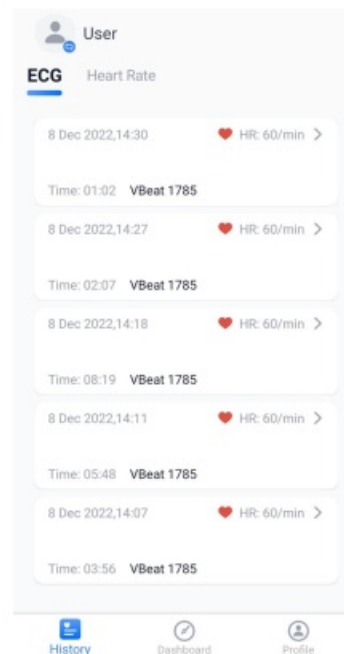

Heart Rate Recording

- Detailed information is displayed in a heart rate recording, including measurement time, maximum heart rate, average heart rate, heart rate motion and trend curves.

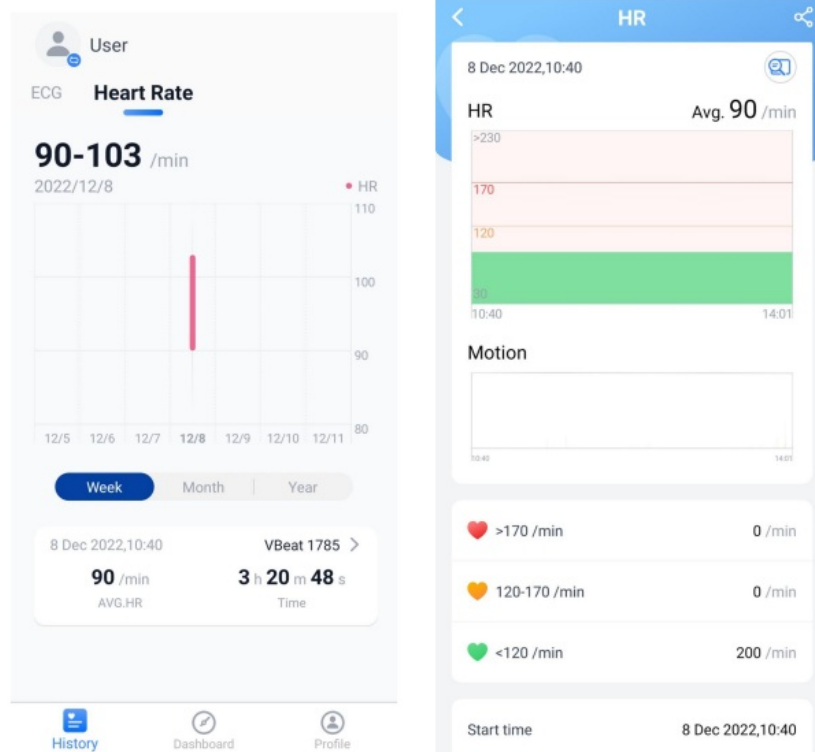

- The different colors in the heart rate zones signify setting heart rate targets. You can adjust the values of [HR Target 1] and [HR Target 2] in the Settings screen.



Heart rate > [HR Target 2]




[HR Target 1] ≤ Heart rate ≤ [HR Target 2]




Heart rate < [HR Target 1]

- **Adding Notes**

- Slide down the screen to input notes about a recording.
- Sharing Heart Rate Recording
- Tap  to share the current heart rate recording as an image.

ECG Recording

The recording data will be displayed in rows of ten seconds. The maximum measurement time is 30 minutes.

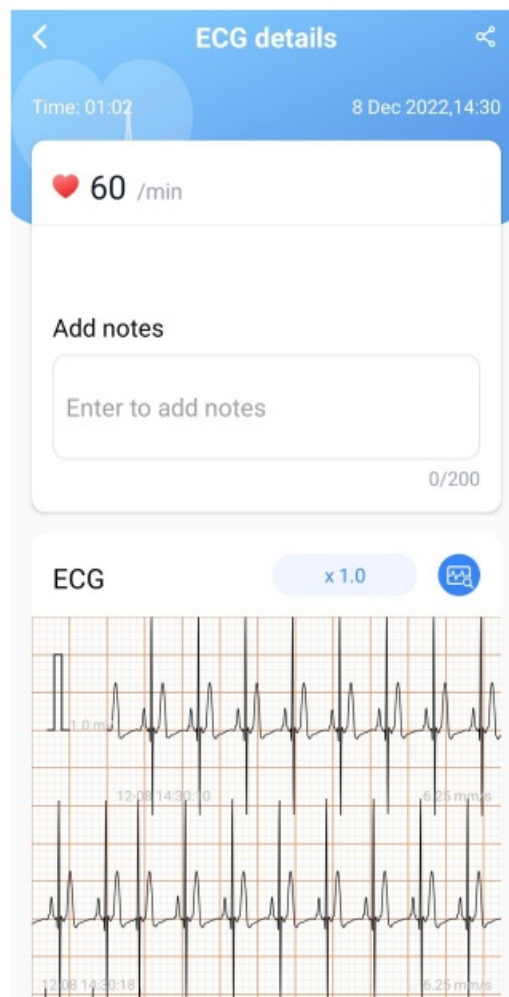

- **Adding Note**

Input notes about a recording.

- **Sharing ECG Record**

Tap to share the current ECG record as a PDF file.

- **Displaying Full Screen Waveform**

Tap  to view the ECG waveform in full screen.


- **Adjusting Waveform Amplitudes**

Tap x1.0 to adjust the amplitude for the ECG waveform. Options: 0.5mV/1mV/2mV

Deleting Records

To delete a record:

1. Swipe a recording to the left.
2. Choose “Delete” to delete the selected recording.

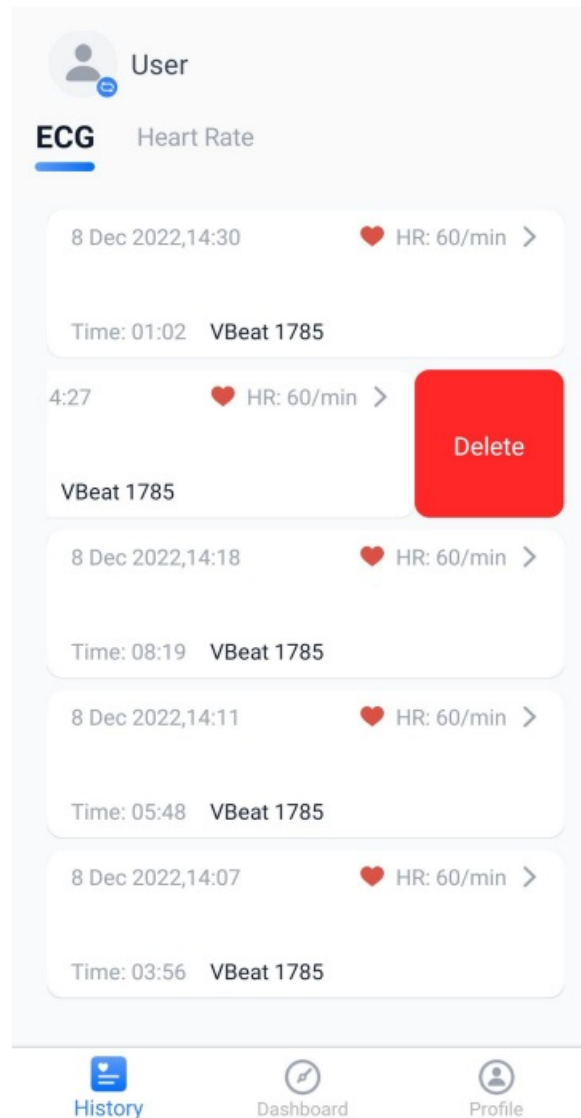


Setting Vibration Alerts

- In the Settings screen, tap [VBeat] ->[HR Target]->[Vibration], then you can turn on/off heart rate vibration alerts.
- When the detected heart rate is higher than [HR Target 1] value or [HR Target 2] value, the vibration alert will be automatically triggered. You can choose the desired target values on the [HR Target] screen.

Note:

- For [HR Target 1] alert, the vibration is triggered every 10 seconds.
- For [HR Target 2] alert, the vibration is triggered every 2 seconds.

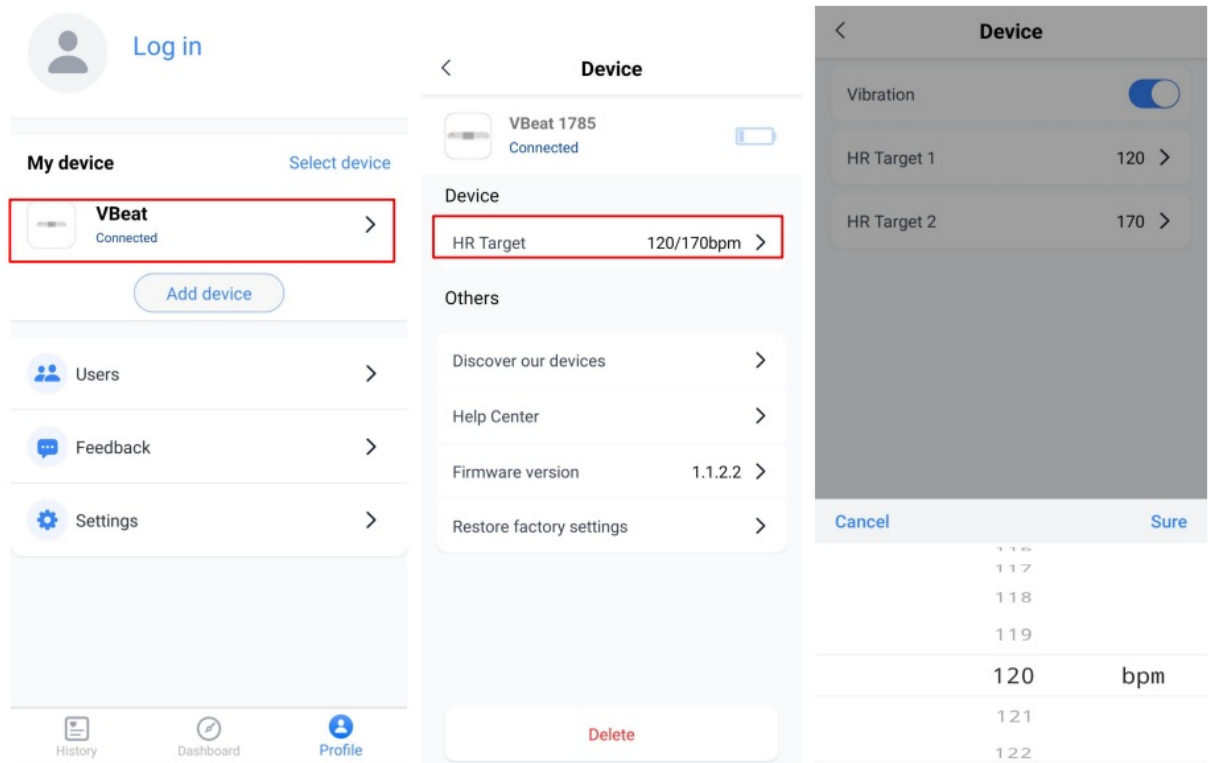

- Disconnect the phone Bluetooth or close the APP, the Bluetooth connection will be disconnected.
- If the user has connected the APP with Bluetooth before use, the data can be transmitted in real time

Note:

- The Bluetooth technology is based on a radio link that offers fast and reliable data transmissions. The Bluetooth uses a license-free, globally available frequency range in the ISM band-intended to ensure communication compatibility worldwide.
- The pairing and transmitting distance of wireless function is 1.5 meters in the normal. If the wireless communication is delay or failure between the phone and the product, you will try to narrow the distance between the phone and the product.
- The product can pair and transmit with the phone under the wireless coexistence environment (e.g. microwaves, cell phones, routers, radios, electromagnetic anti-theft systems, and metal detectors), but other wireless product may still interface with pairing and transmission between the phone and the product under uncertain environment. If the phone and the product display inconsistent, you may need to change the environment.
- Considering the security of app data, certain appropriate antivirus software and firewalls are recommended to be installed for Android system such as AVG, Avast, McAfee, etc. For IOS system, the App can run without antivirus software and firewalls because the closed system and access control of the system.
- There will be pop up to remind users to install the updates when the App has updated version.

Precautions:

The device can store up to 10 part measurement data and up to 168h of measurement data. In order to ensure that every data you collect is able to be viewed smoothly, please export the data in time after each measurement is completed.

Charging

This device uses a rechargeable lithium battery. Charged by connecting a laptop or a power adapter with charging cable. Charging specific steps:

1. Connect the device with the USB clip.
2. Connect the charging cable to the usb port with 5v output voltage for charging. After entering the charging state, The display displays the charging icon. After the charging is complete, the icon of full charge is displayed.

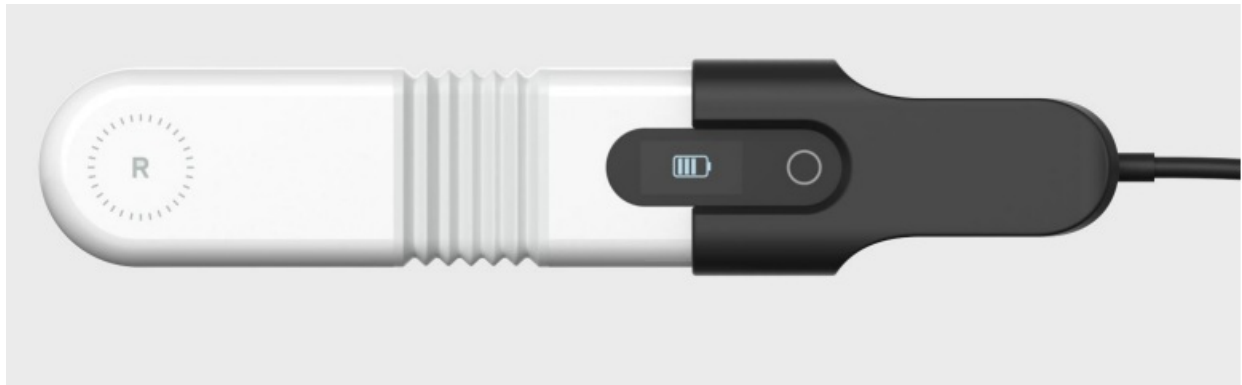


Figure 5

Warnings and Cautionary Advices

- The device cannot be used during charging, and if choosing a third party charging adaptor (Class II), select one that complies with IEC60950 or IEC60601-1.
- Keep out of reach when charging.
- When the long-term storage is not in use, it is necessary to periodically charge the device to maintain battery performance.

Maintenance

Warnings and Cautionary Advices

Have the device repaired by authorized service centers only, otherwise its warranty is invalid

Warranty

The product is warranted to be free from defects in materials and workmanship within warranty period when used in accordance with the provided instructions.

Battery

When the remaining battery power is low, the display displays low power and the device needs to be charged..

Warnings and Cautionary Advices

- The built-in rechargeable lithium-ion battery cannot be replaced. Non-professionals cannot open the enclosure and modify or replace the battery.
- Do not expose the main unit to high temperatures such as ovens, water heaters and microwave ovens. Overheat ing of the battery may explode.
- Do not contaminate or modify the battery. Doing so may cause the battery to leak, overheat, ignite or explode.
- If the battery leaks, keep your skin and eyes free from leaking liquids. If skin or eyes come into contact with leaking liquid, rinse your skin or eyes immediately and go to hospital for treatment.

- Do not throw the battery into a fire. Doing so may cause an explosion.
- When the battery exceeds the service life or no longer holds the power, you should contact the manufacturer for disposal. To dispose of the battery, follow local laws for proper disposal.

Cleaning

- Dynamic ECG recorder and straps need to be cleaned regularly; clean the device per week. carefully swabbing the device with a clean, soft cloth or cotton ball with 70% medical alcohol or water.
- Do not use petrol, thinners or similar solvent.

Warnings and Cautionary Advices

Before using another patient, the device must be cleaned with 70% medical alcohol or water. At the same time, disposable ECG stickers cannot be mixed and must be replaced.

Recycling

Disposal of waste, residues, etc., as well as device and accessories at the end of their useful life shall not be disposed of at random and shall be in accordance with local regulations. When it is intended to discard this device, it must be sent to the appropriate facility for recycling and recycling.

Problem solving

Problem	Possible Cause	Recommended Action
The device cannot perform normal acquisition	1. The battery is low 2. Equipment damage	1. Please charge the device 2. Please contact your local agent
ECG waveform is disordered, and the clutter is large	1. Measurement method is incorrect 2. Poor contact of ECG electrode	1. Please re-measure according to the recommendations of the manual 2. Please clean the ECG electrode according to the method described in the manual.

Accessories

Serial number	Accessory name	Quantity
1	Charging cable	1
2	OTG adapter	1
3	Chest Strap (optional)	1
4	Disposable ECG electrodes (optional)	2

Warnings and Cautionary Advices

1. Use only the accessories specified in this manual, and using other accessories may damage the device.
2. Check if the disposable ECG electrode has expired before use.
3. The disposable ECG electrode used with this device is user-purchased device, which must be a formal device with a medical device registration certificate
4. Disposable ECG electrodes should not be attached to patients with traumatized or scarred skin.
5. Disposable ECG electrodes should be in close contact with the skin. If itching or skin irritation or ulceration occurs, stop using it immediately.

Specifications

Classification		
EC Directive	MDD, 93/42/EEC	
	R&TTE, 2014/53EU	
	ROHS 2.0, 2011/65/EU	
Degree of protection against electrical shock	Type BF	
Environmental		
Item	Operating	Storage
Temperature	5 ~ 45°C	-25 ~ 60°C
Relative humidity (non-condensing)	10% ~ 95%	10% ~ 95%
Atmospheric pressure	700 ~ 1060 hPa	700 ~ 1060 hPa
Degree of dust&water resistance	IP22	
Drop test	1.0 m	
Power supply		
Type of battery	Rechargeable lithium polymer battery	
Battery specification	3.8Vdc, 240mAh	
Battery run time	168 hours (full state)	
Charging input voltage range	4.5 ~ 5.5v DC voltage	
Charging time	2 hours (to 90% power)	
ECG		
Lead type	single-use ECG electrode	
Lead	Lead I	
Input impedance	≥10MΩ, 10Hz	
Linearity and dynamic range	10mV (peak-to-valley)	

Common mode rejection	≥60dB
Frequency response	0.67 ~ 40 Hz
Gain error	Maximum error ±10%
Physical	
Size	100×23×10 mm
Packing size	172×113×59mm
Weight	<20 g (with battery)
Wireless connectivity	Bluetooth connection support Built-in Bluetooth 4.0 BLE
Wireless Quality of Service (QoS)	Transmission Distance: 1.5m
	Transmission Time: ≤10s for one ECG record
	Data integrity: 100%
Expected service life	5 year

FCC Warning:

Any Changes or modifications not expressly approved by the party responsible for compliance could void the user's authority to operate the equipment.

This device complies with part 15 of the FCC Rules. Operation is subject to the following two conditions:

1. This device may not cause harmful interference, and
2. this device must accept any interference received, including interference that may cause undesired operation.

Note: This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates uses and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one or more of the following measures:

- Reorient or relocate the receiving antenna.
- Increase the separation between the equipment and receiver.
- Connect the equipment into an outlet on a circuit different from that to which the receiver is connected.
- Consult the dealer or an experienced radio/TV technician for help.

The device has been evaluated to meet general RF exposure requirement. The device can be used in portable exposure condition without restriction.

Electromagnetic compatibility

The device meets the requirements of IEC 60601-1-2.

Warnings and Cautions

- This device should not be used in the vicinity or on the top of other electronic equipment such as cell phone, transceiver, or radio control products. If you have to do so, the device should be observed to verify normal operation.
- The use of accessories and power cord other than those specified, with the exception of cables sold by the manufacturer of the equipment or system as replacement parts for internal components, may result in increased emissions or decreased immunity of the equipment or system.

Guidance and manufacturer’s declaration– electromagnetic emissions		
The model Dynamic ECG recorder is intended for use in the electromagnetic environment specified below. The customer or the user of the model Dynamic ECG recorder should assure that it is used in such an environment.		
Emissions test	Compliance	Electromagnetic environment – guidance
RF emissions C ISPR 11	Group 1	The model Dynamic ECG recorder uses RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause any interference in nearby electronic equipment.
RF emissions C ISPR 11	Class B	The model Dynamic ECG recorder is suitable for use in all establishments, including domestic establishments and those directly connected to the public low-voltage power supply network that supplies buildings used for domestic purposes.
Harmonic emissions IEC 6100 0-3-2	N/A	
Voltage fluctuations/ flicker emissions IEC 61000-3-3		

Rated maximum	Separation distance according to frequency of transmitter (m)						
output	150kHz		to	80MHz to 800MHz	800MHz	to	2.7GHz
power of transmitter (W)	80MHz	$d = [3.5] P^{1/2}$		$d = [3.5] P^{1/2}$	$d = [1] P^{1/2}$		
0.01	0.12			0.04		0.07	
0.1	0.37			0.12		0.23	
1	1.17			0.35		0.70	
10	3.70			1.11		2.22	
100	11.70			3.50		7.00	

For transmitters rated at a maximum output power not listed above, the recommended separation distance d in metres (m) can be estimated using the equation applicable to the frequency of the transmitter, where p is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer.

NOTE 1 At 80 MHz and 800 MHz, the separation distance for the higher frequency range applies.

NOTE 2 These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.

Recommended separation distances between RF wireless communications equipment						
The device is intended for use in an electromagnetic environment in which radiated RF disturbances are controlled. The customer or the user of the device can help prevent electromagnetic interference by maintaining a minimum distance between RF wireless communications equipment and the device as recommended below, according to the maximum output power of the communications equipment.						
Freq uen cy M Hz	Maxim um Power W	Distan ce	IEC 60601 Test Lev el	Complian ce Level	Electromagnetic Environment – Guidance	
385	1.8	0.3	27	27	RF wireless communications	
450	2	0.3	28	28	equipment should be used	
710					no closer to any part of the	
745	0.2	0.3	9	9	device, including cab les, than the recom	
780					mended	
					separation	
810					distance	
					calculated from the equation	
870	2	0.3	28	28	applicable to the frequency of t	
930					he transmitter.	

172					Recommended separation
0					distance
184 5	2	0.3	28	28	Where P is the maximum
197					output power rating of the
0					transmitter in watts (W) according to the transmitter manufacturer and d is the recommended separation distance in meters (m). Field strengths from fixed RF transmitter, as determined by an
245 0	2	0.3	28	28	
524 0					
550 0					
					electromagnetic site survey,
	0.2	0.3	9	9	should be less than the
578 5					compliance level in each frequency range. Interference may occur in the
					vicinity of equipment marked
					with the following symbol:
Note 1: These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.					

Guidance and manufacturer's declaration – electromagnetic immunity

The model Dynamic ECG recorder is intended for use in the electromagnetic environment specified below. The customer or the user of The model Dynamic ECG recorder should assure that it is used in such an environment.

Immunity test		IEC 60601 test level	Compliance level	Electromagnetic guidance		environment	–
				Portable and mobile RF communications			
				equipment should be used no closer to			
Conducted				any part of The model Dynamic ECG			
d	RF	3Vrms		recorder, including cables,		than the	
IEC61000-4-3		150kHz to 80MHz	N/A	recommended separation distance		distance	
4-6		80MHz		calculated from the equation applicable to			
		10V/m		the frequency of the transmitter.			
Radiated		80MHz to 2.7GHz		Recommended separation distance			
RF		2.7GHz	10V/m				
IEC61000-4-3							
4-3							
				80MHz to 800MHz			

			<p>800MHz to 2.7GHz</p> <p>where P is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer and d is the recommended separation distance in metres(m). Field strengths from fixed RF transmitters, as determined by an electromagnetic site survey,</p> <p>a should be less than the compliance level in each frequency range b</p> <p>Interference may occur in the vicinity of equipment marked with the following symbol:</p>
<p>NOTE 1 At 80 MHz and 800 MHz, the higher frequency range applies.</p> <p>NOTE 2 These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.</p>			

a The ISM (industrial, scientific and medical) bands between 0,15 MHz and 80 MHz are 6,765 MHz to 6,795 MHz; 13,553 MHz to 13,567 MHz; 26,957

MHz to 27,283 MHz; and 40,66 MHz to 40,70 MHz. The amateur radio bands between 0,15 MHz and 80 MHz are 1,8 MHz to 2,0 MHz, 3,5 MHz to

4,0 MHz, 5,3 MHz to 5,4 MHz, 7 MHz to 7,3 MHz, 10,1 MHz to 10,15 MHz,

14 MHz to 14,2 MHz, 18,07 MHz to 18,17 MHz, 21,0 MHz to 21,4 MHz,

24,89 MHz to 24,99 MHz, 28,0 MHz to 29,7 MHz and 50,0 MHz to 54,0 MHz.

b The compliance levels in the ISM frequency bands between 150 kHz and 80 MHz and in the frequency range 80 MHz to 2,7 GHz are intended to decrease the likelihood that mobile/portable communications equipment could cause interference if it is inadvertently brought into patient areas. For this reason, an additional factor of 10/3 has been incorporated into the formulae used in calculating the recommended separation distance for transmitters in these frequency ranges.

c Field strengths from fixed transmitters, such as base stations for radio (cellular/cordless) telephones and land mobile radios, amateur radio, AM and FM radio broadcast and TV broadcast cannot be predicted theoretically with accuracy. To assess the electromagnetic environment due to fixed RF transmitters, an electromagnetic site survey should be considered. If the measured field strength in the location in which The model Dynamic ECG recorder is used exceeds the applicable RF compliance level above, The model Dynamic ECG recorder should be observed to verify normal operation.

Guidance and manufacturer's declaration – electromagnetic immunity

The model Dynamic ECG recorder is intended for use in the electromagnetic environment specified below. The customer or the user of The model Dynamic ECG recorder should assure that it is used in such an environment.

Immunity test	IEC 60601 test level	Compliance level	Electromagnetic environment – guidance
Electrostatic discharge (ESD) IEC 61000-4-2	± 8 kV contact ± 2 kV ± 4 kV ± 8 kV ± 15 kV air	± 8 kV contact ± 2 kV ± 4 kV ± 8 kV ± 15kV air	Floors should be wood, concrete or ceramic tile. If floors are covered with synthetic material, the relative humidity should be at least 30%.



Electrical fast transient/ burst IEC 61000-4-4	± 2 kV for power supply lines ± 1 kV for input/ output lines	n.a.	n.a.
Surge IEC61000-4-5	± 1 kV line to line ± 2 kV line to earth	n.a.	n.a.
Voltage dips, short interruptions and voltage variations on power supply inputs IEC 61000-4-11	$0\% U_T$ 0,5cycle At $0^\circ, 45^\circ, 90^\circ, 135^\circ, 180^\circ, 225^\circ, 270^\circ$ and 315° , $0\% U_T$ 1cycle and $70\% U_T$ 25/30 cycles Single phase: at 0°	n.a.	n.a.
Power frequency (50/60 Hz) magnetic field IEC 61000-4-8	30A/m, 50/60Hz	30A/m,50/60Hz	Power frequency magnetic fields should be at levels characteristic of a typical location in a typical commercial or hospital environment.

NOTE : U_T is the AC mains voltage prior to application of the test level.

N O.	Essential Performance			The description of what the operator of the device can expect if the Essential Performance is lost or degraded due to electromagnetic disturbances
1	Image display		All icons should be displayed as the	
			instrucion for use	
		Input impendence	$\geq 10\text{M}\Omega$, 10Hz	Please stop using the device immediately and
2	EC G	Common mode rejection	$\geq 60\text{dB}$	contact the device manufacturer or
		Frequency response	0.67 ~ 40 Hz	
3	Bluetooth connection		The connection is normal without	distributor for service as soon as possible
			interruption	

ABOUT COMPANY

- Shenzhen Creative Industry Co.,Ltd.
- Floor 5, BLD 9, Baiwangxin High-Tech Industrial Park, Songbai Road, Xili Street, Nanshan District, 518110 Shenzhen, P. R. China
- **Tel:** +86-755-2643 3514
- **Fax:** +86-755-2643 0930
- **E-mail:** info@creative-sz.com
- **Website:** www.creative-sz.com

<div><div>View Manual</div><div>Dynamic ECG recorder</div><div> </div></div>	<div>Creative EHL-1A Dynamic ECG Recorder [pdf] User Manual</div> <div>EHL-1A Dynamic ECG Recorder, EHL-1A, Dynamic ECG Recorder, ECG Recorder, Recorder</div>
--	--

References

- [User Manual](#)

[Manuals+](#), [Privacy Policy](#)

This website is an independent publication and is neither affiliated with nor endorsed by any of the trademark owners. The "Bluetooth®" word mark and logos are registered trademarks owned by Bluetooth SIG, Inc. The "Wi-Fi®" word mark and logos are registered trademarks owned by the Wi-Fi Alliance. Any use of these marks on this website does not imply any affiliation with or endorsement.