



DURR VSA 900 S Suction System with Amalgam Separator Instruction Manual

[Home](#) » [DURR](#) » **DURR VSA 900 S Suction System with Amalgam Separator Instruction Manual** 





Contents

- 1 Short information
- 2 Assembly
- 3 Usage
- 4 Documents / Resources
 - 4.1 References


Short information

CA 4


The current version of the installation and operating instructions is available in the Download Center:



<http://qr.duerndental.com/9000-606-44>



Ambient temperature




70 %

Upper limit of humidity



Only qualified specialists or employees trained by Dürr Dental are permitted to install, connect and start using the unit.

Assembly

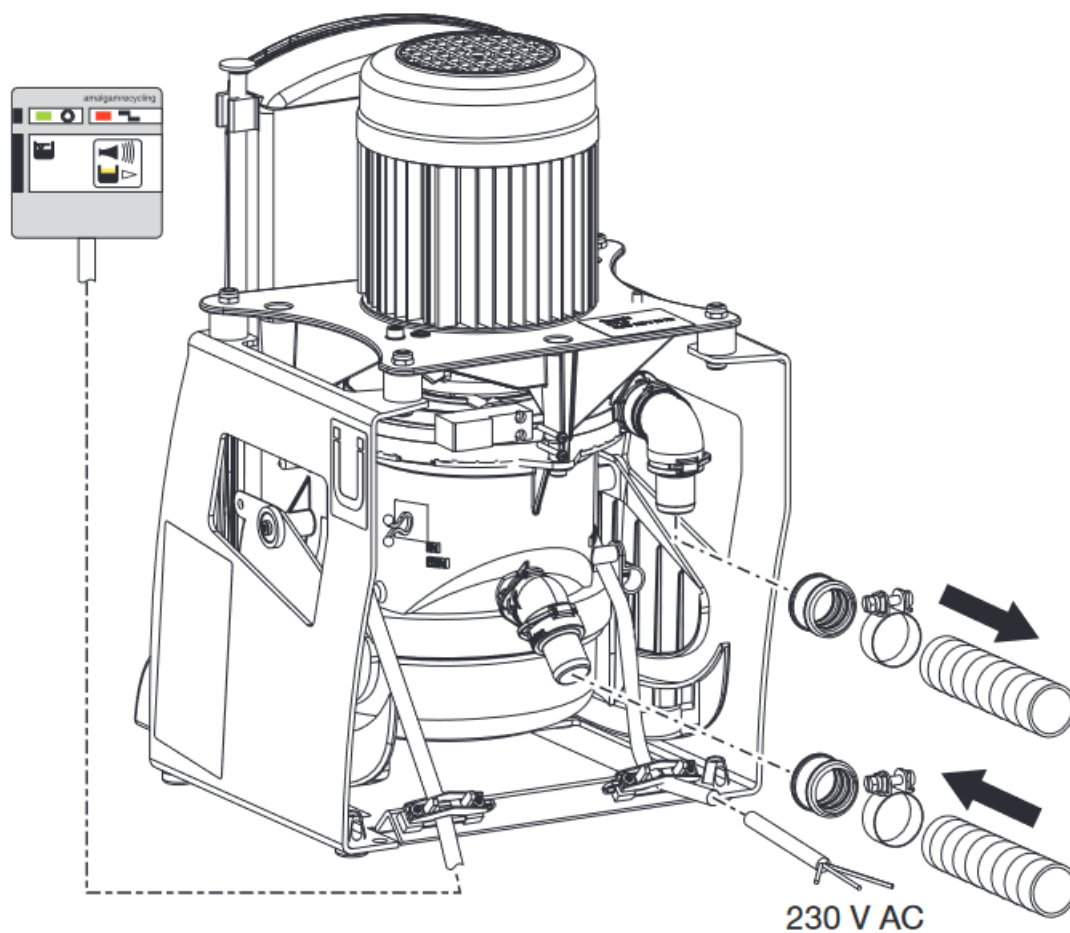


<http://www.duerr-gr.com/75.html>


➤ Use advantages and profit with security. Register your product now!

Usage


Disinfection and cleaning

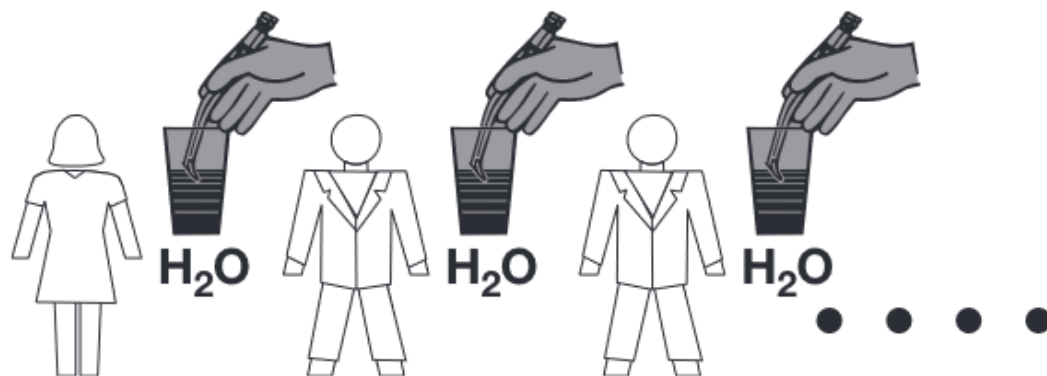


1x / Day
in the evenings

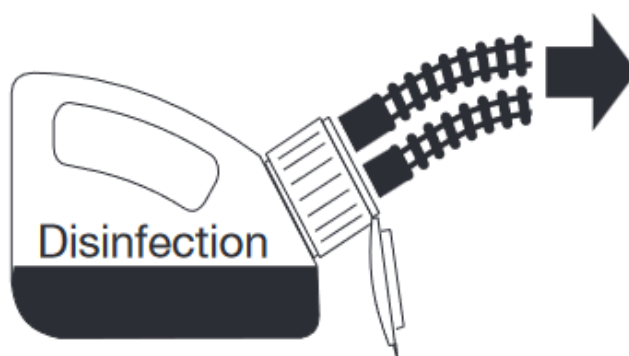

1x / Week
about noon

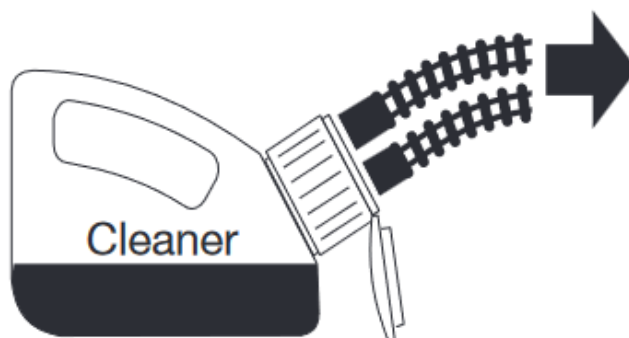


Ready for operation

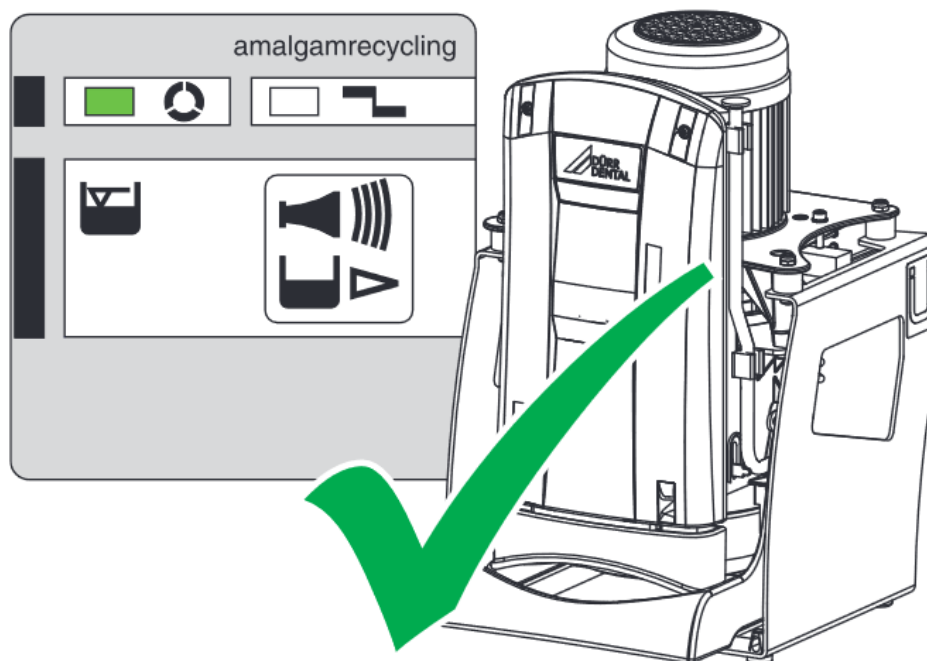


Amalgam collector vessel is 95% full

1

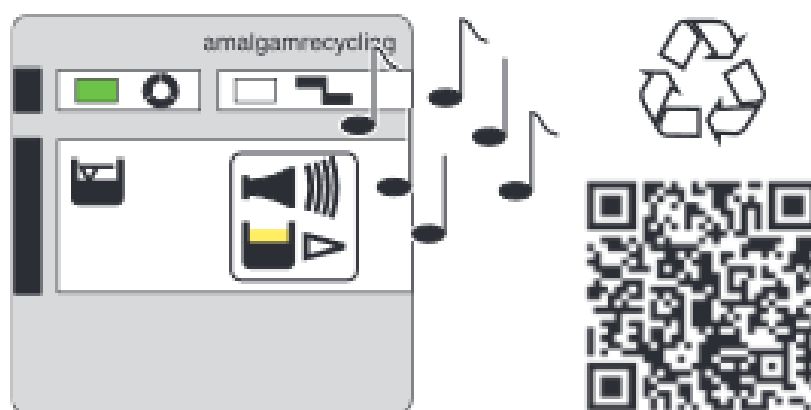

2

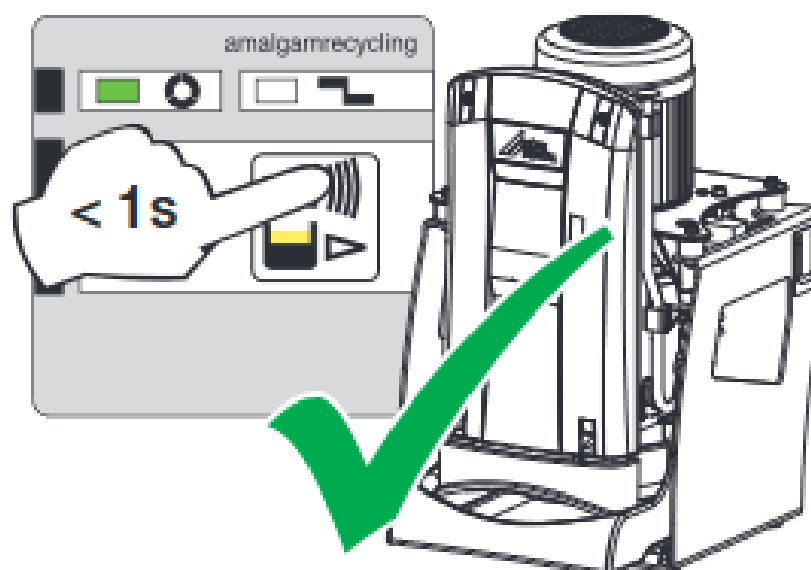

3



<http://www.duerr-gr.com/190.html>

Amalgam collector vessel is 100% full

1




2






3

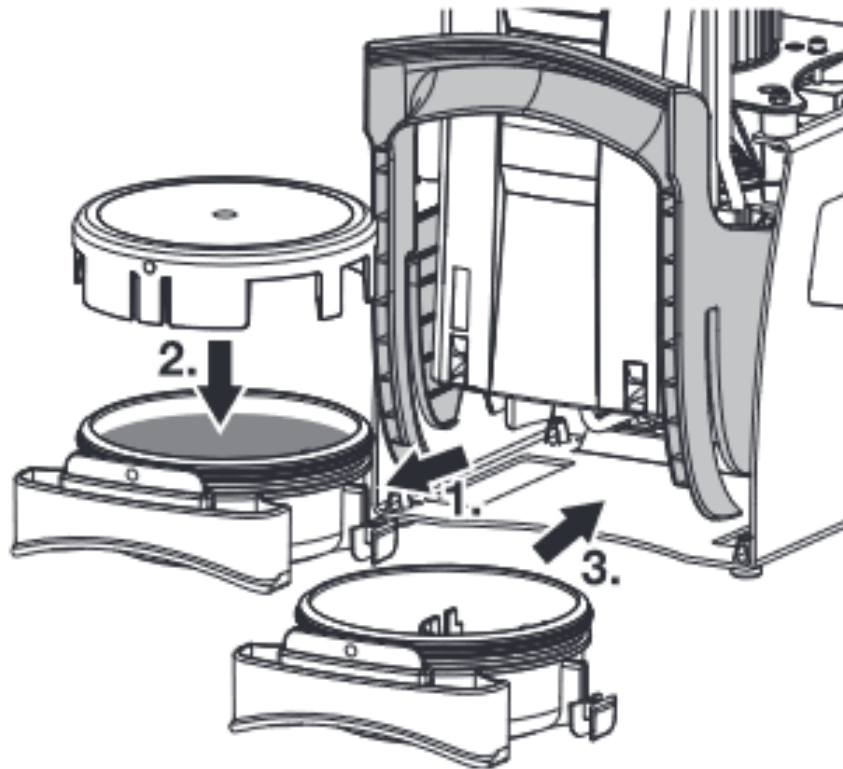


<http://www.duerr-gr.com/190.html>

Amalgam collector vessel not in position


1

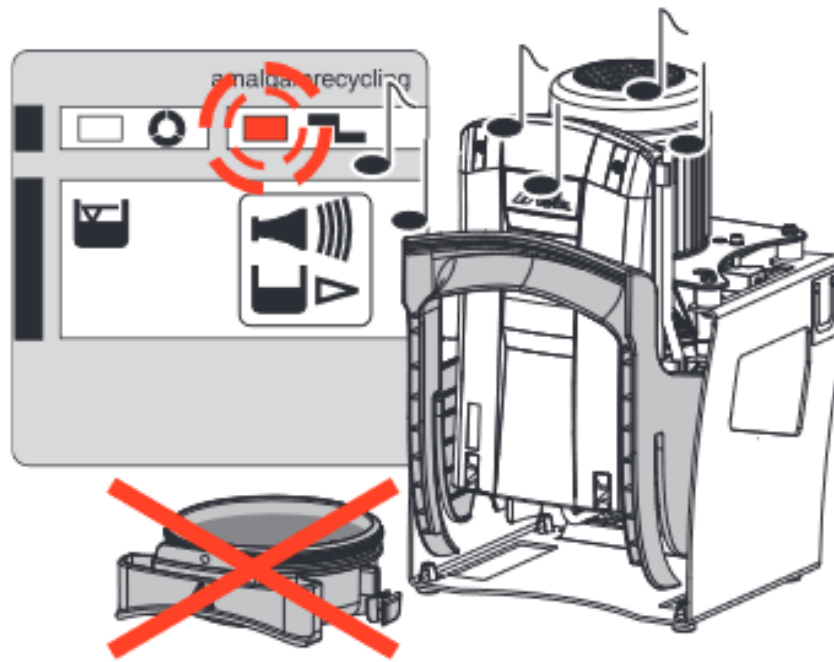


2

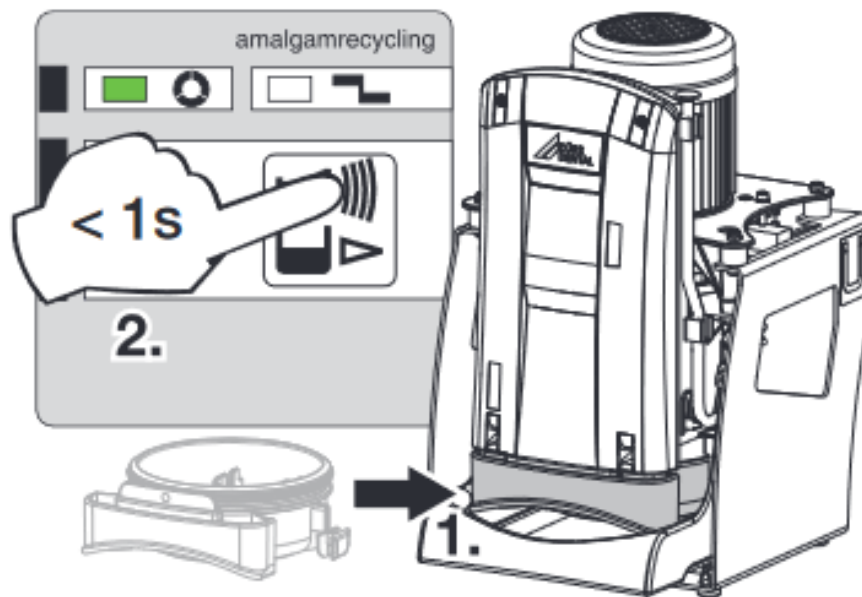

Motor fault

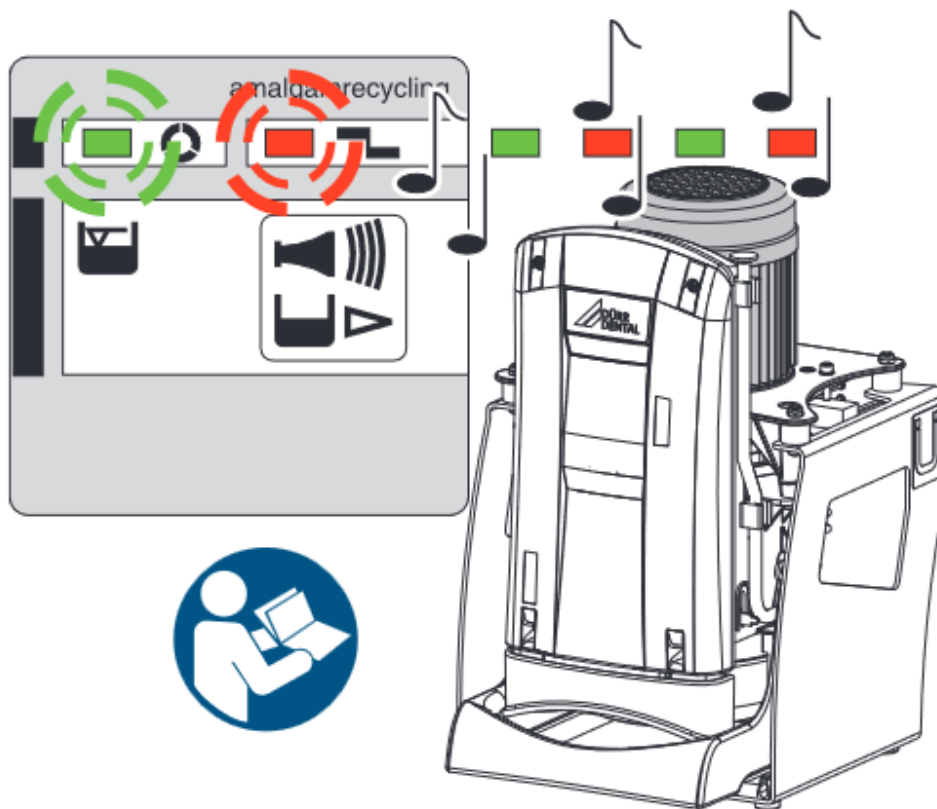


Emergency start sensor in overfill position

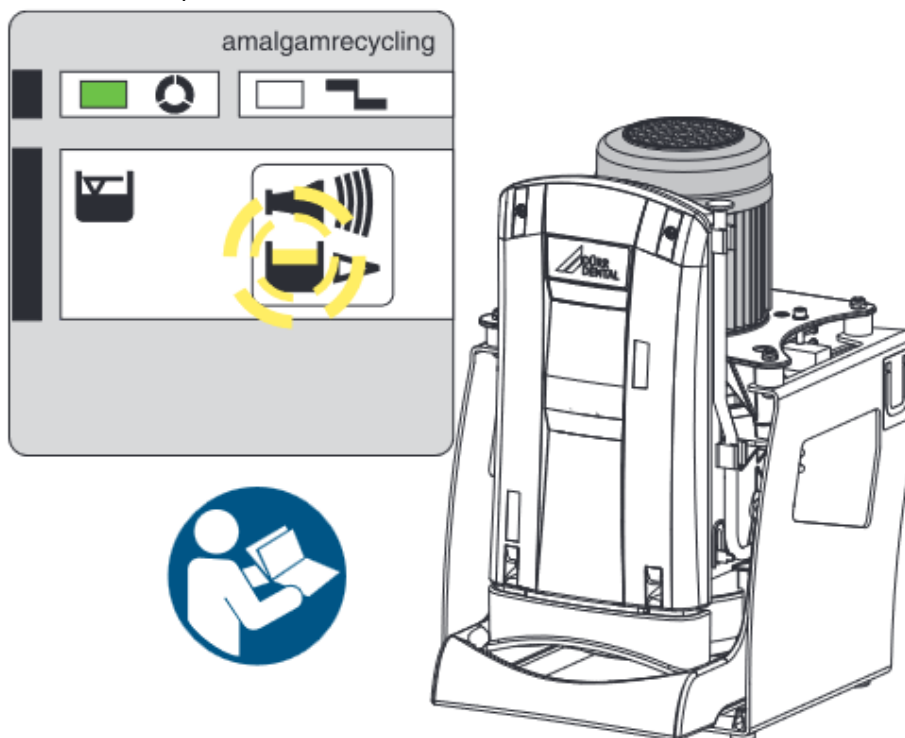

DÜRR DENTAL SE
Höpfigheimer Str. 17
74321 Bietigheim-Bissingen
Germany
7805100014L40
2206V001

Documents / Resources

	DURR VSA 900 S Suction System with Amalgam Separator [pdf] Instruction Manual VSA 900 S Suction System with Amalgam Separator, VSA 900 S, Suction System with Amalgam Separator, Amalgam Separator, Separator
---	--

References

- [Download-Center | Dürr Dental \(GLOBAL\)](#)

Manuals+.