

E-XTEQ E-VLT Leak Detector User Guide

Home » E-XTEQ » E-XTEQ E-VLT Leak Detector User Guide

Contents

- 1 E-XTEQ E-VLT Leak Detector
- 2 E-VLT Quick Start Guide
- 3 User Interface
- 3.1 User Adjustments
- 4 Safety advisory / Warranty
- **5 Preamble**
- 6 Your E-VLT
- 7 User interface
- 8 User adjustments
- 9 FCC Warning
- 10 Specifications
- 11 Documents / Resources
 - 11.1 References
- **12 Related Posts**



E-XTEQ E-VLT Leak Detector



E-VLT Quick Start Guide

Safety Advisory / Warranty

Before using the E-VLT, please read and understand the safety advisory and warranty information provided in the user manual.

Good Practices and Safety Instructions

Please follow the good practices and safety instructions provided in the user manual to ensure safe and proper usage of the E-VLT.

Preamble

The E-VLT is a device designed for testing battery groups. It is important to perform a leak test before using the device.

Principle of Cycle

The E-VLT operates by cycling the battery group through a sequence of charge, discharge, and rest phases. This allows for accurate testing of the battery's capacity and performance.

Your E-VLT

The E-VLT comes with a user interface that includes cycle keys for controlling the testing process. The main menu screen provides options for preparing a program, selecting a battery to test, and starting and stopping a cycle.

User Interface

Overview

The user interface provides access to various features and functions of the E-VLT. The main menu screen displays options for preparing a program, selecting a battery to test, and starting and stopping a cycle.

Keys

The cycle keys are used to control the testing process. The power key is used to turn the device on and off. Other keys are used for selecting options and adjusting settings.

Main Menu Screen

The main menu screen provides options for preparing a program, selecting a battery to test, and starting and stopping a cycle.

Preparing a Program

To prepare a program, navigate to the main menu screen and select the "Preparing a Program" option. Follow the prompts to set the desired program parameters.

Preparing Battery Groups Programs

To prepare battery groups programs, navigate to the main menu screen and select the "Preparing Battery Groups Programs" option. Follow the prompts to set the desired battery group parameters.

Selecting a Battery to Test

To select a battery to test, navigate to the main menu screen and select the "Selecting a Battery to Test" option. Follow the prompts to select the desired battery.

Starting and Stopping Cycle

To start a cycle, navigate to the main menu screen and select the "Starting and Stopping Cycle" option. Follow the prompts to begin the testing process. To stop a cycle, press the stop key.

User Adjustments

The E-VLT allows for user adjustments to program and battery parameters. Navigate to the configuration menu or results menu to make these adjustments.

ATEQ Manufacturer Plants - Measurement Solution, Global Leader.



We continuously work on improving our products. This is why information contained in this man-ual, the device and the technical specifications may be modified without prior notification. Pictures and figures in this manual are non-contractual.

Safety advisory / Warranty

GOOD PRACTICES AND SAFETY INSTRUCTIONS

Safety recommendations

The device is supplied with 100 / 240 V AC, it is mandatory to connect it to the ground with a good link to the ground, to protect against electric hazard or electrocution.

Recommendations for the test environment

Keep the test area as clean as possible.

Recommendations for operators

E-XTEQ recommends that the operators who use the devices have training and a level of qualification that correspond to the job to perform.

General recommendations

- Read the user manual before using the device.
- All electrical connections to the device must be equipped with safety systems (fuses, circuit breakers, etc.) adapted to the needs and in accordance with the applicable standards and rules.
- To avoid electromagnetic interference, electrical connections to the device must be shorter than 2 meters.
- Power supply plug must be grounded.

- Disconnect the device from the mains before performing any maintenance work.
- Shut off the compressed air supply when working on the pneumatic assembly.
- Do not open a connected device.
- Avoid splashing water on the device.

E-XTEQ is at your disposal for any information concerning the use of the device under maxi-mum safety conditions.

We draw your attention to the fact that E-XTEQ cannot be held responsible for any accident related to a misuse of the measuring instrument, the workstation or non-compliance of the in-stallation with safety rules.

In addition, E-XTEQ declines any responsibility for the calibration or the fitting of their instru-ments that is not done by E-XTEQ.

E-XTEQ also declines any responsibility for any modification (program, mechanical or electri-cal) of the device done without their written consent.

Preamble

E-VLT

E-VLT is a leak detector able to test large volume like EV battery housing and cooling.




E-VLT can memorise 128 different test programs and 32 batteries sets of programs.

LEAK TEST

Leak test and Desenzitizes Mode

The test pressure is applied to the input of the test part 3.

The measurement is performed by the pressure sensor 2.




- 1. Device
- 2. Pressure sensor
- 3. Part under test

Desensitized Mode: there is no leak fullscale. The limit is the test Pressure.

PRINCIPE OF CYCLE

The measurement cycle is made of 4 mains phases: fill, stabilization, test, dumping.

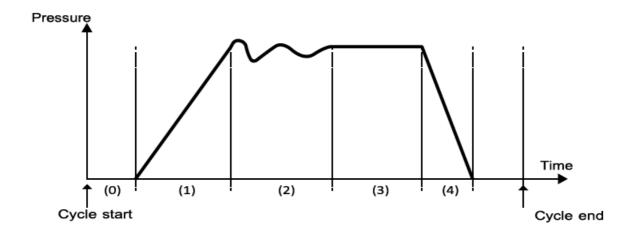

- · Waiting phase
- Fill phase
- Stabilization phase
- Dumping

Your E-VLT

FRONT PANEL

The user interface is located on the front panel.



- 1. Touchscreen Display
- 2. USB Connectors

BACK PANEL



- 1. Part number / Serial number
- 2. Exhaust output
- 3. Test part connector
- 4. Calibration informations
- 5. Connector for 100 / 240 V AC power supply

COUPLERS

Different couplers are mandatories to test Housing or cooling system. They must be connected on the test pipe fast connector.

POWER SUPPLY CONNECTORS

100 / 240 V AC connector (J7)

The device can be connected to a 100 / 240 V AC power supply (option).

This connector has a ON/OFF button.

It is mandatory to connect the device with a good link to the ground, to protect against electric hazard or electrocution.

Interruptor ON/OFF




- 1 ON
- OFF

DIGITAL LINKS

PC USB connectors (on front face)

USB connectors can be used for connecting miscellaneous compatible USB devices. The USB connectors are located under the rubber cover 1 (see figure).



- 1. USB connector to PC
- 2. USB connector to USB key or barcode reader
- 3. Rubber cover

Do not use a cable longer than 2 m.

Push the rubber cover 3 slightly forward for an easy access to USB connectors 1 and 2.

Only use this connection for temporary communication.

Connection to a PC cannot be used permanently because the communication can be disconnected by the PC.

User interface

OVERVIEW



KEYS

Cycle keys

The cycle keys are used to start and to stop a measurement cycle.

Key	Name	Function
	Start	Starts a measurement cycle and opens the Measuremen cycle screen.
STOP	Reset	Stops the measurement cycle in progress.

Keys

The navigation keys are used to select menus/options and change parameter values.

Key	Name	Function
✓	ок	Validation of actual screen.
5	Back	Returns to previous screen.

POWER UP

- 1. Make sure that all the necessary connections are in place.
- 2. Power up your device

When Power up part under pressure must NOT be connected to the instrument. Then the instrument propose an autotest.









MAIN MENU screen

The MAIN MENU screen gives access to different sections for managing the device and the test parameters.



- 1. Battery selection and test Menu
- 2. Results Menu
- 3. Instrument configuration

PREPARING A PROGRAM

Use this process to configure a new test program. On the MAIN MENU screen :

1. Select « Battery » Menu



2. Select « Parameters » Menu (requires Expert Rights)



The program list is displayed.

- Home : returns to main menu
- Group parameters (Batteries)
- Programs parameters
- Special cycles (Autozero, ...)
- Configuration



3. Select the program number you want to edit.



4. Modify parameters

For more details refer to chapter :


User Adjustment / Program parameters



5. Press Home to come back to main menu

PREPARING A BATTERY GROUPS PROGRAMS

- 1. Select « Battery » Menu
- 2. Select the battery group you want to edit

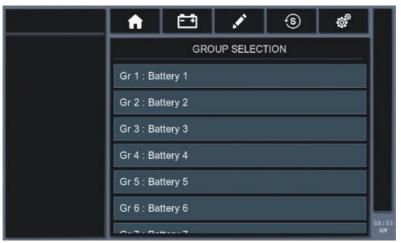

3. Modify parameters

For more details refer to chapter:

User Adjustment / Battery parameters



4. Press HOME to come back to main menu

SELECTING A BATTERY TO TEST

1. Select « Battery » Menu



2. Select « Battery list » Menu



3. Select the correct battery in the list



4. Select TEST TYPE (Housing or Cooling) Prepare and connect the correct coupler



STARTING AND STOPPING CYCLE

When the expected program is selected. Starting a measurement cycle



Press Start.

The cycle phases of program are successively displayed:

FILL

STABILISATION

TEST

DUMP

At the end of the test time, the result is display.

Measurement cycle screen

It displays the different values of the current test (or last one).



- 1. Battery Name
- 2. Step progress
- 3. Battery type of test
- 4. Cloud connection (Not available yet)
- 5. User Right (Normal/Expert)
- 6. Pressure or Leak measurement
- 7. Cycle step (Fill, Stab, Test, Dump, Ready)
- 8. Bargraph: Pressure according to target or leak according to reject level
- 9. Result of the test (Pass, Fail, Alarm code)
- 10. Countdown Bargraph
- 11. Time remaining to finish test
- 12. In the center:

When ready; Start key

Duting cycle: Cycle step icon

When cycle is finished: Result icon (PASS / FAIL / ALA)

13. Quantity program executed / Total in « Auto chain » mode.

Stopping a cycle






1. Press Stop to immediately stop the current measurement.

User adjustments

PROGRAM PARAMETERS

Use this menu to configure the measurement cycle associated to each test program.

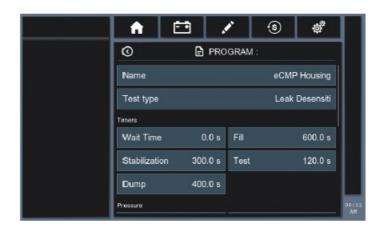

Groups	Parameters	Descriptions
	Name	Text field to easily organise program (Ex: batteryName Hous- ing) Test type : Leak per default
	Waiting time	Time before starting the cycle

1		
	Fill Time	Necessary time to fill the battery at the pressure instruction As soon as the instruction is reached, the fill time is shortened
Timers	Stabilisation time	Necessary time to get a correct measurement during test time
	Test time	Necesary time to get a representative measurement (20 Pa) of the part wit h a leak closed to reject level (ex. leak of 0.1 Pa/s, it is advised to have 180 s test time)
	Dump time	Time required to dump the part through the instrument, for housing (low pre ssure) couplers can be unplug to earn time
	Pressure unit	Select correct unit in the list
Pressure	Set Fill	Pressure instruction (Target)
	Min and Max pressure	At the end of filling time pressure needs to be between these 2 levels
	Leak unit	Select correct unit in the list
Leak	Max reject	Level to declare part under test as FAIL
	Std Patm and Tem perature	Requested parameters when specific unit as sccm is used
	Offset	Manual offset that can be subtracted to the leak measurement. It is a useful I parameter to shorten stabilisation time (Reserved to expert)
	Volume	It's a necessary coeficient to convert pressure decay (in Pa) to leak (in flow unit like ml/min)

	Filter time	Usefull function to limit external pertubation during test time with flow unit, t his time max must be inferior to 0.5*Test time
Options	Sign	Change the sign of the measurement, (vaccum test)
	Leak search	If the part is declared as leaking, the instrument maintains the pressure at t he end of the test to let the operator look for the leak. The test must must be stopped manually

BATTERY PARAMETERS

Use this menu to name and affect Test Programs.



Parameters	Descriptions
Name	Displayed name in the battery list menu
Picture	Displayed pictures in the battery list menu (Not available yet)
Test 1 Housing	Program selected to make Housing TEST
Test 2 Cooling	Program selected to make Cooling TEST

CONFIGURATION MENU

Use this menu to configure your E-VLT device.



Parameters	Descriptions
Date	Define correct Date and Time. it is important for results stored.
Job Mode	Using this mode, the instrument requires to make housing and cooling on a specific bat tery. At the end of the test a special file records the tests.
Autochain	This mode automatically makes the specified quantity of tests and gen- erates a dedicat ed result file.

RESULTS MENU

In this section you can observe the results of the last 50 cycles.



Connecte a USB memory stick and press the white key to transfer data from the instruments :

- Key/SerialNumber/Campaign : all the measurement done with auto chaining mode
- Key/SerialNumber/Results : all the measurement done
- Key/SerialNumber/jobs/: all the measurement done with Job mode

FCC Warning

This device complies with part 15 of the FCC rules. Operation is subject to the following two conditions:

- 1. This device may not cause harmful interference, and
- 2. This device must accept any interference received, including interference that may cause undesired operation.

Changes or modifications not expressly approved by the party responsible for compliance could void the user's authority to operate the equipment.

NOTE: This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates uses and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interferenceto radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one or more of the following measures:

- Reorient or relocate the receiving antenna.
- Increase the separation between the equipment and receiver.
- Connect the equipment into an outlet on a circuit different from that to which the receiver is connected.
- Consult the dealer or an experienced radio/TV technician for help.

Radiation Exposure Statement

This equipment complies with FCC radiation exposure limits set forth for an uncontrolled environment. This equipment should be installed and operated with minimum distance 20cm between the radiator and your body.

Specifications

CARACTERISTICS

Technical characteristics of the device.

Main characteristics:

Characteristics	Values
Mass	About 8,5 kg (18.7 lbs)
Electrical power supply	100 / 240 V AC 55 W – 50/60 Hz
Overvoltage category	II
Air supply	From -10 to 250 kPa
Pneumatic connections:	Fast connector Staubi RBE 03
Operation temperature	+5 °C to + 45 °C (+ 41 °F to 113 °F)
Storage temperature	0 °C to +60 °C (32 °F to 140 °F)
Operation altitude	Up to 2000 m (6500 ft)
Relative humidity	80 % at 31 °C (87 °F) and 50 % at 40 °C (104 °F)

Dimensions (in millimeters) :



Documents / Resources



E-XTEQ E-VLT Leak Detector [pdf] User Guide 2AK5Y-E-VLT, 2AK5YEVLT, CDF 7000, E-VLT Leak Detector, E-VLT, Leak Detector, Detector

References

- E-XTEQ Measurement solutions
- User Manual

Manuals+, Privacy Policy

This website is an independent publication and is neither affiliated with nor endorsed by any of the trademark owners. The "Bluetooth®" word mark and logos are registered trademarks owned by Bluetooth SIG, Inc. The "Wi-Fi®" word mark and logos are registered trademarks owned by the Wi-Fi Alliance. Any use of these marks on this website does not imply any affiliation with or endorsement.