

**EXERGEN  
TAT-5000S-RS232  
Series Accurate  
Temperature**



# EXERGEN TAT-5000S-RS232 Series Accurate Temperature Instruction Manual

[Home](#) » [EXERGEN](#) » EXERGEN TAT-5000S-RS232 Series Accurate Temperature Instruction Manual 

## Contents

- [1 EXERGEN TAT-5000S-RS232 Series Accurate Temperature](#)
- [2 Introduction](#)
- [3 Important Safety Instructions](#)
- [4 Infant Temperature Measurement](#)
- [5 FAQ](#)
- [6 Care and Maintenance](#)
- [7 Display Diagnostics Chart](#)
- [8 CONTACT](#)
- [9 Documents / Resources](#)
  - [9.1 References](#)
- [10 Related Posts](#)

# EXERGEN

EXERGEN TAT-5000S-RS232 Series Accurate Temperature



## Introduction

- The TemporalScanner is an infrared thermometer designed for accurate, completely non-invasive temperature assessment by scanning the temporal artery (TA).
- Temperature is measured by gently stroking the TemporalScanner across the forehead, and includes a momentary touch of the probe to the neck area behind the ear lobe, to account for any cooling of the forehead as a result of diaphoresis.
- The patented arterial heat balance technology (AHB™) automatically measures the temperature of the skin surface over the artery and the ambient temperature. It samples these readings some 1000 times a second, ultimately recording the highest temperature measured (peak) during the measurement.
- The TemporalScanner emits nothing – it only senses the natural thermal radiation emitted from the skin.
- It has been clinically proven in premier university hospitals to be more accurate than ear thermometry, and better tolerated than rectal thermometry, and is supported by more than 70 peer-reviewed published studies covering all ages from premature infants to geriatrics in all clinical care areas. It is a superior method for patients and clinicians alike.
- A 40-page compendium on Temporal Artery Temperature Assessment is available at [www.exergen.com/medical/PDFs/tempassess.pdf](http://www.exergen.com/medical/PDFs/tempassess.pdf), and a complete list of peer-reviewed published clinical studies is available at [www.exergen.com/c](http://www.exergen.com/c).
- Complete multilanguage information on clinical use, instruction manuals, and training is available at [www.exergen.com/s](http://www.exergen.com/s), which includes links to a specialized clinical site <http://www.exergen.com/tathermometry/index.htm>.
- The link to [www.exergen.com/s](http://www.exergen.com/s) appears on the front label of the instrument as a scannable “QR” symbol for



## Important Safety Instructions

### READ ALL INSTRUCTIONS BEFORE USING

Intended Use: The Exergen TemporalScanner is a handheld infrared thermometer used by medical professionals for the intermittent measurement of human body temperature of people of all ages, by scanning the forehead skin over the temporal artery. Intended users are physicians, nurses, and nursing assistants at all levels who normally provide patient care. The thermometer provides a peak temperature reading from plural readings during the step of scanning. Electronic circuitry processes the measured peak temperature to provide a temperature display based on a model of heat balance relative to a detected arterial temperature, the electronic circuitry computing an internal temperature of the body as a function of ambient temperature (Ta) and sensed surface temperature. Training materials that are supplementary to this instruction manual are available at [www.exergen.com/s](http://www.exergen.com/s) and recommended for first-time users.

TAT-5000S Series thermometers are used by medical professionals in clinical environments. Such medical professionals include physicians, nurses, nurses' aides, patient care technicians, and others who are trained to take the temperature of patients. Clinical environments include areas where medical professionals provide medical services for patients, including hospitals, outpatient clinics, primary care offices, and other settings where temperature is taken as part of patient care. Clinical environments include Emergency Medical Services environments. Additionally, the TAT-5000S series thermometers are not for use aboard aircraft or near High-Frequency Surgical Equipment or Radio Frequency shielded rooms, such as MRI (Magnetic Resonance Imaging) areas.

When using the product basic safety precautions should always be followed, including the following:

- Use this product only for its intended use as described in this manual.
- Do not take temperature over scar tissue, open sores or abrasions.
- The operating environmental temperature range for this product is 16 to 40°C (61 to 104°F).
- Always store this thermometer in a clean, dry place where it will not become excessively cold (-20°C/-4°F), or hot (50°C/ 122°F) or humid (max RH 93% non-condensing, at 50 to 106 kPa).
- The thermometer is not shockproof. Do not drop it or expose it to electrical shocks.
- Do not Autoclave. Please note the cleaning and sterilizing procedures in this manual.
- Do not use this thermometer if it is not working properly, if it has been exposed to temperature extremes, damaged, been subject to electrical shocks or immersed in water.
- There are no parts that you can service yourself except for the battery, which you should replace when low by following the instructions in this manual. For service, repair, or adjustments, return your thermometer to Exergen. Warning: no modification of this equipment is allowed.
- Never drop or insert any object into any opening, unless stated in this manual.
- If your thermometer is not used regularly, remove the battery to prevent possible damage due to chemical leakage.
- Follow the battery manufacturer's recommendations or your hospital policy for the disposal of used batteries.
- Not suitable for use in the presence of flammable anesthetic mixtures.
- Do not use corrosive substances on the thermometer.
- Communication cables for the TAT-5000S that are field replaceable are specific to the model and patient

monitor. Only compatible cables may be used, to maintain compliance of the TAT-5000S thermometers with requirements for Emissions and Immunity.

- If the device fails to operate as described above, see the FAQ section of this manual. Additionally, ensure that you are not in the presence of electromagnetic disturbances. If you have any additional questions regarding the use or care of the thermometer, please see [www.exergen.com](http://www.exergen.com) or call customer service at [617-923-9900](tel:617-923-9900).

## **WARNING**

- Use of this equipment adjacent to or stacked with other equipment (other than TAT-5000S compatible patient monitors) should be avoided because it could result in improper operation. If such use is necessary, this equipment and the other equipment should be observed to verify that they are operating normally.

## **WARNING**

- Use of accessories, transducers, and cables other than those specified or provided by the manufacturer of this equipment could result in increased electromagnetic emissions or decreased electromagnetic immunity of this equipment and result in improper operation.

## **WARNING**


- Portable RF communications equipment (including peripherals such as antenna cables and external antennas) should be used no closer than 30 cm (12 inches) to any part of the TAT-5000S thermometer, including cables specified by the manufacturer. Otherwise, degradation of the performance of this equipment could result.

## **WARNING**

- The thermometer contains some substances (i.e., Lead, Nickel, Melamine, etc.) which are in concentrations of  $>0.1\%$  (w/w), and in some cases may cause an allergic reaction. A current list of these declared substances can be found in Exergen's REACH and Proposition 65 (CA) Declaration of Conformity documents by request.

## **Introduction to Temporal Artery Thermometry**

Temporal artery thermometry (TAT) is a completely new method of temperature assessment, using infrared technology to detect the heat naturally emitted from the skin surface. In addition, and of key importance, this method incorporates a patented arterial heat balance system to automatically account for the effects of ambient temperature on the skin.

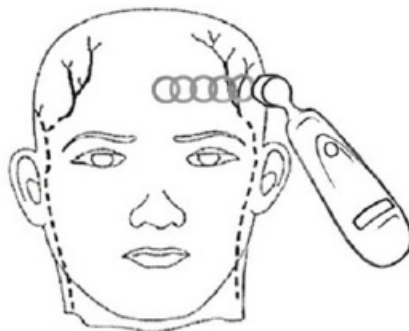

This method of temperature assessment has been shown to improve results and reduce costs by non-invasively measuring body temperature with a degree of clinical accuracy unachievable with any other thermometry method.


## Before Using, Familiarize Yourself with the Instrument

- **To Scan:** Depress the red button. The instrument will continually scan for the highest temperature (peak) as long as the button is depressed.
- **Clicking:** Each fast click indicates a rise to a higher temperature, similar to a radar detector. Slow clicking indicates that the instrument is still scanning, but not finding any higher temperature.
- **To Retain or Lock Reading:** The reading will remain on the display for 30 seconds after the button is released. If measuring room temperature, the temperature will remain on the display for only 5 seconds.
- **To Restart:** Depress the button to restart. It is not necessary to wait until the display is clear, the thermometer will immediately begin a new scan each time the button is depressed.

### Alternate sites when the temporal artery or behind ear are unavailable:

- Femoral artery: slowly slide the probe across the groin.
- Lateral thoracic artery: slowly scan side-to-side in the area ~midway between the axilla and the nipple.

Let the instrument acclimatize for at least 10 minutes in the area in which it will be used.

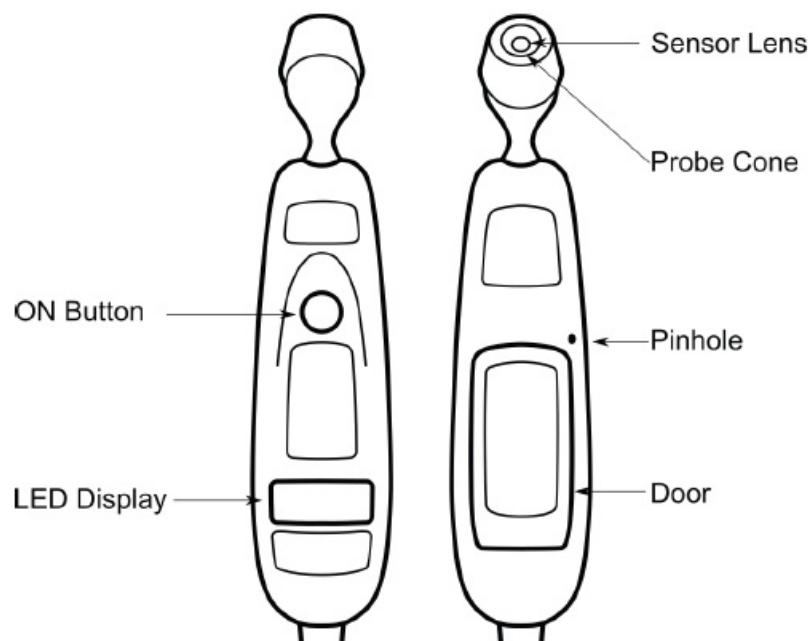

## Infant Temperature Measurement

### 2-Step Infant Temperature Measurement


#### Step 1

- Place the probe flush on the center of the forehead and depress the button. Keeping the button depressed, slowly slide the probe mid-line across the forehead to the hairline.



## Step 2

- Release the button, remove it from the head, and read.

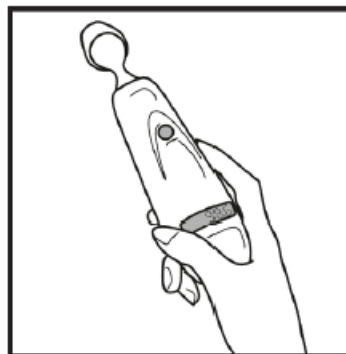

## How to improve the accuracy of your measurements on infants.

- The preferred site is the temporal artery area. Unless visibly diaphoretic, one measurement here is typically all that is required.



- Measure straight across the forehead and not down the side of the face.
- At mid-line, the temporal artery is about 2 mm below the surface but can go deeply below the surface on the side of the face.



- If the temporal artery is covered, then the area behind the ear, if exposed, can be an alternate site.



- Brush the hair aside if covering the area to be measured. The measurement site must be exposed.



### 3-Step Adult Temperature Measurement

#### Step 1


- Slide across the forehead. Place the probe flush on the center of the forehead and depress the button. Keeping the button depressed slowly slide the probe mid-line across the forehead to the hairline.



## Step 2


**Slide behind the ear.**

- Keeping the button depressed, lift the probe from the forehead, touch the behind ear halfway down the mastoid process and slide down to the soft depression behind the earlobe.

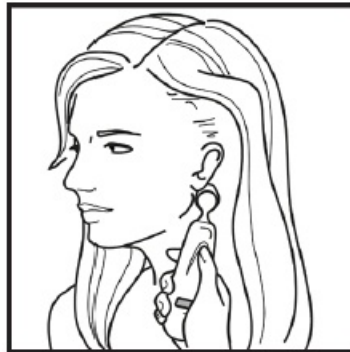

## Step 3

- Release the button, remove it from the head, and read.

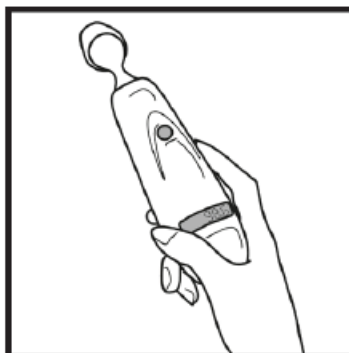

**How to improve the accuracy of your measurements on adults.**

- Measure only the upside on a patient in a lateral position. The down-side will be insulated preventing the heat from dissipating, resulting in falsely high readings.





- Think of a sweatband. Measure straight across the forehead and not down the side of the face. At mid-line, the temporal artery is about 2 mm below the surface but can go deeply below the surface on the side of the face.



- Measure exposed skin. Brush the hair and bangs aside if covering the area to be measured.



- Minimum measuring time: 2 seconds.
- Minimum time between successive measurements: 30 seconds

## FAQ

- Q: How does the temperature from a temporal scanner relate to core temperature?
- A: Temporal artery temperature is considered a core temperature because it has been demonstrated as accurate as the temperature measured by a pulmonary artery and esophageal catheter, and as precise as a rectal temperature on a stable patient. Rule of thumb: Rectal temperature is about 0.5°C (1°F) higher than an oral temperature and 1°C (2°F) higher than an axillary temperature. It will be easy to remember if you think of core temperature as a rectal temperature and apply the same protocol you would use for a rectal temperature. If your thermometer is marked Arterial/Oral and has a serial number beginning with "O" (standard model starts with "A"), it is programmed to compute the normal average cooling effect at the mouth and automatically

reduces the higher arterial temperature by that amount. This calibration allows the hospital to maintain existing protocols for fever workups based on oral temperature, and results in readings consistent with the 37°C (98.6°F) mean normal oral temperature, in the range of 35.9 – 37.5°C (96.6 – 99.5°F) you now see.

- Q: What should I do if I get an abnormally high or low reading, how do I confirm my reading?
- Repeat the reading with the same Temporal Scanner; a correct reading will be reproducible.
- Repeat the reading with another Temporal Scanner. Two Temporal Scanners with the same reading will confirm the reading.
- Sequential readings on the same patient in rapid succession will cool the skin; waiting about 30 seconds for the skin to recover from the cold probe is best.

### Possible causes of abnormal readings

Type of Abnormal Temperature	Possible Cause	Helpful Hint
<b>Abnormally Low Temperature</b>	Dirty Lens	The clean lens of the scanner every two weeks.
	Releasing the button before finishing measuring	Release the button after finishing measuring.
	Measuring when an ice pack or wet compress is on the forehead	Remove the ice pack or wet compress, wait 2 minutes, and re-take temperature.
	Measuring a completely diaphoretic patient	Complete diaphoresis includes diaphoresis of the area behind the ear and suggests that the temperature is rapidly dropping. Use an alternative method of temperature measurement in these cases until the patient is dry and the temporal artery measurement can be repeated.
	Improperly scanning down the side of the face	Scan straight across the forehead. The temporal artery is closest to the skin in that area.
<b>Abnormally High Temperature</b>	Anything covering the area to be measured would insulate and prevent heat from dissipating, resulting in false high readings.	Confirm measurement site has not recently been in contact with heat insulators such as hats, blankets, and hair. Scan the area not covered or wait about 30 seconds for the previously covered area to equilibrate to the environment.

### Care and Maintenance

- **Handling:** The TemporalScanner is designed and built to industrial durability standards to provide long and trouble-free service. However, it is also a high-precision optical instrument and should be accorded the same degree of care in handling as you would provide other precision optical instruments, such as cameras or


otoscopes.

- **Cleaning the case:** The TemporalScanner case can be wiped down using a cloth dampened with 70% isopropyl alcohol. The industrial-grade housing and design of the electronic components allow for completely safe cleaning with 70% isopropyl alcohol but should not be immersed in fluid or autoclaved.
- **Cleaning the sensor lens:** With normal use, the only maintenance required is to keep the lens on the end of the probe clean. It is made of special mirror-like, silicon infrared-transmitting material. However, dirt, greasy films or moisture on the lens will interfere with the passage of infrared heat and affect the accuracy of the instrument. Regularly clean the lens with a cotton swab dipped in alcohol under the instruction label on the instrument (see below). Use only light force for cleaning, to avoid damaging the lens. Water can be used to remove any residual film left by the alcohol. Do not use bleach or other cleaning solutions on the sensor lens.



DO NOT SUBMERSE THE THERMOMETER IN ANY CLEANING SOLUTION.

- **Sterilization:** Sterilization is not recommended for cabled versions of the TemporalScanner.
- **Calibration:** Factory calibration data is installed via a computer that communicates with the TemporalScanner's microprocessor. The instrument automatically self-calibrates each time it is turned on using this data, and will never require recalibration. If **readings** are not correct, the instrument should be returned for repair.
- **Battery:** A standard alkaline 9V battery provides approximately 15,000 readings.\* To replace, insert the end of a bent paper clip into the pinhole on the side of the unit to release the battery compartment door. Disconnect the old battery and replace it with a new one in the same location. Replace the cover. Use only high-quality alkaline batteries.
- Approximate number of readings when scanning for 5 seconds and reading the temperature display for 3 seconds before turning the thermometer off.

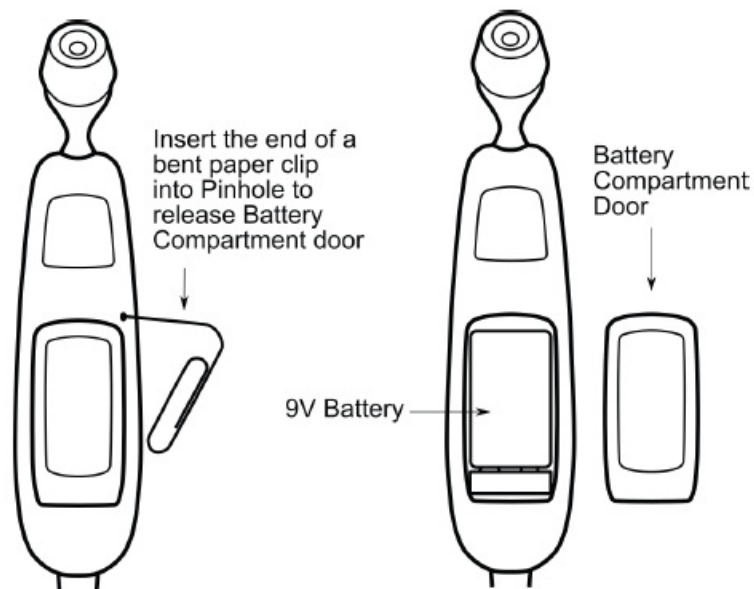

## Display Diagnostics Chart

- The following chart summarizes the conditions that may occur while the TemporalScanner is in use, and the associated indications:

Condition	Display	Range
High Target	HI	> 43 °C (110° F)
Low Target	LO	< 16 °C (61° F)
High Ambient	HI A	> 40 °C (104° F)
Low Ambient	LO A	< 16 °C (61° F)
Low Battery	bAtt	
No or Very Low Battery	blank display	
Processing Error	Err	Restart. Return to Exergen for repair if the error message persists.
Scanning (Normal Operation)	----	


## Fahrenheit or Celsius Conversion

- The TemporalScanner can be used in either °F or °C. To convert from one scale to the other, the only tools necessary are a paper clip and the tip of a small screwdriver.

### For °F/°C Conversion

- Insert the end of a bent paper clip into the pinhole on the side to release and remove the cover. Remove the battery from the compartment.
- Locate the switch, and with the tip of a screwdriver, slide left or right to the opposite position.
- Remove the screwdriver.

- Replace cover.

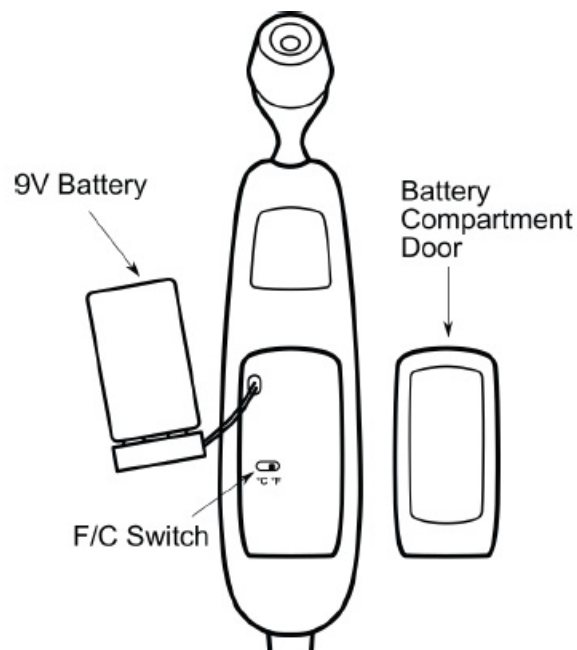

Exergen TAT-5000S-RS232

#### Guidance and Manufacturer's Declaration-Electromagnetic Emissions


The infrared forehead thermometer model TAT-5000S series is intended for use in the electromagnetic environment

specified below. The user of the TAT-5000S series should ensure that it is used in such an environment.

Emissions test	Compliance	Electromagnetic environment-guidance
RF emissions CISPR 11	Group 1	The TAT-5000S series thermometer uses no RF energy- gy therefore any emissions are unlikely to c ause any interference in nearby electronic equipm ent
RF emissions CISPR 11	Class B	The TAT-5000S series thermometer is suitable for use by a healthcare professional in a typical healt hcare environment.
Harmonic emissions	Not applicable	
Voltage fluctuations	Not applicable	

## Guidance and manufacturer's declaration-electromagnetic immunity

The TAT-5000S series thermometer is intended for use in the electromagnetic environment specified below. The user of the TAT-5000S series should ensure that it is used in such an environment.

Immunity test	IEC 60601 test level	Compliance level	Electromagnetic environment-guidance
Conducted RF IEC 61000-4-6	3Vrms 150 kHz to 80 MHz	3Vrms	<p>Portable and mobile RF communications equipment should be used no closer to any part of the TAT-5000S series including cables if applicable, than the recommended separation distance calculated from the equation applicable to the frequency of the transmitter.</p> <p><b>Recommended separation distance</b></p> $d=1,2 \cdot P^{1/2}$ <p><math>d=1,2 \cdot P^{1/2}</math> 80 MHz to 800MHz <math>d=1,2 \cdot P^{1/2}</math> 800MHz to 2,7 GHz</p> <p>Where P is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer and d is the recommended separation distance in meters(m).</p> <p>Field strength from the fixer RF transmitters, as determined by an electromagnetic site survey, a. should be less than the compliance level in each frequency range, and b. interference may occur in the vicinity of equipment with the following symbol:</p> 
Radiated RF IEC 61000-4-3	10V/m 80 MHz to 2,7 GHz	10V/m	

Note 1 At 80MHz and 800MHz, the higher range applies.

Note 2 These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and

reflection from structures, objects, and people.

a. Field strengths from fixed transmitters, such as base stations for radio (cellular/cordless) telephones and land mobile radios, amateur radio, AM and FM radio broadcasts and TV broadcasts cannot be predicted theoretically with accuracy. To assess the electromagnetic environment due to fixed RF transmitters, an electromagnetic site survey should be considered. If the measured field strengths in the location in which the TAT-5000S series thermometer is used exceed the applicable RF compliance level above, the TAT-5000S series thermometer should be observed to verify normal operation. If abnormal performance is observed, additional measures may be necessary, such as reorienting or relocating the TAT-5000S.

b. Over the frequency range 150 kHz to 80 MHz, field strengths should be less than 3V/m.

c. Portable and mobile RF communications equipment can affect performance.

**Guidance and Manufacturer's Declaration-Electromagnetic Immunity (cont)**

The TAT-5000S series thermometer is intended for use in the electromagnetic environment specified below. The user of

the TAT-5000S series should ensure that it is used in such an environment.

<b>Immunity test</b>	<b>IEC 60601 test level</b>	<b>Compliance level</b>	<b>Electromagnetic environment-guidance</b>
Electrostatic discharge (ESD) IEC61000-4-2	8kV contact 15kV air	8kV contact 15kV air	Floors should be wood, concrete or ceramic tile. If floors are covered with synthetic material, the relative humidity should be at least 30%.
Electrical fast transient/burst IEC 61000-4-4	2kV for power supply lines 1kV for input-output lines	Not applicable	Mains power quality should be that of a typical healthcare environment.
Surge IEC 61000-4-5	1kV line(s) to line(s) 2kV line(s) to earth	Not applicable	Mains power quality should be that of a typical healthcare environment.
Interruptions and voltage variations on power supply Input lines IEC 61000-4-11	<5% UT (>95% dip in UT) for 0,5 cycle 40% UT (60% dip in UT) for 5 cycles 70% UT (30% dip in UT) for 25 cycles < 5% UT (>95% dip in UT) for 5 sec.	Not applicable	Mains power is not applicable. The TAT-5000S series is powered by battery and battery only.
Power frequency (50/60 Hz) magnetic field IEC 61000-4-8	30A/m	30A/m	Power frequency magnetic fields should be at the level characteristic of a typical location in a typical healthcare environment.

Note UT is the a.c. mains voltage before the application of the test level

## Recommended separation distances between portable and mobile RF communication equipment and the TAT-5000S Series

The TAT-5000S series forehead thermometer is intended for use in an electromagnetic environment in which radiated RF disturbances are controlled or the user of the TAT-5000S series thermometer can help prevent electromagnetic interference by maintaining a minimum distance between portable and mobile RF communications equipment (transmitters) and the TAT-5000S series thermometer as recommended below, according to the maximum output power of the communications equipment.

Rated maximum output power of the transmitter (W)	Separation distance according to frequency of transmitter m		
	150 KHz to 80 MHz $d=1,2 P^{1/2}$	80 MHz to 800 MHz $d=1,2 P^{1/2}$	800 MHz to 2,7 GHz $d=2,3 P^{1/2}$
0,01	0,12	0,12	0,23
0,1	0,38	0,38	0,73
1	1,2	1,2	2,3
10	3,8	3,8	7,3
100	12	12	23

For transmitters rated at a maximum output power not listed above, the recommended separation distance  $d$  in meters (m) can be estimated using the equation applicable to the frequency of the transmitter, where  $P$  is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer.

Note 1 At 80 MHz and 800 MHz the separation distance for the higher frequency range applies.

Note 2 These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection

from structures, objects, and people.

## Repair

If repair is required, please go to our website at [www.exergen.com/rma](http://www.exergen.com/rma) to request a Return Materials Authorization (RMA) number. You will receive an email response with an RMA number and instructions on where to return your unit. Alternatively, you may contact Exergen customer service at [617-923-9900](tel:617-923-9900) or [service@exergen.com](mailto:service@exergen.com) or contact your local distributor.





Specification †	TAT-5000S-RS232
Clinical Accuracy **	± 0.1°C or 0.2°F Per ASTM E1112
Temperature Range	16 to 43°C (61 to 110°F)
Arterial Heat Balance Range for Body Temperature ***	34.5 to 43°C (94 to 110°F)
Operating Environment	16 to 40°C (61 to 104°F)
Resolution	0.1° C or F
Response Time	~0.04 seconds
Time Displayed On Screen	30 seconds
Size	Instrument : 20 cm X 4.6 cm X 4 cm (7.9" X 1.8" X 1.6" )
Cable	0.8 m (32") retracted
Weight	0.3 kg (0.7 lb)
EMI and RFI Protection	Stainless steel enclosure on the upper part inside of the casing
Storage Conditions	-20 to 50°C (-4 to 122°F)
Display Type and Size	Large bright LED's
Construction Method	<ul style="list-style-type: none"> <li>• Industrial duty impact-resistant casing</li> <li>• Chemically resistant casing and lens</li> <li>• Hermetically sealed sensing system</li> <li>• Chrome-plated alloy cast head</li> </ul>
Warranty	Instrument: Lifetime Cable: 5 years



- The values of quantities stated in SI units are to be regarded as the standard. The values of quantities in parentheses are not in SI and are optional.
- Laboratory accuracy outside the physiological range is +/-0.3 °C (0.5 °F).
- Automatically applied when the temperature is within the normal body temperature range, otherwise reads surface temperature.

#### TAT-5000S-RS232 QR Cable Replacement



1. Bend one leg of a paper clip and insert it into the hole in the side of the plastic housing. Push to release the battery cover, then move the battery out of the way.

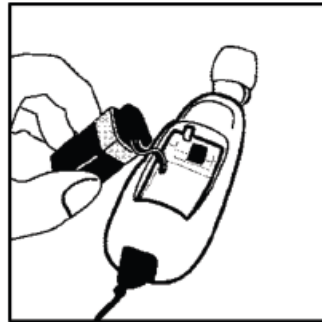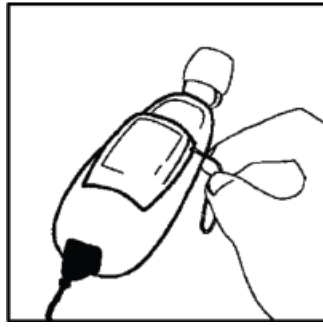



2. Depress the black release button and remove the cable while holding the release button down.

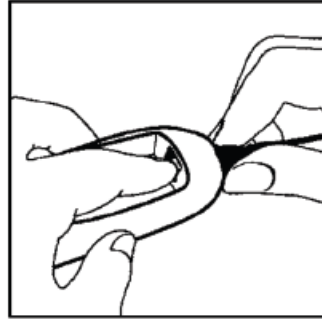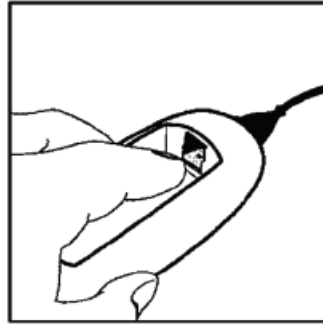

3. Orient the cable plug properly for proper fit into the receptacle hole and install a replacement cable.

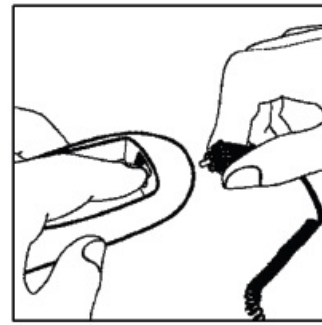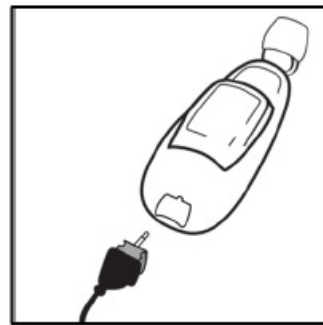

4. Replace the battery in the compartment. Re-install the battery cover.

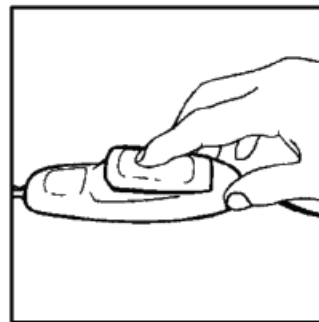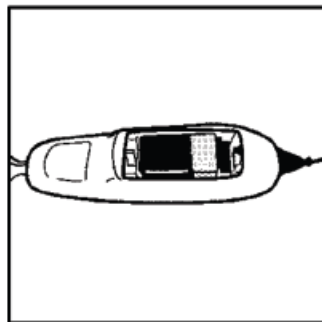

Exergen p/n	Description
124330	QR Replacement Cable, Generic

### Verification Testing

All Exergen infrared thermometers are designed to permanently maintain their accuracy and normally recalibration is not required unless the thermometer has been physically damaged or experiences component failure. In the unlikely event recalibration might be required, the thermometer must be returned to Exergen for the procedure. However, calibration can be verified in the lab or clinical units quite easily using Exergen calibration kits.

See: <https://www.exergen.com/professional-medical-products/products/calibration-verification-kit> and: <https://www.exergen.com/professional-medical-products/products/professional-product-manuals>

### Disposable Caps

Disposable caps, which can be used once and discarded, or reused on the same patient are available for all levels of cross-contamination protection should they be preferred for certain patient populations, and are still very cost

effective..















## Using the Disposable Caps



1. Apply the cap by pushing onto the probe head with your fingers.
2. Remove the cap by pushing the edge forward with the thumb.
3. Caps may be reused on the same patient.

Disposable caps can be discarded in normal trash. The operator is responsible for checking the compatibility of the thermometer, probe cover, and monitoring equipment. Incompatible components can result in degraded performance.

Exergen p/n	Description
134203	Disposable Caps, box of 1000

	Symbol for Manufacturer		Do not throw this device away in the trash, contact Exergen Corp. for disposal and recycling instructions.
	Caution	<b>IPX0</b>	Ordinary Equipment
	Consult Instructions for Use		"On" (only for part of Equipment)
	Degree of Protection Against Electrical Shock Defibrillation-Proof Type BF Applied Part, Battery Operated	<b>CLASSIFIED</b>  E466615	<b>MEDICAL ELECTRICAL EQUIPMENT</b> ANSI/AAMI ES60601-1 (2005) + AMD 1 (2012); CAN/CSA-C22.2 No. 60601-1:14; IEC 60601-1-6; ISO 80601-2-56: Particular Requirements For Basic Safety and Essential Performance of Clinical Thermometers For Body Temperature Measurement
<b>Segurança</b>  	INMETRO		
	Medical Device		EMERGO by UL Westervoortsedijk 60 6827 AT Arnhem The Netherlands
 1434	Conformite Europeenee		MedEnvoy Switzerland Gotthardstrasse 28 6302 Zug Switzerland
UK Representative	Emergo Consulting (UK) Limited c/o Cr360 – UL International Compass House, Vision Park Histon Cambridge CB24 9BZ England, United Kingdom		UK Conformity Assessed

The CLINICAL THERMOMETER is an ADJUSTED MODE CLINICAL THERMOMETER. The correction method is

proprietary. Laboratory testing protocol for laboratory accuracy is available upon request.  
If you have any issues or concerns please contact Exergen [service@exergen.com](mailto:service@exergen.com) or the local Competent Authority.

## CONTACT

- EXERGEN CORPORATION
- 400 PLEASANT STREET WATERTOWN, MA 02472 PH [617-923-9900](tel:617-923-9900)
- [www.exergen.com](http://www.exergen.com)

## Documents / Resources

	<p><a href="#">EXERGEN TAT-5000S-RS232 Series Accurate Temperature</a> [pdf] Instruction Manual TAT-5000S-RS232 Series, TAT-5000S-RS232 Series Accurate Temperature, Accurate Temperature, Temperature</p>
---	--

## References

- [E Home Page - Exergen Corporation](#)
- [E Home Page - Exergen Corporation](#)
- [E Home Page - Exergen Corporation](#)
- [E Professional Product Returns - Exergen Corporation](#)
- [User Manual](#)

### Manuals+, Privacy Policy

This website is an independent publication and is neither affiliated with nor endorsed by any of the trademark owners. The "Bluetooth®" word mark and logos are registered trademarks owned by Bluetooth SIG, Inc. The "Wi-Fi®" word mark and logos are registered trademarks owned by the Wi-Fi Alliance. Any use of these marks on this website does not imply any affiliation with or endorsement.