

FORA®
4183F Total
Cholesterol
Test System



FORA 4183F Total Cholesterol Test System User Guide

[Home](#) » [FORA](#) » FORA 4183F Total Cholesterol Test System User Guide 

Contents

- [1 FORA 4183F Total Cholesterol Test System](#)
- [2 Product Usage Instructions](#)
- [3 HOW TO USE](#)
- [4 Reading the Results](#)
- [5 After Use](#)
- [6 Warranty Registration Card](#)
- [7 Documents / Resources](#)
 - [7.1 References](#)
- [8 Related Posts](#)



FORA 4183F Total Cholesterol Test System



Product Specifications:

- **Intended Use:** Self-testing for in vitro diagnostic use
- **Usage:** For single patient use only, over the counter use
- **Manufacturer:** ForaCare, Inc.
- **Address:** 893 Patriot Drive Suite D, Moorpark, CA 93021 USA

Product Usage Instructions

Preparing for Testing:

Ensure you have all the necessary components ready for testing.

Performing the Test:

Follow the instructions provided in the user manual carefully.

Reading the Results:

Interpret the results based on the guidelines provided.

Cleaning and Maintenance:

After use, clean the device as per the instructions to ensure proper hygiene and longevity.

Frequently Asked Questions

Can this device be used in healthcare settings?

No, this device is not intended for use in healthcare or assisted-use settings such as hospitals, physician offices, or long-term care facilities.

Are alcohol pads included in the test kit?

No, alcohol pads are not included in the test kit and should be purchased separately.





How to contact ForaCare for assistance?

You can visit www.foracare.com or call 315-4183600-012 for assistance. For after-hours support, contact your healthcare professional.

Quick Start User Guide




For self-testing. Read instructions before use. For In vitro diagnostic use. For single patient use only.
For over the counter use only.

HOW TO USE

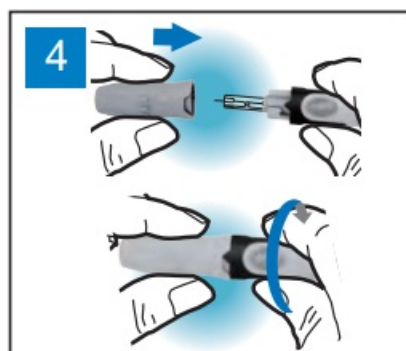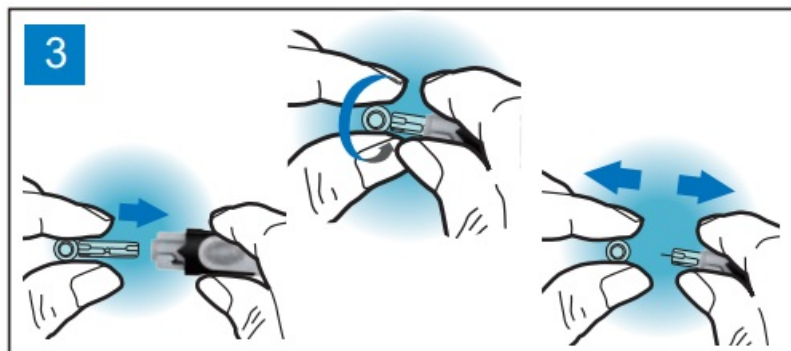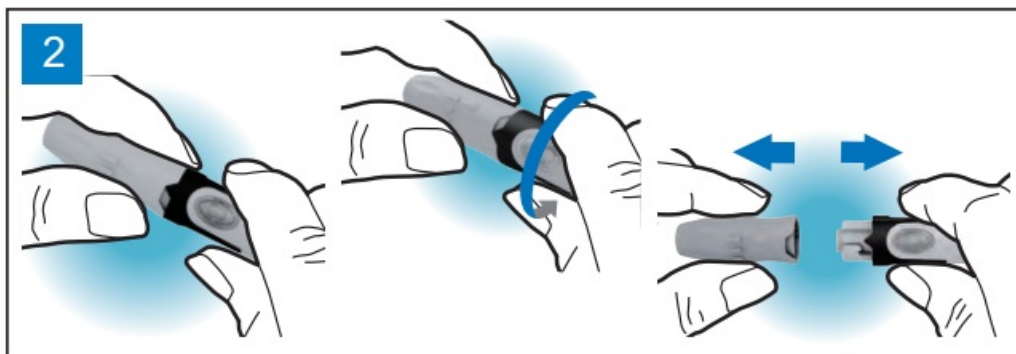
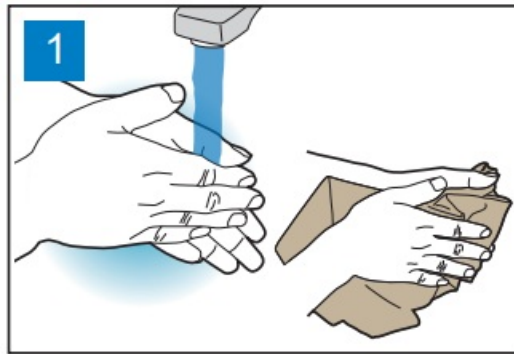





Reading the Results

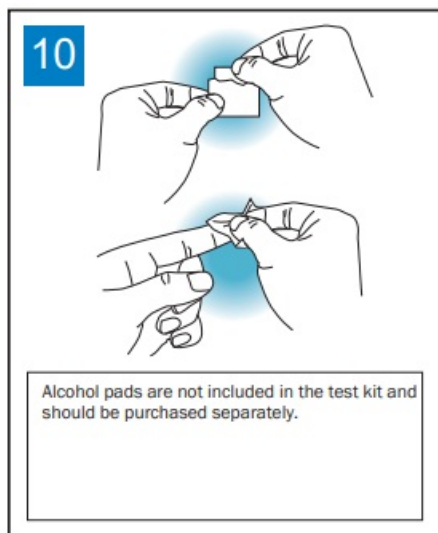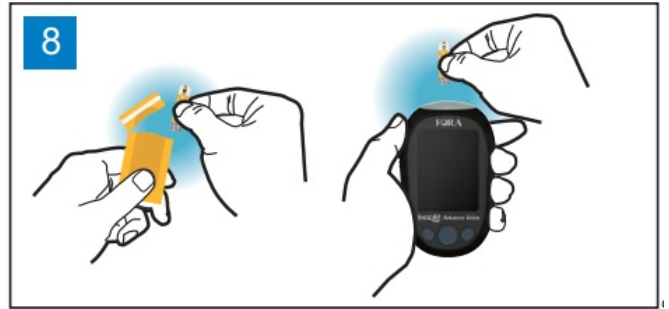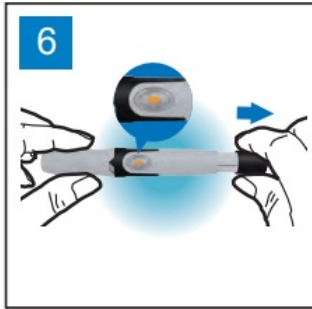

NOTE

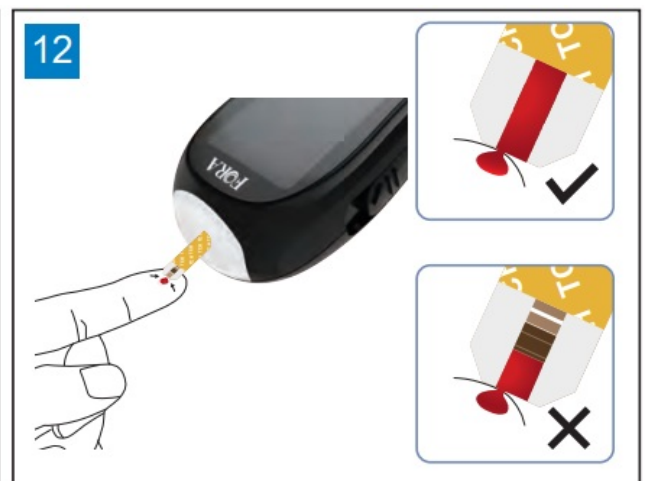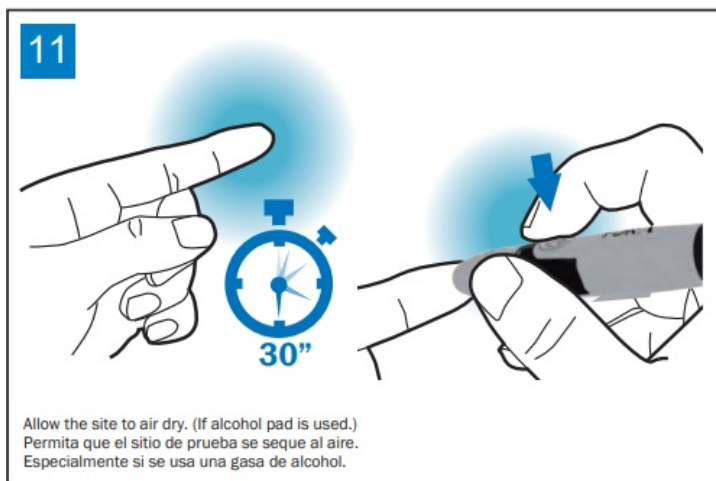

After Use

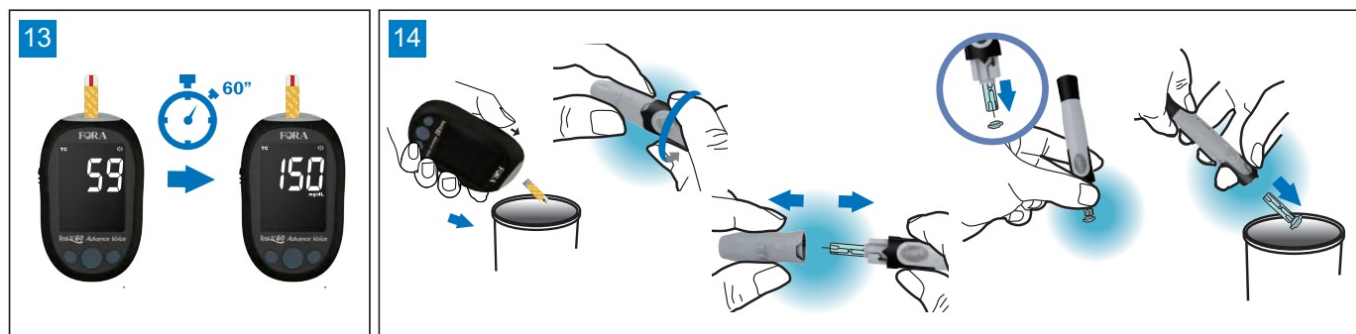

This device is NOT intended for use in healthcare or assisted-use settings such as hospitals, physician offices, or long-term care facilities. Use of this device on multiple patients may lead to transmission of Human Immunodeficiency Virus (HIV), Hepatitis C Virus (HCV), Hepatitis B Virus (HBV), or other bloodborne pathogens.

Warranty Registration Card

Five Years Warranty Registration Card


Name										E-mail									
Street Address / Dirección																			
APT#					City										Country				
State					Zip										Home Telephone				
Meter Serial Number (See label on back of meter) /															Date of Purchase (Month-Day-Year) /				

acknowledge that ForaCare has the right to contact me with updates, promotions, or meter upgrade offers

ForaCare, Inc. Online Warranty Registration and Detailed Warranty Coverage at www.foracare.com/support.html

www.foracare.com

Documents / Resources

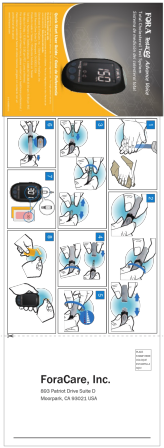

[FORA 4183F Total Cholesterol Test System](#) [pdf] User Guide

4183F, 4183F Total Cholesterol Test System, Total Cholesterol Test System, Cholesterol Test System, Test System, System

References

- [User Manual](#)

[Manuals+](#), [Privacy Policy](#)

This website is an independent publication and is neither affiliated with nor endorsed by any of the trademark owners. The "Bluetooth®" word mark and logos are registered trademarks owned by Bluetooth SIG, Inc. The "Wi-Fi®" word mark and logos are registered trademarks owned by the Wi-Fi Alliance. Any use of these marks on this website does not imply any affiliation with or endorsement.