

graham field JB0112-067 Nebulizer Compressor User Manual

Home » graham field » graham field JB0112-067 Nebulizer Compressor User Manual







Contents

- 1 INTRODUCTION
- **2 IMPORTANT SAFETY**

PRECAUTIONS

- **3 PRODUCT DESCRIPTION**
- 4 SETUP
- **5 OPERATION**
- **6 MAINTENANCE**
- **7 TROUBLESHOOTING**
- **8 SPECIFICATIONS**
- **9 LIMITED WARRANTY**
- 10 Support
- 11 Documents / Resources
- 12 Related Posts

INTRODUCTION

This user manual contains important information and safety precautions for the John Bunn Neb-u-Tyke Speedster

Nebulizer Compressor. Before using your Nebulizer Compressor, please read and understand this entire user manual. Take special note of all safety precautions marked DANGER and WARNING. Save this user manual for future reference.

Intended Use

The Neb-u-Tyke Speedster Compressor Nebulizer System is designed to provide a source of compressed air for aerosol therapy. It is used in conjunction with a jet (pneumatic) nebulizer to produce medicated aerosols for inhalation by pediatric and adult patients with respiratory symptoms. Indications for therapy include asthma, chronic bronchitis, infection of the upper respiratory tract, chronic obstructive pulmonary disease, and other respiratory disorders in accordance with a physician's prescription. Do not use this product for any other purpose than the preceding. This device can be used with adult or pediatric patients under physician's prescription.

Symbols Key

0	Off
1	On
~	Alternating current
IPX0	Enclosed equipment without protection against ingress of water
<u>\(\) \(\) \(\) \(\)</u>	Attention (read the instructions)
II	Class II (not applicable for UL1431)
床	BF: This product is in accordance with the degree of protection against electric shock for type BF eq uipment. (not applicable for UL1431)
<u> </u>	Disposal of Electrical & Electronic Equipment (WEEE): This product should not be treated as house hold waste, but submitted to an appropriate collectionpoint for the recycling of electrical and electronic equipment. For more detailed information about the recycling of this product, please contact your local city office, household waste disposal service, or the Graham-Field authorized dist ributor from whom you purchased this product.

IMPORTANT SAFETY PRECAUTIONS

When using electrical products, especially when children are present, always follow basic safety precautions, including the following:

DANGER: Indicates a potential hazard situation or unsafe practice that, if not avoided, will result in death or serious personal injury.

WARNING: Indicates a potential hazard situation or unsafe practice that, if not avoided, could result in death or serious personal injury.

CAUTION: Indicates a potential hazard or unsafe practice that, if not avoided, could result in minor or moderate personal injury.

NOTICE: Indicates a potential hazard or unsafe practicethat, if not avoided, could result in product or property damage.

Info: Provides application recommendations or other useful information to ensure that you get the most

READ ALL INSTRUCTIONS BEFORE USING

DANGER: To reduce the risk of electrocution:

- 1. Always unplug this product immediately after use.
- 2. Do not use this product while bathing, showering, washing dishes, or close to water sources of any kind.
- 3. Do not place or store device where it can fall or be pulled into a tub or sink.
- 4. Do not place device in or drop into water or other liquid.
- 5. Do not reach for a device that has fallen into water. Unplug it immediately



WARNING: To reduce the risk of burns, electrocution, fire or personal injury:

- 1. Never leave this device unattended when plugged in.
- 2. This product contains small parts that may present a choking hazard to small children, and the tubing may present a strangulation hazard. Always use close supervision when this device is used by or near children or those who require close supervision.
- 3. Children under the age of 3, or any patient who is unable to use a mouthpiece properly under supervision, should use a mask.
- 4. Use this device only as intended and described in this manual. Do not use attachments or accessories not recommended by GF Health Products, Inc.
- 5. Never operate this product if:
 - a. it has a damaged cord or plug,
 - **b.** it is not working properly,
 - c. it has been dropped or damaged, or
 - d. it has been dropped into water. Return the product to your Graham-Field authorized distributor for examination and repair.
- 6. Keep the cord away from heated surfaces.
- 7. Never block the air openings of this product or place it on a soft surface, such as a bed or couch, where the air openings may be blocked. Keep the air openings free of lint, hair and the like.
- 8. Never drop or insert any object into any openings or hose.
- 9. Never use this device while drowsy or sleeping.
- 10. Do not use this device outdoors or operate where aerosol (spray) products are being used.
- 11. Do not use this device in the presence of flammable anesthesia or where oxygen or nitrous oxide is being administered. This device has no AP or APG protection.
- 12. Connect this device to a properly grounded outlet only.
- 13. This device has a polarized plug (one blade is wider than the other). As a safety feature, this plug will fit into a polarized outlet only one way. If the plug does not fit fully into the outlet, reverse the plug. If it still does not fit, contact a qualified electrician. Do not modify the plug in any way. Do not attempt to defeat this safety feature.
- 14. Unplug the device before filling or cleaning the nebulizer.
- 15. This device is oil-free. Do not lubricate.
- 16. Do not remove the jet nebulizer while the device is operating.


- 17. Do not leave medication inside the jet nebulizer when it is not in use.
- 18. Use the nebulizer intermittently; the maximum operating period is 30 minutes. The nebulizer must stand unused for 30 minutes between uses.
- 19. The mouthpiece (and optional mask) are for use by one person only; in order to avoid infection, do not share them.
- 20. Notice for California Customers- California Proposition 65

WARNING: This product contains a chemical known to the State of California to cause cancer and reproductive or developmental harm.

PRODUCT DESCRIPTION

Features and Components

Please note nebulizer features and components, labeled in the illustration below.

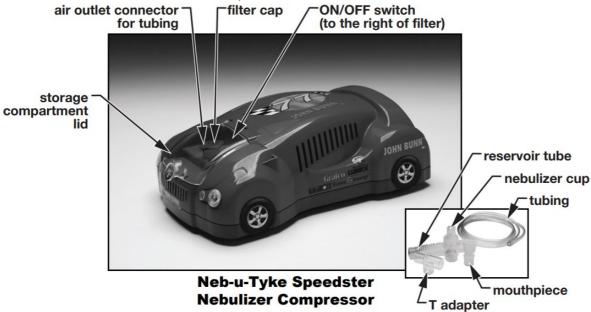

Item No.	Description	
JB77200	Neb-u-Tyke Speedster Nebulizer Compressor complete with Garage Bag	
JB0112-067	Neb-u-Tyke Speedster Nebulizer Compressor without Garage Bag	
JB76220	Garage Bag only	

SETUP

Info: Before initial operation, clean the nebulizer cup assembly following the instructions given in


MAINTENANCE/Cleaning the Nebulizer Cup.

 \bigwedge

/!\ WARNING: Ensure that the nebulizer compressor is unplugged during setup.

- 1. Before each use, inspect the compressor and nebulizer cup assembly for damage or wear; replace as needed.
- 2. Place the compressor on a table or other flat stable surface (not on the floor), in an area that is clean and dustfree. Be sure you can easily reach the controls when seated.

- 3. Open the nebulizer medication cup: Twist the cap counter-clockwise until it stops, then lift cap off.
- 4. Pour the prescribed medication into the nebulizer medication cup. Do not fill with more than 5 ml per treatment.
- 5. Install cap on cup. Turn clockwise to tighten.




6. If using the mouthpiece for treatment, proceed to step 7. If using an optional mask, install the bottom part of the mask directly onto the top of the nebulizer medication cup cap as shown at right. Proceed to step 9.




7. Insert mouthpiece into large end of T adapter.

Info: The reservoir tube, shown in the illustration earlier in this manual, acts as a holding tank for the mist, reducing the amount lost during treatment. Its use is optional. If you wish to use the reservoir tube, install it now on the small end of the T adapter.



- 8. Install T adapter onto top of nebulizer medication cup cap.
- 9. Connect the tubing to the adapter on the bottom of the nebulizer medication cup.



10. Connect the tubing's other end to the compressor air outlet connector.

WARNING: Before use, check that all parts are securely connected. Use of an improperly assembled nebulizer could diminish or prevent adequate delivery of medication and the effectiveness of the treatment.

OPERATION

NOTICE: The Neb-u-Tyke Speedster Nebulizer Compressor is designed for intermittent use only. Do not operate it continuously for more than 30 minutes for a single use without turning it off and allowing a cooling period of least 30 minutes.

- 1. Ensure that the ON/OFF switch is in the OFF position.
- 2. Plug the power cord into a properly grounded electrical wall outlet.
- 3. Move the ON/OFF switch to the ON position to start the compressor.
- 4. Place the nebulizer mouthpiece between teeth and close mouth (or install the optional mask on face).
- 5. As aerosol starts flowing, inhale deeply and slowly through mouthpiece (or optional mask).

WARNING: Never use a nebulizer with a clogged nozzle. If the nozzle is clogged, the aerosol mist will be reduced, altered or stopped, which will diminish or eliminate the effectiveness of the treatment. If clogging occurs, replace the nebulizer.

Info: If you need to interrupt treatment, move the ON/OFF switch to the OFF position.

- 6. When the treatment is complete, move the ON/OFF switch to the OFF position to turn off the compressor.
- 7. Unplug the compressor from power outlet.
- 8. Disconnect nebulizer from tubing.
- 9. Clean nebulizer as instructed in MAINTENANCE/ Cleaning the Nebulizer Cup.

Safety Overload

NOTICE: Do not exceed 30 minutes of continuous operation

- 1. The motor of this device has a built-in thermal overload protector. Should the motor overheat, the protector will automatically shut off the motor. Should this occur, move the ON/OFF switch to the OFF position and allow the motor to cool down for approximately 30 minutes\ before turning it on again.
- 2. If the overload protector shuts off the motor frequently, you may have an unstable voltage situation.

3. If the device shuts down and cannot restart, it may need to be replaced. Call your Graham-Field authorized distributor immediately.

MAINTENANCE

Cleaning the Compressor's Outer Case

VARNING: Electrical shock hazard. Do not remove the outer case of the device. All disassembly and maintenance of the device must be performed by a qualified service technician. Refer service to qualified service personnel.

WARNING: This device does not require oil. Do not attempt to lubricate any internal parts.

/!\ WARNING: Unplug device before cleaning. Do not submerge in water for cleaning

Wipe the compressor's outer case with a clean, damp cloth weekly to keep it dust-free. Do not use any powdered type cleaners or soap

Cleaning the Nebulizer Cup

All parts of the disposable nebulizer, except tubing, should be thoroughly cleaned after each use. If your physician specifies a specific cleaning procedure, follow that procedure.

riangle **WARNING:** To prevent possible risk of infection from contaminated medication, clean the nebulizer after each treatment.

- 1. After each use, disassemble the nebulizer cup, T adapter and mouthpiece completely, wash all parts in warm soapy water, and rinse thoroughly. Allow to air dry. Store in a clean, dry location.
- 2. Once daily, after washing as above, soak nebulizer components in a fresh solution consisting of one part warm water and one part white vinegar for 30 minutes followed by a warm water rinse. Allow to air dry. Store in a clean, dry location.

Replacing the Filter

NOTICE: Change the filter once every 30 days or when filter turns gray

- 1. Ensure that ON/OFF switch is in the OFF position. Open the filter cap located next to the ON/OFF switch.
- 2. Remove the dirty filter with a small, pointed object. Discard the filter.
- 3. Replace with a clean filter. Additional filters are available from your Graham-Field authorized distributor.
- 4. Replace the filter cap.

NOTICE: Do not use cotton or other materials as a filter.

NOTICE: Do not wash or clean the filter.

NOTICE: Do not reuse the filter. Do not operate compressor without a filter. Compressor damage can result.

NARNING: The disposable nebulizer kit is for single patient use only

Storage

Keep the device and accessories dry. Avoid exposure to direct sunlight.

TROUBLESHOOTING

If your Neb-u-Tyke Speedster Nebulizer Compressor fails to function, consult the following Troubleshooting guide. If the problem persists, consult your Graham-Field authorized distributor

Problem	Cause and Solution		
	Check if plug is properly fit into a grounded electrical outlet.		
Device doesn't operat e	When device has been run continuously for more than 30 minutes just before using, auto-shut-down may have been activated by the built-in thermal protector; ensure that device is OFF for at least 30 minutes before next usage.		
	Check for proper electrical voltage.		
Nebulization is weak	Check tubing for blockage or air leakage at connection to Neb-u-Tyke compressor or n ebulizer cup; replace as needed.		
Nebulization is weak	Check that the nebulizer cup is properly assembled and not damaged. If there is any d amage, replace as needed.		
	Check if filter is dirty; replace filter as needed.		

SPECIFICATIONS

Specification	Description		
Max pressure (compressor)	30.5 psi		
Max flow rate	Approximately 12 LPM		
Nebulization rate	.33 ml/min		
Particle dimension	.5 – 5 microns		
Capacity	5 ml		
Filter	Sponge		
Dimensions (LxWxH)	10.2" ×6.9" × 3.7" (25.9 cm x 17.5 cm x 9.4 cm)		
Weight	3.8 lb (1.73 kg)		
Electrical requirement	115VAC/60Hz		
Current	1.2A (rate)		
Fuse	2.5A 250V		
Power cord	Black, 7 ft (84") / 213.4 cm		
Plug	2-prong type		
Sound level	54dba		
	Temperature	Operation: 41°F to 104°F (5°C to 40°C)	
Environment		Storage: 14°F to 158°F (-10°C to 70°C)	
Liviloninent	Humidity	Operation: 30% to 95% RH	
		Storage: 10% to 95% RH	

LIMITED WARRANTY

SCOPE OF WARRANTY

GF Health Products, Inc. ("GF") warrants to the original purchaser only that it will replace or repair components, at GF's sole discretion, that are defective in material or workmanship under normal use and service. All warranties are conditioned upon the proper use of the products strictly in accordance with good commercial practice and applicable GF instructions and manuals, including proper use and maintenance. To the extent that a component is warranted by a third party, GF conveys all of its rights under that warranty to the original purchaser, to the extent permitted.

This limited warranty shall only apply to defects that are reported to GF's customer service team within the applicable warranty period and which, upon examination by GF or its authorized representative, prove to be a warranty item. This limited warranty is not transferable.

The warranted components and time period are set forth below:

Compressor: five years

Accessories: six months

The applicable warranty period shall commence from date of shipment to the original customer, unless there is an expiration date on the component in which case the warranty shall expire on the earlier of warranty period or the

OBTAINING WARRANTY SERVICE

A GF Customer Service Representative must authorize warranty service.

EXCLUSIONS

The warranty does not cover and GF shall not be liable for the following:

- 1. Defects, damage, or other conditions caused, in whole or in part, by misuse, abuse, negligence, alteration, accident, freight damage, tampering or failure to seek and obtain repair or replacement in a timely manner;
- 2. Products which are not installed, used, or properly cleaned and maintained as required in the official manual for the applicable product;
- 3. Products considered to be of a non-durable nature including, but not limited to: casters, filters, fuses, gaskets, lubricants, and charts;
- 4. Accessories or parts not provided by GF;
- 5. Charges by anyone for adjustments, repairs, replacement parts, installation or other work performed upon or in connection with such products whichare not expressly authorized in writing, in advance, by GF;
- 6. Any labor or shipping charges incurred in the replacement part installation or repair;
- 7. Costs and expenses of regular maintenance and cleaning; and
- 8. Representations and warranties made by any person or entity other than GF.

ENTIRE WARRANTY, EXCLUSIVE REMEDY AND CONSEQUENTIAL DAMAGES DISCLAIMER

THIS WARRANTY IS GF'S ONLY WARRANTY AND IS IN LIEU OF ALL OTHER WARRANTIES, EXPRESS OR IMPLIED. GF MAKES NO IMPLIED WARRANTIES OF ANY KIND INCLUDING ANY IMPLIED WARRANTIES OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE.

IF ANY MODEL OR SAMPLE WAS SHOWN TO THE CUSTOMER, SUCH MODEL OR SAMPLE WAS USED MERELY TO ILLUSTRATE THE GENERAL TYPE AND QUALITY OF THE PRODUCT AND NOT TO REPRESENT THAT THE PRODUCT WOULD NECESSARILY CONFORM TO THE MODEL OR SAMPLE IN ALL RESPECTS.

THIS WARRANTY IS LIMITED TO THE REPAIR OR REPLACEMENT OF THE DEFECTIVE PARTS. GF SHALL NOT BE LIABLE FOR AND HEREBY DISCLAIMS ANY DIRECT, SPECIAL, INDIRECT, INCIDENTAL, EXEMPLARY OR CONSEQUENTIAL DAMAGES, INCLUDING, BUT NOT LIMITED TO: DAMAGES FOR LOSS OF PROFITS OR INCOME, LOSS OF USE, DOWNTIME, COVER, OR EMPLOYEE OR INDEPENDENT CONTRACTOR WAGES, PAYMENTS AND BENEFITS

The warranties contained herein contain all the representations and warranties with respect to the subject matter of this document, and supersede all prior negotiations, agreements and understandings with respect thereto. The recipient of this document hereby acknowledges and represents that it has not relied on any representation, assertion, guarantee, warranty, collateral contract or other assurance, except those set out in this document. For additional information on this product or this warranty, please contact a GF Customer Service Representative.

NOTES:

- 1. Additional terms and conditions may apply.
- 2. Freight claims must be notated on the Bill of Lading and must be made with immediacy. The ICC regulations

govern specific requirements for freight claims. Failure to abide by those regulations may result in a denial of the freight claim. GF will assist you in filing the freight claim.

3. Claims for any short shipment must be made within thirty (30) days of the invoice date

Support

Manufactured for: GF Health Products, Inc. 2935 Northeast Parkway Atlanta, Georgia 30360 USA Telephone: 770-368-4700

Fax: 770-368-2386

Documents / Resources



graham field JB0112-067 Nebulizer Compressor [pdf] User Manual JB0112-067 Nebulizer Compressor, JB0112-067, Nebulizer Compressor, Compressor

Manuals+,