


healthdirect Real Time Device Monitoring App Owner's Manual

[Home](#) » [healthdirect](#) » healthdirect Real Time Device Monitoring App Owner's Manual 



Real Time Device Monitoring App Owner's Manual

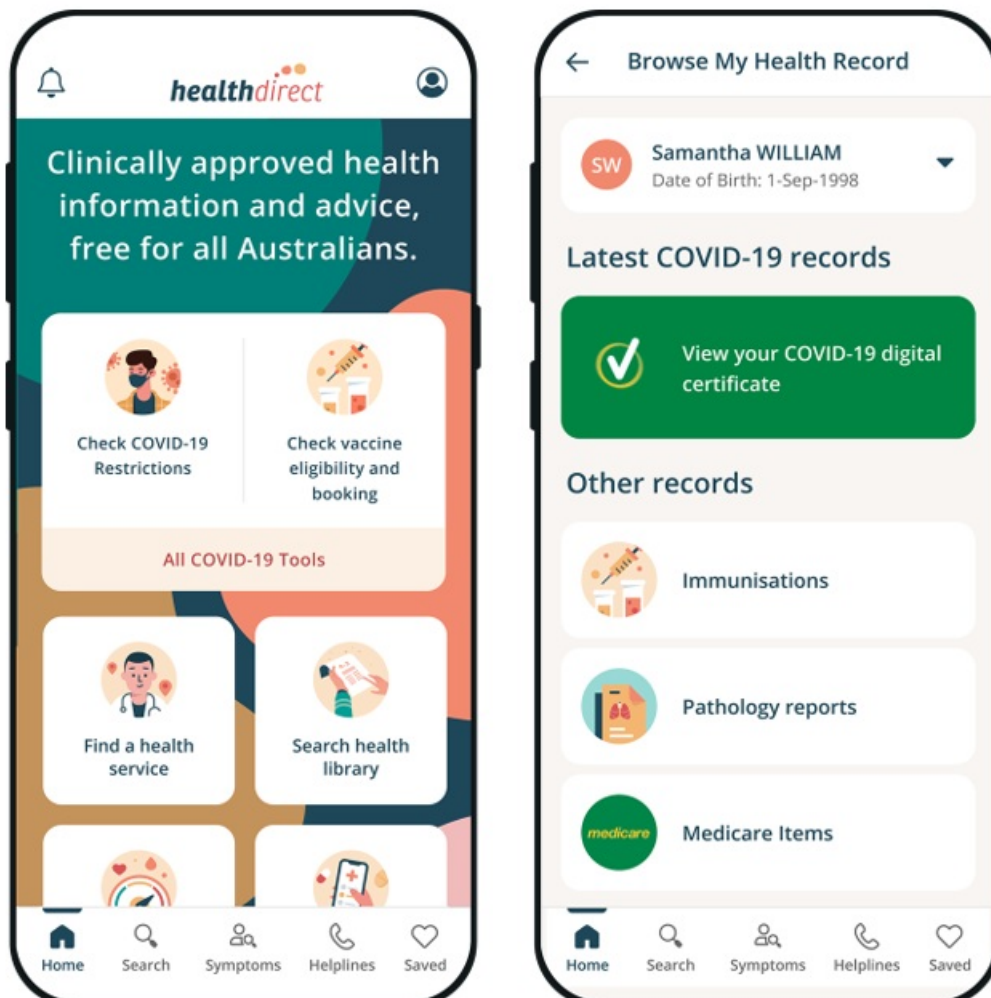

Contents


- 1 Real Time Device Monitoring App
- 2 Documents / Resources
 - 2.1 References
- 3 Related Posts

Real Time Device Monitoring App


Patient guide: Real-time device monitoring Connecting your monitoring device to your Video Call
Please note: the screenshots below are a guide and may differ slightly depending on your device or screen orientation. If using a mobile phone, please ensure you are using a smartphone for your consultation.

1. Turn on Bluetooth and your monitoring device and do a Pre-call check, to check that the device can connect to your Video Call before your appointment day:


<https://pmcheck.videocall.org.au/>

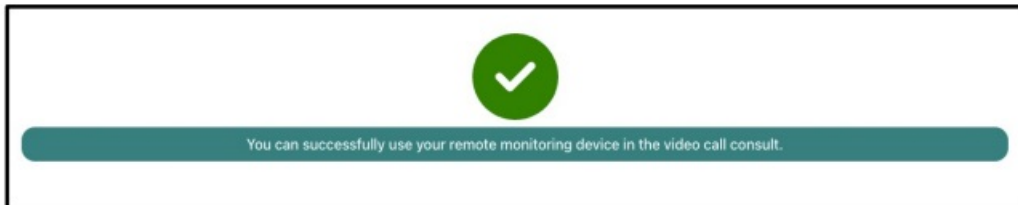


2. On appointment day, ensure Bluetooth is turned on and start the Video Call using the link provided by your healthcare provider. Ensure the monitoring device is nearby.
3. When your clinician joins, you will be given instructions to turn on and pair your monitoring device via Bluetooth.
4. When you see the green button on the screen to connect to your monitoring device, click on Click here to connect to your device.

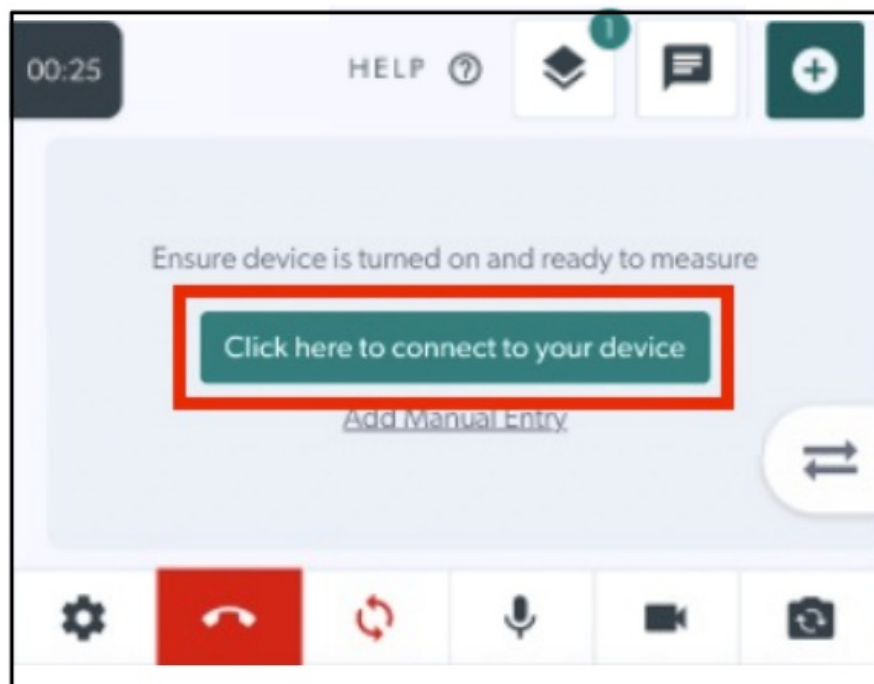


5. A pop-up will appear with the name of the monitoring device available to pair. Select your device and click on Pair.

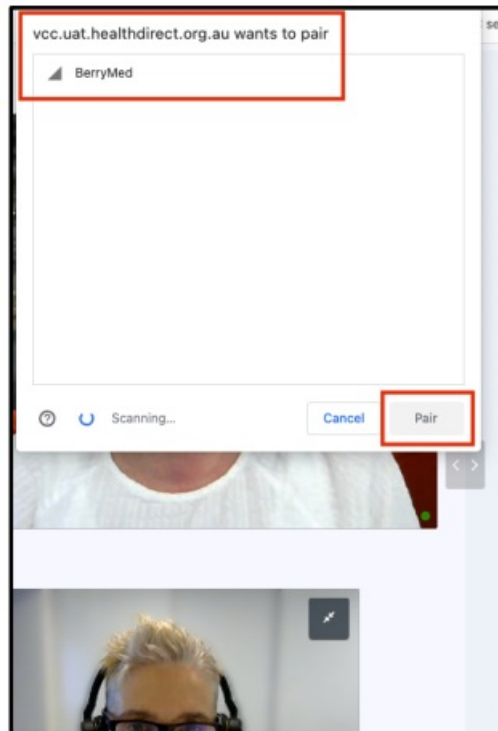

6. Your readings should now display on the screen. These may take a moment to appear.

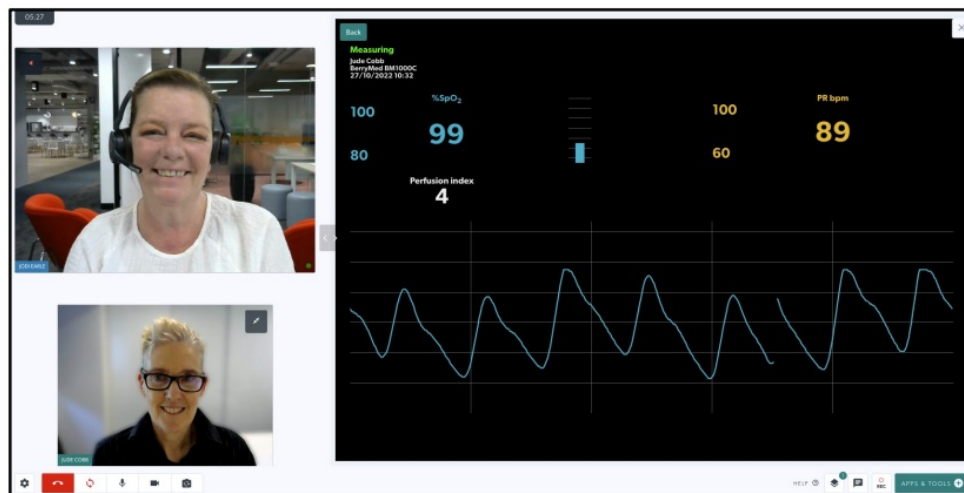


7. If your readings do not appear, your doctor may ask you to select Add Manual Entry instead.

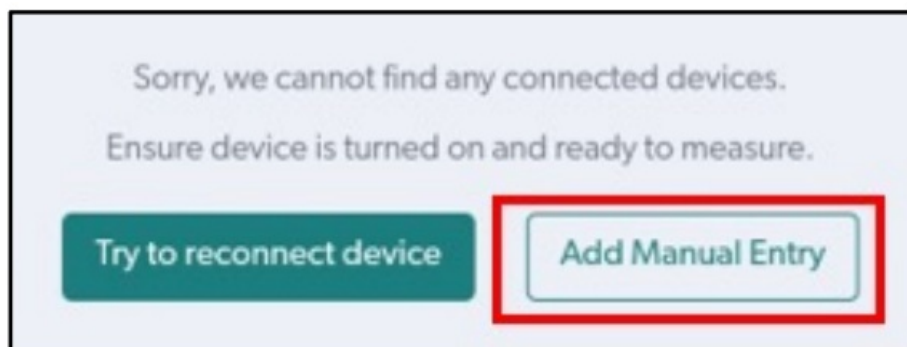

8. To manually enter your results, type the readings displayed on your monitoring device into the fields shown below. Click on Confirm Results to send them to your clinician.

Back Thursday 11:29am 13/10/2022



Please enter the results below for SpO2 and PR bpm reading on your pulse oximeter

SpO2
%

PR bpm
❤️/min

CONFIRM RESULTS

9. You will see a notification at the top of your screen, confirming the results were successfully sent to your clinician.

Your results were sent to the clinician



<https://help.vcc.healthdirect.org.au/remote-patient-monitoring>


Use this link: help.vcc.healthdirect.org.au/remote-patient-monitoring or scan the QR code for more information, including how to use the Wobbled browser for iOS and the patient support video UNOFFICIAL



For iPhones and iPads please download and use the Wobbled browser for your health direct Video Call:

<https://apps.apple.com/au/app/webble/id1193531073>

Documents / Resources



[healthdirect Real Time Device Monitoring App](#) [pdf] Owner's Manual
Real Time Device Monitoring App, Device Monitoring App, Monitoring App

References

- [Real-time remote physiological monitoring - Healthdirect Australia](#)
- [Patient Monitoring Device Check](#)