



HOVERTECH Q2Roller Lateral Turning Device User Manual

[Home](#) » [HOVERTECH](#) » HOVERTECH Q2Roller Lateral Turning Device User Manual 



Q2Roller Lateral Turning Device User Manual



Contents

[1 Intended Use and Precautions](#)

[2 PRECAUTIONS – HOVERTECH INTERNATIONAL AIR SUPPLY](#)

[3 Air Supply Keypad Functions](#)

[4 Instructions for Use](#)

[5 Product Specifications](#)

[6 Cleaning & Maintenance](#)

[7 Returns and Repairs](#)

[8 HoverTech Symbols](#)

[9 Documents / Resources](#)

[9.1 References](#)

[10 Related Posts](#)

Intended Use and Precautions

INDICATIONS FOR USE

Patients who are unable to turn or laterally position themselves

CONTRAINDICATIONS

Patients who are experiencing thoracic, cervical or lumbar fractures that are deemed unstable

INTENDED CARE SETTINGS

Hospitals, long-term or extended care facilities


PRECAUTIONS

- Ensure the Q2Roller meets the patient's needs before using it.
- Always use a minimum of two caregivers when operating the Q2Roller.
- Ensure valves are not in contact with the patient while on the Q2Roller.
- Product should only be used by trained personnel.
- Only use attachments and/or accessories that are authorized by HoverTech International.
- Use of this device with products or accessories not authorized by HoverTech International could result in injury or equipment malfunction and may void the Manufacturer's Warranty. HoverTech International will not be held responsible for any injuries or damages caused due to the improper use of this device.
- Use the Q2Roller according to instructions.
- Only for use with the HT-Air air supply adjustable button.
- Make sure patient is centered on the Q2Roller before inflating. Reference Center Line Indicator on the Q2Roller.
- Caregivers must ensure patient is attended and stabilized during 2Roller inflation, deflation or when inflated at angles greater than 30 degrees.
- Do not launder.
- Reference product-specific user manuals for additional operating instructions.


PRECAUTIONS – HOVERTECH INTERNATIONAL AIR SUPPLY

- Route the power cord in a manner to ensure freedom from hazard.
- Avoid blocking the air intakes of the air supply.
- Use this product only for its intended purpose as described in this manual.
- **CAUTION:** Avoid electric shock. Do not open air supply.

Part Identification – Q2Roller

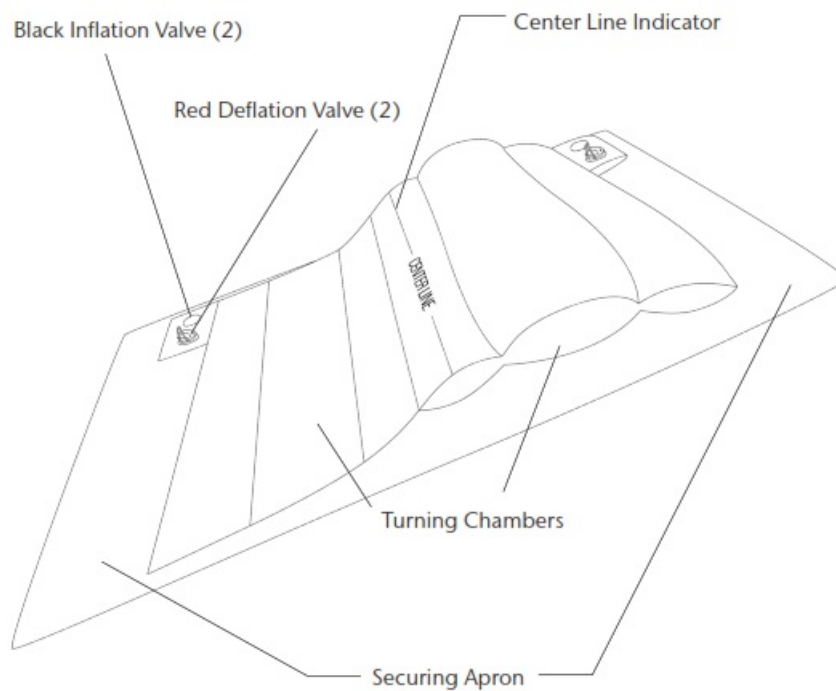

Part Identification – Air Supply

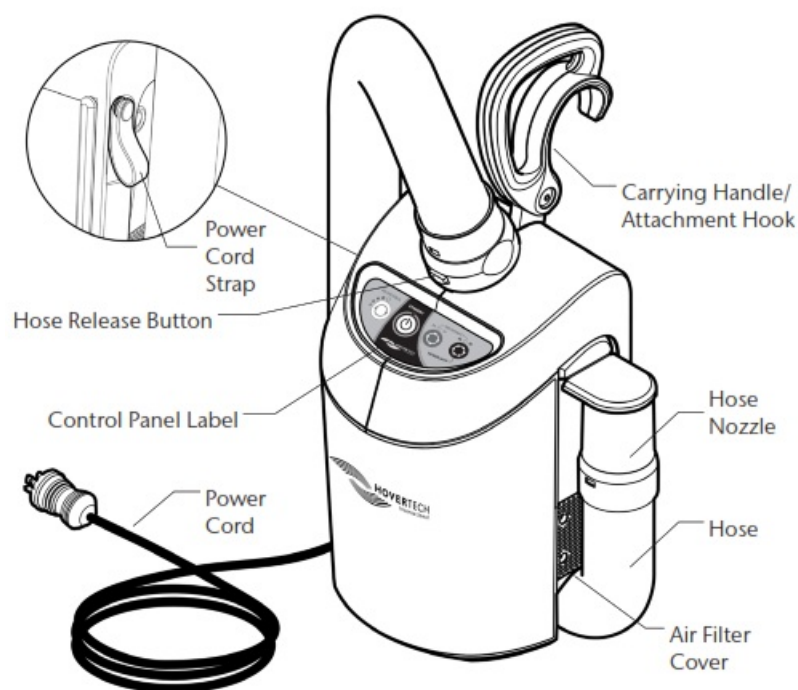


WARNING: The HT-Air is not compatible with DC power supplies. The HT-Air is not intended for use with the HoverJack Battery Cart.

CAUTION: NO USER-SERVICEABLE PARTS.

Only qualified service personnel shall perform repairs on the HoverTech International Air Supply.

Air Supply Keypad Functions

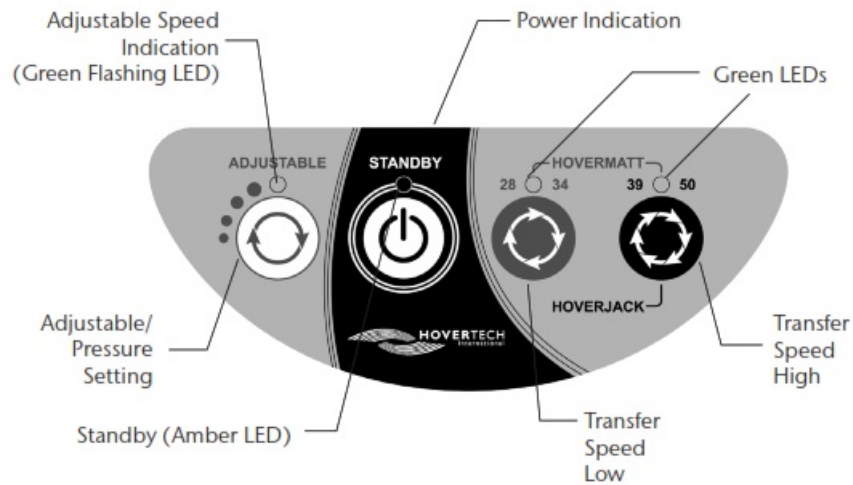

The **ADJUSTABLE** keypad function has four different settings. Each press of the button increases the air pressure and rate of inflation. The Green Flashing LED will indicate the inflation speed by the number of flashes (i.e. two flashes equals the second inflation speed).



STANDBY: Used to stop inflation/air flow (Amber LED indicates STANDBY mode).

Instructions for Use

1. Ensure the red deflation valves are capped tightly before beginning inflation.
2. Place the Q2Roller on the bed mattress, and center using the Center Line Indicator.
3. Tuck the securing apron of the Q2Roller under the bed mattress to keep it in place during use.
4. Remove the backing from the adhesive strips on the Q2R Pad, and center it on top of the Q2Roller (if the patient is already on the mattress, place the device and pad under the patient using a log-rolling technique).
5. With the patient-centered on the device, ensure all bed/stretchers rails are up, or follow your facility's protocol.
6. Locate the inflation valve on the **OPPOSITE** side of the turn direction, and place the air supply hose over the valve. Press the **ADJUSTABLE** button on the HT-Air keypad to initiate airflow. If necessary, press this button up to 3 more times to increase airflow and rate of inflation.
7. When the turn is complete, remove the hose from the valve and press the **STANDBY** button on the air supply keypad to stop airflow. Chamber may not need to be fully inflated to achieve desired position.
8. To quickly deflate the Q2Roller, remove the red cap from the deflation valve. To slowly deflate or adjust the chamber, depress the center of the black inflation valve.

Product Specifications

Q2ROLLER® LATERAL TURNING DEVICE

Material:	Polyurethane
Construction:	RF Welded
Width:	Chambers: 46.5" (118 cm) (combined chamber width) Apron: 72" (183cm)
Length:	Chambers: 44.5" (113 cm) Apron: 44" (112 cm)

LATEX FREE

Model #: HTR-200

Patient Weight Limit: 600 lbs. (272 kg)

Single-Patient Use

Q2R® PAD

Material:	Non-Woven, Breathable PE
Construction:	Thermal Bonding
Width:	39" (99 cm)
Length:	39" (99 cm)

Model #: HTR-CHX-5PACK (5 ea.)

Model #: HTR-CHX-CASE (50 ea.)

REQUIRED ACCESSORY:

Model #: HTAIR1200 (North American Version) – 120V~, 60 Hz, 10A

Model #: HTAIR2300 (European Version) – 230V~, 50 Hz, 6A

Model #: HTAIR1000 (Japanese Version) – 100V~, 50/60 Hz, 12.5A

Model #: HTAIR2356 (Korean Version) – 230V~, 50/60 Hz, 6A

Cleaning & Maintenance

CLEANING

The Q2Roller is a single-patient use device. If the device becomes soiled, completely wipe it down using a germicidal cleaner (phenolic disinfectant, quaternary solution or another intermediate level disinfectant according to facility procedure) to disinfect. For best results, follow the cleaner manufacturer's recommended dwell time and instructions for use. Apply germicidal cleaner directly into hard-to-reach areas. Let air dry. Do not launder.

INFECTION CONTROL

The Q2R Pad is recommended to cover the Q2Roller to keep the device from getting soiled (also available for separate purchase). Other materials, such as pads or linens, may also be placed on top of the Q2Roller to keep it clean.

If the Q2Roller is used on an isolation patient, the hospital should employ the same protocols/procedures it utilizes for the bed mattress and/or for the linen in that patient room.

AIR SUPPLY CLEANING AND MAINTENANCE

See air supply manual for reference.

NOTE: CHECK YOUR LOCAL/STATE/FEDERAL/INTERNATIONAL GUIDELINES BEFORE DISPOSAL.

PREVENTIVE MAINTENANCE

Prior to use, a visual inspection should be performed on the Q2Roller to ensure that there is no visible damage that would render the Q2Roller unusable. The Q2Roller should be periodically inspected to ensure the following:

- All inflation valves are self-sealing with no evidence of leakage
- There are no punctures or tears in the Q2Roller

If any damage is found that would cause the Q2Roller not to function as intended, the Q2Roller should be discarded.

Returns and Repairs

All products being returned to HoverTech International (HTI) must have a Return Goods Authorization (RGA) number issued by the company. Please call 800-471-2776 and ask for a member of the RGA Team, who will issue you an RGA number. Any product returned without an RGA number will cause a delay in the repair time.

Returned products should be sent to:

















HoverTech International

4482 Innovation Way
 Allentown, PA 18109
 Attn: RGA # _____
 Phone: 800-471-2776
 Fax: 610-694-9601

For European companies, send returned products to:

Attn: RGA # _____
 Kista Science Tower
 SE-164 51 Kista, Sweden
www.Etac.com
OrderExport@Etac.com

HoverTech Symbols



 CE MARKING OF CONFORMITY	 SINGLE PATIENT
 CAUTION	 ELECTRICAL AN
 OPERATING INSTRUCTIONS	 UNIQUE DEVIC
 MEDICAL DEVICE	 KEEP DRY
 HUMIDITY LIMITATION	 TEMPERATURE LIM
 AUTHORIZED REPRESENTATIVE	 MANUFACTURE
 SERIAL NUMBER	 LOT NUMBER
 HoverTech International 4482 Innovation Way Allentown, PA 18109 www.HoverMatt.com Info@hovermatt.com These products comply with the standards applicable for Class 1 products in the Medical Device Regulation (EU) 2017/745 on medical devices. ManualSymbols, Rev. A Date Revised: 5/20/21	
 CEpartner4U , NETHERLANDS. www.cepartner4u.com In case an adverse ever reported to our authorized represen information to the manu www.HoverMatt.com	



4482 Innovation Way
 Allentown, PA 18109
 800.471.2776
 Fax 610.694.9601
www.HoverMatt.com
Info@HoverMatt.com

Visit www.HoverMatt.com for other languages

Documents / Resources

	<p>HOVERTECH Q2Roller Lateral Turning Device [pdf] User Manual Q2Roller, Lateral Turning Device, Q2Roller Lateral Turning Device</p>
	<p>HOVERTECH Q2Roller Lateral Turning Device [pdf] User Manual Q2Roller Lateral Turning Device, Q2Roller, Lateral Turning Device, Lateral Device, Turning Device</p>

References

-  [Medical Device CE marking - CEpartner4U](#)
-  [Etac - A world-leading developer of assistive devices](#)