



ibidi Clamp for Sticky Slides Instructions

[Home](#) » [ibidi](#) » ibidi Clamp for Sticky Slides Instructions 

ibidi Clamp for Sticky Slides Instructions




Contents

- [1 Introductions](#)
- [2 Material](#)
- [3 Specifications](#)
- [4 Handling of the Clamp for sticky-Slides](#)
- [5 Ordering Information](#)
- [6 Documents / Resources](#)
 - [6.1 References](#)
- [7 Related Posts](#)

Introductions

The Clamp for sticky-Slides is an instrument to support the assembling of the ibidi stickySlides with a bottom material. The assembled sticky-Slide is inserted into an adapter, which is then compressed between the brackets of the Clamp for sticky-Slides. The applied force is homogeneous on the overall area, to guarantee an optimal adhesive bond between the sticky-Slide and the substrate (e.g. glass coverslip).

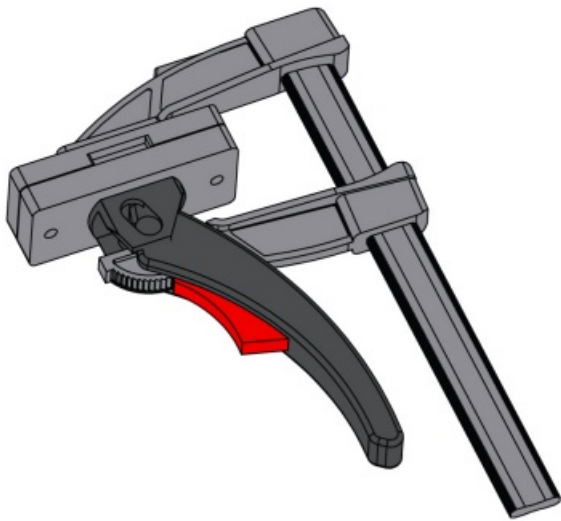

Material

The materials of the Clamp for sticky-Slides and the adapters are anodized aluminum and plastic. There are magnets integrated in both parts of the adapters to keep the two parts together.

The Clamp for sticky-Slides and the adapters are not autoclavable since they are temperature stable up to 60°C/140°F only. For sterilization we recommend cleaning all surfaces with an ethanol-soaked tissue.

Specifications

The Clamp for sticky-Slides is available with adapters for several types of sticky-Slides. For detailed information about the handling of the sticky-Slides please refer to the sticky-Slide instructions.

Specifications

Clamping force: 1.2 kN

Material: Anodized aluminium, plastic

Sterilization: Ethanol

Available adapters

sticky-Slide 8 Well / 18 Well

sticky-Slide I Luer

sticky-Slide VI 0.4

sticky-Slide Chemotaxis

Dimensions of Compatible Coverslip


Width: 75 mm

Length: 25 mm

Thickness: 0.1-1.0 mm


Handling of the Clamp for sticky-Slides

The working principle and the order of insertion of the parts of the Clamp for sticky-Slides is shown in the following picture:

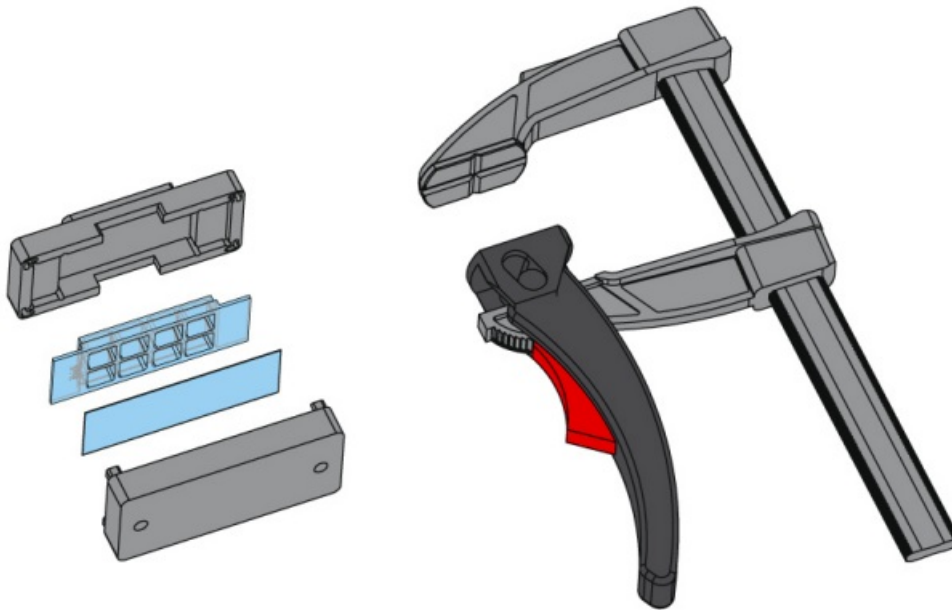


For optimal results please follow the proceeding of the protocol below:


1. Take the desired sticky-Slide out of the packaging and remove the protection film of the adhesive surface.
2. Bring the coverslip in position and glue it to the lower side of the sticky-Slide.

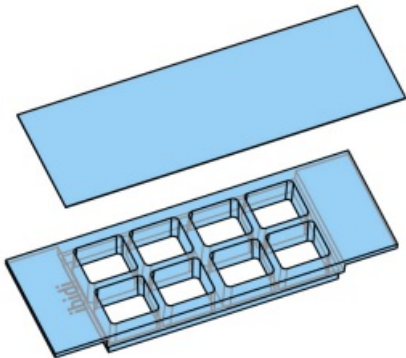

3. Put the assembled sticky-Slide in the adapter.

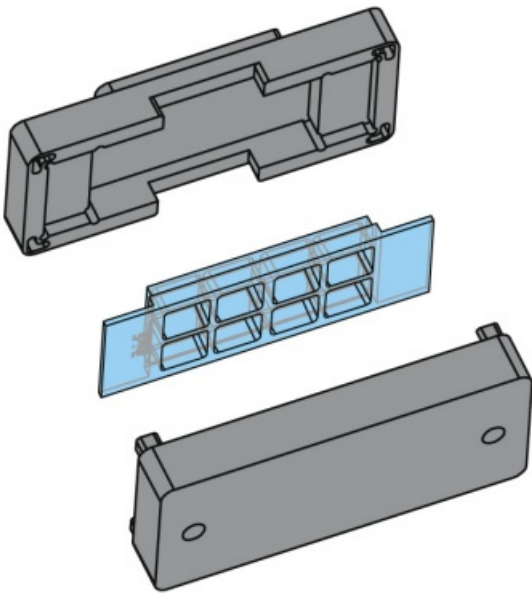


4. Mount the adapter onto the upper bracket of the clamp.

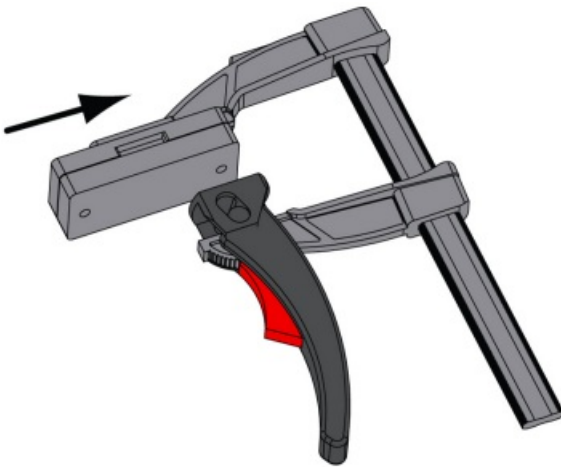

5. Move the lower bracket upwards until it pushes against the adapter. Make sure the lever is opened all the way.


6. Pull the lever to apply pressure on the adapter.

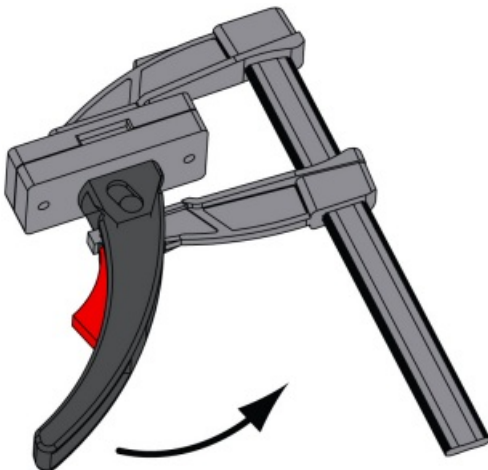


Warnings:

- Always handle with care, because the glass coverslip might break during the procedure!
- Please take care not to trap your hand or fingers between the brackets!

7. Keep the sticky-Slide pressed for approximately 1 min.

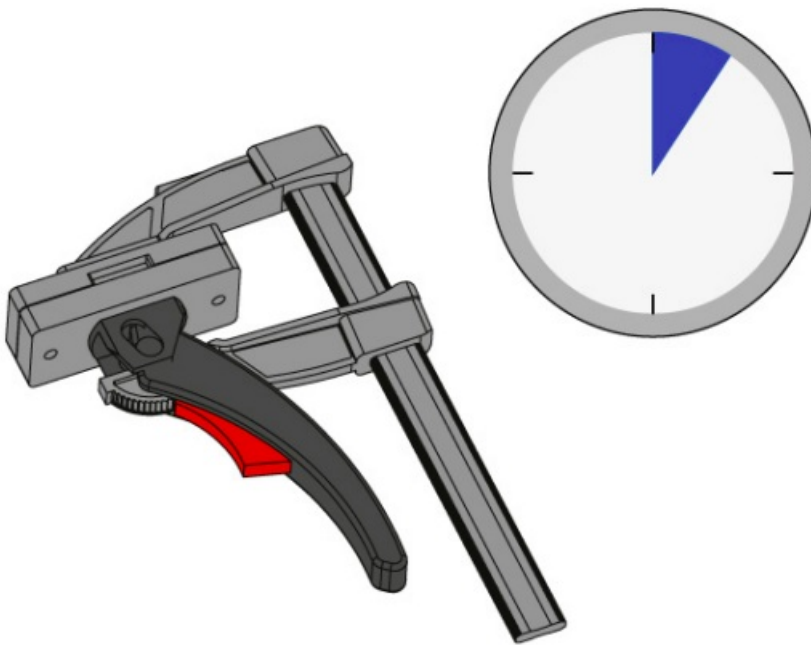

8. Open the clamp by pressing the red button and releasing the lever.

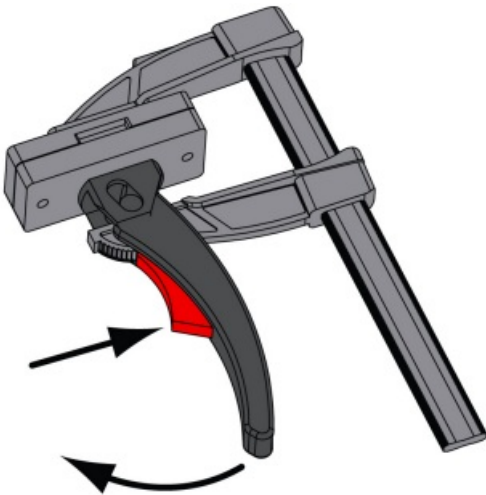

9. Remove the adapter from the clamp.

10. Open the adapter and remove the sticky-Slide.

11. For best results, incubate the finished sticky-Slide for 8 hours at 37°C in a dry or humid incubator.

Ordering Information

The Clamp for sticky-Slides is available with adapters for several types of sticky-Slides.

Cat. No. Description

80040 Clamp for sticky-Slides

80042 Adapter for sticky-Slide I Luer

80043 Adapter for sticky-Slide VI 0.4

80044 Adapter for sticky-Slide Chemotaxis

80045 Adapter for sticky-Slide 8 Well / 18 Well

For research use only!


Further information can be found at www.ibidi.com.

For questions and suggestions please contact us by e mail info@ibidi.de or by telephone +49 (0)89/520 4617 0.

© ibidi GmbH, Lochhamer Schlag 11, 82166 Grafelfing, Germany



Documents / Resources

	<p>ibidi Clamp for Sticky Slides [pdf] Instructions Clamp for Sticky Slides, Clamp, for Sticky Slides, Sticky Slides</p>
---	--

References

- [ibidi – cells in focus](#)
- [ibidi – cells in focus](#)
- [sticky-Slides](#)