



Image Engineering iQ-Defocus User Manual

[Home](#) » [Image Engineering](#) » Image Engineering iQ-Defocus User Manual 

Contents

- [1 Image Engineering iQ-Defocus](#)
- [2 INTRODUCTION](#)
- [3 GETTING STARTED](#)
- [4 OPERATING INSTRUCTIONS](#)
- [HARDWARE](#)
- [5 TECHNICAL DATA SHEET](#)
- [6 Documents / Resources](#)
 - [6.1 References](#)
- [7 Related Posts](#)



Image Engineering iQ-Defocus



INTRODUCTION

Important information: Read the manual carefully before using this device. Inappropriate utilization may cause damage to the device, to the DUT (device under test), and/or other components of your setup. Keep these instructions in a safe place and pass them on to any future user.

Conformity

We, Image Engineering GmbH & Co. KG, hereby declare that the iQ-Defocus corresponds to the essential requirements of the following EC directive:

- Electromagnetic Compatibility – 2014/30/EU

Intended use

iQ-Defocus is used to defocus the automatic focusing system of a camera with high temporal accuracy. A typical use of iQ-Defocus is to measure the camera release time in conjunction with the LED-Panel.

- Only suitable for indoor use.

Foreseeable misuse

Connect only to LED-Panel and DTS

iQ-Defocus can only be connected to LED-Panel and DTS. Usage with unsupported devices will cause irreversible damage to the iQ-Defocus.

General safety information

Do not open the device without instructions from the Image Engineering support team or when connected to a power supply.

GETTING STARTED

Scope of delivery

- iQ-Defocus
- 7.5 m extension cable for iQ-Trigger-T (6.3 mm TRS connector)

Commissioning

The iQ-Defocus comes ready to use. Follow the steps in chapter 3 to set up the measurement environment.


OPERATING INSTRUCTIONS HARDWARE

Setup

The setup of the iQ-Defocus depends on the measurement periphery.

Using iQ-Defocus on an iQ-Mobilemount


The iQ-Defocus is designed for seamless integration into the measurement workflow with the iQ-Mobilemount.

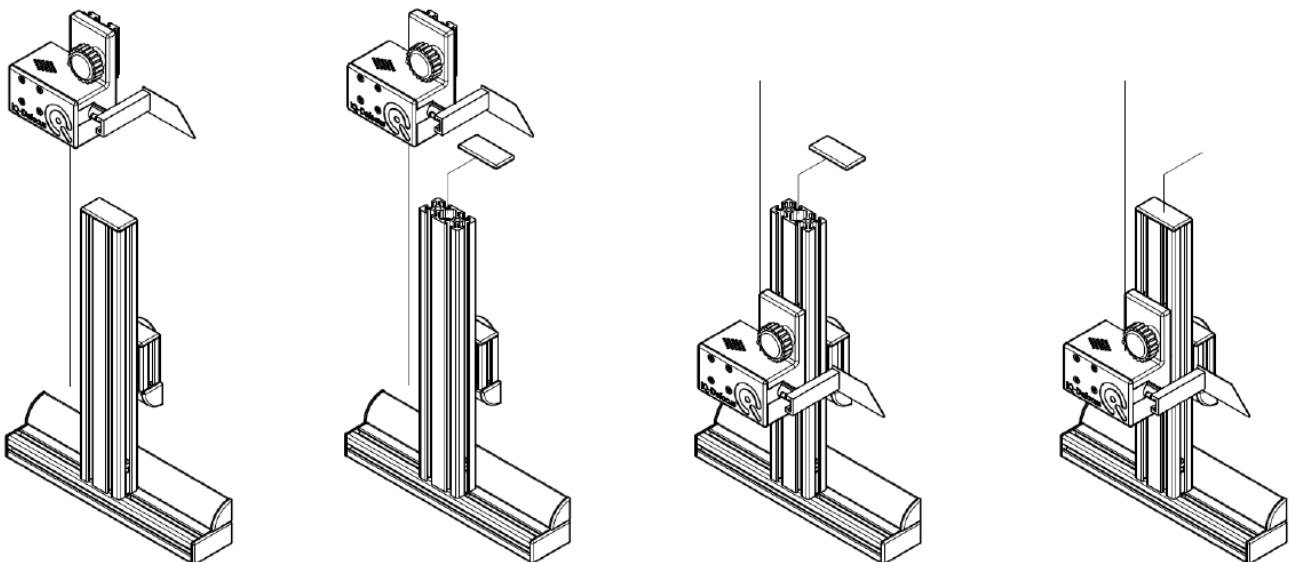

To attach the iQ-Defocus to the iQ-Mobilemount:


- Remove the top cover of the iQ-Mobilemount (use a thin screwdriver as a lever)
- Make sure the tightening hand screw of the iQ-Defocus is loose
- Slide the iQ-Defocus into the grooves of the iQ-Mobilemount, as shown in Figure 1
- Place the cover back on the iQ-Mobilemount

Using iQ-Defocus on a third-party mount

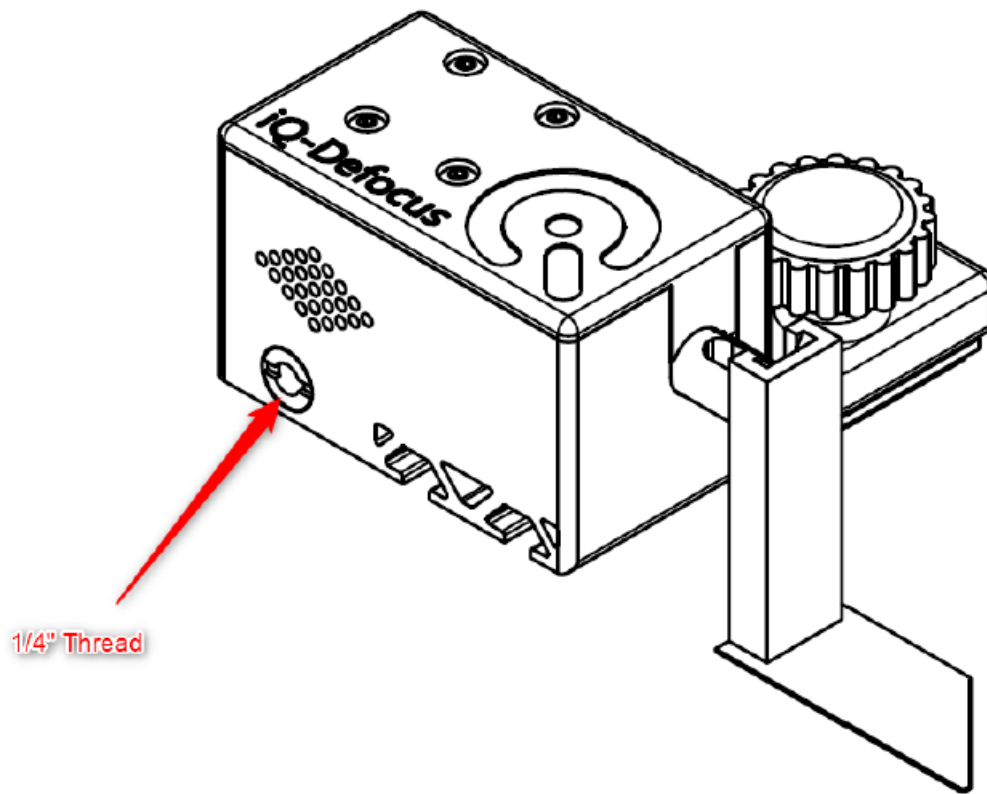

The iQ-Defocus can be attached to a tripod using the 1/4" thread on the bottom of the device. We recommend using a boom stand when the iQ-Defocus is not mounted to the iQ-Mobilemount.


Adjusting for lens depth

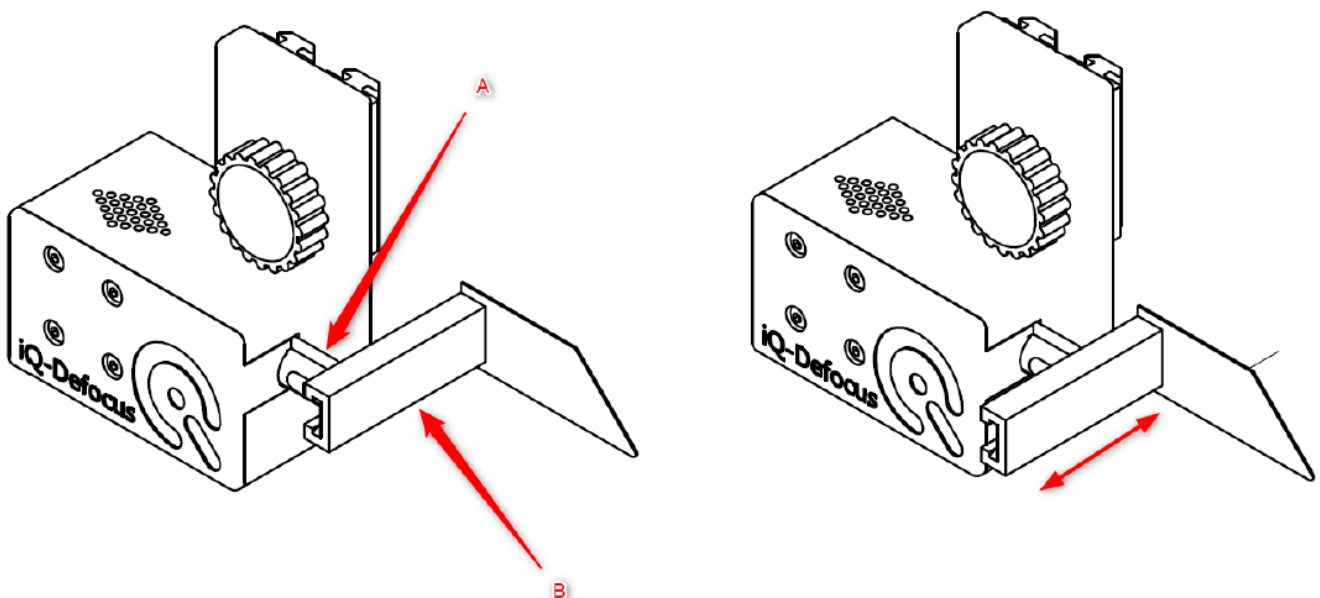

The iQ-Defocus shutter blade can be easily adjusted for different lens depths. Apply pressure to the clip (A) and slide the shutter blade adjustment profile (B) to the desired position.

Using iQ-Defocus with other IE measurement devices

LED-Panel (timing measurement)

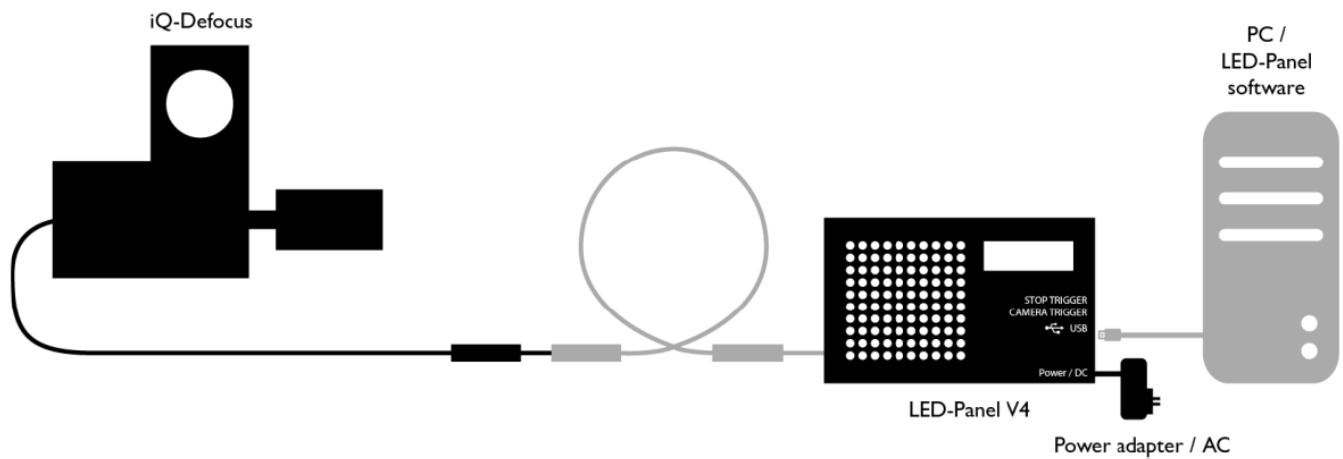

Mount iQ-Defocus in front of the device under test and connect the TRS connector (6.5 mm “jack plug”) to the LED-Panel (over an optional extension cable). Please refer to the LED-Panel manual for details on how to measure different timings (shutter lag, autofocus time, etc.) and how to interpret the captured images.

DTS (Dynamic Test Stand)

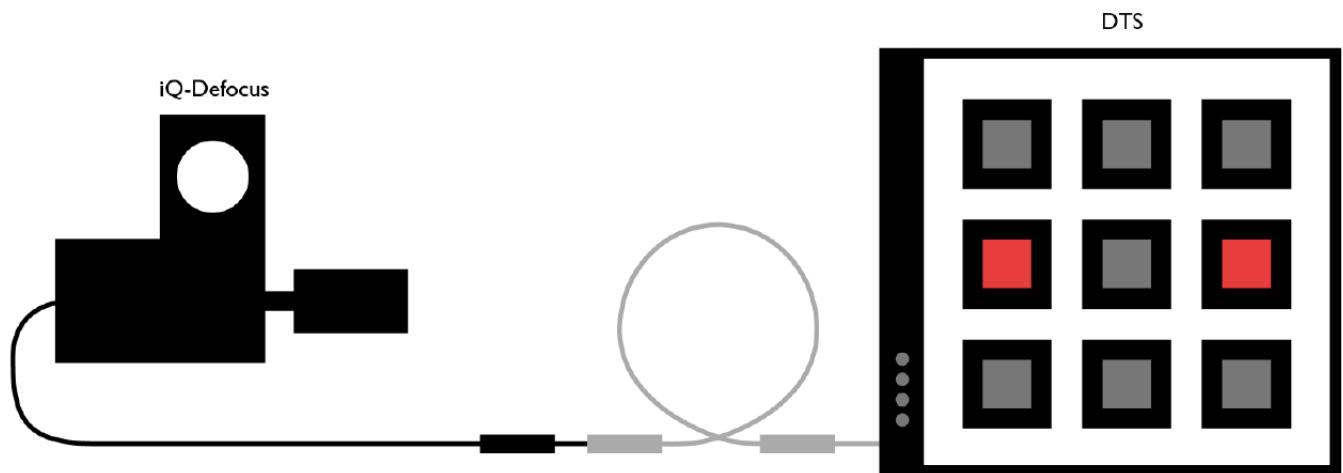


Figure 5 Connection scheme iQ-Defocus and LED-Panel

Mount iQ-Defocus on the device under test and connect the TRS connector (6.5 mm jack plug) to the DTS (over an optional extension cable). Please refer to the DTS manual for details on how to measure global flicker or modulated light mitigation probability.

Care instructions

- Always store the iQ-Defocus in the supplied case
- Avoid contact with water
- Do not use any chemical cleaning agents
- Use compressed air or a dust blower to remove dust

ADDITIONAL INFORMATION

Storage and transport

Ensure that the iQ-Defocus is fixed and the device is wrapped correctly for transport to avoid damage to the shutter blade. Unplug all cables/devices from iQ-Defocus before storage/transport.

Disposal instructions

After the service life of iQ-Defocus, it must be disposed of properly. Electrical and electromechanical components are included in iQ-Defocus. Observe your national regulations and ensure that third parties cannot use iQ-Defocus after disposing of it.


Contact Image Engineering if assistance for disposal is required.

TECHNICAL DATA SHEET

See annex for the technical data sheet. It can also be downloaded from the website of Image Engineering:

<https://image-engineering.de/support/downloads>

Documents / Resources

 <p>The image shows the cover of the 'iQ-Defocus User Manual'. At the top is the Image Engineering logo. Below it, the text 'iQ-Defocus' is displayed. Further down, it says 'User Manual' and 'March 15, 2019'. At the bottom, there is a small image of the iQ-Defocus device and some technical specifications.</p>	<p>Image Engineering iQ-Defocus [pdf] User Manual iQ-Defocus, Defocus</p>
---	---

References

- [Image Engineering - Solutions to test image Quality](#)
- [Downloads](#)