KEITHLEY 2601B Pulse System Source Meter





KEITHLEY 2601B Pulse System Source Meter User Guide

Home » KEITHLEY » KEITHLEY 2601B Pulse System Source Meter User Guide 1

Contents

- 1 KEITHLEY 2601B Pulse System Source Meter
- **2 Product Information**
- **3 Product Usage Instructions**
- **4 GENERAL INFORMATION**
- **5 SUPPORTED OPERATING SYSTEMS**
- **6 INSTALL ACS BASIC**
- 7 UPDATE PREVIOUS VERSIONS OF ACS BASIC FILES
- **8 SUPPORTED MODELS AND TEST**

CONFIGURATIONS

- 9 SUPPORTED COMMUNICATION INTERFACES
- **10 SOFTWARE LICENSE**
- 11 ACS BASIC VERSION 3.3
- **12 RESOLVED ISSUES**
- 13 SOFTWARE COMPATIBILITY
- **14 USAGE NOTES**
- 15 Documents / Resources
 - 15.1 References



KEITHLEY 2601B Pulse System Source Meter



Product Information

Specifications

• Product Name: ACS Basic Edition

Version: 3.3

• Release Date: November 2023

· Manufacturer: Keithley Instruments

• Operating System Compatibility: Refer to supported operating systems section

Product Usage Instructions

Install ACS Basic

- 1. Log in to your computer as an Administrator.
- 2. Open the ACS Basic executable file.
- 3. Follow the software installation instructions.
- 4. Select Yes if you have an older version of ACS Basic installed.
- 5. Follow the instructions to specify how you want to install the software on your system.
- 6. For backup or restore from a previous version, see Update previous versions of ACS Basic files.

Install ACS Basic on a 4200A-SCS Parameter Analyzer

If installing on a 4200A-SCS Parameter Analyzer, follow the specific dialog box instructions provided.

Update Previous Versions of ACS Basic Files

- 1. Go to C:ACS_BASICUpgradeTool.
- 2. Double-click UpgradeTool.exe.
- 3. Choose the items in the folder you want to update.
- 4. Select Copy to update the files.

Manually Copy Projects and Libraries

1. Copy and paste projects and libraries from the previous version by following the provided steps.

Frequently Asked Questions (FAQ)

Q: Can ACS Basic files before version 3.0 be converted using UpgradeTool.exe?

A: No, ACS Basic files before version 3.0 cannot be converted using UpgradeTool.exe.

• Q: What should I do if I have ACS Basic version 2.1.5 or later?

A: If you have ACS Basic version 2.1.5 or later, you must manually copy the projects and libraries following the provided steps.

ACS Basic Edition

Version 3.3 Release Notes

Keithley Instruments

28775 Aurora Road Cleveland, Ohio 44139 1-800-833-9200 tek.com/keithley

GENERAL INFORMATION

- This document describes the features added to the Keithley Instruments Automated Characterization Suite (ACS) Basic Edition software (version 3.3).
- The Keithley Instruments ACS Basic Edition software supports component characterization testing of packaged parts and wafer-level testing using a manual probe station. ACS Basic Edition software can be installed on any computer, including Keithley Instruments Model 4200A-SCS Parameter Analyzer, or Model 4200 Semiconductor Characterization System (4200-SCS).

SUPPORTED OPERATING SYSTEMS

ACS Basic Edition software is supported on the following operating systems:

- Microsoft® Windows® 11, 64-bit
- Microsoft Windows 10, 64-bit
- Microsoft Windows 10, 32-bit
- Microsoft Windows 7, 64-bit (with Service Pack 1)
- Microsoft Windows 7, 32-bit (with Service Pack 1)

ACS BASIC EDITION REVISION HISTORY


Version	Release date
3.3	November 2023
3.2.1	March 2023
3.2	November 2022
3.1	March 2022
3.0	August 2021
2.1.5	November 2017
2.1	November 2015
2.0	September 2012
1.3	July 2011
1.2	September 2010

INSTALL ACS BASIC

To install ACS software on a personal computer:

- 1. Log in to your computer as an Administrator.
- 2. Open the ACS Basic executable file.
- 3. Follow the software installation instructions.
- 4. Select Yes if you have an older version of ACS Basic installed, as shown in the following figure.

Figure 1: ACS Basic Software installation

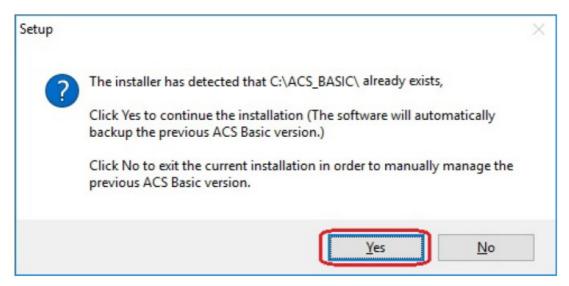

- 5. Follow the instructions to specify how you want to install the software on your system.
- 6. If you have projects you need to backup or restore from a previous version of ACS Basic, see Update previous versions of ACS Basic files.


Note

If you are installing ACS on a Model 4200A-SCS Parameter Analyzer, see the following information.

Install ACS Basic on a 4200A-SCS Parameter Analyzer

If you are installing ACS Basic on a 4200A-SCS Parameter Analyzer, the following dialog box displays indicating that the applications identified are needed for installation. Make sure you select Do not close applications and Next to install (see the following figure).

Figure 2: ACS Basic 3.3 prepare to install

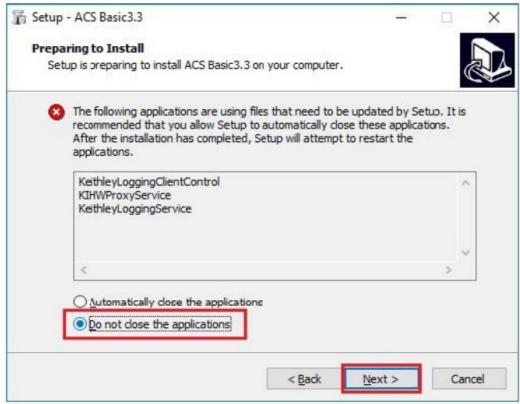

Note

If you are installing Clarius+ and ACS Basic on the same system, Clarius+ must be installed first.

UPDATE PREVIOUS VERSIONS OF ACS BASIC FILES


Note

Once ACS Basic is installed, you can use UpgradeTool.exe to convert your ACS Basic version 3.0 files or later to the present version, which includes projects, libraries, and settings from previous versions. ACS Basic files before version 3.0 cannot be converted using this method.

To update previous software files:

- 1. Go to C:\ACS_BASIC\UpgradeTool\.
- 2. Double-click UpgradeTool.exe.
- 3. Choose the items in the folder you want to update (see the following figure).

Figure 3: ACS Basic Upgrade Tool

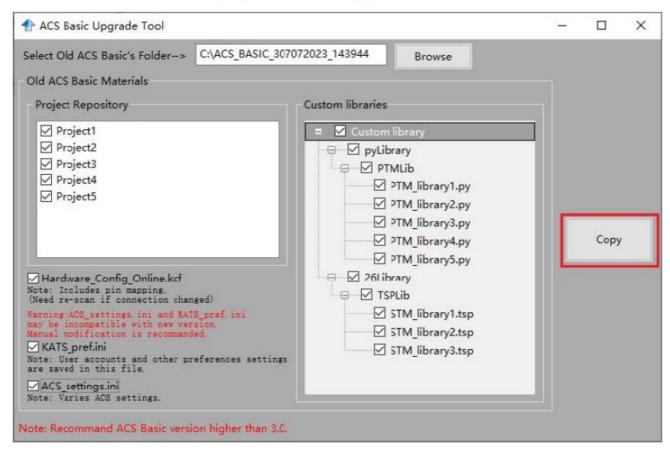

4. Select Copy.

When the updated version of ACS Basic is installed, the previous version is renamed. You can copy the projects and libraries from the previous version using the following steps.

Note

If you have ACS Basic version 2.1.5 or later, you must manually copy the projects and libraries by following the steps below.

To copy and paste folders:

- 1. Find the C:\ACS BASIC DDMMYYYY HHMMSS\Projects\ folder.
- 2. Copy and paste to the present C:\ACS_BASIC\Projects\ folder.
- Find the C:\ACS_BASIC_DDMMYYYY_HHMMSS\library\pyLibrary\PTMLib\ folder.
- 4. Copy and paste to the present C:\ACS_BASIC\library\pyLibrary\PTMLib\ folder.
- 5. Find the C:\ACS_BASIC_DDMMYYYY_HHMMSS\library\26library\ folder.
- 6. Copy and paste to the present C:\ACS_BASIC\library\26library\ folder.

Note

ACS Basic 3.3 is based on the Python 3.7 programming language. If you customized your projects in a previous version of ACS Basic you may need to change the projects created in the older version of ACS Basic, which includes the Python language test module (PTM) script libraries. You can go to this site to review the Python changes for more detail:


https://docs.python.org/3/whatsnew/3.7.html#porting-to-python-37

Install ACS Basic after installing NI-488.2 drivers

If you are installing ACS Basic on a system that contains NI-488.2 drivers, the following dialog box displays indicating that the applications identified are needed for installation. Make sure you select Do not close

applications and Next to install (see the following figure).

Figure 4: ACS Basic 3.3, Preparing to Install

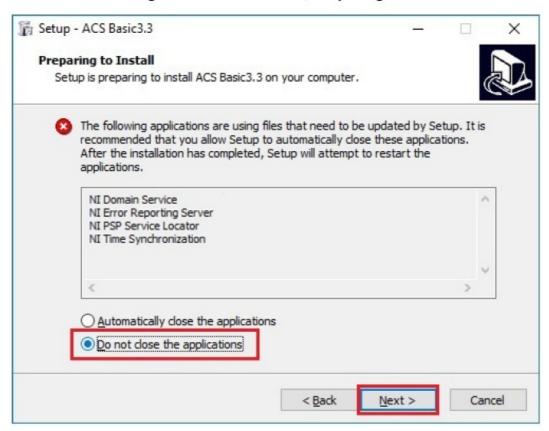

SUPPORTED MODELS AND TEST CONFIGURATIONS

- ACS Basic Edition software is used to characterize semiconductor devices with a variety of Keithley
 Instruments products in a variety of different configurations. The ACS Basic Reference Manual (part number
 ACSBASIC-901-01) contains detailed information about the supported hardware and test configurations.
- The following table summarizes the instruments supported in the ACS Basic test libraries.

Instrument type	Supported models
	2600B Series: 2601B, 2602B, 2604B, 2611B, 2612B, 2614B, 2634B, 2635B, 26 36B
	2600A Series: 2601A, 2602A ,2611A, 2612A, 2635A, 2636A
SMU Instruments	2400 Graphical Series SMU (KI24XX): 2450, 2460, 2460-NFP, 2460-NFP-RACK , 2460-RACK, 2461, 2461-SYS, 2470
	2400 Standard Series SMU: 2401, 2410, 2420, 2430, 2440
	2650 Series for High Power: 2651A, 2657A
Parameter Analyzers	4200A and supported cards/modules: 4210-CVU, 4215-CVU, 4225-PMU/4225-RPM, 4225-RPM-LR, 4200-SMU, 4201-SMU, 4210-SMU, 4211-SMU, 4200-PA, 4200A-CVIV
DMMs	DMM6500, DMM7510, 2010 Series
Ultra-sensitive Current Sourc es and Nanovoltmeter	6220,6221, 2182A
Switching and data acquisition systems	DAQ6510, 707A/B, 708A/B, 3700A
Pulse Generators	3400 Series

Note

- The graphical interactive test module (ITM) supports 24xx Graphical Series SMU instruments and 26xx instruments at the same time. The 24xx instrument should be connected as the primary instrument, and the 26xx connected as the subordinate.
- You can control any Test Script Processor (TSPTM) instrument using a script test module (STM) script.
- You can control any instrument using a Python language test module (PTM) script, including instrumentation from other vendors.
- Existing ACS Basic STM and PTM libraries support specific instruments based on the library definition.

SUPPORTED COMMUNICATION INTERFACES

- GPIB
- LAN (Auto Scan and LAN)
- USB
- RS-232

Note

If you are using an RS-232 connection, the instrument is not automatically added to the hardware configuration. Add instruments connected with RS-232 manually and change the hardware configuration file that is in the following directory on your computer to the following:

C:\ACS_BASIC\HardwareManagementTool\HWCFG_pref.ini. In this file you can change the baud rate, parity, byte, and stopBit settings. Review the following figure for details.


Figure 5: RS-232 connection



SOFTWARE LICENSE

ACS Basic allows you to create tests, manipulate settings, and view previous data without a license. However, you must have a license for ACS Basic in to control and retrieve data from a physical instrument. You can launch a one-time, 60-day trial for ACS Basic after the initial installation. Once the license expires, you need to purchase a full license to use the software.

Figure 6: ACS Basic 3.3 license information

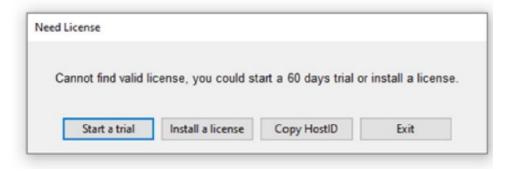


LICENSE MANAGEMENT

The ACS Basic software license is managed using the Tektronix Asset Management System (TekAMS). **To generate a license file:**

- 1. You must submit your Host ID to TekAMS. For more information on TekAMS, see <a href="tek.com/products/produc
- 3. Select Install.

Figure 7: ACS Basic Host ID 3.3 license information

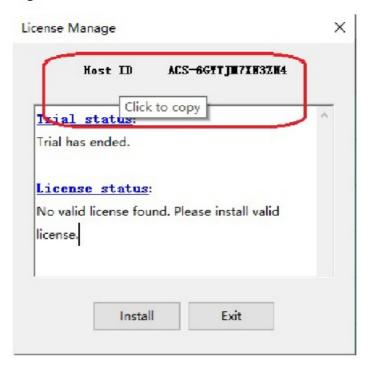

ACS BASIC VERSION 3.3

ENHANCEMENTS

Hardware configuration	
Issue number:	ACS-784, CAS-209266-Y5K4F1
Enhancement:	Support for the Keysight E4980A added.
Issue number:	ACS-716
Enhancement:	Support for TSP-Link connections to the DMM6500 and DMM7510.
	ACS-677
	Add Hardware Scan Tool support scanning for:
Issue number: E nhancement:	6221 through GPIB and ethernet
Timanoomonia	6220 through GPIB
	2182 and 2182A through RS232 or Trigger Link cable to the 6220 or 6221

ACS Basic software and libraries	
Issue number:	ACS-766, CAS-199477-J6M6T8
Enhancement:	Switching speed when switching between PTMs and ITMs has been optimized.
Issue number:	ACS-762
Enhancement:	Support added for saving data to the Excel® format, .xlsx.
Issue number: E	ACS-724
nhancement:	Shared-Stress App: Added an example library and project to show how to use the built-in shared stress functions.
Issue number: E	ACS-718
nhancement:	DMM7510 and DMM6500 support: Added TSP library DMM_SMU_lib.tsp including the functions FIMV_Sweep and FIMV_Sample.
Issue number:	ACS-717
Enhancement:	2601B and DMM7510 support: Added LIV_Lib.tsp library.
Issue number:	ACS-713, ACS-712
Enhancement:	Added test library VTH_SiC under device PowerMosfet for ACS Basic.
Issue number:	ACS-690, ACS-689
Enhancement:	Added the standard PTM KI622x_2182_Lib.py library to support delta and differential measur ements using the Keithley Instruments Model 6220 or 6221 used with a Model 2182A.
Issue number:	ACS-681, ACS-680, ACS-679
Enhancement:	Added Shared-Stress App: Added python library Share_Stress_App.py and shared_Stress_Demo.py.
Issue number:	ACS-676
Enhancement:	Add a PTM demo script to run a UTM library remotely on the 4200A-SCS through KXCI.
Issue number:	ACS-664, CAS-143278-Z7L7T3
Enhancement:	Added support for generalized Shared-Stress testing.
Issue number:	ACS-653, CAS-124875-V3W1G7
Enhancement:	UpgradeTool.exe was added to help convert your ACS 6.0 files or later to the present version , including projects, libraries, and settings from previous versions.

ACS Basic manual updates	
Issue number:	ACS-757, ACS-744, ACS-743, ACS-733, ACS-711
Enhancement:	Automated Characterization Suite (ACS) Basic Software Reference Manual update.
Issue number:	ACS-790, ACS-785, ACS-719, ACS-715, ACS-714, ACS-711
Enhancement:	Automated Characterization Suite (ACS) Basic Edition Libraries Reference Manual update.
Issue number:	ACS-711
Enhancement:	ACS Basic Software Quick Start Guide update.

RESOLVED ISSUES

Issue number:	ACS-763, CAS-198461-L5X8W7
Enhancement: Resolution:	When ACS Formulator formula VTCI returns #REF, the data cannot be saved to an .xls file. T his issue has been corrected.
	ACS-758
Issue number: E nhancement: R esolution:	ITM 2461 Pulse mode incorrectly reached compliance at current lower than the limiti setting.
	This issue has been corrected.

Issue number:	ACS-755
Enhancement: Resolution:	Formulator from the last device-level running file is copied to all ITMs. This issue has been co rrected.
Issue number:	ACS-753, CAS-191970-C6C2F3
Enhancement: Resolution:	ACS Basic graph problem: Fixed Scale applied incorrectly to Y2. This issue has been correct ed.
Issue number:	ACS-752, CAS-191977-V4N4T0
Enhancement: Resolution:	ACS Basic graph problem with Log Scale. This issue has been corrected.
Issue number:	ACS-751, CAS-191987-Q2T8Q5
Enhancement: Resolution:	ACS Basic graph scale format error (scientific linear). This issue has been corrected.
Issue number:	ACS-750, CAS-191988-X7C2L0
Enhancement: Resolution:	ACS Basic graph scale format error (scientific LOG). This issue has been corrected.


Issue number:	ACS-740
Enhancement: Resolution:	The 2450, DMM6500, and DAQ6510 report errors when starting ACS Basic. This issue has b een corrected.
Issue number:	ACS-737, CAS-183556-J8P1L6
Enhancement: Resolution:	Cannot enable High C mode in an ITM when connected to a Model 2657A. This issue has be en corrected.
Issue number:	ACS-732
Enhancement: Resolution:	Cannot enable High C mode in an ITM when connected to a Model 2657A. This issue has be en corrected.
Issue number:	ACS-706
Enhancement: Resolution:	sintgv() is missing in TSPLPT. This issue has been corrected.
Issue number: E	ACS-705
nhancement: Resolution:	The Combine SMU button is disabled in configure demo mode in the Hardware Management Tool. This issue has been corrected.
lagua numban F	ACS-704, CAS-168192-R6R9C0
Issue number: E nhancement: Resolution:	When measuring a CF sweep (from 10 kHz to 100 kHz) on a sample that has a capacitance value of about 100 pF, inaccurate data was shown at 10 kHz frequency. This issue has been corrected.
	ACS-699
Issue number: E nhancement: Resolution:	When a customer enters a pattern, subsite, or device name that starts with a number, the project is damaged. This issue has been corrected by displaying a message if the user tries to use a name that st arts with a number.
Issue number: Enhancement: Resolution:	ACS-695
	TSPLPT delcon command is not working correctly. This issue has been corrected.
Issue number: E nhancement: Resolution:	ACS-688
	ACS Basic cannot scan a Model 707B Switching System that contains a 7072B cards in the Hardware Management Tool. This issue has been corrected.

Issue number:	ACS-687, CAS-157136-K7R9R0
Enhancement: Resolution:	High Open Offset Capacitance issue on PCT HVCV Test. This issue has been corrected.
Issue number:	ACS-686
Enhancement: Resolution:	Added ACSLPT sweepX, bsweepX functions for 4200A SMU. This issue has been corrected.
Issue number:	ACS-685
Enhancement: Resolution:	Y1/Y2 min/max scale in the plot setting is automatically changed when running a test. This is sue has been corrected.

SOFTWARE COMPATIBILITY

	N/A
Issue number: R esolution:	When you start ACS Basic on a 4200A-SCS that has Clarius software version 1.4 or later (with the Windows 10 operating system), a warning message may appear indicating that KXCI did not start successfully. Select Cancel to dismiss the warning.


Figure 8: KXCI did not start

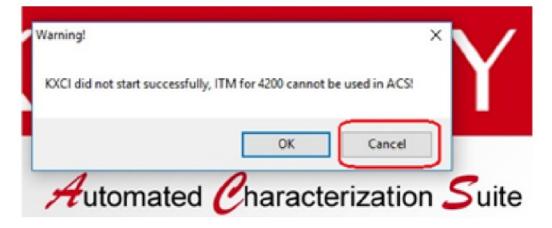

To manually configure the compatibility settings:

- 1. Right-click the ACS Basic icon and select Properties.
- 2. Open the Compatibility tab.
- 3. Select Run this program as an administrator and select OK to save.

Figure 9: ACS Basic properties

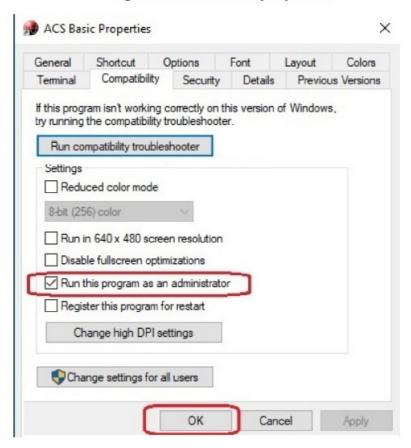

USAGE NOTES





Figure 10: ACS Basic command compatible

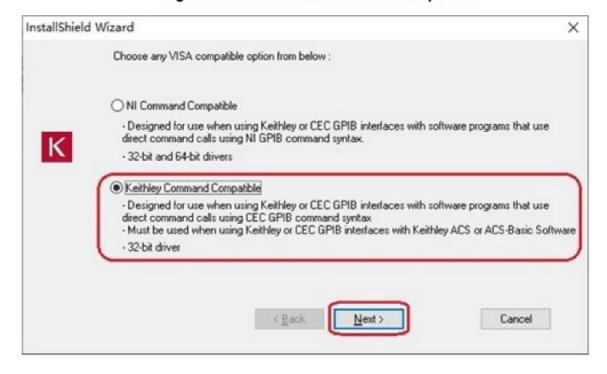

ACS-691, CAS-162126-B3Y7Y6

Microsoft® Windows® mapped network drive error.

When installing ACS Basic on a personal computer, Microsoft policy settings can limit ACS Basic from accessing mapped network drives in its file windows. Modifying the registry fixes this issue. *To modify the registry:*

Issue number : Resolution:

- 1. Run regedit.
- 2. Navigate to

HKEY_LOCAL_MACHINE/SOFTWARE/Microsoft/Windows/CurrentVersion/Policies/ System.

- 3. If one does not exist, create a new DWORD (32-bit) entry named EnableLinkedConnections.
- 4. Set the value to 1.
- 5. Restart the computer.

Documents / Resources



KEITHLEY 2601B Pulse System Source Meter [pdf] User Guide

2601B Pulse System Source Meter, 2601B, Pulse System Source Meter, System Source Meter, Source Meter

References

- W Keithley Instruments & Products | Tektronix
- Product License | Tektronix
- What's New In Python 3.7 Python 3.12.2 documentation
- User Manual

Manuals+, Privacy Policy

This website is an independent publication and is neither affiliated with nor endorsed by any of the trademark owners. The "Bluetooth®" word mark and logos are registered trademarks owned by Bluetooth SIG, Inc. The "Wi-Fi®" word mark and logos are registered trademarks owned by the Wi-Fi Alliance. Any use of these marks on this website does not imply any affiliation with or endorsement.