

# KLHA KM53B98 Wind Speed and Direction Integrated Sensor **User Manual**

Home » KLHA » KLHA KM53B98 Wind Speed and Direction Integrated Sensor User Manual





KM53B98 User Manual

http://www.klha.com/

File Version: V21.12.24



KM53B98 using the standard RS485 bus MODBUS-RTU protocol, easy access to PLCDCS and other instruments or systems for monitoring wind speed, conductivity, temperature, humidity state quantities. The internal use of high-precision sensing core and related devices to ensure high reliability and excellent long-term stability can be customized

RS232,RS485,CAN,4-20mA,DC0~5V10V,ZIGBEE,Lora,WIFI,GPRS and other output methods.


#### **Contents**

- **1 Technical Parameters**
- 2 Product Size
- **3 Communication Protocol** 
  - 3.1 Read Data (Function id 0x03)
  - 3.2 Data Address Table
- 4 Disclaimer
- **5 Contact Us**
- 6 Documents / Resources
  - **6.1 References**
- **7 Related Posts**

# **Technical Parameters**

| Technical parameter            | Parameter value |
|--------------------------------|-----------------|
| Brand                          | КНА             |
| Wind speed range               | 0-30m/s         |
| Start wind                     | 0.2m/s          |
| Wind speed accuracy            | ±3%             |
| Shell material                 | aluminum        |
| Wind direction range           | 0-360°          |
| Wind direction resolution      | 22.5°           |
| Temperature measuring range    | -30°C-80°C      |
| Temperature measuring accuracy | ± 0.5°C @25°C   |
| Humidity measuring range       | 0-100°/0RH      |
| Humidity accuracy              | ±3%RH @25°C     |
| Communication Interface        | RS485           |
| Default baud rate              | 9600 8 n 1      |
| Power                          | DC6-24V 1 A     |
| Running temperature            | -40-80°C        |
| Working humidity               | 5%RH-90%RH      |


# **Product Size**

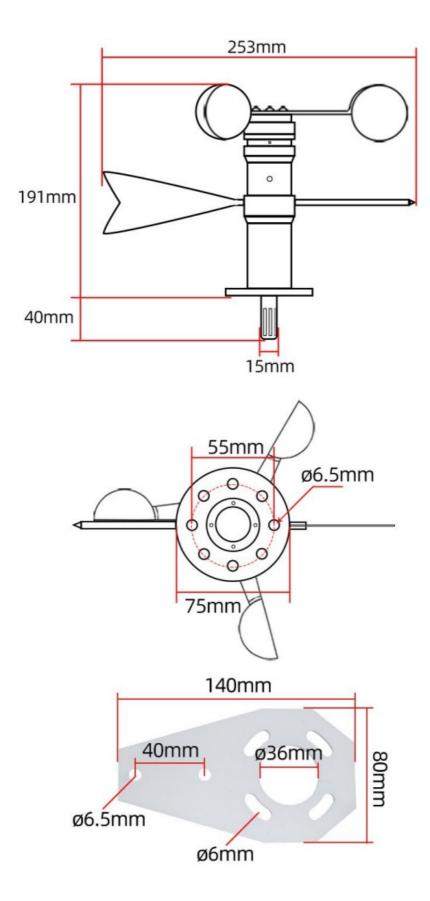


How to wiring?

# RS485 Wiring RD PWR+ GN PWR YE RS485 A+ BU RS485 B-

# **Application solution**

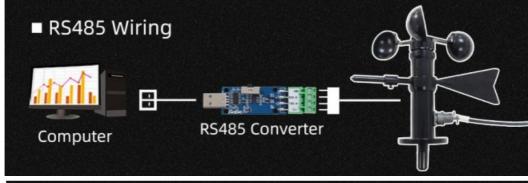

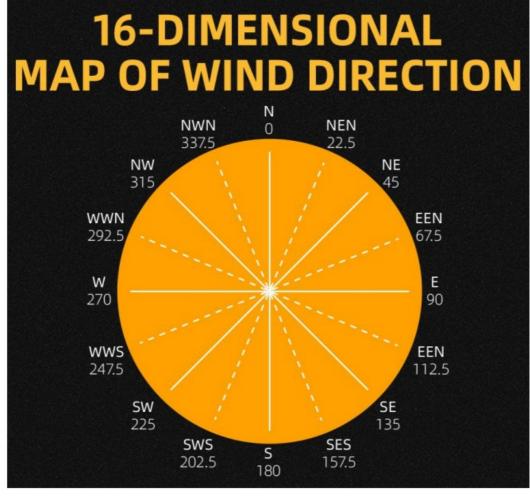

<sup>\*</sup> **Note:** When wiring, connect the positive and negative poles of the power supply first and then connect the signal wire



# **Communication Protocol**

The product uses RS485 MODBUS-RTU standard protocol format, all operation or reply commands are hexadecimal data. The default device address is 1 when the device is shipped, the default baud rate is 9600, 8, n, 1

# Read Data (Function id 0x03)

Inquiry frame (hexadecimal), sending example: Query 1# device 1 data, the host computer sends the command:01 03 00 00 00 04 44 09.

| Device ID | Function id | Start Address | Data Length | CRC16 |
|-----------|-------------|---------------|-------------|-------|
| 01        | 03          | 00 00         | 00 04       | 44 09 |

For the correct query frame, the device will respond with data:01 03 08 00 7C 00 00 00 00 00 00 28 10, the response format is parsed as follows:

| Device ID | Function id | Data Lengt<br>h | Data 1 | Data 2 | Data 3 | Data 4 | Check Cod<br>e |
|-----------|-------------|-----------------|--------|--------|--------|--------|----------------|
| 01        | 03          | 08              | 00 79  | 00 7A  | 00 7B  | 00 7C  | 28 10          |

Data Description: The data in the command is hexadecimal. Take data 1 as an example. 00 79 is converted to a decimal value of 121. If the data magnification is 100, the actual value is 121/100=1.21. Others and so on.

#### **Data Address Table**

| Address | Start Address | Description  | Data type  | Value range |
|---------|---------------|--------------|------------|-------------|
| 40001   | 00 00         | wind speed   | Read Only  | 065535      |
| 40002   | 00 01         | conductivity | Read Only  | 065535      |
| 40003   | 00 02         | temperature  | Read Only  | 065535      |
| 40004   | 00 03         | humidity     | Read Only  | 065535      |
| 40101   | 00 64         | model code   | read/write | 0-65535     |
| 40102   | 00 65         | total points | read/write | 1-20        |
| 40103   | 00 66         | Device ID    | read/write | 1-249       |
| 40104   | 00 67         | baud rate    | read/write | 0-6         |
| 40105   | 00 68         | mode         | read/write | 1~4         |
| 40106   | 00 69         | protocol     | read/write | 1~10        |

# 3 read and modify device address

# 1. Read or query device address

If you don't know the current device address and there is only one device on the bus, you can use the command FA 03 00 64 00 02 90 5F Query device address.

| Device ID | Function id | Start Address | Data Length | CRC16 |
|-----------|-------------|---------------|-------------|-------|
| FA        | 03          | 00 64         | 00 02       | 905F  |

FA is 250 for the general address. When you don't know the address, you can use 250 to get the real device address. 00 64 is the device model register.

For the correct query command, the device will respond, for example, the response data is 01 03 02 07 12 3A 79, the format of which is as shown in the following table:

| Device ID | Function id | Start Address | Model Code  | CRC16 |
|-----------|-------------|---------------|-------------|-------|
| 01        | 03          | 02            | 55 3C 00 01 | 3A 79 |

The response should be in the data. the first byte 01 indicates that the real address of the current device is. 55 3C converted to decimal 20182 indicates that the parent device's main model is 21820. the last two bytes 00

#### 2. Change devise address

For example, if the current device ad&ess is 1. we want to change to 02. the command is:01 06 00 66 00 02 E8 14.

| Device ID | Function id | Start Address | Destination | CRC16 |
|-----------|-------------|---------------|-------------|-------|
| 01        | 06          | 00 66         | 00 02       | E8 14 |

After the change is successful. the device will return information: 02 06 00 66 00 02 E8 27. its format is parsed as shown in the following table:

| Device ID | Function id | Start Address | Destination | CRC16 |
|-----------|-------------|---------------|-------------|-------|
| 01        | 06          | 00 66         | 00 02       | E8 27 |

The response should be in the data, after the modification is successful, the first byte is the new device address. After the general device address is changed, it wit take effect immediately. At this time, the user needs to change the query command of the software at the same time.

FA is 250 for the general address. When you don't know the address, you can use 250 to get the real device address. 00 64 is the device model register.

For the correct query command, the device will respond, for example, the response data is 01 03 02 07 12 3A 79, the format of which is as shown in the following table:

| Device ID | Function id | Start Address | Model Code  | CRC16 |
|-----------|-------------|---------------|-------------|-------|
| 01        | 03          | 02            | 55 3C 00 01 | 3A 79 |

The response should be in the data. the first byte 01 indicates that the real address of the current device is. 55 3C converted to decimal 20182 indicates that the parent device's main model is 21820. the last two bytes 00 01 Indicates that the device has a status quantity.

# (2)Change device address

For example, if the current device ad&ess is 1. we want to change to 02. the command is:01 06 00 66 00 02 E8 14.

| Device ID | Function id | Start Address | Destination | CRC16 |
|-----------|-------------|---------------|-------------|-------|
| 01        | 06          | 00 66         | 00 02       | E8 14 |

After the change is successful. the device will return information: 02 06 00 66 00 02 E8 27. its format is parsed

as shown in the following table:

| Device ID | Function id | Start Address | Destination | CRC16 |
|-----------|-------------|---------------|-------------|-------|
| 01        | 06          | 00 66         | 00 02       | E8 27 |

The response should be in the data, after the modification is successful, the first byte is the new device address. After the general device address is changed, it wit take effect immediately. At this time, the user needs to change the query command of the software at the same time.

# 4 Read and Modify Baud Rate

#### 1. Read baud rate

The device's default factory baud rate is 9600. If you need to change it, you can change it according to the following table and the corresponding communication protocol. For example, read the current device's baud rate ID, the command is:01 03 00 67 00 01 35 05, its format is parsed as follows.

| Device ID | Function id | Start Address | Data Length | CRC16 |
|-----------|-------------|---------------|-------------|-------|
| 01        | 03          | 00 67         | 00 01       | 35 05 |

Read the baud ate encoding of the current device. Baud rate encoring: 1 is 2400:2 is 4800:3 is 9600: 4 is 19200:5 is 38400:6 is 115200.

For the correct query command, the device will respond, for example, the response data is 01 03 02 00 03 F8 45, the format of which is as shown in the following table:

| Device ID | Function id | Data Length | Rate ID | CRC16 |
|-----------|-------------|-------------|---------|-------|
| 01        | 03          | 02          | 00 03   | F845  |

coded according to the baud rate. 03 is 9600. ie the current device has a baud rate of 9600. (2)Change the baud rate, For example, changing the baud rate from 9600 to 38400, ie changing the code from 3 to 5, the command is: 01 06 00 67 00 05 F8 1601 03 00 66 00 01 64 15.

| Device ID | Function id | Start Address | Target Baud Rate | CRC16 |
|-----------|-------------|---------------|------------------|-------|
| 01        | 03          | 00 66         | 00 01            | 64 15 |

Change the baud rate from 9600 to 38400, changing the code from 3 to 5. The new baud rate will take effect immediately, at which point the device will lose its response and the baud rate of the device should be queried accordingly. Modified.

#### **5 Read Correction Value**

#### 1. Read Correction Value

When there is an error between the data and the reference standard, we can reduce the display error by adjusting the correction value. The correction difference can be modified to be plus or minus 1000, that is, the value range is 0-1000 or 64535 -65535. For example, when the display value is too small, we can correct it by adding 100. The command is: 01 03 00 6B 00 01 F5 06. In the command 100 is hex 0x64 If you need to reduce, you can set a negative value, such as -100, corresponding to the hexadecimal value of FF 9C, which is calculated as 100-65535=65435, and then converted to hexadecimal to Ox FF 9C. The correction value starts from 00 6B. We take the first parameter as an example. The correction value is read and modified in the same way for multiple parameters.

| Device ID | Function id | Start Address | Data Length | CRC16 |
|-----------|-------------|---------------|-------------|-------|
| 01        | 03          | 00 68         | 00 01       | F5 D6 |

For the correct query command, the device will respond, for example, the response data is 01 03 02 00 64 B9 AF, the format of which is as shown in the following table:

| Device ID | Function id | Data Length | Data value | CRC16 |
|-----------|-------------|-------------|------------|-------|
| 01        | 03          | 02          | 00 64      | B9 AF |

In the response data, the first byte 01 indicates the real address of the current device, and 00 6B is the first state quantity correction value register. If the device has multiple parameters, other parameters operate in this way. The same, the general temperature, humidity have this parameter, the light generally does not have this item.

#### 2. Change correction value

For example, the current state quantity is too small, we want to add 1 to its true value, and the current value plus 100 correction operation command is:01 06 00 6B 00 64 F9 FD.

| Device ID | Function id | Start Address | Destination | CRC16 |
|-----------|-------------|---------------|-------------|-------|
| 01        | 06          | 00 6B         | 00 64       | F9 FD |

After the operation is successful, the device will return information: 01 06 00 6B 00 64 F9 FD, the parameters take effect immediately after a successful change.

#### **Disclaimer**

This document provides all information about the product, does not grant any license to intellectual property, does not express or imply, and prohibits any other means of granting any intellectual property rights, such as the statement of sales terms and conditions of this product, other issues. No liability is assumed. Furthermore, our company makes no warranties, express or implied, regarding the sale and use of this product, including the suitability for the specific use of the product, the marketability, or the infringement liability for any patent, copyright, or other intellectual property rights, etc. Product specifications and product descriptions may be modified at any time without notice.

#### **Contact Us**

Company: Shanghai Sonbest Industrial Co., Ltd KLHA Brand Division

Address: Building 8, No.215 Northeast Road, Baoshan District, Shanghai, China

Web: <a href="http://www.klha.com">http://www.klha.com</a> Web: <a href="http://www.klha.com">http://www.klha.com</a>

SKYPE: soobuu

Email: sale@sonbest.com

Tel: 86-021-51083595 / 66862055 / 66862075 / 66861077

# Sha nghai Sonbest Industrial Co., Ltd KLHA Brand Division

# **Documents / Resources**



KLHA KM53B98 Wind Speed and Direction Integrated Sensor [pdf] User Manual KM53B98, Wind Speed and Direction Integrated Sensor, KM53B98 Wind Speed and Direction I ntegrated Sensor

#### References

- <sup>O</sup> Home-KLHAå¿«ä¹æμ·å²¸ç‰©è"ç½¹
- <sup>O</sup> Home-KLHAå¿«ä¹æμ·å²¸ç‰©è"ç½¹

Manuals+,