

## CA 4

The current version of the installation and operating instructions is available in the Download Center:



<http://qr.duerdental.com/9000-606-44>



Ambient temperature



Upper limit of humidity




Only qualified specialists or employees trained by Dürr Dental are permitted to install, connect and start using the unit.



## Assembly

1

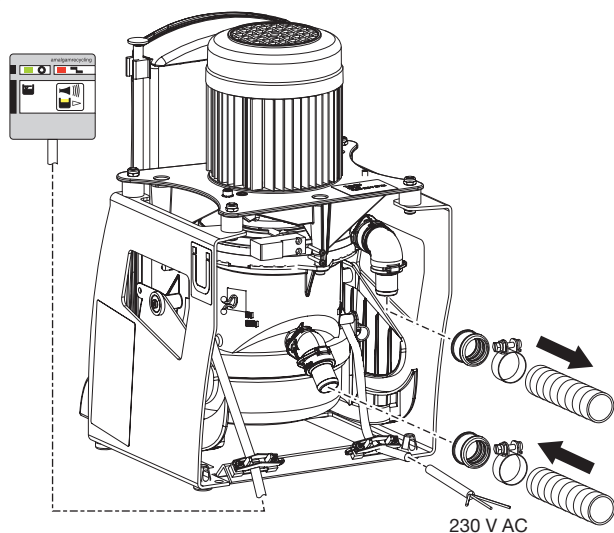

2




► Use advantages and profit with security. Register your product now!

## Usage


## Disinfection and cleaning

1

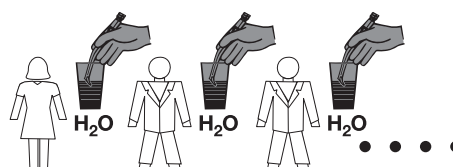


2

1x / Day  
in the evenings




1x / Week  
about noon




## Ready for operation


1

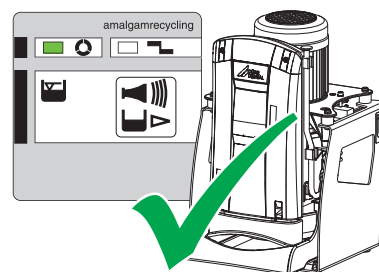


Amalgam collector vessel is 95% full

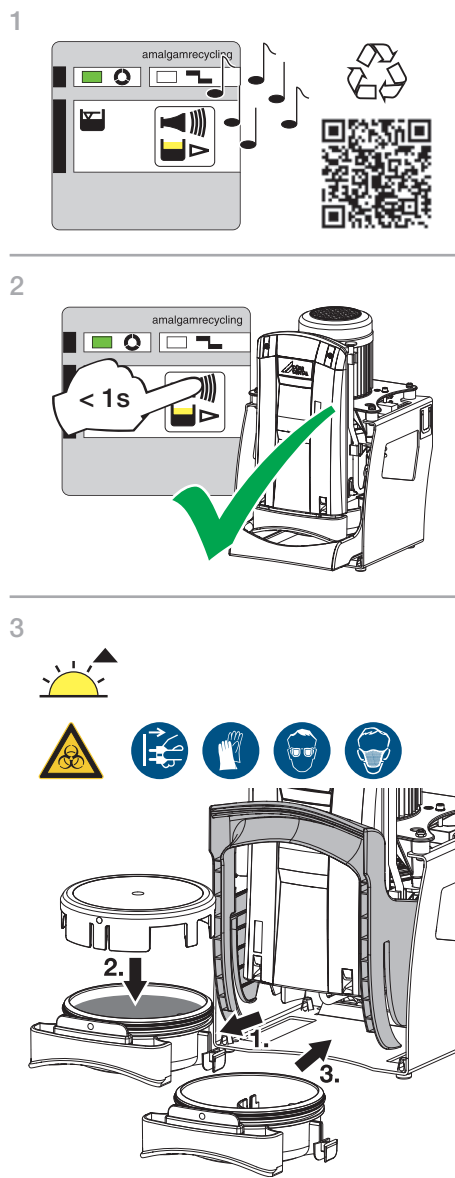


Amalgam collector vessel is 100% full

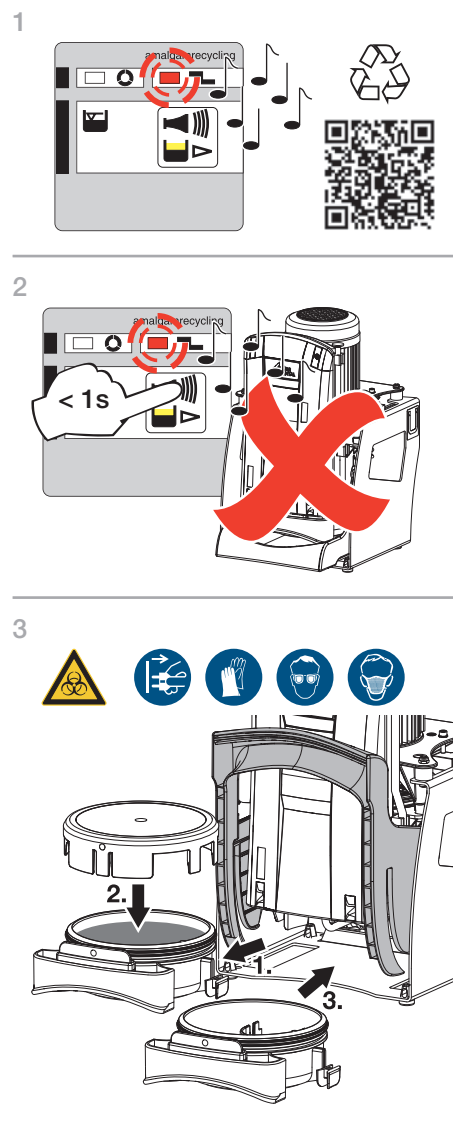

Amalgam collector vessel not in position

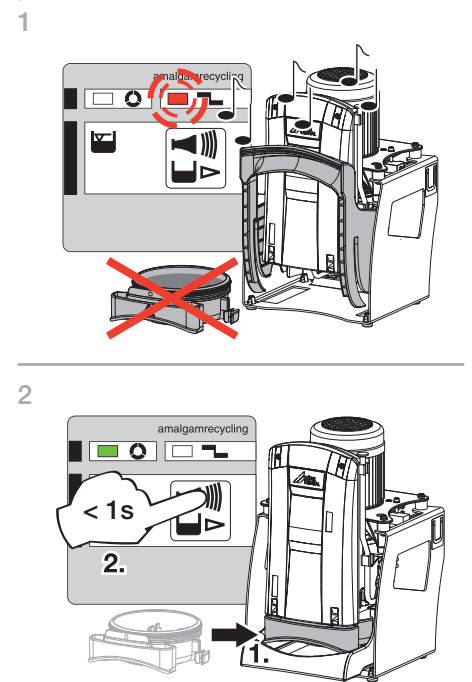

Motor fault

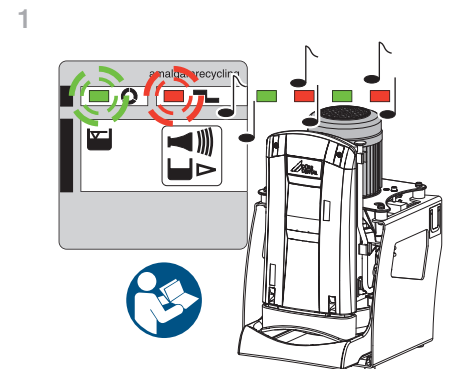

Emergency start sensor in overflow position

