


VISCOJECT-BIO 2.2 Injector Set


Handling instruction for 4-point haptic IOLs



Seeing beyond

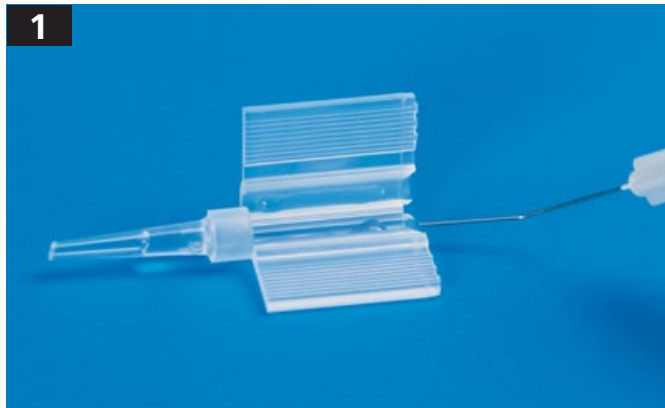


1
Place a small amount of OVD* in the cartridge tip.
Place a line of OVD in each channel of the cartridge.
Do not touch the tip of the cartridge.

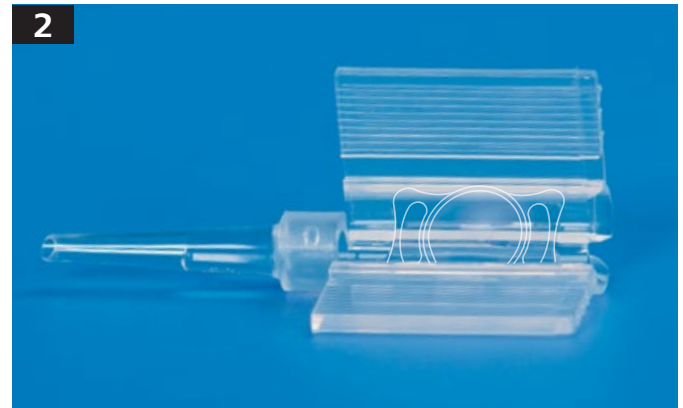

2
Place the lens in the center of the open cartridge. Push down on the edges of the optic to ensure that the optic haptics are positioned under the ledges of the cartridge.



3
For toric and multifocal IOLs, mind the orientation holes and the meridian marks.

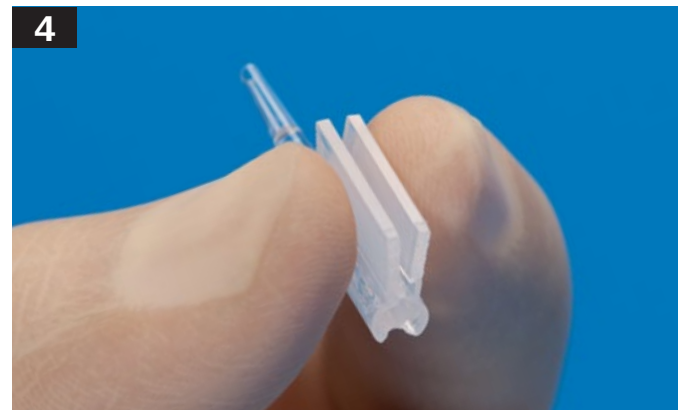

4
Maintain the IOL in place with the folding forceps while folding the cartridge. Close the cartridge until you hear a click.



5
Place the cartridge into the injector and move it forward as far as it will go. The lens is ready for implantation.



6
Place the bevelled edge downward and gently push the plunger to inject the IOL.

**Carl Zeiss Meditec recommends the use of ZEISS OVDs.*



0482

VISCOJECT-Bio 2.2 Injector Set



Medicel AG

Dornierstrasse 11

9423 Altenrhein

Switzerland

www.zeiss.com/injectors

www.zeiss.com/med/contacts