

# Labnet Prism™ Microcentrifuge

## Instruction Manual

### Catalog Numbers:

C2500  
C2500-230V  
C2500-100V



## Table of Contents

1.0 Introduction .....	1
2.0 Safety Information .....	1
2.1 Operation Safety Precautions.....	1
3.0 Specifications .....	2
4.0 Package Contents .....	2
5.0 Installation.....	2
6.0 Installation of Rotors and Rotor Maintenance.....	3
6.1 Rotors and Accessories .....	3
6.2 Rotor Maintenance .....	4
6.3 Removing and Installing the Angle Rotor.....	4
6.4 Loading the Rotor.....	4
6.5 Overloading Rotors .....	4
7.0 Operation.....	5
7.1 Attaching Rotor Lid .....	5
7.2 Closing the Lid.....	5
7.3 Lid Release .....	5
7.4 Lid Lock .....	5
7.5 Speed Selection.....	5
7.6 Selection of Operating Time, Momentary Operation, Start/Stop.....	5
8.0 Service and Maintenance .....	6
8.1 Centrifuge Service .....	6
8.2 Cleaning .....	6
8.3 Replacing Fuses.....	6
9.0 Troubleshooting Guide .....	6
10.0 Determination of G-values.....	7
11.0 Limited Warranty.....	8
12.0 Equipment Disposal .....	8

## 1.0 Introduction

The Labnet Prism™ microcentrifuge is a small benchtop centrifuge designed for separation of various research samples. The motor is brushless and requires no routine maintenance. This microcentrifuge is supplied with a 24 x 1.5/2.0 mL rotor for microsample tubes. Adapters are available for tubes smaller than 1.5 mL. This reaches speeds of up to 15,000 rpm/21,200 x g.

## 2.0 Safety Information

Before using the Labnet Prism microcentrifuge for the first time, please read this entire manual carefully. If the equipment is used in a manner not specified by the manufacturer, the protection provided by the equipment may be impaired.



This symbol indicates a potential risk and alerts you to proceed with caution.

### 2.1 Operation Safety Precautions

- ▶ Never use the centrifuge in any manner not specified in these instructions.
- ▶ Never operate the centrifuge without a rotor properly attached to the shaft.
- ▶ Always use a wrench to tighten the rotor nut. Never tighten rotor nut by hand only.
- ▶ Never fill tubes while they are in the rotor. Liquid spillage may harm unit.
- ▶ Never put hands in the rotor area unless the rotor is completely stopped.
- ▶ Never move the centrifuge while the rotor is spinning.
- ▶ Never use solvents or flammables near this or other electrical equipment.
- ▶ Never centrifuge flammable, explosive, or corrosive materials.
- ▶ Never centrifuge hazardous materials outside of a hood or a proper containment facility.
- ▶ Always load the rotor symmetrically. Each tube should be counter-balanced by another tube of the same type and weight.
- ▶ Always locate the centrifuge within easy access to an electrical outlet.
- ▶ Always use only microcentrifuge tubes made from plastic and designed to withstand centrifugal forces of at least 21,200 x g.
- ▶ Always use a wrench to tighten the rotor nut.

Do not operate the centrifuge if any of the following conditions exist:

- ▶ The centrifuge has not been installed properly.
- ▶ The centrifuge is partially dismantled.
- ▶ Service has been attempted by unauthorized or unqualified personnel.
- ▶ The rotor has not been installed securely on the motor shaft.
- ▶ Rotors and accessories outside of the standard range are not to be used without permission from the manufacturer.  
Exception: Microcentrifuge tubes made of plastic, normally available in the laboratory.
- ▶ The centrifuge is located in an explosive atmosphere.
- ▶ Materials to be centrifuged are combustible and/or explosive.
- ▶ Materials to be centrifuged are chemically reactive.
- ▶ The rotor load is not properly balanced.
- ▶ The rotor nut was not tightened with a wrench.

### 3.0 Specifications

Dimensions (W x D x H)	10.1 x 14.2 x 7.6 in. (25.7 x 36.0 x 19.4 cm)
Maximum Speed	15,000 rpm
Maximum RCF	21,200 x g
Maximum Volume	24 x 2.2 mL
Timer	0.5 to 99 minutes or continuous
Admissible Sample Density	1.2 kg/dm <sup>3</sup>
Electrical/Fuse Rating	
C2500	120V~, 50/60 Hz, 250W, 3.4A
C2500-230V	230V~, 50/60 Hz, 200W, 1.4A
C2500-100V	100V~, 50/60 Hz, 230W, 3.5A
Temperature Range	5°C to 40°C (up to 80% RH at 31°C, decreasing linearly to 50% RH at 40°C)
Protection Class	IP21

The Labnet Prism™ microcentrifuge is designed to be safe at least when operated under the following conditions:

- ▶ Indoor use only
- ▶ Altitude up to 2,000 meters
- ▶ Pollution Degree 2

Changes or modifications not expressly approved by the party responsible for compliance could void the user's authority to operate the equipment.

**NOTE:** This equipment has been tested and found to comply with the limits for a Class A digital device, pursuant to Part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference when the equipment is operated in a commercial environment. The equipment generates, uses, and can radiate radio frequency energy and, if not installed and used in accordance with the user manual, may cause harmful interference to radio communications. Operation of equipment in a residential area is likely to cause harmful interference in which case the user will be required to correct the interference.



**CAUTION:** This equipment is not intended for use in residential environments and may not provide adequate protection to radio reception in such environments.

This ISM device complies with Canadian ICES-001.

*Cet appareil ISM est conforme à la norme NMB-001 du Canada.*

### 4.0 Package Contents

- ▶ Labnet Prism microcentrifuge
- ▶ Standard angle rotor (Cat. No. 24D-RTR)
- ▶ Rotor removal tool
- ▶ Power cord
- ▶ Instruction manual

### 5.0 Installation

The centrifuge should be installed on a rigid, even surface such as a stable laboratory bench, countertop, etc. To guarantee sufficient ventilation, ensure that the centrifuge has at least 6 inches (15 cm) of free space on all sides, including the rear. The centrifuge should not be located in areas subject to excessive heat such as in direct sunlight or near radiators or the exhaust of a compressor, as a buildup of heat may occur within the chamber.

Before operating the centrifuge, check that the power source (electrical outlet on the wall) corresponds to that on the manufacturer's rating label, then connect the power cord to the centrifuge and the power source.

## 6.0 Installation of Rotors and Rotor Maintenance

### 6.1 Rotors and Accessories

The following accessories are included or available for the Labnet Prism™ microcentrifuge:

#### Angle Rotor for 24 x 1.5 mL/2.0 mL Tubes (included)

Cat. No.	24D-RTR
Tube Measurement	1.5 mL/2.0 mL (10 x 40 mm)
Maximum Speed	15,000 rpm
Centrifuging Radius	3.3 in. (8.4 cm)
Maximum RCF (G-value)	21,200 x g

#### Rotor Wrench (included)

Cat. No.	AM190
----------	-------

#### Rotor Lid (included)

Cat. No.	C2400-RC1
----------	-----------

#### Rotor Securing Screw (included)

Cat. No.	AR110
----------	-------

#### Strip Spin Adapter

Cat. No.	C2400-SS
Tubes Accepted	0.2 mL tubes or 8 x 0.2 mL strips
Maximum Speed	15,000 rpm
Centrifuge Radius Range	4.32 to 5.33 cm
RCF (G-value) Range	10,874 to 13,405 x g

#### Adapter for 0.5 mL Tubes (6/Pk)

Cat. No.	C-1205
Tube Measurement	8 x 30 mm
Maximum Speed	15,000 rpm
Centrifuging Radius	7.53 cm
RCF (G-value)	18,942 x g

#### Adapter for 0.4 mL Tubes (6/Pk)

Cat. No.	C-1206
Tube Measurement	6 x 47 mm
Maximum Speed	15,000 rpm
Centrifuging Radius	8.4 cm
RCF (G-value)	21,200 x g

#### Adapter for 0.2 mL Tubes (6/Pk)

Cat. No.	C-1222
Tube Measurement	6 x 21 mm
Maximum Speed	15,000 rpm
Centrifuging Radius	7.03 cm
RCF (G-value)	17,684 x g

## 6.2 Rotor Maintenance

The rotor should be cleaned thoroughly after each use. **NOTE:** Thorough cleaning must be performed when spinning samples containing phenol or phenol chloroform. Periodically inspect the rotor for dents, dings, scratches, discoloration, and cracks. If any damage to the rotor is found, discontinue use of the rotor immediately and replace.

## 6.3 Removing and Installing the Angle Rotor

The Labnet Prism™ microcentrifuge comes complete with a standard 24-place rotor installed. To remove the rotor for cleaning, using the rotor wrench remove the rotor securing screw from the motor shaft by turning the screw counterclockwise. Lift the rotor directly upward in a straight vertical motion.



Figure 1. Loading the rotor to achieve balance.

To replace the rotor, first make sure the motor shaft and rotor mounting hole are clean. Place the rotor on the motor shaft. Reinstall the rotor securing screw on the motor shaft by turning it clockwise. Hold the rotor with one hand and tighten the rotor securing screw, using the rotor wrench.

## 6.4 Loading the Rotor

Tubes to be loaded should be filled equally by eye. The difference in the weight between the tubes should not exceed 0.1 gram. Tubes should always be loaded so there is equal spacing between all tubes. One or two additional loaded tubes may need to be added to achieve this. See Figure 1 for a typical balancing scheme.

## 6.5 Overloading Rotors

The maximum load of the rotor and maximum speed has been established by the manufacturer. Do not attempt to exceed these values. The maximum speed of the rotor has been established for liquids having a homogeneous density of 1.2 g/mL or less. In order to centrifuge liquids with a higher density it is necessary to reduce the speed. **NOTE:** Failure to reduce the speed may result in damage to the rotor and centrifuge. The revised maximum speed can be calculated with the following formula:

$$\text{Reduced speed } (n_{\text{red}}) = \sqrt{\frac{1.2}{\text{higher density value}}} \times \text{max. speed } (n_{\text{max}})$$

**Example:** Where the density of the liquid is 1.7, the new maximum speed would be calculated as follows:

$$(n_{\text{red}}) = \sqrt{\frac{1.2}{1.7}} \times 15,000 = 12,602 \text{ rpm}$$

If in doubt concerning maximum speeds, please contact the manufacturer for assistance.

## 7.0 Operation

**CAUTION:** Never attempt to operate the centrifuge with rotors or adapters that show signs of corrosion or mechanical damage. Never centrifuge strongly corrosive materials that may damage the rotors, accessories, or bowl of the unit.

### 7.1 Attaching Rotor Lid

After the rotor has been properly secured and loaded, attach the rotor lid to the rotor. Always use the rotor lid for safety and to allow the rotor to reach proper speed. Make sure the rotor lid snaps securely into place, by pressing down on center catch.

### 7.2 Closing the Lid

Close the centrifuge lid. This microcentrifuge has a lid lock that activates only when a run is started.

### 7.3 Lid Release

The lid will remain locked during a centrifuge run. Once the run has been completed and the rotor has come to a stop, a beep will indicate the end of a run, and the lid will unlock automatically.



**CAUTION:** Do not attempt to open the lid of any centrifuge until the rotor has come to a complete stop.

In the event of a power failure or malfunction, it may be necessary to open the lid manually.

1. Disconnect the power cord from the wall socket.
2. Remove the plastic plug, located on the left side of the unit.
3. Pull the wire (attached to the plug) to open the lid lock manually.

### 7.4 Lid Lock

The centrifuge can be started only when the lid is securely closed. When a run is started, the lid lock automatically activates.

**CAUTION:** Do not attempt to open the lid during a centrifuge run. At the end of the run, the lid will automatically unlock. Never attempt to override the lid lock mechanism. Doing so is dangerous and could damage the centrifuge.

### 7.5 Speed Selection



Figure 2. Labnet Prism™ microcentrifuge control panel layout.

The speed (rpm or g-force) can be selected from 500 to 15,000 rpm in 100 rpm increments or from 100 to 21,200 x g with the control knob. The speed is selected by pressing the RPM or RCF button. The speed signal will begin to blink. Then, turn the control knob to increase or decrease the value.

### 7.6 Selection of Operating Time, Momentary Operation, Start/Stop

Operating time can be selected from 0.5 min. to 99 min. by pressing the TIME button and adjusting with the control knob. The time can be set in 0.5-minute increments from 0 to 10 minutes and in 1-minute increments from 10 to 99 minutes. After 99 minutes, the display shows "--" which indicates continuous run. In this mode, the centrifuge will run until manually stopped. To start a run, press the control knob. When the preselected time expires, the centrifuge will stop automatically. To stop the centrifuge prior to the expiration of set time, press the control knob. The centrifuge may be operated for a short run by pressing and holding the control knob. The centrifuge will continue to run as long as the control knob is depressed, the time (in seconds) will count up on the time display.

## 8.0 Service and Maintenance

### 8.1 Centrifuge Service

The brushless motor in this microcentrifuge requires no routine maintenance. Any required service should be performed by authorized, qualified personnel only. Repairs performed by unauthorized personnel may void the warranty.

### 8.2 Cleaning

Always keep the centrifuge housing, rotor chamber, rotor and rotor accessories clean. All parts should be wiped down periodically with a soft cloth. For more thorough cleaning, use a neutral cleaning agent (pH between 6 and 8) applied with a soft cloth. Excessive amounts of liquid should be avoided. Liquid should not come into contact with the motor. After cleaning, ensure that all parts are dried thoroughly by hand or in a warm air cabinet (maximum temperature 50°C).

The rotor should be cleaned after each use. When spinning samples containing phenol or phenol chloroform, the rotor should be cleaned immediately after use.

Should a spill of infectious materials occur within the rotor or chamber, the unit should be disinfected. This should be performed by qualified personnel with proper protective equipment.

### 8.3 Replacing Fuses

Check the fuse when it is recommended (see Troubleshooting Guide section). Disconnect the power cord from the wall socket before checking the fuses. The fuse holder is located in the power inlet on the rear of the unit. Open the fuse holder drawer by inserting a small screwdriver under the tab and prying it open. Remove the innermost (operative) fuse from its retaining tabs, and replace the fuse if necessary. A spare fuse is located in the outermost chamber of the fuse drawer. Replace only with a fuse of exactly the same value as the original. See Section 3.0 for information on fuse type.

## 9.0 Troubleshooting Guide


Problem	Possible Cause	Solution
Centrifuge will not start	No power supply	<ul style="list-style-type: none"><li>▶ Check if power is being supplied to the outlet.</li><li>▶ Check if the power cord is plugged into both the wall outlet and the back of the centrifuge.</li><li>▶ Check if the power cord is damaged.</li></ul>
	Blown fuse	Check the fuse and replace if necessary.
Lid lock will not release	Defective lid lock	Open manually, and have the unit serviced.
	No power from the PC board	Call for service.
	Lid lock is jammed	Call for service.
	Centrifuge is not receiving power	See “Centrifuge will not start”.
Centrifuge cannot be started, although power is On	Lid is not closed correctly	Close the lid correctly.
	No speed or time has been selected	Set the speed and/or time.
bAL (Error Message) indicates imbalance	Tubes are not inserted symmetrically in the rotor holes	Load the tubes symmetrically (see Section 6.4: Loading the Rotor).
	Sample liquid in the tubes is not balanced	Make sure the same volume of liquid is in each tube.
	Defective or improperly adjusted balance sensor	Call for service.
Lid (Error Message) lid not closed	Lid is not closed completely	Close the lid.
	Lid lock or sensor is defective	Call for service.
Other Error Messages Er on Display	—	<ul style="list-style-type: none"><li>▶ Press the time or speed button to clear the error.</li><li>▶ Call for service.</li></ul>

Should you have a question about the operation of the Labnet Prism™ Microcentrifuge or if service is required, contact Corning Customer Service. Do not send in a unit for service without first calling to obtain a repair authorization number. Should the unit require return for service, it should be properly packed to avoid damage. Any damage resulting from improper packaging shall be the responsibility of the user.



## 10.0 Determination of G-values

The centrifuging radius of the 1.5/2.0 mL rotor is 8.23 cm. The Labnet Prism™ microcentrifuge has an automatic g-force conversion program, so g-values are automatically calculated and can be displayed on the control panel, for this centrifuging radius. If adapters or smaller tubes are used, the centrifuging radius changes as does the g-force. The chart below can be used to manually determine g-values for any centrifuging radius.

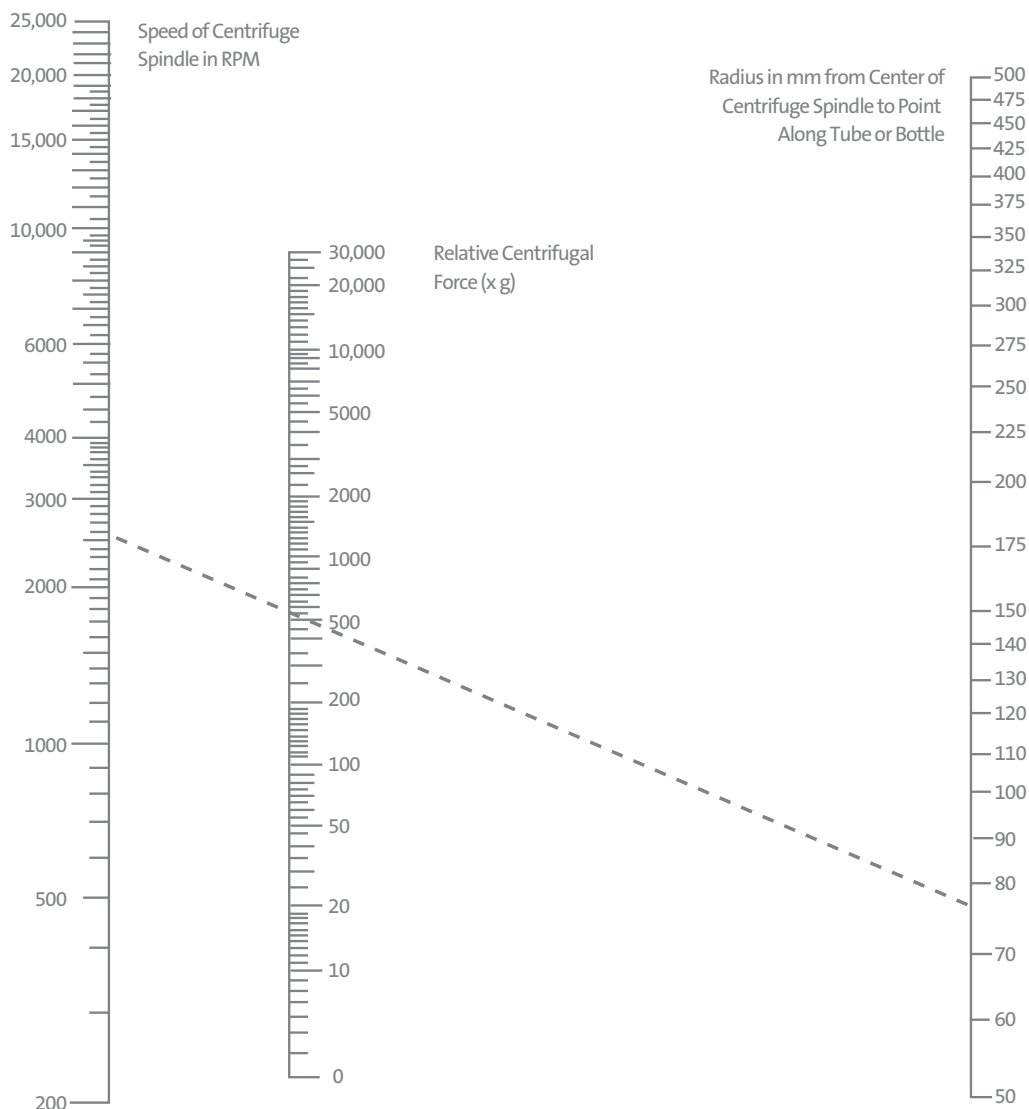

To calculate the RCF value at any point along the tube or bottle, measure the radius (in mm), from the center of the centrifuge spindle to the particular point. Draw a line from the radius value on the right-hand column to the appropriate centrifuge speed on the left-hand column. The RCF value is the point where the line crosses the center column. The nomogram is based on the formula:

$$RCF = (11/17 \times 10^{-7}) RN^2$$

where:

R = Radius in mm from centrifuge spindle to point in tube bottom

N = Speed of spindle in RPM

## 11.0 Limited Warranty

Corning Incorporated (Corning) warrants that this product will be free from defects in material and workmanship for a period of one (1) year from date of purchase. CORNING DISCLAIMS ALL OTHER WARRANTIES WHETHER EXPRESSED OR IMPLIED, INCLUDING ANY IMPLIED WARRANTIES OF MERCHANTABILITY OR OF FITNESS FOR A PARTICULAR PURPOSE. Corning's sole obligation shall be to repair or replace, at its option, any product or part thereof that proves defective in material or workmanship within the warranty period, provided the purchaser notifies Corning of any such defect. Corning is not liable for any incidental or consequential damages, commercial loss or any other damages from the use of this product.

This warranty is valid only if the product is used for its intended purpose and within the guidelines specified in the supplied instruction manual. This warranty does not cover damage caused by accident, neglect, misuse, improper service, natural forces or other causes not arising from defects in original material or workmanship. This warranty does not cover motor brushes, fuses, light bulbs, batteries or damage to paint or finish. Claims for transit damage should be filed with the transportation carrier.

In the event this product fails within the specified period of time because of a defect in material or workmanship, contact Corning Customer Service at: USA/Canada 1.800.492.1110, outside the U.S. +1.978.442.2200, visit [www.corning.com/lifesciences](http://www.corning.com/lifesciences), or contact your local support office.

Corning's Customer Service team will help arrange local service where available or coordinate a return authorization number and shipping instructions. Products received without proper authorization will be returned. All items returned for service should be sent postage prepaid in the original packaging or other suitable carton, padded to avoid damage. Corning will not be responsible for damage incurred by improper packaging. Corning may elect for onsite service for larger equipment.

Some states do not allow limitation on the length of implied warranties or the exclusion or limitation of incidental or consequential damages. This warranty gives you specific legal rights. You may have other rights which vary from state to state.

No individual may accept for, or on behalf of Corning, any other obligation of liability, or extend the period of this warranty.

For your reference, make a note of the serial and model number, date of purchase, and supplier here.

Serial No. \_\_\_\_\_ Date Purchased \_\_\_\_\_

Model No. \_\_\_\_\_ Supplier \_\_\_\_\_

## 12.0 Equipment Disposal



According to Directive 2012/19/EU of the European Parliament and of the Council of 4 July 2012 on waste electrical and electronic equipment (WEEE), this product is marked with the crossed-out wheeled bin and must not be disposed of with domestic waste.

Consequently, the buyer shall follow the instructions for reuse and recycling of waste electronic and electrical equipment (WEEE) provided with the products and available at [www.corning.com/weee](http://www.corning.com/weee).

To request certificates, please contact us at [www.labnetlink.com](http://www.labnetlink.com).

**Warranty/Disclaimer:** Unless otherwise specified, all products are for research use or general laboratory use only.\* Not intended for use in diagnostic or therapeutic procedures. Not for use in humans. These products are not intended to mitigate the presence of microorganisms on surfaces or in the environment, where such organisms can be deleterious to humans or the environment. Corning Life Sciences makes no claims regarding the performance of these products for clinical or diagnostic applications. \*For a listing of US medical devices, regulatory classifications or specific information on claims, visit [www.corning.com/resources](http://www.corning.com/resources).

*Corning's products are not specifically designed and tested for diagnostic testing. Many Corning products, though not specific for diagnostic testing, can be used in the workflow and preparation of the test at the customers discretion. Customers may use these products to support their claims. We cannot make any claims or statements that our products are approved for diagnostic testing either directly or indirectly. The customer is responsible for any testing, validation, and/or regulatory submissions that may be required to support the safety and efficacy of their intended application.*

# CORNING

Corning Incorporated  
Life Sciences

[www.corning.com/lifesciences](http://www.corning.com/lifesciences)

## NORTH AMERICA

t 800.492.1110  
t 978.442.2200

## ASIA/PACIFIC

Australia/New Zealand  
t 61 427286832  
Chinese Mainland  
t 86 21 3338 4338

## India

t 91 124 4604000

## Japan

t 81 3-3586 1996

## Korea

t 82 2-796-9500

## Singapore

t 65 6572-9740

## Taiwan

t 886 2-2716-0338

## EUROPE

CSEurope@corning.com

## LATIN AMERICA

grupoLA@corning.com

## Brazil

t 55 (11) 3089-7400

## Mexico

t (52-81) 8158-8400