
MOMCOZY

Wearable Breast Pump

V1 Pro

Model number: BP137
USER MANUAL

(For OTC Type of Use)

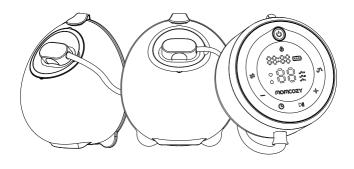

Read this user manual carefully before using this device and keep this manual for future reference.





TABLE OF CONTENTS

) 2
)2
)3
)4
)4
)6
)9
28
28
28
30
30
30
32
32
32
39
40
40
40



1. Product Introduction

The Momcozy Wearable Breast Pump is intended to be used by lactating women to express and collect milk from their breasts. The Momcozy Wearable Breast Pump forms a vacuum around the nipple to express breast milk. The milk is collected in a milk collector. The device includes stimulation mode, expression mode, and mixed mode. In stimulation mode, the breast pump begins with a quick and short sucking pattern to get your milk to start flowing. In expression mode, the breast pump begins with a slow and long sucking pattern for milk expression, sucking more deeply and more slowly. In mixed mode, the breast pump begins with a quick and short sucking pattern, followed by a slow and long sucking pattern. To prevent milk from flowing into the vacuum system, the milk collection sets include a silicone diaphragm that physically separates the milk-contacting pathway from the vacuum system.

The device is intended for a single user.

2. Warning Instructions and Precautions

The warning signs and graphic symbols in the manual are intended to enable you to use the product safely and correctly and to prevent harm to you and others. Warning marks and graphic symbols are described as follows:

Warning/precautions symbols		
<u>!</u> Warning	A warning alerts the reader about a situation that, if not avoided, could result in death or serious injury. It may also describe potential serious adverse reactions and safety hazards.	
Precautions	Indicating a hazard alert that warns the reader of a potentially hazardous situation which, if not avoided, may result in minor or moderate injury to the user or patient or damage to the equipment or other property. It may also be used to alert against unsafe practices. This includes the special care necessary for the safe and effective use of the device and the care necessary to avoid damage to a device that may occur as a result of use or misuse.	
Contraindications	Contraindications are conditions under which the device should not be used because the risk of use clearly outweighs any possible benefit. There may be persons for whom the device should not be used because of their health status.	
Notes	Indicates the need for attention, if not attention may lead to incorrect use of the product or property device damage.	

Symbol Description

*	Keep Dry	∑ 5 ■	Pile Limit 5 layers	
†	Applied part of type BF	(3)	Refer to instruction manual.	
LOT	Batch code		Manufacture date	
	Manufacturer information: The manufacturer name and address	SN	Serial Number	
*	Distribution packages shall not be exposed to sunlight	521	For food contact	
IP22	The first number 2: Protected against solid foreign objects of 12.5mm diameter and greater. The second number 2: Protected against vertically falling water drops when enclosure titled up to 15°.			
<u>Z</u>	Disposal in accordance with Directive 2012/19/EU (WEEE)			
MR	This device has not been tested for use in an MR environment and should not be used exposed to MR environments while patients are wearing the device. Keep it outside the MRI scanner room.			
F©	FCC logo			

3. Indications for Use

[Intended use]

The Momcozy Wearable Breast Pump (model: BP137) is a powered breast pump intended to express milk from lactating women in order to collect milk from their breasts. The device is intended for a single user.

[Intended users]

Can read and understand the user manual The PATIENT is an intended OPERATOR

[Patient Population]

Lactating women

4. Contraindications

No known Contraindications

Home Healthcare Environment

5. Safety Information

When using electrical products, especially if children are present, the following basic safety information should always be maintained.

5.1 Warning

- Do not use this device if you have a cardiac pacemaker, implanted defibrillator, or other implanted metallic or electronic device. Such use could cause electrical interference, or death.
- 2) This breast pump is not intended for use by persons (including children) with reduced physical, sensory or mental capabilities, or lack of experience and knowledge. Such persons can only use this breast pump if they are supervised by or have received proper instruction concerning use of the appliance by a person responsible for their safety.
- 3) Danger: To reduce the risk of electrocution:
- Always unplug electrical devices immediately after charging.
- Do not use it while bathing, showering, driving or swimming.
- Do not reach for electrical product that has fallen into water, please unplug the power adapter from wall outlet immediately.
- 4) The Momcozy Wearable Breast Pump is a personal care item and for hygienic reasons should never be shared between mothers or resold from one mother to another. Either of these actions will void the warranty.
- 5) If you are a mother who is infected with Hepatitis B, Hepatitis C or Human Immunodeficiency Virus (HIV), pumping breast milk using the Momcozy Wearable Breast Pump will not reduce or remove the risk of transmitting the virus to your baby through your breast milk.
- 6) Close supervision is necessary when product is used near children or invalids. Do not allow children or pets to play with the motor unit, packaging materials or accessories.
- 7) Use product only for intended use as described in this manual.
- 8) Do not use attachments or other milk collection components other than those recommended by manufacturer.
- 9) Check the power adapter before charging, never use the damaged power adapter.
- 10) Never leave product unattended while charging.
- 11) Keep the product and all attachments away from heated surfaces.
- 12) Never use it while sleeping or drowsy.
- Do not operate where aerosol spray products are being used or oxygen is being administered.
- 14) Do not use the device around explosive or flammable material, in an MRI environment, in a hyperbaric chamber, or near a fireplace or radiant heater.



- 15) Avoid strangulation resulting from Charging cable.
- 16) Users are not allowed to repair the product. If you do so, your warranty becomes invalid. For repairs, sent to the manufacturer or a designated franchise distributor.
- 17) Always switch off the breast pump before you remove the pump body from your breast, in order to release the vacuum.
- 18) Powered breast pumps that are designed for single users should never be rented or shared
- 19) Never use the breast pump while you are pregnant, as pumping can induce labor.
- 20) The high level temperature of applied part can reach max.43.9°C, excessive temperature may cause skin burns, please make sure that your skin of breast must be intact and healthy before use. If you feel overheated, please turn off the device. In order to avoid high temperature burn, the maximum continuous use shall not exceed 30min each time, the interval between two uses shall be at least 5min to allow the device to cool down.

21) For product service life (i.e. working life)

The device has no shelf life, and the service life of the product is 500 hours. The expected operating life of the washable parts is one to three months. Please check whether the product can run normally before use. Use beyond the service life may lead to the degradation of product performance. Such as, if the product cannot control the vacuum correctly, excessive vacuum may cause injuries.

22) Keep the product away form children or pets, and avoid swallowing small parts.



- Do not place or store where the product can fall or be pulled into a bathtub, sink or pool.
- Do not place or drop the product into water or other liquid.
- Do not immerse in any liquid for any reason or subject the unit to extreme shocks, such as dropping the pump.
- Do not continue pumping for more than five minutes at a time if you do not succeed in expressing any milk. Try to express at another time during the day.
- If discomfort is felt, then suction can be broken by inserting a finger between the breast and the flange.
- If irritation or discomfort occurs, discontinue use and see a health care provider.
- If the power adapter casing or wiring becomes loose, separated, or frayed, stop use
 of the power adapter immediately and contact the device manufacturer. Stop using
 the device immediately if you note any smoke or burning from the pump unit or
 power adapter.
- Before each use visually inspect the individual components for cracks, chips, tears, discoloration, or deterioration. In the event that damage to the device is observed, please discontinue use until the parts have been replaced.
 Statement: If you feel excessive warmth from the Wearable breast pump while pumping, stop pumping immediately and remove pump.


Notes:

Avoid direct sunlight to the main unit.



6. Product Description

The product is mainly composed of main unit and milk collection set.




Description of breast pump unit				
NO.	Item Description			
0	Double-sealed flange (24mm)			
2	Tubing			
3	Valve	All of these components make up		
4	Milk collector			
6	Main unit	Pump motor		
6	USB Type-C cable	Input end is USB 2.0 interface, the output end is Type-C interface		

EN

Other Accessories Included:

Flange Insert Valve Flange Cover Quick Start Guide Flange Size Ruler User Manual



- On/Off: Long-press to turn on/off the device;
- 4 Battery Display
- Mode Selection
- •
- Increase

- 6 Mode Indicator
 - 8 Cycle Selection
 - 11 Timer

Screen Lock

- 3 Running Time
- 6 Cycle Indicator
- O Decrease
- Pause / Continue

Suction Level Display

Buttons and LEDs	Functions		
(4)	Long-press to turn on/off the device; Short-press to put the screen to sleep and press any button to activate the screen.		
►II	Pause/Continue your pumping session.		
÷	Mode Selection		
_	Decrease suction level		
+	Increase suction level		



\bigcirc	Stimulation Mode In this mode, the breast pump begins with a quick and short sucking pattern to get your milk to start flowing.	
٥	Expression Mode The breast pump begins with a slow and long sucking pattern for milk expression, where the suction is deeper.	
\bigcirc 0	Mixed Mode In this mode, the breast pump begins with a quick and short sucking pattern, followed by a slow and long sucking pattern.	
88	Running Time Display	
∂	Screen Lock	
√	Cycle Selection	
<u> </u>	Timer	



7. Operating Instructions

7.1 Powering the Breast Pump

There are two power options available for your pumping session.

7.1.1 By the rechargeable built-in battery

Charge the pump for two hours before its first use. There are three indicator bars when the pump is fully charged.


7.1.2 By the charging cable

Plug the charging cable into the port on top of the pump motor.

7.2 Charging battery

Please charge the product before using it for the first time. The breast pump is powered by the internal rechargeable lithium battery.

Our product comes with a charging cable (USB2.0/Type-C line) but not with a power adapter. Please purchase the power adapter by yourself before charging. Make sure to buy the power adapter which matches the USB 2.0 interface, and please make sure the input power of the power adapter is AC 100-240V 50/60 Hz and the output power is DC 5V==2A



Charge the battery as below:

- a. Insert the USB end of Charging cable into the USB interface of power adapter;
- b. Insert power adapter plug into AC socket;
- c. Insert the Type-C end of Charging cable into the charging port.






Fig. 4 Position of Charging port

The device will take approximately 120 minutes to fully charge. When the pump is charged, the battery indicator bar increases one by one, from one bar to three bars, then switches off and repeats this process until the pump is fully charged. The display of three bars indicates that the battery is full.

Unplug the power adapter from the socket, disconnect the charging cable from the power adapter and main unit after charging is completed.



- The charging cable is only used to connect between the power adapter and the Momcozy wearable breast pump unit for charging, please do not connect to other equipment, otherwise, it may cause electric shock accident!
- If the power adapter casing becomes loose, separated, or frayed, stop the use of the power adapter immediately and contact the manufacturer of power adapter.
- If the charging cable is damaged, broken or cracked, stop the use of the charging cable immediately and contact the manufacturer to replace a new one (See the last page of this manual for contact information).
- Stop using the device immediately if you note any smoke or burning from the pump unit or power adapter.



Using the wrong type of adapter or purchasing a poor-quality adapter may reduce the device's safety, and may damage your property and health. Please purchase the medical adapter that meets the IEC 60601–1 and IEC 60601–1-2 standards in professional medical markets, and make sure the output of the power adapter is DC 5V=2A.



Notes:

- After fully charging the battery, if the working time of the battery is shorter than before and you want to replace it, don't try to replace the rechargeable battery by yourself. Please contact the manufacturer for replacement. Self-disassembly and replacement of the battery may cause damage to the main unit and battery.
- When the product is not used for a long time, the battery will discharge slowly. In order to avoid battery damage due to low voltage for a long time, please charge the device every three months.

7.3 Cleaning and disinfection

7.3.1 General description/requirement

Providing breast milk is one of the best things you can do for your baby's health and development. Pumping your milk is one way to provide breast milk to your baby. Keeping the parts of your pump clean is critical because germs can grow quickly in breast milk or breast milk residue that remains on pump parts. Following these steps can help prevent contamination and protect your baby from infection. If your baby was born prematurely or has other health concerns, your baby's health care providers may have more recommendations for pumping breast milk safely.

1) BEFORE EVERY USE

Inspect and assemble a clean pump kit.
Clean pump motor with disinfectant wipes.

2) AFTER EVERY USE

Store milk safely: Use breast milk storage bags or clean, food-grade containers to store expressed breast milk. Make sure the containers are made of glass or plastic and have tight-fitting lids, and label them with the date and time, and immediately place them in a refrigerator, freezer, or cooler bag with ice packs.

Clean pumping area: Clean the surface of the pump motor with disinfectant wipes.

Parts that need to be cleaned and disinfected


Clean and disinfect all parts that come into contact with breast and breast milk before you use the breast pump for the first time and after every use. Cleaning and sanitizing are not the same. It's necessary to clean and disinfect the pump separately, so as to keep moms and babies safe and maintain the breast pump's performance.

 Parts contacting with the breast milk and breast skin: parts of milk collection set, including flange, lid, diaphragm, valve, and milk collector.



4) Before cleaning / disinfection:

- a. Please Wash your hands well with soap and water for 20 seconds.
 - b. Please disassemble all parts as follows:

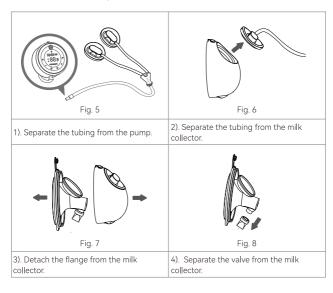



Never put the main unit, charging cable or the adapter (If you have purchased an adapter) in water or a dishwasher, as this causes permanent damage to these parts.

7.3.2 Cleaning and disinfecting parts contacting with the breast milk

Step 1: Cleaning

Please manually clean the device! The safety of using a dishwasher to clean and disinfect this product has not been verified.





Do not use antibacterial or abrasive cleaning agents to clean the breast pump parts as this may cause damage.

- 1) Prepare the below items:
- Soap and hot water
- Drinking-quality water
- Clean wash basin used only for infant feeding items
- Clean brush used only for infant feeding items
- Unused dish towel or paper towel
- 2) Rinse: Rinse parts of milk collection set and any other feeding items by holding them under running water to remove the remaining milk or dirt. The water can be warm or cold, whatever you prefer.




Fig. 9

- 3) Wash milk collection parts:
- Place parts of the milk collection set in a clean wash basin used only for infant feeding items. Do not wash directly in the sink because it may contain germs that could contaminate these items.
- Soak parts of the milk collection set in warm 40–60 $^{\circ}$ C (104–140 $^{\circ}$ F), soapy water for 3~5 minutes.



Fig. 10



- Using a clean brush used only for infant feeding items to scrub items.
- 4) Rinse again: Rinse by holding items under running water, or by submerging them in fresh water in a separate basin that is used only for cleaning infant feeding items. If there is still dirt, repeat step 3 and re-rinse until there is no visible dirt.
- 5) Air-dry thoroughly: Place parts of the milk collection set, wash basin, and bottle brush on a clean, unused dish towel or paper towel in an area protected from dirt and dust. Do not use a dish towel to rub or pat items dry because doing so may transfer germs to the items!



Fig. 11

6) Clean wash basin and bottle brush: Rinse the wash basins and brush well and allow them to air-dry after each use. Wash them every few days by hand with soap and warm water. If your baby is less than 3 months old, was born prematurely, or has a weakened immune system due to illness (such as HIV) or medical treatment (such as chemotherapy for cancer), wash basin and bottle brush after every use.

After Cleaning:

For extra germ removal, disinfect the parts of milk collection set, wash basin, and bottle brush at least once daily after they have been cleaned. Items can be disinfected using boiling water with a disinfection setting. Disinfection is especially important if your baby is less than 3 months old, was born prematurely, or has a weak immune system due to illness or medical treatment.

For the disinfection of milk contact parts, please refer to step 2.

Step 2: Disinfection

Caution:

- Do not sterilize pump parts in a microwave or UV sterilizer. High temperature(> 110 $^{\circ}$ C) will shorten their service life and cause safety hazards.
- Do not sterilize the lid

Before disinfection, make sure you have a cleaned milk collection set, bottle brushes, and wash basins using the methods above. Disinfect all items in contact with milk (even the bottle brush and wash basin!) by using one of the following methods.



- 1) Prepare the below items:
- A household pot
- Drinking-quality water
- Clean tongs



During disinfection with boiling water, prevent the bottle or other parts from touching the sides of the pot. This can cause irreversible product deformation or damage.

2) Place the disassembled milk collection set in the pot and fill the pot with enough water to cover the components to disinfect. Let the water boil for 5-10 minutes, making sure the parts do not touch the sides of the pot.



Fig. 12

3) Remove items with clean tongs.



Fig. 13






Fig. 14

Step 3: Store safely

Store dry items safely until needed. Ensure the clean pump parts, bottle brushes, and wash basins have air-dried thoroughly before storing. Items must be completely dry to help prevent germs and mold from growing. Store dry items in a clean, protected area to prevent contamination.

- 1. Wash hands: Wash hands well with soap and water.
- 2. Put back together: Put together the clean, dry pump parts.
- Store safely. Place reassembled pump parts and other feeding items, wash basin, and dry bottle brush in a clean, protected area such as inside a closed kitchen cabinet that is used only to store clean dishes.

7.3.3 Clean/Disinfect the other parts

The shell of the main unit need to be cleaned and disinfected for the first time and after each use. The other parts, do not come into contact with the human body nor the milk during pumping, and only need to be cleaned when it is dirty.

Cleaning/disinfecting the items at room temperature 5 °C~ 40 °C as below:

Prepare the below items:

- Disinfection
- 70% isopropyl alcohol wipes
- Clean soft cloth

Cleaning method:

- 1. Before performing this cleaning procedure, wash your hands with hand disinfection first.
- 2. Remove all residues from the main unit and/or charging cable using a clean soft cloth.
- 3. Take a piece of 70% isopropyl alcohol wipes to swab on the parts until no visible contaminants remain.
- 4. Dry the device by placing it at room temperature for 10min to evaporate the residual cleaning reagent solution on the product.



Disinfection method:

Cleaning the shell of the main unit as the above method before disinfection.

- 1. Disinfect the shell of the main unit with a soft cloth dampened with the 70% isopropanol for 3 minutes.
- 2. Dry it by placing the main unit at room temperature for 10min to evaporate the residual disinfection solution.

7.4 Direction for use

7.4.1 Preparation before use



- 1. Wash hands with soap and water, and inspect and assemble a clean pump kit.
- 2. Duration of pumping session:

This product is powered by a rechargeable lithium battery, after being fully charged, it can be used for 8-9 sessions (about 270 minutes) of pumping, 30 minutes per session. A typical pumping session lasts about 10-15 minutes per breast, but you should only pump as long as it is comfortable and productive for you.

1. Select Flange Size

This pump includes a 24mm silicone flange. If the flange provided does not fit, you can find flange or flange inserts of 21mm, 19mm, and 17mm available for purchase on Amazon / "momcozy.com". Type "momcozy breast pump accessories" in the search bar and find the flange size and flange insert that fits you.



Fig. 15 select right size

Nipple Measurement (mm)	11-13	13-15	15-17	17-20	20-23	23-26	26-29
Flange (mm)	15	17	19	21	24	27	30

Fig. 16 Flange size chart




2. Stimulate the Nipple

- a) Stimulate your nipple to get a full size (do not skip this step!).
- b) Place the nipple into the smallest hole you can comfortably fit into without forcing it.
- c) Select the hole that can comfortably fit the very base of your nipple.
- d) Get your measurement based on the sizing chart.

3. Test the Flange Fit

- A. To find the suitable size flange, first, you need to make sure you place the flange in the right place on your breast.
- B. Please press the flange on your breast until there is no gap. Make sure your nipple is right in the middle of the flange.



Too Small

Too small: During pumping, if your nipple continues to rub against the inner wall of the flange, then this flange is too small for you.

Good Fit

Suitable fitting: During pumping, if your nipple moves smoothly without rubbing or touching the inner wall of the flange, and almost no areola is sucked inside, then this flange is right for you.

Too Large

Too large: During pumping, if a large area of areola is sucked inside, then this flange is too big for you.





Fig. 19

- Made of stretchy fabric
- No underwire or padding

3 Has a flap

4 Full coverage



Fig. 20



Fig. 21

NO GAP

When you put the pump inside your bra, the silicone flange of this pump should be firmly pressed against your skin without a gap.

IF IT MOVES

If you feel the pump moves during use, please tighten your bra strap to adjust the pump again, or choose another bra.

5. RECOMMEND POSTURE



Always sit or stand upright while pumping to prevent the milk from leaking. This pump is not to be used when lying down or sleeping to ensure the proper orientation is maintained during use.



POSTURE

Make sure the pump and the milk collector always stay at a vertical angle. Otherwise, the milk will spill out.



Fig. 22 right posture

7.4.2 Assembling the Pump



Make sure you have cleaned and disinfected the parts of the breast pump that come into contact with milk or breast.



Warning


- Be careful, when you have disinfected the breast pump parts by boiling them, they
 can be very hot. To prevent burns, only start assembling the breast pump when
 disinfected parts have cooled down.
- Wash your hands thoroughly with soap and water before you touch breast pump parts and breasts to prevent contamination. Avoid touching the inside of milk collection set.

Notes:


 Before each use visually inspect the individual components for cracks, chips, tears, discoloration, or deterioration. In the event that damage to the device is observed, please discontinue use until the parts have been replaced.



Wash your hands thoroughly with soap and water, then assembling the pump as follows:

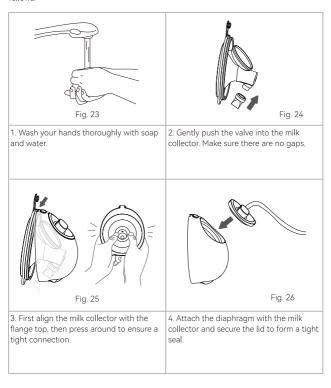



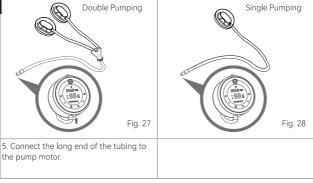

The breast pump is now ready for use.

7.4.3 Pumping instructions



Warning

- · Before you remove the pump body from your breast, always switch off the breast pump to release the vacuum.
- Do not continue pumping for more than 5 minutes at a time if you do not succeed in expressing any milk. Try to express at another time during the day.
- If the process becomes very uncomfortable or painful, stop using the pump and consult your healthcare professional.



Caution:

1. Monitoring milk level during pumping to ensure overfill does not occur.


2.Pumping

- a. Assemble two milk collectors.
- b. Assemble the pump for double pumping.
- c. Put the pump in your bra.




3. Alignment

a. Before pumping, please make sure the pump is pressed tightly on your breast without a gap.



b. To align, hold the flange against your breast so you can see if your nipple is centered in the flange tunnel. You may need to bend forward.

c. After you've aligned, look through the flange to confirm your nipple is centered before pumping. The tip of your nipple should NOT touch the top, sides or bottom of the flange tunnel. If it does, try again.



Correct Alignment Milk expression

Incorrect Alignment
Try again

Fig. 30

Notes:

Correct nipple alignment is key to comfort expression and performance.


Nipple must be positioned correctly in flange tunnel before pumping to avoid discomfort.

Nipple must be positioned correctly in flange tunnel before pumping to avoid discomfort. See Section 7.4.1 Preparation before use-Select Flange Size.

4. Secure pump in bra

Secure Pump in place by bra, taking care to keep Pump pressed firmly against breast. If necessary, tighten bra to keep pump securely in place and start pumping.





5. Starting pumping

Do not slide the pump directly into your bra, follow the step-by-step instructions. Disconnect from charger before use.

A. Turn on the pump

Long press the On/Off O button to turn on the pump.

B. Select the mode

Modes: Stimulation Mode ♥ & Expression Mode ♠ & Mixed Mode (Short press the Mode Selection button to change from 3 modes.

C. Select the vacuum level

Momcozy pump has 15 vacuum pressure settings for each mode, giving you control over what feels comfortable and works most efficiently in all modes. Once you feel uncomfortable, use the Increase / Decrease + - button to adjust the vacuum

D. Screen Lock

After starting the breast pump, if there is no operation for 30 seconds, the lock screen & will begin to flash and remain steady after 3 seconds. The keypad lights will also turn off to ensure that you won't disrupt your breast pumping settings due to accidental key presses. Simply press the power button \bigcup briefly to unlock.

After the screen is locked, and there is no operation for 10 seconds, both the screen and keypad lights will automatically turn off. Touching any key will illuminate the screen, and a brief press of the power button (1) will unlock it.

E. Pressure

Always ensure you are pumping at a comfortable level.

F. Cycle Selection

Under each suction level, there are three cycle options to choose from:

H-**^**∗corresponds to a high cycle under the current suction level.

M- - corresponds to a medium cycle under the current suction level,

L- A-corresponds to a low cycle under the current suction level.

The breast pump defaults to a medium cycle under each suction level upon startup; you can change the cycle by using the cycle adjustment button N to find a comfortable breast pumping rhythm. When you switch to another mode, the breast pump will remember the current level and cycle under that mode.



Every woman is different, so adjust the cycle speed setting to find the speed that works best for you.

G. Setting the Breast Pump Timer

The default timer on the breast pump will start counting down from 30 minutes. If you want to set a different time, follow the steps below:

Before starting breast pumping, press the timer button . The time indicator \$33.33 will start flashing. Use the "+" and "-" keys + — to set the pumping time in five-minute increments. You can set a timer for a maximum of 40 minutes and a minimum of 5 minutes.

Tip: A higher vacuum pressure does not always mean a higher volume of milk. Putting your nipple under excess stress can reduce milk production. Always ensure you are pumping at a comfortable level. If you don't feel suction, please check the pump is assembled correctly.



- * pump should not be used while lying down, engaging in strenuous activities or performing activities with risk of harm.
- * Using a breast pump should not cause pain. Do not try to express with a vacuum pressure setting that is too high or uncomfortable. If excessive discomfort or pain is felt during pumping, stop pumping, break the seal around your nipple and discontinue the session.

6. Pause / Continue Pumping

Press the Pause / Continue button to stop pumping and you will see the pumping time in the LFD screen

Press the Pause / Continue button again to continue your pumping session.


7. Turn off the pump

Long press the On / Off button to turn off the pump.

8. Remove the pump

Use your finger to break the seal between the flange and the breast tissue. Lean slightly forward to remove the pump from the breast after your pumping session, then keep the flange opening side up to prevent milk from pouring over.





We recommend the user stop the pumping session once the expressed milk volume of the milk collector approaches 230 ml to avoid overflow.



• Refrigerate or freeze expressed milk immediately or keep it at a temperature of 16 $^{\circ}$ C $^{\circ}$ C for 2-4 hours before you feed your baby.

7.5 Storing breast milk

7.5.1 Proper storage of breast milk

Following the recommended storage and preparation techniques can maintain the safety and quality of expressed breast milk for the baby's health.

These are general guidelines for storing human milk at different temperatures. Various factors affect how long human milk can be stored safely. Such factors include milk volume, room temperature when milk is expressed, temperature fluctuations in the refrigerator and freezer, and cleanliness of the environment.

Storing breast milk after expressing:

- Refrigerate or chill milk right after it is pumped, if possible. You can put it in the
 refrigerator, place it in a cooler or insulated cooler pack, or freeze it in small (2 to 4
 ounce) batches for later feedings.
- Use breast milk storage bags or clean, food-grade containers to store expressed breast milk. Make sure the containers are made of glass or plastic and have tight-fitting lids.
 - -- Avoid bottles with the recycle symbol number 7, which indicates that the container may be made of BPA-containing plastic.
- Remove air before sealing.
- \bullet Lay bags flat to freeze. To prevent sticking between bags, please separate the bags with paper towels.
- Never store breast milk in disposable bottle liners or plastic bags that are not intended for storing breast milk.
- Gently swirl the container to mix the cream part of the breast milk that may rise to the top back into the rest of the milk. Do not shake the milk. This can make some of the milk's valuable parts break down.
- · Freshly expressed or pumped milk can be stored:



	Storage Location and Temperatures			
Type of Breast Milk	Countertop 77 °F (25 °C) or Colder (room temperature)	Refrigerator 40 °F (4 °C)	Freezer 0°F (-18 °C) or Colder	
Freshly Expressed or Pumped	Up to 4 Hours	Up to 4 Days	Within 6 months is best Up to 12 months is acceptable	
Thawed, Previously Frozen	1–2 Hours	Up to 1 Day (24 hours)	NEVER refreeze human milk after it has been thawed	
Leftover from a Feeding (baby did not finish the bottle)	Use within 2 hours after the baby is finished feeding			

These guidelines are for healthy full-term babies only and may vary for premature or sick babies. Check with your health care provider.

Storage tips:

- Clearly label the storage container with the date it was expressed, including your child's name, if you are giving the milk to a childcare provider.
- Do not store breast milk in the door of the refrigerator or freezer. This will help protect the breast milk from temperature changes from the door opening and closing.
- If you don't think you will use freshly expressed breast milk within 4 days, freeze it right away. This will help to protect the quality of the breast milk.
- When freezing breast milk:
- ·Store small amounts to avoid wasting milk that might not be finished. Store in 2 to 4 ounces or the amount offered at one feeding.
- ·Leave about one inch of space at the top of the container because breast milk expands as it freezes.
- Breast milk can be stored in an insulated cooler with frozen ice packs for up to 24 hours when you are traveling. At your destination, use the milk right away, store it in the refrigerator, or freeze it.

7.5.2 Safe thawing of breast milk

- Always thaw the oldest breast milk first. Remember first in, first out. Over time, the quality of breast milk can decrease.
- There are several ways to thaw your breast milk:
- In the refrigerator overnight.
- ·Set in a container of warm or lukewarm water.
- ·Under lukewarm running water.



- Never thaw or heat breast milk in a microwave. Microwaving can destroy nutrients in breast milk and create hot spots, which can burn a baby's mouth.
- If you thaw breast milk in the refrigerator, use it within 24 hours. Start counting the 24 hours when the breast milk is completely thawed, not from the time when you took it out of the freezer.
- · Once breast milk is brought to room temperature or warmed, use it within 2 hours.
- · Never refreeze breast milk after it has thawed.

8. Transfer

When traveling, please use the charging cable provided and adjust it to the right power source for your current location. Before boarding the plane, please consult the airline for advice about carrying or using this pump on the plane.

Temperature: -20 to 60 °C/-4 to 140 °F Relative Humidity: 15% - 90% Ambient Pressure: 70 - 106kPa

9. Storage Condition

How to store the pump

- * Short-term storage
- * Please keep the breast pump out of direct sunlight. Store the breast pump and its accessories in a safe, clean, and dry place, and away from children.
- * Long-term storage

First, please charge the pump before long-term storage in which way the service life of this pump can be prolonged. Second, keep it in a place away from direct sunlight in avoidance of discoloration. Third, clean and dry the washable parts before storing them.

- * Temperature: -20 to 60 °C / -4 to 140 °F
- * Relative Humidity: 15% 90%
- * Ambient Pressure: 70 to 106 kPa
- * Generally 30 minutes is required to warm from the minimum storage temperature and/or cool from the maximum storage temperature until is is ready for operation.

10. Specification

Model	BP137	
Name	Wearable Breast Pump	
Power requirements	Input: 100-240Vac, 50/60Hz; Output: 5V == 2A (Charge through provided USB 2.0/Type-C Charging cable and self-purchased power adapter)	
Power supply	DC 3.7 V / 2300mAh Rechargeable lithium battery	
Rated power	10W	



Suction modes	Stimulation mode, expression mode, and mixed mode
Vacuum range	Stimulation mode: -55~-175mmHg Expression mode:-100~-300 mmHg Mixed mode: -55~-300 mmHg
Cycle speed	Stimulation mode: 48~98 cycle/min Expression mode: 20~67 cycle/min Mixed mode: 40~83 cycle/min
Dimensions	97.09mm X 104.12mm X 50mm (pump motor) 123mm X 111mm X 72mm (milk collector)
Weight	240g (pump motor weight) 130g (single milk collector weight)
Product use life	500 hours
Noise level	≤48dBA
Type of protection against electric shock	Internally powered equipment
Degree of protection against electric shock	Type BF applied part (milk collection set)
Operating conditions	Temperature: 0°C to 40°C; Humidity: 15% to 90%, Atmospheric pressure: 70 kPa to 106 kPa
Transportation & storage environment	Temperature: -20 °C to 60 °C; Humidity: 15% to 90%, Atmospheric pressure: 70 kPa to 106 kPa
Battery charging time	120 minutes
Battery usage time	270 minutes



11. Maintenance and Replacement Parts

The device contains no user serviceable parts inside: Opening or tampering with this device will void the warranty. In the event the device requires repair, it should be returned to the medical equipment company or to retailer directly. Modification of any kind is prohibited.

The MANUFACTURER will make available on request circuit diagrams, component part lists, descriptions, calibration instructions, or other information that will assist SERVICE PERSONNEL to repair those parts of the device that are designated by the MANUFACTURER as repairable by the SERVICE PERSONNEL. When the product is not used for a long time, the battery will discharge slowly. In order to avoid battery damage due to low voltage for a long time, please charge the device every three months.



The replacement of lithium batteries by inadequately trained personnel could result in a hazard.

Do not clean or maintain the device while the device is in use or while charging.

12. Declaration of Conformity

Shenzhen Root Innovation Technology Co., Ltd. declares that the device conforms to the following standards IEC60601-1, IEC60601-1-2, IEC60601-1-11, IEC62304, ISO10993-5, ISO10993-10, ISO10993-23, ISO10993-1, ISO 14971.

13. Troubleshooting

Problems	Solutions
Pump does not work	If let-down has not yet occurred, consider leaving the pump on breast for longer period of time to observe for possible delayed let-down. Note: Initial milk let-down time is unique for each person and varies by many factors. Check nipple alignment, pause the pump, and remove it from breast. Realign the pump as described below. You may not have the correct Flange size.
Milk does not flow	Pause the pump and remove it from breast. Realign it correctly. You may also separate the pump from the flange to realign. Then, center your nipple in the flange tunnel and bring the pump to your breast.



Need to realign	Pause the pump and remove it from breast. Realign it correctly. You may also separate the pump from the flange to realign. Then, center your nipple in the flange tunnel and bring the pump to your breast.
Feel discomfort while pumping	If you're experiencing excessive discomfort, please try the following: Make sure to press the pump firmly against your breast during Stimulation mode. Tighten bra to make sure the pump is held firmly against the breast. Decrease suction level. Realign the pump. You may be pumping for too long. This pump shuts off automatically after running for 30 minutes. You may not have the correct flange size. Stop and see a medical professional or breastfeeding specialist.
Decreased (low) pump suction	The Pump has 15 suction settings. Press the increase button to increase suction level. Check the condition of your washable parts. They should be replaced after three months of use. If that does not work, try the following: Check connections between all washable parts to ensure all are secure. Susually inspect all washable parts and replace them if damaged. Check that power is on.
Stop pumping	This pump shuts off automatically after running for 30 minutes. Short press Pause/Continue button will pause the pump, press again will resume.
Pump does not stop pumping	Press the Pause/Continue button. If the issue persists, then break the seal by inserting a finger between the breast tissue and the flange. Then press the On/Off button to turn the pump off.
Pump or Charger gets wet (immersed in water).	Dry the pump immediately. Prop the pump upright with charger port down and suction controls up, and let it air dry overnight. Do not use the pump or charger within 24 hours. Contact Customer Care.
Pump is not charging.	Ensure the USB Type-C cable with standard charger (not included) is fully plugged into the pump charging port.

Remark: If the above methods still do not solve the problem, please contact the manufacturer, see the last page for contact information.



14. Disposal



At the end of the product life cycle, do not throw this product into the normal household garbage, but bring it to a collection point for the recycling of electronic equipment and battery. Waste Electrical and Electronic Equipment may have potentially harmful effects on the environment. Improper disposal may lead to the accumulation of harmful toxins in the air, water, and soil, which is harmful to human health. you have obligation to dispose of the device correctly. Consult your municipal authority for information about disposal.

15. Warranty

Please contact the manufacturer in case of a claim under the warranty, the contact information please refer to last page of this user manual. If you have to send the unit, enclose a copy of your receipt with clear statement of defect description.

The warranty terms are as below:

- In case of a warranty claim, the date of purchase has to be proven by means of the sales receipt or invoice.
- 2. Repairs under warranty do not extend the warranty period either for the device or for the replacement parts.
- 3. The following cases are excluded under the warranty
- All damages which are arisen due to improper treatment, e.g. nonobservance of the user instruction.
- All damages which are arisen due to repairs or tampering by the customer or unauthorized third parties.
- Damages which are arisen during transport from the manufacturer to the consumer or during transport to the service center.
- · Accessories which are subject to normal wear and tear.
- · Device damage due to privately disassemble devices.
- Liability for direct or indirect consequential losses caused by the unit is excluded even if the damage to the unit is accepted as a warranty claim.

16. EMC Information

The equipment with following ESSENTIAL PERFORMANCE is intended used in Home healthcare environment facility environment.





Device- Specific Function	Device-Specific Pass/Fail Criteria	Detection/ Testi ng Method
Vacuum strength (mmHg)	Stimulation mode: -55~-175mmHg Expression mode:-100~-300 mmHg Mixed mode: -55~-300 mmHg	Vacuum manometer Observation
Cycle speed (cycles / min)	Stimulation mode: 48~98 cycle/min Expression mode: 20~67 cycle/min Mixed mode: 40~83 cycle/min	Observation
Maximum vacuum	≤-300mmHg	Vacuum manometer Observation
Software for suction pressure regulation	≤-300mmHg	Vacuum manometer Observation
Backflow prevention mechanism	No leakage at maximum vacuum	Observation

If Essential Performance is lost or degraded due to electromagnetic disturbances, this may result in loss of product function or injury to patients, please read below important information before to avoid possible electromagnetic disturbances.



 Using cell phone or microwave oven, HF surgical equipment, magnetic resonance imaging or other radio radiant equipment near this product may cause malfunction.



- Use of this equipment adjacent to or stacked with other equipment should be avoided because it could result in improper operation. If such use is necessary, this equipment and the other equipment should be observed to verify that they are operating normally.
- Portable RF communications equipment (including peripherals such as antenna cables and external antennas) should be used no closer than 30 cm (12 inches) to any part of the Momcozy Wearable Breast Pump, including cables specified by the manufacturer. Otherwise, degradation of the performance of this equipment could result.
- Use of accessories, transducers and cables other than those specified or provided by the manufacturer of this equipment could result in increased electromagnetic emissions or decreased electromagnetic immunity of this equipment and result in improper operation.



- 1) Security, antitheft, and radiofrequency identification (RFID) devices. Some electromagnetic anti- theft systems and metal detectors such as those used at entrances or exits of department stores, libraries, and other public places, and airport security screening devices may affect the Momcozy Wearable Breast Pump. Please do not use Momcozy Wearable Breast Pump near these places. Additionally, RFID devices, which are often used to read identification badges, as well as some tag deactivation devices, such as those used at payment counters at stores and loan desks at libraries, may also affect the Momcozy Wearable Breast Pump. Please do not use Momcozy Wearable Breast Pump are these places. If you have to go through one of these devices, turn off your Momcozy Wearable Breast Pump to ensure it can operate normally.
- 2) Using short-wave diathermy, microwave diathermy, or therapeutic ultrasound diathermy (all now referred to as diathermy) and electrocautery devices near this product may cause malfunction or lead to loss of performance, please do not use Momcozy Wearable Breast Pump near this equipment.

A list of cables and maximum length of cables is as follows:

Cables name	Cable length	Whether shielding
Charging cable	1000±10mm	No



Guidance and manufacture's declaration - electromagnetic emission

The Momcozy Wearable Breast Pump is intended for use in the electromagnetic environment specified below. The customer of the user of the Momcozy Wearable Breast Pump should assure that it is used in such an environment.

Emission test	Compliance	Electromagnetic environment – guidance	
Conducted and Radiated RF emissions CISPR 11	Group 1 Class B	The Momcozy Wearable Breast Pump uses RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause any inter	
Conducted and Radiated RF emissions CISPR 11	Group 1 Class B	The Momcozy Wearable Breast Pump is suitable for use in all establishments, including domestic and those directly connected to the public low-voltage power supply network that supplies buildings used for domestic purposes	
Harmonic emissions IEC 61000-3-2	Class A		
Voltage fluctuations/flicker emissions IEC 61000-3-3	Complies	except for near active HF surgical equipment and the RF shielded room for magnetic resonance imaging.	

Guidance and Manufacturer's Declaration - Electromagnetic Immunity

The Momcozy Wearable Breast Pump is intended for use in the electromagnetic environment specified below. The customer or the user of the Momcozy Wearable Breast Pump should assure that it is used in such an environment.

Immunity Test	IEC 60601-1-2 Test level	Compliance level	Electromagnetic environment- guidance
Electrostatic discharge IEC 61000-4-2	±8 kV contact ±2 kV, ±4kV, ±8 kV, ±15 kV air	±8 kV contact ±2 kV, ±4kV, ±8 kV, ±15 kV air	Floors should be wood, concrete or ceramic tile. If floors are covered with synthetic material, the relative humidity should be at least 30%.



Radiated RF EM fields IEC 61000-4-3	10V/m (Home healthcare environment), 80MHz – 2.7GHz 80% AM at 1kHz	10V/m (Home healthcare environment), 80MHz – 2.7GHz 80% AM at 1kHz	
Electrical fast transients/bursts IEC 61000-4-4	±2kV AC power supply lines; ±1kV DC power/Signal lines. 100 kHz repetition frequency	±2kV AC lines;	power quality should be that of a HOME HEALTHCARE ENVIRONMENT.
Surges IEC 61000-4-5	±0.5kV, ±1kV lines to lines; ±0.5kV, ±1kV, ±2kV lines to earth	±0.5kV, ±1kV lines to lines;	power quality should be that of a HOME HEALTHCARE ENVIRONMENT.
Conducted disturbances induced by RF fields IEC 61000-4-6	3V 0.15MHz – 80MHz, 6V in ISM bands between 0.15MHz and 80MHz 80% AM at 1kHz	3V 0.15MHz – 80MHz, 6V in ISM bands between 0.15MHz and 80MHz 80% AM at 1kHz	power quality should be that of a HOME HEALTHCARE ENVIRONMENT.

Note: The ISM (industrial, scientific and medical) bands between 0,15 MHz and 80 MHz are 6,765 MHz to 6,795 MHz to 13,553 MHz to 13,557 MHz to 27,253 MHz; and 40,66 MHz to 40,70 MHz. The amateur radio bands between 0,15 MHz and 80 MHz are 1,84 MHz to 20 MHz, 3,5 MHz to 4,0 MHz, 3,5 MHz to 10,15 MHz, 14 MHz to 14,2 MHz, 18,07 MHz to 18,17 MHz, 21,0 MHz to 12,4 MHz, 18,07 MHz to 18,17 MHz, 21,0 MHz to 21,4 MHz, 24,89 MHz to 24,99 MHz, 28,0 MHz to 29,7 MHz and 50,0 MHz to 54,0 MHz.

Rated power frequency magnetic fields IEC 61000-4-8	30A/m 50Hz or 60Hz	30A/m 50Hz or 60Hz	Power frequency magnetic fields should be at levels characteristic of a HOME HEALTHCARE ENVIRONMENT.
Voltage dips IEC 61000-4-11	0% UT , 0.5 cycle At 0°, 45°, 90°, 135°, 180°, 225°, 270° and 315°; 0% UT , 1 cycle and 70% UT , 25/30 cycle Single phase: at 0°	Applicable	power quality should be that of a HOME HEALTHCARE FNVIRONMENT
Voltage interruptions IEC 61000-4-11	0% UT , 250/300 cycle	Applicable	ENVIRONIFICIAL.

NOTE: UT is the a.c. mains voltage prior to application of the test level. E.g.: 25/30 means 25 periods at 50 Hz or 30 periods at 60 Hz.



Guidance and manufacture's declaration - electromagnetic immunity

The Momcozy Wearable Breast Pump is intended for use in the electromagnetic environment specified below. The customer or the user of the Momcozy Wearable Breast Pump should assure that it is used in such an environment.

Immunity test	IEC 60601-1- 2 test level	Compliance level	Electromagnetic environment – guidance
Proximity fields from RF wireless communications equipment IEC 61000-4-3	See the following table	Complies	
Proximity magnetic fields IEC 61000-4-39	See the following table	Complies	



Test specifications for ENCLOSURE PORT IMMUNITY to RF wireless communications equipment

Test frequency (MHz)	Band a) (MHz)	Service a)	Modulation	Immunity Test Level (V/m)
385	380 - 390	TETRA 400	Pulse modulation ^{b)} 18 Hz	27
450	430 - 470	GMRS 460, FRS 460	FM a ± 5 kHz deviation 1 kHz sine	28
710				
745	704 – 787	LTE Band 13, 17	Pulse modulation ^{b)} 217 Hz	9
780				
810		GSM 800/900,		
870	800 – 960	TETRA OOO IDENI	Pulse modulation ^{b)} 18 Hz	28
930		LTE Band 5		
1720		GSM 1800; CDMA		
1845	1700 – 1990	1900; GSM 1900; DECT; LTE Band 1, 3.	Pulse modulation ^{b)} 217 Hz	28
1970		4, 25; ÚMTS		
2450	2400 – 2570	Bluetooth, WLAN, 802.11 b/g/n, RFID 2450, LTE Band 7	Pulse modulation ^{b)} 217 Hz	28
5240				
5500	5100 - 5800	WLAN 802.11 a/n	Pulse modulation ^{b)} 217 Hz	9
5785				

NOTE If necessary to achieve the IMMUNITY TEST LEVEL, the distance between the transmitting antenna and the ME EQUIPMENT or ME SYSTEM may be reduced to 1 m. The 1 m test distance is permitted by IEC 61000-4-3.

b) The carrier shall be modulated using a 50 % duty cycle square wave signal.

a) For some services, only the uplink frequencies are included.

c) As an alternative to FM modulation, the carrier may be pulse modulated using a 50% duty cycle squire wave signal at 18 Hz, While it does not represent actual modulation, it would be worst case.



Test specifications for enclosure port immunity to proximity magnetic files

Test frequency	Modulation	Immunity test level (A/M)
30 kHz ^{a)}	CW	8
134.2 kHz	Pulse modulation ^{b)} 2.1 kHz	65 ^{c)}
13.56 MHz	Pulse modulation b) 50 kHz	7.5 ⁰

a) This test is applicable only to ME EQUIPMENT and ME SYSTEMS intended for use in the home he althcare environment.

17. Reporting Adverse Events

MedWatch is the Food and Drug Administration's (FDA) program for reporting serious reactions, product quality problems, therapeutic inequivalence/failure, and product use errors with human medical products, including drugs, biologic products, medical devices, dietary supplements, infant formula, and cosmetics.

If you think you or someone in your family has experienced a serious reaction to a medical product, you are encouraged to take the reporting form to your doctor. Your health care provider can provide clinical information based on your medical record that can help FDA evaluate your report.

However, we understand that for a variety of reasons, you may not wish to have the form filled out by your health care provider, or your health care provider may choose not to complete the form. Your health care provider is NOT required to report to the FDA. In these situations, you may complete the Online Reporting Form yourself. You will receive an acknowledgement from FDA when your report is received. Reports are reviewed by FDA staff. You will be personally contacted only if we need additional information.

Submitting Adverse Event Reports to FDA

Use one of the methods below to submit voluntary adverse event reports to the FDA:

1) Report Online at:

www.access data.fda.gov/scripts/medwatch/index.cfm? action=reporting.home

2) Consumer Reporting Form FDA 3500B. Follow the instructions on the form to either fax or mail it in for submission. For help filling out the form, see MedWatchLearn. The form is available at:

www.fda.gov/downloads/aboutFDA/reportsmanualsforms/forms/ucm349464.pdf

- 3) Call FDA at 1-800-FDA-1088 to report by telephone
- a) Reporting Form FDA 3500 commonly used by health professionals. The form is available at:

www.fda.gov/downloads/aboutFDA/reportmanualsforms/forms/ucm163919.pdf

b) The carrier shall be modulated using a 50% duty cycle square wave signal.

c) r.m.s, before modulation is applied



18. Travel or International Use Statement

Since the performance of the Momcozy Wearable Breast Pump may be affected by the external environment, in view of the uncertainty and instability of the travel environment, please do not use the device during travel or on the aircraft.

The Momcozy Wearable Breast Pump can be internationally used, but it must be used and stored in the environment specified in this user manual, and please make sure the input power of your power adapter is AC 100-240V 50/60 Hz and output power is DC 5V==2A, and please make sure you have a converter to convert to the proper voltage of the target country. To ensure that the Momcozy Wearable Breast Pump is not affected during carrying, please check the following items before use to ensure it can operate normally:

- Check the Momcozy Wearable Breast Pump to ensure that it is free from damage and cracks.
- $\bullet\,$ Before each usage, check the status of your Momcozy Wearable Breast Pump to ensure it can operate normally.

If there is any abnormality, please stop using it.

19. Manufacturer Information



Shenzhen Root Innovation Technology Co.,Ltd. #2-201, Floor 2, Hasee Computer Building, No.2 Beier Rd, Bantian Street, Longgang, Shenzhen, Guangdong, China, 518129

E-mail: support@momcozy.com

If assistance in setting up, using, or maintaining the device when needed or to report unexpected operation or events, please contact us.

20.FCC Compliance Statement

Any Changes or modifications not expressly approved by the party responsible for compliance could void the user's authority to operate the equipment.

This device complies with part 15 of the FCC Rules. Operation is subject to the following two conditions: (1) This device may not cause harmful interference, and (2) this device must accept any interference received, including interference that may cause undesired operation.

IMPORTANT NOTE:

Note: This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates, uses and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one or more of the following measures:

- Reorient or relocate the receiving antenna.
- Increase the separation between the equipment and receiver.
- Connect the equipment into an outlet on a circuit different from that to which the receiver is connected.
- Consult the dealer or an experienced radio/TV technician for help.