### Omnipod® 5 Automated Insulin Delivery System


# **HCP Quick Glance Guide**



## **CGM VALUES & TRENDS**

## How CGM Values & Trends Affect Automated Insulin Delivery

Every 5 minutes, SmartAdjust™ technology receives a CGM value and predicts where glucose will be 60 minutes into the future. It then automatically increases, decreases or pauses insulin delivery based upon the user's chosen Target Glucose value.

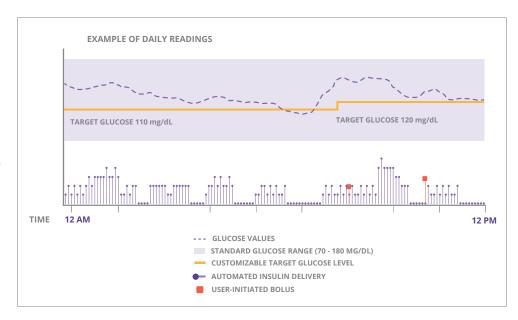

## **Adjustable Settings**

#### **AUTOMATED MODE**

**Target Glucose** is the ONLY adjustable setting that directly impacts automated insulin delivery.

- Customizable and can include up to 8 time segments.
- Ranges from 110-150 mg/dL in 10 mg/dL increments.
- Used as the target for BOTH automated insulin delivery AND correction bolus dosing.

#### **MANUAL MODE**

**Basal Programs** for basal insulin delivery.

Adjusting basal rates ONLY impacts Manual Mode basal insulin delivery.

## SMARTBOLUS CALCULATOR AUTOMATED & MANUAL MODE

SmartBolus Calculator settings impact suggested bolus doses in BOTH modes. These include:

- Target Glucose & Correct Above
- Insulin to Carb Ratio
- Correction Factor
- Reverse Correction
- Duration of Insulin Action
- Minimum Glucose for Calculations

#### NOTE:

 Insulin to Carb Ratios can be programmed in 0.1 g carb/U increments



## **HCP Quick Glance Guide**

# omni pod 5

#### **HOW TO EDIT TARGET GLUCOSE**



• Tap the Menu button on the Home screen



 Tap **Settings** to expand list

Tap Bolus



 Tap Target Glucose & Correct Above



Tap **NEXT**



 Tap on the segment you want to edit. Edit time, Target Glucose and/or Correct Above.

 Tap **NEXT** to add/edit more segments as needed.



 Review changes and tap **SAVE**.

#### NOTE:

Follow these steps to adjust settings for:

- Insulin to Carb Ratio
- Correction Factor
- Reverse Correction
- Duration of Insulin Action
- Minimum Glucose for Calculations

#### **HOW TO VIEW HISTORY & CGM GRAPH**



• Tap the Menu button on the Home screen



Tap History Detail



 The SUMMARY section includes CGM, Insulin, and Carb details.



 Tap AUTO EVENTS to see automated event details

#### **CGM GRAPH**

The CGM graph shows most recent CGM readings as well as insulin delivery history. This includes times that SmartAdjust technology paused insulin, maximum basal insulin was delivered, or a bolus was given.



 Tap View on the Home screen



The Omnipod® 5 Automated Insulin Delivery System is indicated for use by individuals with Type 1 diabetes mellitus in persons 2 years of age and older. The Omnipod 5 System is intended for single patient, home use and requires a prescription. The Omnipod 5 System is compatible with the following U-100 insulins: NovoLog®, Humalog®, and Admelog®.

Refer to the Omnipod 5 Automated Insulin Delivery System User Guide at www.omnipod.com/safety for complete safety information including indications, contraindications, warnings, cautions, and instructions. ©2022 Insulet Corporation. Omnipod, the Omnipod 5 logo and SmartAdjust are trademarks or registered trademarks of Insulet Corporation in the United States of America and other various jurisdictions. All rights reserved. All other trademarks are the property of their respective owners. The use of third party trademarks does not constitute an endorsement or imply a relationship or other affiliation. INS-OHS-11-2021-00012 V.2.0