


SOLAR CELL I-V TEST SYSTEM (AUTOMATED) USER MANUAL

Manual Version: 1.0.G

Product Code: T2003

Product Version: 2.0

Software Version: 1.0

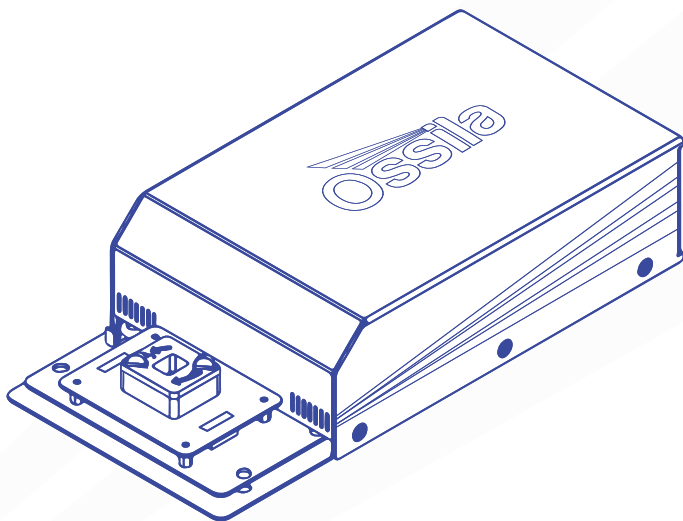

Contents

1. Overview.....	4
2. EU Declaration of Conformity (DoC).....	5
3. Safety	8
3.1 Use of Equipment.....	8
3.2 Hazard Icons.....	8
3.3 General Hazards	8
3.4 Power Cord Safety.....	8
3.5 Servicing.....	9
3.6 Health and Safety – Servicing.....	9
4. Requirements	9
5. Unpacking	10
5.1 Packing List	10
5.2 Damage Inspection.....	10
6. Specifications	10
7. System Components.....	11
8. Installation	12
9. Operation	12
9.1 Measurement Types	12
9.2 Quickstart Guide	14
9.3 Shared Software Settings.....	15
9.4 Solar Cell Characterisation Settings	17
9.5 Solar Lifetime Measurement Settings.....	18
9.6 Stabilised Current Output Settings	20
9.7 Saving and Loading Settings	20
9.8 Saving Results.....	21
9.9 Controls.....	23
9.10 Test Device.....	24
10. Troubleshooting.....	26
11. Related Products.....	27
11.1 Related Consumables.....	27
11.2 Related Equipment.....	27

1. Overview

The Ossila Solar Cell I-V Test System is a low-cost solution for reliable current-voltage characterisation of solar cells. The system is controlled by specially-designed software which can perform multiple I-V measurements, determine key metrics of solar cells, and measure these properties over long periods of time. The automated version of the system enables automatic switching between pixels, making measurements faster and easier.



2. EU Declaration of Conformity (DoC)

We

Company Name: Ossila Limited

Postal Address: Solpro Business Park, Windsor Street.

Postcode: S4 7WB

City: Sheffield

Telephone number: +44 (0)114 2999 180

Email Address: info@ossila.com

**declare that the DoC is issued under our sole responsibility
and belongs to the following product:**

Product: Solar Cell I-V Test System – Automated (T2003A2 / T2003B2 / T2003C2 /
T2003E2)

Serial number: T2003A2-xxxx, T2003B2-xxxx, T2003C2-xxxx, T2003E2-xxxx

Object of declaration:

Solar Cell I-V Test System – Automated (T2003A2 / T2003B2 / T2003C2 / T2003E2)

**The object of declaration described above is in conformity
with the relevant Union harmonisation legislation:**

EMC Directive 2014/30/EU

RoHS Directive 2011/65/EU

Signed:



Name: Dr James Kingsley

Place: Sheffield

Date: 07/12/2020

[Декларация] за съответствие на ЕС

Производител: Ossila Ltd., Solpro Business Park, Windsor Street, S4 7WD, Великобритания

Декларира с цялата си отговорност, че посоченото оборудване съответства на приложимото законодателство на ЕС за хармонизиране, посочено на предходната(-ите) страница(-и) на настоящия документ.

[Čeština] Prohlášení o shodě EU

Výrobce: Ossila Ltd., Solpro Business Park, Windsor Street, S4 7WD, Spojené Království

Prohlášíme na vlastní odpovědnost, že uvedené zařízení je v souladu s příslušnými harmonizačními předpisy EU uvedenými na předchozích stranách tohoto dokumentu.

[Dansk] EU-overensstemme Iserklæring

Producent: Ossila Ltd., Solpro Business Park, Windsor Street, S4 7WD, UK

Erklærer herved, at vi alene er ansvarlige for, at det nævnte udstyr er i overensstemmelse med den relevante EU-harmoniseringslovgivning, der er anført på den/de foregående side(r) i dette dokument.

[Deutsch] EU-Konformitätserklärung

Hersteller: Ossila Ltd., Solpro Business Park, Windsor Street, S4 7WD, Vereinigtes Königreich

Wir erklären in alleiniger Verantwortung, dass das aufgeführte Gerät konform mit der relevanten EU-Harmonisierungsgesetzgebung auf den vorangegangenen Seiten dieses Dokuments ist.

[Eesti keel] ELi vastavusavaldus

Tootja: Ossila Ltd., Solpro Business Park, Windsor Street, S4 7WD, UK

Kinnitame oma ainuvastutust, et loetletud seadmed on kooskõlas antud dokumendi eelmisel leheküljel / eelmistel lehekülgedel ära toodud asjaomaste ELi ühtlustamise õigusaktidega.

[Ελληνικά] Δήλωση πιστότητας ΕΕ

Κατασκευαστής: Ossila Ltd., Solpro Business Park, Windsor Street, S4 7WD, Ηνωμένο Βασίλειο

Δηλώνουμε υπεύθυνα ότι ο αναφερόμενος εξοπλισμός συμμορφώνεται με τη σχετική νομοθεσία εναρμόνισης της ΕΕ που υπάρχει στις προηγούμενες σελίδες του παρόντος εγγράφου.

[Español] Declaración de conformidad UE

Fabricante: Ossila Ltd., Solpro Business Park, Windsor Street, S4 7WD, Reino Unido

Declaramos bajo nuestra única responsabilidad que el siguiente producto se ajusta a la pertinente legislación de armonización de la UE enumerada en las páginas anteriores de este documento.

[Français] Déclaration de conformité UE

Fabricant: Ossila Ltd., Solpro Business Park, Windsor Street, S4 7WD, Royaume-Uni

Déclarons sous notre seule responsabilité que le matériel mentionné est conforme à la législation en vigueur de l'UE présentée sur la/les page(s) précédente(s) de ce document.

[Hrvatski] E.U izjava o sukladnosti

Proizvođač: Ossila Ltd., Solpro Business Park, Windsor Street, S4 7WD, Velika Britanija

Izjavljujemo na vlastitu odgovornost da je navedena oprema sukladna s mjerodavnim zakonodavstvom EU-a o usklađivanju koje je navedeno na prethodnoj(nim) stranici(ama) ovoga dokumenta.

[Italiano] Dichiarazione di conformità UE

Produttore: Ossila Ltd., Solpro Business Park, Windsor Street, S4 7WD, UK

Si dichiara sotto la propria personale responsabilità che l'apparecchiatura in elenco è conforme alla normativa di armonizzazione UE rilevante indicata nelle pagine precedenti del presente documento.

[Latviešu] ES atbilstības deklarācija

Ražotājs: Ossila Ltd., Solpro Business Park, Windsor Street, S4 7WD, UK

Ar pilnu atbildību paziņojam, ka uzskaitītais aprīkojums atbilst attiecīgajiem ES saskaņošanas tiesību aktiem, kas minēti iepriekšējās šī dokumenta lapās.

[Lietuvių k.]

ES atitikties deklaracija

Gamintojas: Ossila Ltd., Solpro Business Park, Windsor Street, S4 7WD, UK

atsakingai pareiškia, kad išvardinta įranga atitinka aktualius ES harmonizavimo teisės aktus, nurodytus ankstesniuose šio dokumento

[Magyar]

EU-s megfelelőségi nyilatkozat

Gyártó: Ossila Ltd., Solpro Business Park, Windsor Street, S4 7WD, UK

Kizárólagos felelősségünk mellett kijelentjük, hogy a felsorolt eszköz megfelel az ezen dokumentum előző oldalán/oldalain található EU-s összehangolt jogszabályokra vonatkozó rendelkezéseinek.

[Nederlands]

EU-Conformiteitsverklaring

Fabrikant: Ossila Ltd., Solpro Business Park, Windsor Street, S4 7WD, UK

Verklaart onder onze uitsluitende verantwoordelijkheid dat de vermelde apparatuur in overeenstemming is met de relevante harmonisatiewetgeving van de EU op de vorige pagina(s) van dit document.

[Norsk]

EU-samsvarserklæring

Produsent: Ossila Ltd., Solpro Business Park, Windsor Street, S4 7WD, UK

Erklærer under vårt eneansvar at utstyret oppført er i overholdelse med relevant EU-harmoniseringslovverk som står på de(n) forrige siden(e) i dette dokumentet.

[Polski]

Deklaracja zgodności Unii Europejskiej

Producent: Ossila Ltd., Solpro Business Park, Windsor Street, S4 7WD, UK

Oświadczamy na własną odpowiedzialność, że podane urządzenie jest zgodne ze stosownymi przepisami harmonizacyjnymi Unii Europejskiej, które przedstawiono na poprzednich stronach niniejszego dokumentu.

[Por tuuguês]

Declaração de Conformidade UE

Fabricante: Ossila Ltd., Solpro Business Park, Windsor Street, S4 7WD, Reino Unido

Declara sob sua exclusiva responsabilidade que o equipamento indicado está em conformidade com a legislação de harmonização relevante da UE mencionada na(s) página(s) anterior(es) deste documento.

[Română]

Declarație de conformitate UE

Producător: Ossila Ltd., Solpro Business Park, Windsor Street, S4 7WD, Regatul Unit

Declară pe proprie răspundere că echipamentul prezentat este în conformitate cu prevederile legislației UE de armonizare aplicabile prezentate la pagina/paginile anterioare a/ale acestui document.

[Slovensky]

Vyhlasenie o zhode pre EÚ

Výrobca: Ossila Ltd., Solpro Business Park, Windsor Street, S4 7WD, Spojené kráľovstvo

Na vlastnú zodpovednosť prehlasuje, že uvedené zariadenie je v súlade s príslušnými právnymi predpismi EÚ o harmonizácii uvedenými na predchádzajúcich stranách tohto dokumentu.

[Slovenščina]

Izjava EU o skladnosti

Proizvajalec: Ossila Ltd., Solpro Business Park, Windsor Street, S4 7WD, UK

s polno odgovornostjo izjavlja, da je navedena oprema skladna z veljavno uskladitveno zakonodajo EU, navedeno na prejšnji strani/ prejšnjih straneh tega dokumenta.

[Suomi]

EU-vaatimusten mukaisuusvakuutus

Valmistaja: Ossila Ltd., Solpro Business Park, Windsor Street, S4 7WD, UK

Vakuutamme täten olevamme yksin vastuussa siitä, että tässä asiakirjassa luettellut laitteet ovat tämän asiakirjan sivuilla edellisillä sivuilla kuvattujen olennaisen yhdenmukaistamista koskevien EU-säädösten vaatimusten mukaisia.

[Svenska]

EU-försäkran om överensstämmelse

Tillverkare: Ossila Ltd., Solpro Business Park, Windsor Street, S4 7WD, Storbritannien

Vi intygar härmed att den utrustning som förtecknas överensstämmer med relevanta förordningar gällande EU-harmonisering som finns på föregående sidor i detta dokument.

3. Safety

3.1 Use of Equipment

The Ossila Solar Cell I-V Test System (Automated) is designed to be used as instructed. It is intended for use under the following conditions:

- Indoors in a laboratory environment (Pollution Degree 2)
- Altitudes up to 2000m
- Temperatures of 5°C to 40°C; maximum relative humidity of 80% up to 31°C.

The unit is supplied with a 24 VDC/ 2A power adapter with a power cord for the country of purchase, in accordance with European Commission regulations and British Standards. Use of any other electrical power cables, adaptors, or transformers is not recommended

3.2 Hazard Icons

The following symbols can be found at points throughout the manual. Note and read each warning before attempting any associated operations associated with it:

Table 3.1. Hazard warning labels used in this manual.

Symbol	Associated Hazard
	Electrical shock

3.3 General Hazards

Before installing or operating the Solar Cell I-V Test System (Automated), there are several health and safety precautions which must be observed to ensure safe installation and operation.

3.4 Power Cord Safety



Emergency power disconnect options: use the power cord as a disconnecting method and remove from wall. To facilitate disconnect, make sure the power outlet for this cord is readily accessible to the operator.

3.5 Servicing

If servicing is required, please return the unit to Ossila Ltd. The warranty will be invalidated if:

- Modification or service has been carried out by anyone other than an Ossila engineer.
- The Unit has been subjected to chemical damage through improper use.
- The Unit has been operated outside the usage parameters stated in the user documentation associated with the Unit.
- The Unit has been rendered inoperable through accident, misuse, contamination, improper maintenance, modification, or other external causes.

3.6 Health and Safety – Servicing



Servicing should only be performed by an Ossila engineer. Any modification or alteration may damage the equipment, cause injury, or death. It will also void your equipment's warranty.

4. Requirements

The system requires a computer running Windows (Vista or newer) with an available USB port or a network connection. Further details are given in **Table 4.1**.

Table 4.1. Solar Cell I-V Test System requirements.

Power	24 VDC / 2A
Operating System	Windows 10
CPU	Dual Core 2 GHz or faster
RAM	2 GB
Available Hard Drive Space	178 MB
Monitor Resolution	1680 x 1050 or larger
Connectivity	USB 2.0 or newer, or Ethernet (requires DHCP)

5. Unpacking

5.1 Packing List

The standard items included with the Ossila Solar Cell I-V Test System – Automated are:

- Ossila Solar Cell I-V Test System – Automated.
- 24 VDC / 2A power adapter with a cord set specifically for country of operation (UK, USA, EU, or AU).
- USB-B cable.
- USB memory stick pre-loaded with the user manual, quality control data, and software installer.
- Printed copy of the user manual.

5.2 Damage Inspection

Examine the components for evidence of shipping damage. If damage has occurred, please contact Ossila directly for further action. The shipping packaging will come with a shock indicator to show if there has been any mishandling of the package during transportation.

6. Specifications

The Solar Cell I-V Test System – Automated specifications are shown in **Table 6.1**,

Table 6.1. Solar Cell I-V Test System – Automated specifications.

Voltage range	$\pm 333\text{ }\mu\text{V}$ to $\pm 10\text{ V}$
Current range	$\pm 10\text{ nA}$ to $\pm 150\text{ mA}$
Substrate Size	20 mm x 15 mm
Substrate Compatibility (T2003A)	S101 (OLED substrates)
Substrate Compatibility (T2003B)	S211 (PV substrates)
Substrate Compatibility (T2003C)	S171 (Pixelated cathode substrates)
Overall Dimensions	Width: 155 mm Height: 73 mm Depth: 317 mm

7. System Components

The Solar Cell I-V Test System – Automated comprises three items: the Solar Cell I-V Test System (**Figure 7.1**), power adaptor (**Figure 7.2**), and the Solar Cell I-V software (**Figure 7.3**).

Figure 7.1. Solar Cell I-V Test System.

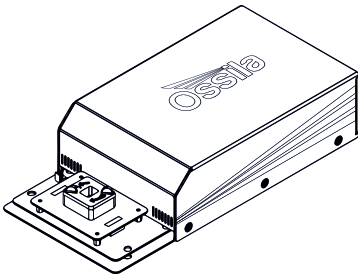


Figure 7.2. The 18V DC power adaptor


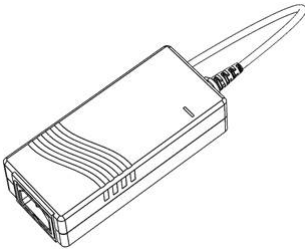


Figure 7.3. Solar Cell I-V Test System software.

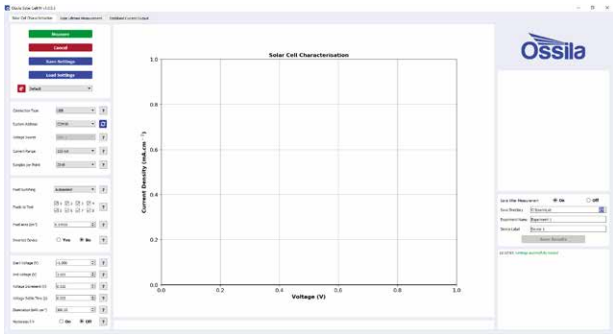

8. Installation

1. Install the Solar Cell I-V software on your PC.
 - I. Run the file 'Ossila-Solar-Cell-IV-Installer-vX-X-X-X.exe' on the USB memory stick provided.
 - II. Follow the on-screen instructions to install the software.
2. Connect the 24 VDC power adaptor to the power socket on the rear of the unit.
3. Connect the unit to your PC using the provided USB-B cable, or an Ethernet cable if preferred.

Note: The Solar Cell I-V software can also be downloaded from
www.ossila.com/pages/downloads

9. Operation

9.1 Measurement Types

The Solar Cell I-V software can perform three different types of measurements. Each measurement type can be selected using the tabs at the top of the window. The available measurements are:

1. Solar Cell Characterisation (**Section 9.1.1**).
2. Solar Lifetime Measurement (**Section 9.1.2**).
3. Stabilised Current Output (**Section 9.1.3**).


Each measurement type requires several settings to be selected before it can be performed. Settings that are shared between all measurements are detailed in **Section 9.2**. Measurement-specific settings are detailed in **Sections 9.4, 9.5, and 9.6**.

9.1.1 Solar Cell Characterisation

The Solar Cell Characterisation tab performs current-voltage (I-V) measurement and analysis of solar cells. The analysis calculates the following properties:

- Power conversion efficiency (PCE)
- Fill factor (FF)
- Short-circuit current density (J_{sc})
- Open-circuit voltage (V_{oc})
- Shunt resistance (R_{sh})
- Series resistance (R_s)


Figure 9.2. Solar Cell I-V software: The Solar Lifetime Measurement tab.

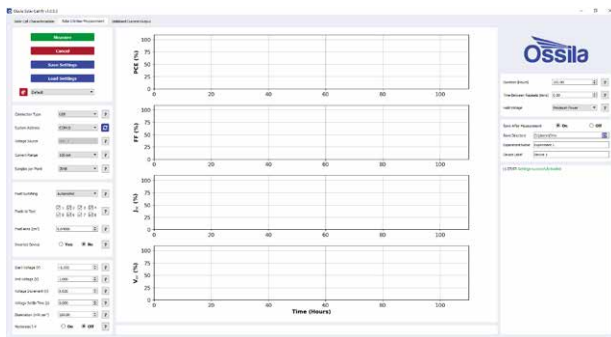

9.1.3 Stabilised Current Output

The Stabilised Current Output tab lets you measure the evolution of the photogenerated current at specific voltages.

Figure 9.3. Solar Cell I-V software: The Stabilised Current Output tab.

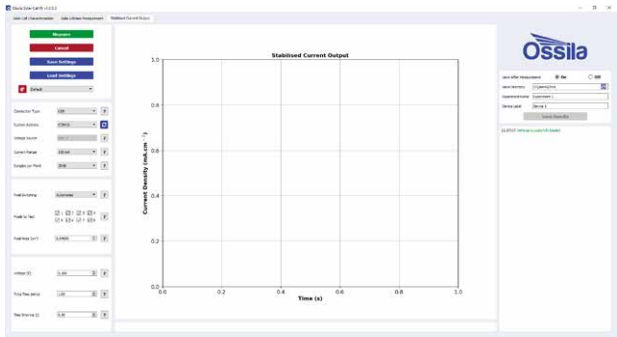

9.2 Quickstart Guide

1. Start the Ossila Solar Cell I-V software. The window shown in **Figure 9.1** will open.
2. Choose a measurement type as described in **Section 9.1**.
3. Place your sample in the test board.
4. Place the test board beneath your solar simulator.
5. Set the appropriate settings in the software (explained in more detail in **Sections 9.4 - 9.8**).
 - I. Set 'Pixel Switching' to 'Automated'.
6. Open the shutter of your solar simulator.
7. Click the 'Measure' button.
 - I. For each pixel, measurements are performed using the chosen measurement settings.
 - II. After the measurement has completed, the results are displayed in the central plot.
 - III. This process is repeated until all pixels have been measured.
8. If automatic saving is turned on, the measurement data and settings will then be saved.

9.3 Shared Software Settings

The settings in these sections are shared between all measurement types.

9.3.1 Connection

Figure 9.4. Connection settings.

Connection Type	USB	?
System Address	COM10	↻

(I) **Connection Type**

- Select the type of connection you are using (either USB or Ethernet).
 - I. Any connected units will be automatically detected when a selection is made and the 'System Address' box will be populated.
- The software will search for units connected via USB on start-up.
 - I. To rescan for connected units (in case the connection is changed), click the refresh icon next to the 'System Address' box.

(II) **System Address**

- Select the COM port or IP address of the connected unit you intend to use (USB and Ethernet connection respectively).
 - I. This box will be populated automatically with the addresses of any units connected to the computer via the method selected in the 'Connection Type' box.

9.3.2 System Settings

Figure 9.5. System settings.

Voltage Source	SMU 1	?
Current Range	150 mA	?
Samples per Point	2048	?

(I) **Voltage Source**

- SMU 1' will be automatically selected when pixel switching is set to 'Automated'.

(II) Range

- Select the range of currents to be used for the measurement.
 - I. This defines the upper limit and accuracy of current measurements that can be performed by the unit. The values for each range are given in Table 9.1.
 - II. The maximum current values for each range are also shown in the range selection box.

Table 9.1. Maximum current and accuracy for the different range settings for the Solar Cell I-V Test System.

Range	Maximum Current	Accuracy
1	±150 mA	±200 µA
2	±20 mA	±10 µA
3	±2000 µA	±1 µA
4	±200 µA	±100 nA
5	±20 µA	±10 nA

9.3.3 Device Details

Figure 9.6. Device Details settings.

Pixel Switching

Automated

?

Pixels to Test

☒ 1 ☒ 2 ☒ 3 ☒ 4

☒ 5 ☒ 6 ☒ 7 ☒ 8

?

Pixel Area (cm²)

0.04000

?

Inverted Device

☐ Yes ☒ No

?

(I) Pixel Switching

- Select 'Automated' in the pixel switching setting.

(II) Pixels to Test

- Select which pixels to measure.
 - I. The pixel numbers are labelled on the test board.

(III) Pixel Area

- Set the are in cm^2 of each pixel in the device.

(IV) Inverted Device

- Set whether the device to be measured is inverted.
 - I. This option should be on if the anode of your device connects to the 'cathode' pins in the device holder.

9.4 Solar Cell Characterisation Settings

9.4.1 Measurement Settings

Figure 9.7. Measurement Settings for the solar characterisation and lifetime measurements.

Start Voltage (V)	-1.000	?
End Voltage (V)	1.000	?
Voltage Increment (V)	0.020	?
Voltage Settle Time (s)	0.000	?
Illumination ($\text{mW} \cdot \text{cm}^{-2}$)	100.00	?
Hysteresis I-V	☐ On ☒ Off	?

(I) Start Voltage

- Set the voltage in volts at which to start the current-voltage measurement.
 - I. This can be set between -10 V and +10 V.

(II) End Voltage

- Set the voltage in volts at which to end the current-voltage measurement.
 - I. This can be set between -10 V and +10 V.

(III) Voltage Increment

- Set the step size in volts for changing the voltage during current-voltage measurement.

(IV) Voltage Settle Time

- Set the time in seconds between applying a voltage and measuring the current.
I. This has a maximum of 10 seconds.

(V) Illumination

- Set the illumination intensity (in mA.cm^{-2}) being used during the measurement.

(VI) Hysteresis I-V

- This option performs a reverse current-voltage measurement after the forward current-voltage measurement has completed.
I. This reverses the set start and end voltages and uses the same voltage increment and settle time as the forward measurement.

9.5 Solar Lifetime Measurement Settings

9.5.1 Measurement Settings

Figure 9.8. Measurement Settings for the solar characterisation and lifetime measurements.

Start Voltage (V)	-1.000	<input "="" type="button" value="?"/>
End Voltage (V)	1.000	<input "="" type="button" value="?"/>
Voltage Increment (V)	0.020	<input "="" type="button" value="?"/>
Voltage Settle Time (s)	0.000	<input "="" type="button" value="?"/>
Illumination (mW.cm^{-2})	100.00	<input "="" type="button" value="?"/>
Hysteresis I-V	☐ On ☒ Off	?

(I) Start Voltage

- Set the voltage in volts at which to start the current-voltage measurement.
I. This can be set between -10 V and +10 V.

(II) End Voltage

- Set the voltage in volts at which to end the current-voltage measurement.
I. This can be set between -10 V and +10 V.

(III) Voltage Increment

- Set the step size in volts for changing the voltage during current-voltage measurement.

(IV) Voltage Settle Time

- Set the time in seconds between applying a voltage and measuring the current.
 - I. This has a maximum of 10 seconds.

(V) Illumination

- Set the illumination intensity (in mA.cm⁻²) being used during the measurement.

(VI) Hysteresis I-V

- This option performs a reverse current-voltage measurement after the forward current-voltage measurement has completed.
 - I. This reverses the set start and end voltages and uses the same voltage increment and settle time as the forward measurement.

9.5.2 Lifetime Parameters

Figure 9.9. Lifetime Parameters settings.

Duration (Hours)	100.00	?
Time Between Repeats (mins)	0.00	?
Hold Voltage	Maximum Power	?

(I) Duration

- Set the total duration in hours of the lifetime measurement.

(II) Time Between Repeats

- Set the time interval in minutes between performing repeat current-voltage measurements of the device.

(III) Hold Voltage


- Set the voltage that all pixels will be held at between measurements.
- This can be set as:
 - I. Short-Circuit – hold at 0 V.
 - II. Maximum Power – hold at the average maximum power point determined from most recent current-voltage curve.
 - III. Open-Circuit – hold at the average open-circuit voltage determined from the most recent current-voltage curve.

Note: As the voltage source is only a single channel, the hold voltage will be the same for all pixels being tested.

9.6 Stabilised Current Output Settings

9.6.1 Measurement Settings

Figure 9.10. Experimental Parameters settings for the Stabilised Current Output.

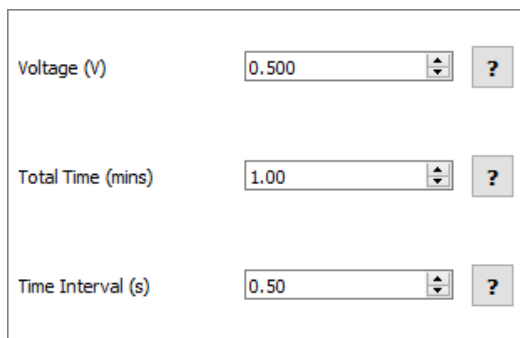

Voltage (V)	0.500	?
Total Time (mins)	1.00	?
Time Interval (s)	0.50	?

(I) Voltage

- Set the voltage to apply to the sample for the measurement.
 - I. This can be set between -10 V and +10 V.

(II) Total Time


- Set the total length of the measurement in minutes.

(III) Time Interval

- Set the time between each current measurement in seconds.
 - I. This has a minimum of 0.1 seconds.

9.7 Saving and Loading Settings

Figure 9.11. Controls for saving and loading settings profiles.

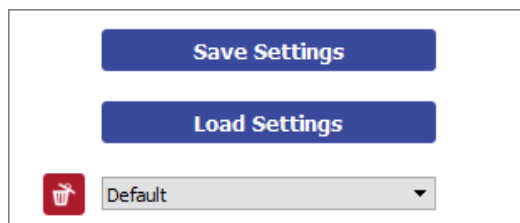

Save Settings

Load Settings

 Default

(I) Save Settings

- Saves the current settings as a profile that can be loaded quickly for use at another time.
- When clicked, you will be prompted to name the settings profile.
 - I. If the name is already in use, you will be asked if you wish to overwrite the previous profile.
 - II. The name cannot contain the characters: \ / : * ? " < > |
 - III. You can change the default settings by choosing the name 'Default'.
- The settings profile will be added to the drop-down box using the given name.

(II) Load Settings


- Opens a dialog box to navigate to a settings file that has been created as part of a previous measurement.
 - I. The settings fields will be populated with the values in the settings file.

(III) Settings Profiles

- Select a saved settings profile from the drop-down box.
 - I. The settings fields will be populated with the saved values.
- Settings profiles can be deleted by selecting the profile, and then clicking the red 'delete' icon next to the drop-down box.

9.8 Saving Results

Figure 9.12. Saving measurement data settings.

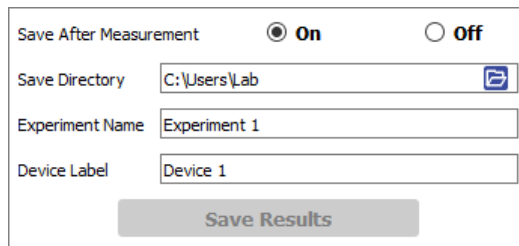

Save After Measurement ☒ On ☐ Off

Save Directory

Experiment Name

Device Label

Save Results

(I) Save After Measurement

- Set whether the measurement data will be saved after the measurement has completed.

Warning: Automatic saving can be turned off for lifetime measurements. However, **manual saving is unavailable for lifetime measurements**, so you will not be able to save your data if it is off.

- The program allows for data to be saved automatically (and manually) once the measurement is complete.
 - I. To enable or disable automatic saving, choose the appropriate option from the drop-down box.
 - II. For automatic saving, the 'Saving' fields must be filled in before the measurement can start, these are detailed below.
 - III. The 'Save Results' button is enabled once a measurement has been completed.
- For all measurements, a save directory must be specified. This can be done either by:
 - I. Manually typing the directory into the 'Save Directory' field,
 - II. Copy and pasting from your file explorer,
 - III. Clicking the 'Select Directory' button, which will open a dialog box to allow the selection of a folder to save to.
- All output files are comma separated variable (.csv) files.

(II) Save Directory

- Set the directory in which to create the data files.
- This can be filled in by:
 - I. Manually typing the directory into the 'Save Directory' field,
 - II. Copy and pasting from your file explorer,
 - III. Clicking the 'Select Directory' button, which will open a dialog box to allow the selection of a folder to save to.

(III) Experiment Name

- Set the name of the folder that the data will be saved into.
- For the solar cell characterisation measurements, this will also be used to name the file containing the device properties.
- This field cannot contain the following characters:
 - I. \ / : * ? " < > |

(IV) Device Label

- Set the name of the device being tested.
- This is used to label the files for I-V data and measurement settings.
- This field cannot contain the following characters:
 - I. \ / : * ? " < > |

(V) Save Data Format

- All data is saved as .csv (comma separated value) files.
- All data will be saved into a folder with the Experiment Name.
- The figures below show the files that are created when saving data for each of the measurements.

Figure 9.13. Solar Cell Characterisation save data format.




Figure 9.14. Stabilised Current Output save data format.






Figure 9.15. Solar Lifetime Measurement save data.

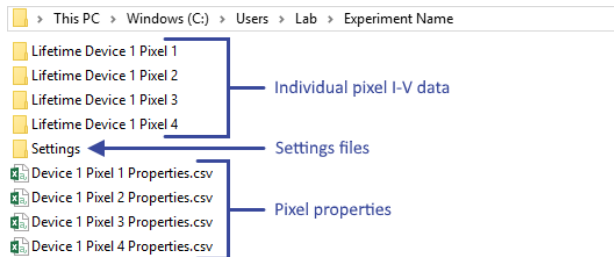

9.9 Controls

Figure 9.16. Controls for the measurements.

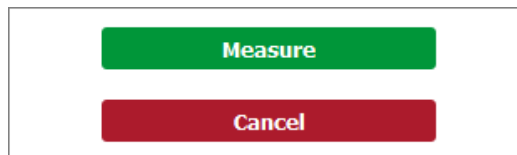

(I) Measure

- Clicking this button will start the measurement using the chosen settings.
- This button cannot be clicked if the software has not detected the test system.

(II) Cancel

- Stops a measurement that is currently in progress.
 - I. Note that if the measurement is stopped before it completes, the user will be unable to save the experimental data.

9.10 Test Device

The system is shipped with a test device that can be used to verify the correct operation of the system by mimicking the response of a solar cell. It has semiconductor photodiodes arranged in the geometry of the substrate pixels. The appearance of the test device will depend on the substrate system being used (**Figure 9.17**).

Figure 9.17. Test device configurations



9.10.1 Taking a Measurement

1. Place the test device in the substrate holder with the photodiodes facing upwards.
2. Start the Solar Cell I-V software and enter the following settings:


Figure 9.18. Measurement Settings for the solar characterisation and lifetime measurements.

Start Voltage (V)	-1.000	↕	?
End Voltage (V)	0.400	↕	?
Voltage Increment (V)	0.020	↕	?
Voltage Settle Time (s)	0.000	↕	?
Illumination (mW.cm ⁻²)	100.00	↕	?
Hysteresis I-V	☐ On ☒ Off		?

The other settings can be left as default.

3. Place the test system under a solar simulator and select 'Measure'. The system should record the classic diode response (no response for negative bias and exponentially increasing current for increasing positive bias, **Figure 9.19**). The test can also be performed without the use of a solar simulator, however the current density will not be shifted below zero.

Figure 9.19. Software settings and photodiode response

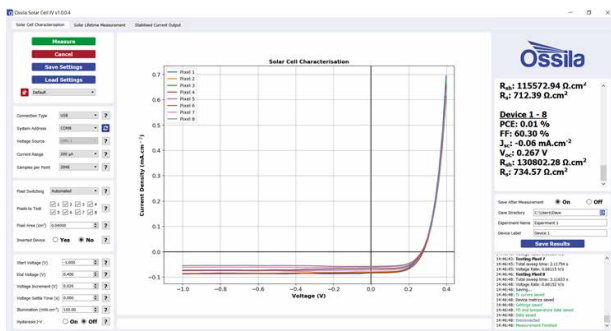

10. Troubleshooting

Most of the issues that may arise will be detailed here. However, if you encounter any issues that are not listed here, then contact us by email at info@ossila.com. We will respond as soon as possible.

Table 10.1. Troubleshooting guidelines for the Ossila I-V Test System (Automated)

Problem	Possible cause	Action
No power / display	a. The power supply may not be connected properly. b. The power supply adaptor has a fault.	a. Ensure the system is firmly plugged into the power supply, and that the plug is connected to both the adaptor and a working power socket. b. Contact Ossila for a replacement power supply adaptor.
Software does not start	a. The wrong version of Windows is installed on the computer. b. The software has not installed properly.	a. Install the software on a computer with Windows 10. b. Try reinstalling the software.
Cannot connect to the system via USB	a. The USB cable may not be connected properly. b. The USB cable may not be connected to a working USB port. c. The USB cable is defective.	a. Ensure the USB cable is firmly plugged in at both ends. b. Try connecting the unit to a different USB port on the computer. c. Use a different USB-B cable, and contact Ossila if necessary.
Cannot connect to the system via network	a. The MAC address of the unit is not registered with the internal network. b. The Ethernet cable may not be connected properly. c. The Ethernet cable is defective.	a. Register the system on the network using the MAC address obtained via a USB connection (see Source Measure Unit manual). b. Ensure the Ethernet cable is firmly plugged in at both ends. c. Try using a different Ethernet cable.

11. Related Products

11.1 Related Consumables



ITO Substrates

Our range of 15 x 20 mm ITO substrates for OPV, OLED and sensing applications.

Product codes: S111 / S101 / S211 / S281 / S171



Flat tip tweezers

Provides a good substrate grip without scratching.

Product codes: C121



FTO Coated Glass Substrates

Designed to be used in the fabrication of transparent electrodes for thin-film photovoltaics.

Product code: S301 / S302 / S303 / S304



Substrate Cleaning Rack

Holds 20 substrates for a variety of processing techniques.

Product code: E101

11.2 Related Equipment



Spin Coater

Produce high-quality coatings without any substrate warping. Perfect for busy labs with limited space.

Product code: L2001A3



Syringe Pump

High-precision, programmable single and dual syringe pumps for the automatic dispensing of solutions.

Product codes: L2003S1 / L2003D1



UV Ozone Cleaner

For removing contamination on the surface of samples, providing you with ultraclean surfaces within minutes.

Product code: L2002A2




Source Measure Unit

Source voltage, measure current, get data. Simplify and accelerate your data collection!

Product code: P2005A2



THE QUEEN'S AWARDS
FOR ENTERPRISE:
INTERNATIONAL TRADE
2018



**INNOVATION
AWARD 2017**

IOP Institute of Physics

Copyright © Ossila 2020

Ossila.com