

SPECTRA DEW 350

User Manual



speCtra[®]
AUSTRALIA & NEW ZEALAND

WELCOME TO YOUR SPECTRA DEW 350

Congratulations on becoming the owner of a Spectra DEW 350 hospital grade double electric breast pump. Your Spectra Dew 350 is a hospital grade breast pump with a single smooth, powerful, yet gentle pumping action that will support milk supply and allow you to make short work of expressing. If you have any questions about using your DEW 350, please check out our website for more information or get in touch with our customer service team at any time.

Features

- **Double-Sided Pumping:** Your Spectra DEW 350 comes with everything you need for double pumping. Expressing from both breasts at once saves you time and better supports milk supply.
- **Fully Adjustable Vacuum Settings:** Simply turn the dial to increase or decrease vacuum strength to your comfort level.
- **Very Quiet:** The motor has a soft, constant quiet noise so you can pump next to your baby or at work without worrying.
- **Stylish, Portable Design:** Spectra has endeavoured to make the most portable and convenient hospital grade pump ever, with an integrated handle to make life a little easier.

General Safety Guidelines

- Close supervision is necessary when used near children.
- Use the product only for its intended use and with attachments recommended by the manufacturer.
- Handle the power cord and plug with care; do not leave on a heated surface, do not pull or twist the cord, and do not wrap the cord around the breast pump.
- Do not use near water.
- Do not use in the presence of concentrated oxygen or pressurised gases.
- Unplug and store out of reach of children when not in use.



IMPORTANT SAFEGUARDS

Carefully read the instructions prior to using the Spectra DEW 350. Follow the safety guidelines above when using your pump. Failure to follow these guidelines could result in damage to the pump and/or injury to yourself and those around you.

INCLUDED WITH YOUR DEW 350

Your Spectra DEW 350 comes with everything you need to double pump, including two sets of tubing, backflow filters, breastshields, valves, and bottle kits.



PUMP MOTOR



TUBING (x 2)



SHORT TUBING (x 2)



BACKFLOW FILTER (x 4)



BREASTSHIELD (x 2)



VALVE (x 2)

TUBING CONNECTORS (x 2)



TEAT (x 2)



BOTTLE CAP (x 2)



BOTTLE NECK (x 2)



BOTTLE (x 2)

- Sterilise all parts prior to first use except for tubing, backflow filters, and pump motor.
- Do not get the pump motor or tubing wet. Washing or sterilising the tubing can cause milk or moisture to enter the pump motor, leading to mould or bacteria growth. Once milk or moisture enters the tubing it can no longer be assured as hygienic and the tubing should be replaced.
- Sterilise bottles before use. Inspect teat before each feeding and discard if torn.
- Our milk collection bottles are freezer safe.

QUICK START GUIDE



1. Sterilise Parts

Sterilise all parts **except for tubing, backflow filters and pump motor**. To sterilise by boiling disassemble all parts and cover with water in a large stock pot. Bring to a boil for 5 minutes. Use tongs to remove parts from pot and set to air dry on a clean paper towel.




2. Assemble

Firmly press valve into the bottom of the breastshield, then twist breastshield onto collection bottle. Place short tubing onto backflow filter, and place other end onto the connector and insert into breastshield. Attach long tubing to other end of backflow filter and onto air ports on pump motor.



3. Fit to Breast

Place breastshield so nipple is centred within the flange. While pumping your nipple should move freely within the flange with 2-3mm space, not rubbing on the sides and without excess areola being drawn in. You should not feel any pain. See our website for more on breastshield sizing.

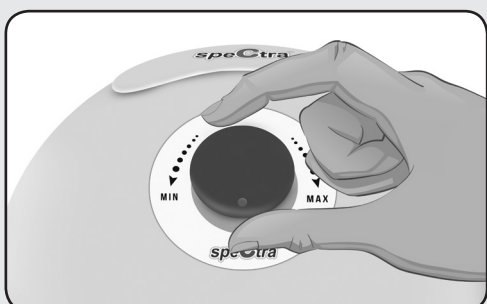

4. Understanding Settings

You should plan on trying out different settings to find what works best for you. To start, begin at a low vacuum setting. Slowly increase vacuum strength to trigger milkflow. Pumping shouldn't be painful - never set vacuum higher than your comfort level.

Pumping Tips

Relax and stay hydrated. Set yourself up with a glass of water, snacks and try to minimise interruptions for the next 15-30 minutes.

Remember who you are pumping for. Try pumping with a picture or video of your baby, or a piece of your baby's clothing, to encourage milkflow.


Massage your breasts to encourage milkflow. Before and during pumping, massage your milk ducts by pressing in small gentle circles starting at the top of the breast and working down.

Free a hand. With practice, you may be able to use the crook of your elbow to support one collection bottle while holding the other, or invest in a hands free pumping bra.

ASSEMBLING YOUR MILK COLLECTION KIT

Before assembling, make sure you've sterilised and washed your milk collection kit (**except** for the tubing and backflow filters). Make sure all parts have been able to completely air dry prior to assembling.

Start by inserting the valve firmly into the breastshield. Then, screw the breastshield onto the milk collection bottle. Attach the short tubing to the backflow filter, and then to the breastshield as shown below. Then, attach the long tubing to the other end of the backflow filter.

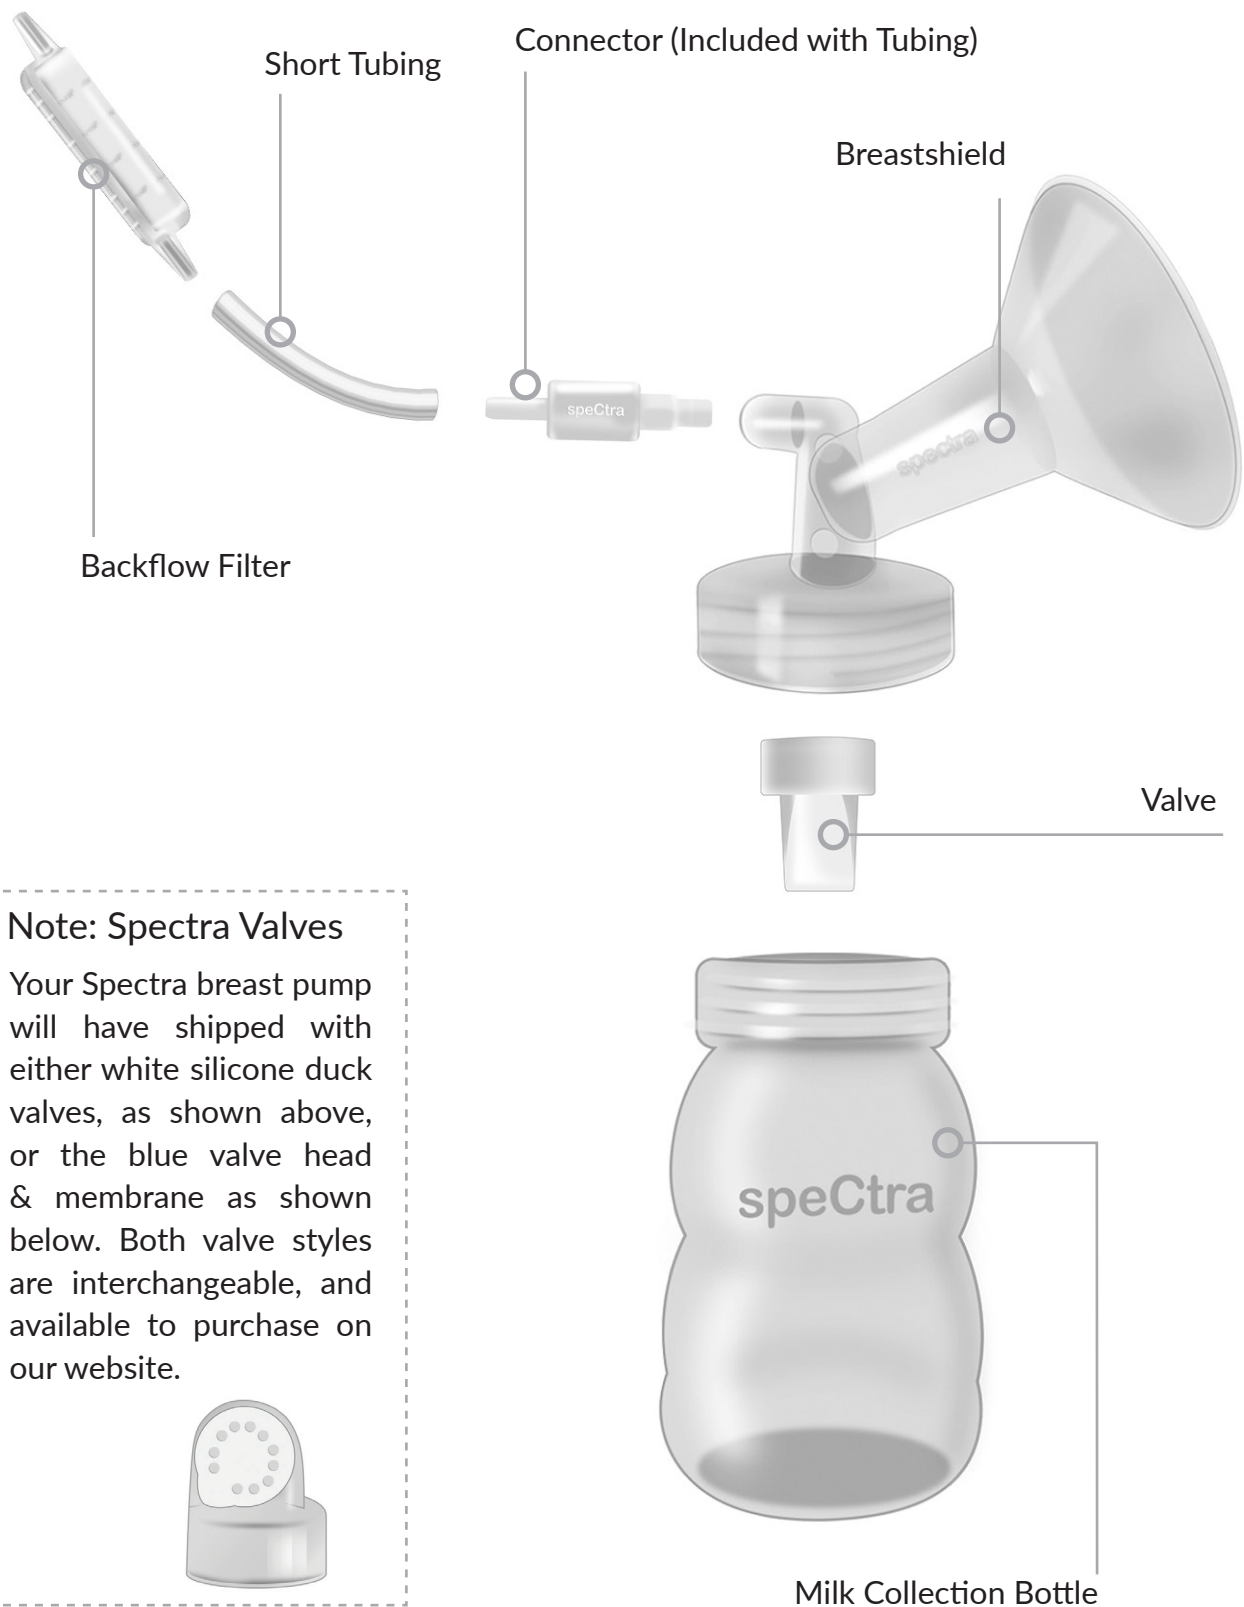

ASSEMBLING YOUR DEW 350


HOW TO ASSEMBLE YOUR BREAST PUMP FOR USE



1. Attach Tubing

Assemble the milk collection kit as shown on the previous page. Make sure all parts are completely dry prior to assembly. Attach tubing firmly onto the backflow filter.


Note on short tubing: The DEW 350 ships with the connector inserted into the long tubing, which puts the backflow filters all the way down by the pump motor. You can insert the connector into the short tubing if you have a strong letdown or you're concerned about moisture in the tubing. This puts the backflow filters up by your breastshield, protecting the long tubing. You may wish to do this because the short tubing can be cleaned.

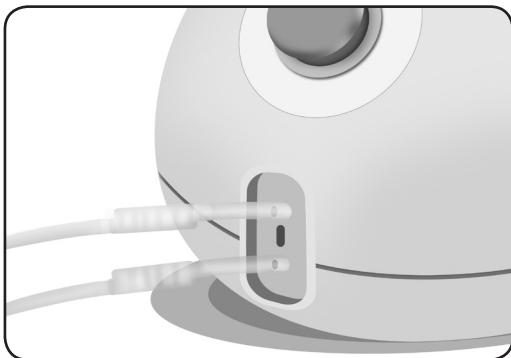

2. Double Pumping


Insert tubing firmly over each air port. Make sure tubing is firmly placed onto backflow filters and into breastshields.

Tip: If you're having trouble removing the cap over the second air port, try using a pair of tweezers and gently rocking it back and forth.

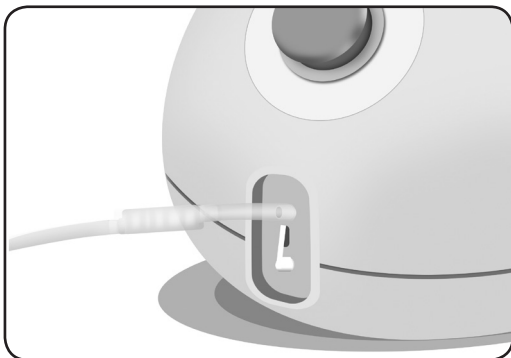

3. Single Pumping

Insert tubing firmly over one air port. Make sure cap is firmly and completely covering the second air port.

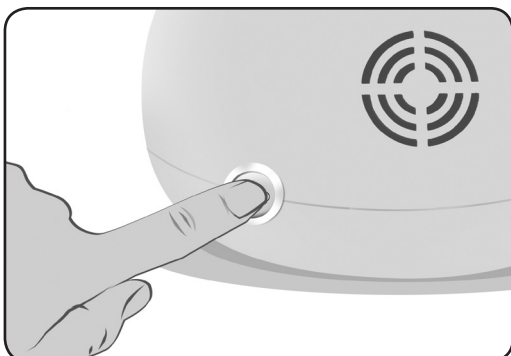

4. Powering the DEW 350

Plug the DEW 350 power cable into mains. To power on the pump, flip the switch on the back side as shown.

PUMPING INSTRUCTIONS



To begin pumping, place the breastshield over the nipple. Use one hand to hold the breast and the other to hold the breastshield as you adjust your breast into the nipple so the nipple is centred in the flange and an airtight seal is formed around your breast or areola. Repeat for double pumping.

Tip: Use the inside of your elbow to hold the first breastshield in place while you adjust the second.

- For your safety, before powering on make sure vacuum is at its lowest setting by turning the dial all the way to the left.
- Flip the power switch on the back of the pump. The pump will initiate.
- Adjust the vacuum to comfort level. Start off with the vacuum on low, and then gradually increase the vacuum setting to your comfort level by turning dial to the right. Never set the vacuum level higher than your comfort level.
- Express milk for 10-15 minutes per breast. To maintain supply for an exclusively breastfed baby, we recommend pumping every 2-3 hours, or 7-8 times per day for long enough to completely drain the breast; then, an additional 5 minutes to signal the demand for the body to make more milk.
- When you wish to stop expressing, flip the power switch and then remove the milk collection kits from your breasts. Do not attempt to remove the collection kits without first breaking suction. Turning off the pump will break suction.


CONTROLS



Power Switch


Vacuum Strength

The strength of the suction. Adjustable by turning the dial to the right to increase suction strength, and to the left to decrease.

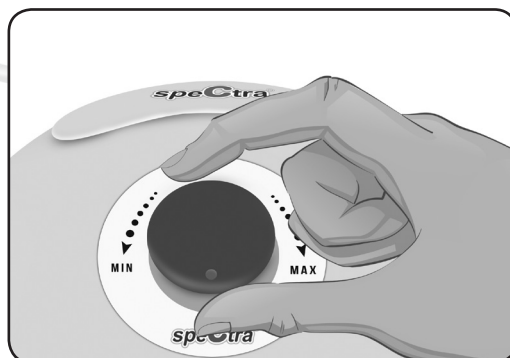

BREASTSHIELD SIZING GUIDE

The DEW 350 comes with size 24mm breastshields. This is the most commonly fitted shield size; however, many women will fit better in other sizes. A properly sized breastshield is important to ensure the best performance of your pump. An improperly fitted breastshield can hinder milk output, cause discomfort, and in extreme cases cause injury. To determine the shield size you need, pump for 5 minutes using the provided shields. Your nipples will expand while milk is being expressed so it's important to measure after they have swollen to ensure the size you select will provide enough room. After you pump, measure the diameter of the nipples at the base as illustrated in the image to the right. Repeat the process a few times to make sure you have the right measurement. Select a shield size that is 2-3mm larger than this measurement.

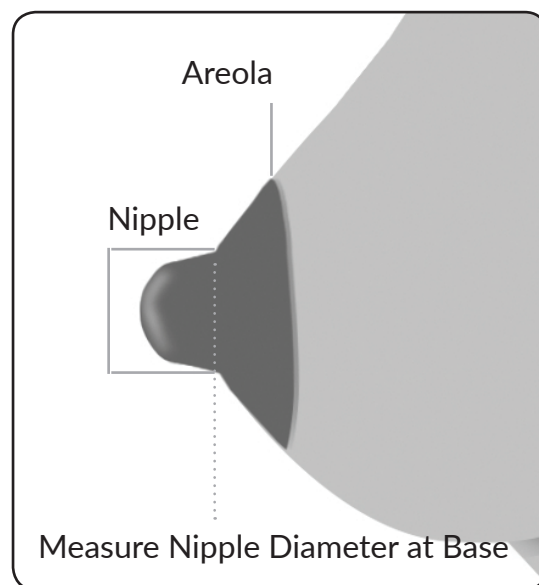

Signs your breastshield may be too small

- Painful rubbing of nipple in flange.
- Nipple not moving freely inside of flange.
- Redness of the nipple.
- Whiteness of the nipple and/or a white ring around the base of the nipple.
- Little milk is being expressed.
- General discomfort while pumping.

Signs your breastshield may be too large


- Excess areola is drawn into the flange (a small amount of areola may enter the flange for some women; however, it should never be uncomfortable or painful).
- Sensation of pulling and/or pulling pain.
- Nipple is pulled to the end of the flange.
- Shield falls from the breast while pumping or milk pools between shield and breast.
- Little milk is being expressed.
- General discomfort while pumping.

MORE INFORMATION ABOUT SHIELD SIZING

- You should check your shield size every so often throughout your pumping journey, especially if you are noticing a decrease in milk output.
- We suggest taking measurements of the swollen nipple after pumping (rather than the unswollen nipple before pumping) because every woman's nipples will respond differently to pumping.
- Your measurements might be different throughout the day. For example, you might be fuller in the morning after going a few hours without pumping and/or feeding at night, warranting a larger size. You might also be smaller in the evening after consistent pumping or feeding throughout the day.
- You might be larger at the beginning of a pumping session, and smaller after some milk has been expressed.
- Your measurements might change after your milk supply is well-established (about 10 weeks postpartum).
- One breast may perform better with a different sized breastshield than the other.

CLEANING & STERILISATION

STERILISE BEFORE FIRST USE

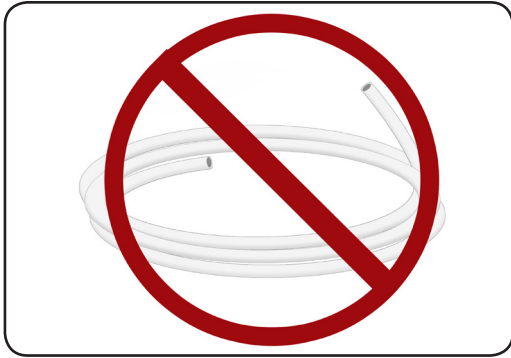


What to Sterilise

Sterilise all parts before first use except tubing, backflow filters, and pump motor. Sterilise all parts that might come in contact with your breastmilk, including bottles, breastshields, valves, bottle necks, sealing discs, caps, and teats.



Boiling Water Method

Select a large stock pot large enough for all of your pump parts to fit without pressing against each other. Place parts into pot, making sure they are completely disassembled. Fill the pot with more than enough water to cover all of your pump parts. Make sure there are no air pocket and that parts are not nestled together (check that bottles don't have any air pockets or smaller parts like valves in them).

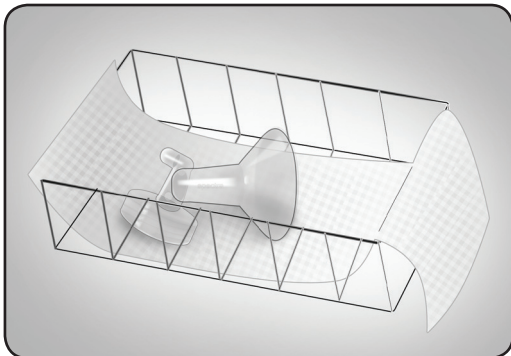

Place the pot on the stovetop and turn on the heat. Heat until a rolling boil: boil for 5 minutes. Do not let the water run dry as this will melt your parts.

After 5 minutes, remove from heat. Use a pair of tongs to carefully remove each part and set on a clean paper towel. Allow to completely air dry prior to assembling.

Steam Sterilisers / Other Methods

If you're using a microwave steam steriliser, a chemical solution, or another sterilisation method please follow the manufacturer's instructions. We don't normally recommend chemical solutions unless you don't have access potable water.

Precautions

- Do not get the tubing wet. Moisture can cause irreparable damage to the motor and invite mould and bacteria to grow inside of your pump.
- Do not overcrowd when using the boiling water method because this can cause parts to permanently warp. Repeat the process multiple times in a smaller pot if you don't have a large enough pot.
- Sterilisation can cause discoloration of the plastic. This is normal and safe for use.
- Over-sterilisation can cause parts to wear down more quickly than they should. Following a good cleaning method (see next page) means you don't need sterilise more than just once.
- 9 • If your care provider has given you alternative cleaning & sterilisation instructions, always adhere to those.

CLEANING & STERILISATION

CLEAN YOUR PARTS DAILY

What Needs to be Cleaned



Clean all parts that come in contact with breastmilk after using them. You don't have to clean your parts after each use (unless your care provider has advised you to), but make sure you keep your pump parts in a sealed container in the refrigerator between uses. **Do not wash the tubing or backflow filters.**


Note on short tubing: You can clean the short tubing as needed with a pipe cleaner or bottle brush if you have it assembled so that it's between the backflow filter and connector on your breastshield (see Assembly on pg. 6). Thoroughly rinse and allow to air dry. Do not boil or sterilise tubing.

Hand Washing Parts



To hand wash parts you'll need access to potable water, regular dish soap, a dedicated wash basin & sponge or bottle brush for your pump parts, and paper towels. Add your pump parts to your wash basin and fill with warm soapy water. Make sure they are fully disassembled (check that valves are removed from breastshields and so on). Wash the surfaces, interior and crevices of each part, and be especially careful with the valve. Rinse thoroughly under a stream of cool, clean water, and set to air dry on a clean paper towel. Allow parts to completely air dry prior to assembly.

Washing in the Dishwasher

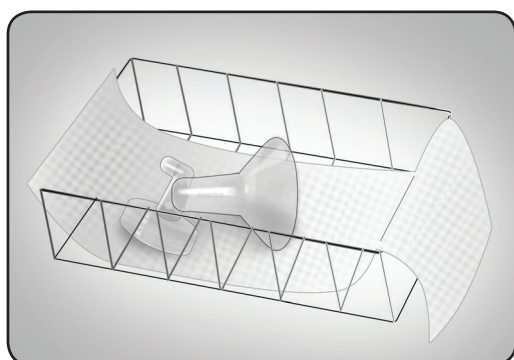

You can wash your breast pump parts in the top rack of the dishwasher on a normal dish washing setting. A dishwashing basket with a closing lid is great for preventing small parts from getting lost. Make sure that your dishwasher is set to air dry, **not to heat dry**, as that can cause your parts to warp. Try to handwash the valves and membranes whenever possible as these are delicate and easily lost.

Allow parts to completely dry in dishwasher or remove and air dry on a clean paper towel, prior to assembling.

Other Cleaning Methods

If you're following another cleaning method, such as a cleaning wipes, always follow the manufacturer's instructions. We recommend hand washing or washing in the dishwasher whenever possible.

TIPS FOR EXPRESSING BREASTMILK

- **Relax and Stay Hydrated:** Set yourself up with a glass of water and snacks, and minimise interruptions for the next 15-30 minutes as much as possible.
- **Set the Stage:** Have a regular pumping location. Choose a seat that is comfortable and provides back support so you can relax while still sitting up straight. Keeping a small towel nearby will help you clean as needed.
- **Routine and Ritual:** You can condition your body to express easily by pumping with the same setup each time. For example, try always using the bathroom first, then fix your favorite drink, grab your clean milk collection kits, sit down in your regular spot, have your drink, and then start pumping. Try always expressing after brushing your teeth, or playing the same game on your phone while you express. Your body will start to recognise what's going on.
- **Visualise Success!** Just as ritual can help contribute to effective pumping, some creative visualisation can also help. Think of a gushing faucet, a flowing river, or simply visualise your milk coming out.
- **Remember Who You are Pumping For:** Some women find a picture of their baby, a baby item or item of clothing that smells like their baby can help trigger letdown. Some find that a recording of their baby's cry is a powerful letdown trigger.
- **Massage to Start:** Stimulate your breasts before pumping can ease letdown. Rub in small circles all around the breast (don't forget in the armpit area) on both sides before you turn your pump on.
- **Massage to Continue:** When you notice your milkflow starting to slow, massaging your breast while focussing on any areas that seem to still contain milk can sometimes restart milkflow or encourage another letdown.
- **Pump more Often:** Increasing the frequency of your pumping sessions rather than the amount of time you pump is generally more effective at increasing the volume you can express.
- **Pump on Schedule:** Pumping at the same time each day can help teach your breasts to be ready to let the milk flow. Some women find pumping in the morning brings about the biggest 'payoff' while other pump after their baby's bedtime, a much more relaxed time of day.
- **Free a Hand:** With practice, you may be able to use a cushion or the crook of your arm to support one milk collection kit while you hold the other. This gives you a free hand to turn pages, scroll down screens, or use the remote. If you are serious about getting things done while pumping, a hands-free pumping bra will free up both your hands.
- **Pain should not be "Pushed Through":** If you are experiencing discomfort or pain while pumping, turn the suction down, try a little bit of lubricant such as coconut oil on the shield, and contact your care provider or Spectra Customer Support ASAP if the pain continues.

Note: When you express and how often will depend on your specific situation. We have provided some basic instructions here, but you may wish to ask your care provider for additional help. More information is also provided on our website and through customer support. Contact us if you need assistance.

BREASTMILK STORAGE

Freshly Expressed Breastmilk

At room temperature (up to 26°C / 78°F)	4 - 8 hours
In the cooler bag with an ice pack (up to 15°C / 59°F)	12 - 24 hours
In the back of the refrigerator (up to 4°C / 78°F)	3 - 8 days

Frozen Breastmilk Prior to Feeding

At room temperature (up to 26°C / 78°F)	<i>Should never be thawed at room temperature! Always thaw in the refrigerator.</i>
In the cooler bag with an ice pack (up to 15°C / 59°F)	Until thawed.
In the back of the refrigerator (up to 4°C / 78°F)	24 - 48 hours

Fresh Breastmilk after Feeding

At room temperature (up to 26°C / 78°F)	1 - 2 hours
In the cooler bag with an ice pack (up to 15°C / 59°F)	Up to 4 hours
In the back of the refrigerator (up to 4°C / 78°F)	Up to 24 hours
In the freezer (-18-20°C / -4-0°F)	<i>You should never freeze breastmilk after feeding.</i>

Note: These guidelines are based on current international recommendations for a healthy, full-term baby. You should always adhere to your care provider's advice.

BREASTMILK STORAGE (CONTINUED)

Previously Refrigerated or Frozen Breastmilk after Feeding

At room temperature (up to 26°C / 78°F)	1 hour
In the cooler bag with an ice pack (up to 15°C / 59°F)	1 - 2 hours
In the back of the refrigerator (up to 4°C / 39°F)	1 - 2 hours
In the freezer (-18-20°C / -4-0°F)	<i>You should never refreeze breastmilk.</i>

In the Freezer

In the Freezer Compartment of a Refrigerator (-15°C / 5°F)	1 - 2 weeks
Conventional freezer (-18-20°C / -4-0°F)	3 - 6 months
Deep Freeze (-20°C / -4°F or lower)	Up to 1 year

Tip: Check your freezer often to make sure it's working. Should the power go out, try not to open your freezer to keep the contents, including your frozen breastmilk, cool and insulated as long as possible. Breastmilk is still considered frozen when there is any amount of ice remaining in it.

Note: These guidelines are based on current international recommendations for a healthy, full-term baby. You should always adhere to your care provider's advice.

TROUBLESHOOTING

Pump Will Not Turn On

Possible Problem	Possible Solution
Plugged in, no power	• Check that the power cable is plugged into mains. • Check that power switch is in the “on” position. • Check that the mains outlet is working properly.
Loose rattling sound inside	• Contact customer support.

No / Low Suction

Vacuum settings have accidentally been changed	• Try increasing vacuum intensity settings.
On just one side	• Is valve seated correctly on breastshield? • Check the valve for tears & replace valve. • Check that tubing is snugly attached.
Tubing	• Check for snug attachment on air ports and backflow protectors. • Check for damage.
While Single Pumping	• Make sure cap is fully covering unused air port on pump.
Air is leaking between breastshield and breast	• Make sure breast is inserted correctly into breastshield so that vacuum is maintained constantly as pump sucks and releases. • Check breastshield sizing (pg. 8).
Internal tubing has come loose	• Place finger directly over air ports and turn on the pump. If you do not feel suction, contact customer support.

CARING FOR YOUR DEW 350

Replacing Parts

To properly maintain your DEW 350, you'll need to replace parts on a regular basis. Not replacing parts will make your pump work harder, leading to unnecessary wear and tear on the motor.

- Valve Membrane: Replace every 2 - 8 weeks, or when you notice a decrease in suction.
- Duck Valve: Replace every 2 - 3 months, or when you notice a decrease in suction.
- Backflow Filter: Pink lines will turn blurry when they need replacement.
- Breastshield: Replace every 6 months.
- Tubing: Replace should moisture ever enter the tubing.

Warranty & Repair

This product is warranted by the supplier to be free from defects in material and workmanship for a period of 2 years from the date of purchase. This warranty does not cover damage caused by accident, misuse, abuse, improper maintenance, unauthorised modification, or connection to an improper power supply. For warranty claims, service, and repair please contact customer support.

Spectra Baby services and repairs pumps outside of warranty coverage. For more information on services provided, cost, or to book a service, visit our website.

Disposal

- Spectra Baby encourages used pumps in working order to be donated.
- Milk collection kits, bottles, and other breast pump accessories are for single-person use only and are unhygienic to be used by more than one person. They should not be reused second-hand.
- Breastshields, bottles, and other hard plastic parts can normally be recycled; check with your local authority.
- Silicone parts including duck valves, membranes, tubing, and teats cannot be recycled and must be thrown away.
- The Spectra DEW 350 breast pump must not be disposed of with your regular household waste. It must be taken to a designated electronics recycling location. For more information about where you can dispose of electronic waste, please contact your local authority. This is to comply with EU Directive 2002/96/EC on Wasted Electrical and Electronic Equipment (WEEE).

TECHNICAL SPECIFICATIONS

Vacuum Strength	350mmHg
Grade	Hospital Grade
Massage / Letdown Mode	No
Cycle Speed	46 Cycles per Minute (CPM)
Power	Mains
Double Pumping	Yes
Weight	2kg
Warranty	2 Years
Motor Life	1500 Hours
Country of Origin	South Korea
Certifications	CE, FDA, ISO13485, ISO9001
Electromagnetic Compatibility	Compliant with IEC 60601-1-2:2007 Portable communications devices (i.e. mobile phones & 2-way radios) can impact the functionality of the Spectra S2. Should you experience interference, we recommend moving the Spectra S2 at least 1 metre away from these devices while in use.

Environmental Conditions

Operating Temperature	5°C - 40°C
Operating Humidity	20% - 80% non-condensing
Storage Temperature	-20°C - 50°C
Storage Humidity	20% - 95% non-condensing



© 2018 Chabalala Pte Ltd
Tel: +61 (07) 3053 8669
support@spectra-baby.com.au
spectra-baby.com.au