## 12.3.2 Managing Representative Information

tton to create
esentative
profile.
tton to edit
esentative
profile.
tton to delete
esentative
profile.



Figure 14 - Representative Information Screen

## 12.3.3 To Set Control Permissions

- 1. Access the Control Permissions screen.
- 2. For each connected motor, set control permissions as necessary (*Figure 15*).



Figure 15 – Control Permissions Screen

## 12.3.4 To Import and Exporting Preset(s)

**NOTE:** A USB data storage device must be inserted into the USB port to access the Import/Export screen.

- 1. Access the Import/Export screen.
- 2. Touch the **Import** or **Export** menu tab (depending on required outcome).
- 3. Touch the **SELECT ALL** button or touch the individual preset(s) to import/export (*Figure 16*).
- 4. Touch **(Confirm**).

NOTE: A pop-up message will appear upon completion.



Figure 16 - Import/Export Screen

## 12.3.5 To Manage Irrigation Settings

**NOTE:** An irrigation cassette must be inserted into the irrigation port to access the Irrigation Settings screen.

- 1. Access the Irrigation Settings screen.
- 2. Adjust settings as necessary (Figure 17).

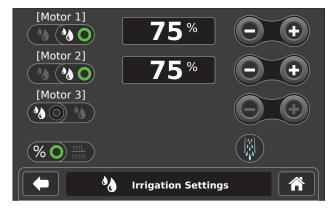


Figure 17 - Irrigation Settings Screen

# 12.3.6 Preparing the Irrigation Cassette

# *12.3.6.1 To Prime the Irrigation Cassette* NOTES:

- The prime feature is used to fill the irrigation tubing with sterile fluid and remove air pockets.
- After inserting an irrigation cassette, the Irrigation Settings screen will automatically be displayed.
- 1. (If required) Access the Irrigation Settings screen.
- 2. Touch (Initial Prime) to prime the irrigation cassette (Figure 18).

NOTE: A pop-up message will appear upon completion.

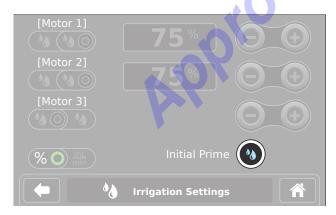


Figure 18 - Irrigation Settings (Initial Prime)

#### 12.3.6.2 To Flush the Irrigation Cassette

**NOTE:** The flush feature is only available if the irrigation cassette has been primed and is used to maximize fluid flow through the irrigation tubing to remove lodged debris.

3. Touch and hold (Flush) until lodged debris is removed (Figure 19).



Figure 19 - Irrigation Settings (Flush)

## 12.3.7 To Access General Information

**NOTE:** The General Info screen provides URLs and QR codes to access electronic versions of the Instructions For Use and Open Source Software disclosures for the console (*Figure 20*).

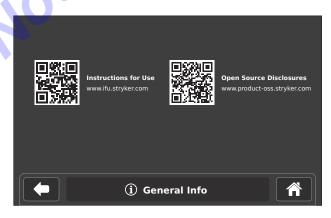


Figure 20 - General Info Screen

## 12.3.8 Managing Motor Settings

**NOTE:** Available motor settings may vary. The console will only display settings that are available for the connected device.

## 12.3.8.1 General (Motor Settings)

SYMBOL	DEFINITION	FUNCTION
Ö	General	Use this menu tab to adjust various motor settings.



Figure 21 - General Menu Tab

#### 12.3.8.2 Irrigation (Motor Settings)

SYMBOL	YMBOL DEFINITION FUNCTION	
٥٥	Irrigation	Use this menu tab to adjust various motor irrigation settings.
Ö	8	

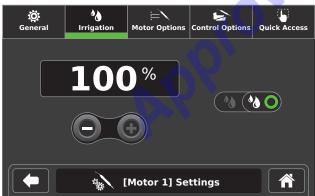


Figure 22 - Irrigation Menu Tab

#### 12.3.8.3 Motor Options (Motor Settings)

SYMBOL	SYMBOL DEFINITION FUNCTION	
=\	Motor Options	Use this menu tab to adjust various motor options.

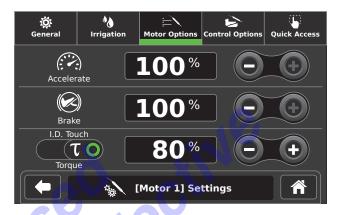


Figure 23 - Motor Options Menu Tab

## 12.3.8.4 Control Options (Motor Settings)

SYMBOL	DEFINITION	FUNCTION
	Control Options	Use this menu tab to adjust various control options.

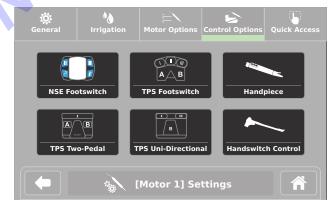


Figure 24 - Control Options Menu Tab

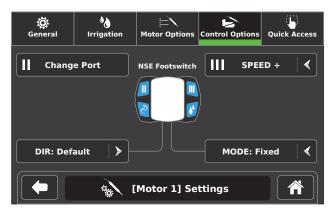


Figure 25 - NSE Footswitch Control Options

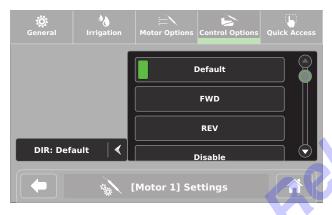


Figure 26 - Direction Options List

## 12.3.8.5 Quick Access (Motor Settings)

SYMBOL	DEFINITION	FUNCTION
	Quick Access	Use this menu tab to set direction, irrigation, mode, or I.D. Touch (torque) to be accessible from the Home screen.  Choosing the No Quick Access option will remove the quick access button from the Home screen.  The PREVIEW area displays a glimpse of the quick access area on the Home screen (Figure 27).

**NOTE:** In *Figure 27*, the Irrigation Control option was touched and appears in the PREVIEW area.

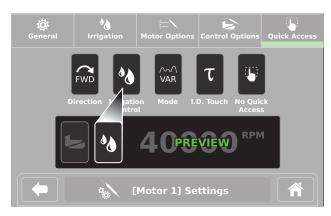


Figure 27 - Quick Access Menu Tab

# 12.4 Network Devices Screen

**NOTE:** The Network Devices screen displays connected external devices. Only Stryker supported devices will appear after successfully connecting with the CORE 2 Console. For example, this screen is used to confirm the Q Guidance System is connected (*Figure 28*).

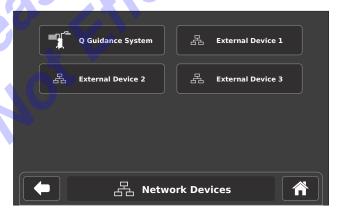


Figure 28 - Network Device Screen

FΝ 5400-052-700-EN Rev-AH

# 13 Cleaning and Disinfection



## **WARNINGS:**

- ALWAYS clean and disinfect the equipment as indicated upon initial receipt and before each use. Failure to comply may cause infection and result in patient or healthcare staff injury.
- ALWAYS consult the Instructions For Use that accompanies motors, footswitches, and attachments for product specific cleaning requirements.

#### **CAUTIONS:**

- DO NOT immerse the equipment in liquid. DO NOT allow liquids or moisture to enter any electrical connection.
- DO NOT sterilize the console.
- DO NOT use solvents, lubricants, or other chemicals, including glutaraldehyde or similar chemical cleaners, unless otherwise specified.
- Use of unapproved disinfectants may cause damage to equipment.

## 13.1 Recommended Materials

- PPE as recommended by the disinfectant manufacturer
- Soft, lint-free cloth
- Brushes
- United States Environmental Protection Agency (US EPA) registered disinfectant with a claim for activity against Hepatitis B. The following disinfectants have been validated for use on the exterior surfaces of the Stryker CORE 2 Console:
  - Quaternary Ammonium Based CaviCide® Disinfectant (EPA Registration #46781-6)
  - Sodium Hypochlorite Based Clorox® Clean-Up® Disinfectant Cleaner with Bleach (EPA Registration #67619-17)

## 13.2 Clean and Disinfect Procedure

1. Lightly wipe all external surfaces of the console and power cord with a soft, lint-free cloth moistened with a non-abrasive, hospital disinfectant prepared according to the manufacturer's instructions. Clean surfaces until all visible soil is removed.

- 2. Wipe critical areas such as the area around the power button, irrigation cassette door, and any other areas that may have become soiled. Use appropriate brushes to remove soil from difficult to clean locations on the console that could not be thoroughly cleaned by wiping alone.
- 3. After removing all visible gross soil, use a clean cloth moistened with disinfectant and wipe all surfaces. Make sure all surfaces remain visibly wet at room temperature for at least the minimum time specified in the Instructions For Use supplied by the disinfectant manufacturer.
- 4. Remove any excess disinfectant solution using a soft, lint-free cloth moistened with water if required by the instructions supplied by the disinfectant manufacturer.

CAUTION: DO NOT use an aerosol spray directly on the console screen.

5. Apply glass cleaner to a soft, lint-free cloth and clean the console screen.

# **Troubleshooting**



WARNING: DO NOT disassemble, modify, service. or repair any equipment without the authorization of the manufacturer. For assistance, contact Stryker.

	PROBLEM	CORRECTIVE ACTION
	Console powers OFF unexpectedly.	Verify the power cord is connected properly.
	Console powers OFF due to elevated temperature.	Disconnect the console power cord from the hospital-grade power outlet for a minimum of five minutes before attempting to use the console again.
not recognize a properly. I		Verify the device is connected properly. If necessary, remove and replace the device cord.
	Electrical interference is experienced.	Turn off all equipment not in use in the operating room. Verify equipment is not placed too close to the console.

20 www.stryker.com Date Released: <unreleased>

# 15 Maintenance

# 15.1 Fuse Replacement



## WARNINGS:

- ALWAYS disconnect the power cord from the console before replacing the fuses. Failure to comply may cause an electrical shock hazard.
- ALWAYS use the same type and rated fuse when replacing fuses. Failure to comply may cause a fire hazard. See Section 18.10 Appendix J: Specifications for fuse information.
- DO NOT use the console if a fuse immediately fails after replacement. For assistance, contact Stryker.
- 1. Remove power from the console as follows:

**CAUTION:** Some power cords have a locking mechanism, press the colored tab prior to disconnection.

- 1.1. Disconnect the power cord from the console.
- 1.2. If used, disconnect the equipotential cable.
- 2. Using a small flat blade screwdriver, gently pry open the cover of the fuse holder.
- 3. Remove the fuse holder from the console.
- Remove the two fuses from the fuse holder and properly dispose of the fuses. See Section 17 Disposal/Recycle for disposal information.
- 5. Install two new fuses into the fuse holder (Figure 29)
- 6. Securely install the fuse holder into the console.




Figure 29 - Fuse Replacement

# 16 Storage and Handling

#### **CAUTIONS:**

- ALWAYS save the original packaging container for reuse. Failure to comply may result in damage during transport to the Stryker Service Center.
- ALWAYS store the equipment within the specified environmental condition values (Section 18.10).

# 17 Disposal/Recycle



**WARNING:** ALWAYS follow the current local recommendations and/or regulations governing environmental protection and the risks associated with recycling or disposing of the equipment.



To comply with European Community
Waste Electrical and Electronic Equipment
(WEEE) Directive 2012/19/EU, this device
should be collected separately for recycling.
Do not dispose of as unsorted municipal
waste. Contact local distributor for disposal
information. Ensure infected equipment is
decontaminated prior to recycling.



Infected units should be decontaminated before they are sent for recycling. If it is not possible to decontaminate the unit for recycling, the hospital should not attempt to remove the batteries from waste equipment. Continued disposal of small amounts of portable batteries to landfill and incineration is allowed under Directive 2006/66/ EC and Member State regulations.



廢電池請回收

(Taiwan - Recycle Waste Batteries)

# 18 Appendices

# 18.1 Appendix A: Acronyms

ACRONYM	DEFINITION		
DIR	Direction		
EMC	Electromagnetic Compatibility		
ENT	Ear, Nose, Throat		
ES6	Electronic System 6		
FWD	Forward		
I.D.	Identification		
IFU	Instructions For Use		
IRR	Irrigation		
MRI	Magnetic Resonance Imaging		
OSC	Oscillating		
OSS	Open Source Software		
PPE	Personal Protective Equipment		
QR	Quick-response Code		
REV	Reverse		
RF	Radio Frequency		
RFID	Radio Frequency Identification		
RPM	Rotations Per Minute		
TPS	Total Performance System		
UHT	Universal High Torque		
UI	User Interface		
URL	Uniform Resource Locator		
USB	Universal Serial Bus		
VAR	Variable		

# 18.2 Appendix B: Audio Output

TYPE	DESCRIPTION	
Button Press	A quick low pitched beep to denote actuation of a button.  A quick low pitched beep to denote volume of a button press.  Slightly elongated chime to denote completion of a task.  Two tone set of beeps to indicate the motor is rotating in reverse (counterclockwise).  Two tone ascending beep to indicate a notification.	
Footswitch Mapping		
Volume Change		
Confirm		
Motor Reverse		
Notice		
Error	High two tone descending beep to indicate an error.	
Prohibited	Low two tone descending beep to denote prohibited actions.	

# 18.3 Appendix C: Colors

## 18.3.1 User Interface Colors

COLOR	DEFINITION
	Selected/Active
	Disabled/Inactive/Inaccessible

#### 18.3.2 Power Button Illumination Colors

COLOR	DEFINITION	
<b>Ф</b>	Console On	
0	Console Standby Mode	

# 18.4 Appendix D: Equipotential Bonding

Equipotential bonding involves the joining together of all metalwork and conductive items that are in the same potential (voltage) everywhere and is an important countermeasure in reducing the risk of equipment damage and personal injury. For additional information, refer to *IEC 60601-1 Clause 16*.

22

# 18.5 Appendix E: Power Cords

## 18.5.1 Power Cord General Specifications

Current Rating:	10 A	Connector Type:
Voltage Rating:	250 VAC minimum	Cable Type:
Frequency Rating:	50/60 Hz	Cable Length:
Copper Conductor Size Rating:	3 X 1.00 mm <sup>2</sup> ≤ Conductor Size < 3 X 1.50 mm <sup>2</sup>	18.7 Appendi
Connector Type:	IEC 60320 C13	• • •
	3.0 m, 2.5 m	Property
Cord Lengths:	<b>NOTE:</b> The 2.5 m cord is not for use in Canada or the US.	<b>18.7.1 Software</b> See the <i>Software Lice</i>
Temperature Rating:	0 °C to 70 °C minimum	REF 5400-052-704 st
Flammability Rating:	UL 94 V-2 minimum, IEC 60332-1	18.7.2 Trademarl
Cord Type:	SJT, H05VV-F, HVCTF, RVV or equivalent (unshielded)	Trademarks not the p
Dielectric Withstand:	1500 VAC for 60-seconds between Line/Neutral and Protective Earth	250 64
Mains:	Plug shall have a ground/ earthing pin	(Go. C)
Certification:	All applicable in-country medical electrical requirements	10
18.5.2 Additional Pov	ver Cord Requirements	B

## **18.5.2 Additional Power Cord Requirements**

The Canadian and US power supply cord shall have a tag or label in English and French indicating that "GROUNDING RELIABILITY CAN ONLY BE ACHIEVED WHEN EQUIPMENT IS CONNECTED TO AN EQUIVALENT RECEPTACLE MARKED 'HOSPITAL ONLY' OR 'HOSPITAL GRADE' " or equivalent wording.

Agency Approval: CSA Certified for Canada and US or ம் UL Recognized for Canada and US.

# 18.6 Appendix F: Ethernet Cables

## **18.6.1 Ethernet Cable General Specifications**

Connector Type: RJ45	
Cable Type:	CAT6 (shielded or unshielded)
Cable Length:	Up to 5 meters maximum

# 18.7 Appendix G: Intellectual **Property**

## 18.7.1 Software Licensing

See the Software License Addendum REF 5400-052-704 supplied with the console.

### 18.7.2 Trademarks

Trademarks not the property of Stryker Corporation are the property of their respective owners.

# 18.8 Appendix H: Footswitch Pedal/Pad Options



**WARNING:** ALWAYS consult the Instructions For Use that accompanies motors, footswitches, and attachments for product specific duty cycles and additional information.

NOTE: Available options may vary. The console will only display options that are available for the connected device.

## **18.8.1 Footswitch Pedal Direction Options**

OPTION	FUNCTION		
Default	These settings may be factory default settings of the connected motor or user programmed settings.		
Disable	Disables the footswitch pedal.		
Forward (FWD)	Pressure on the pedal will cause the motor to rotate in the forward (clockwise) direction.		
Reverse (REV)	Pressure on the pedal will cause the motor to rotate in the reverse (counterclockwise) direction.		
Oscillate (OSC)	Pressure on the footswitch pedal will cause the motor to oscillate.		

# 18.8.2 Footswitch Pedal Mode Options

OPTION	FUNCTION
Default	Causes the motor to operate according to the factory default setting of the connected motor.
	Specific default settings vary based on how the motor was programmed at the factory.
Variable	Varying pressure on the footswitch pedal will cause the motor speed to vary.
Fixed	Pressure on the footswitch pedal will cause the motor to operate at a constant speed as set on the
	Home screen.
1Touch	Press and release the footswitch pedal to activate the motor to operate at a constant speed as set
	on the Home screen. Press and release the footswitch pedal again to deactivate the motor operation.

## 18.8.3 Footswitch Pad Options

**NOTE:** The IRR On/Off and FWD<>REV buttons on the NSE Footswitch cannot be programmed to any footswitch pad options.

OPTION	FUNCTION		
Disable	Disables the footswitch pad.		
SPEED +	Pressure on the pad will increment the set point speed.		
SPEED -	Pressure on the pad will decrement the set point speed.		
IRR +	Pressure on the footswitch pad will increment the pump flow set point and increase irrigation to the motor cutting accessory.		
IRR -	Pressure on the footswitch pad will decrement the pump flow set point and decrease irrigation to the motor cutting accessory.		
IRR On/Off	Pressure on the footswitch pad will toggle the irrigation pump on and off.		
Change Port	Pressure on the footswitch pad will change the footswitch assignment to another assigned motor.		
Flush	Pressure on the pad will turn the irrigation pump on at the flush rate (300%).		
OSC<>Normal	Pressure on the pad will toggle the operating mode of the motor.		
FWD<>REV	Pressure on the pad will toggle the direction of the motor rotation.		
Change Attachment	Pressure on the footswitch pad will toggle through the list of available attachments for the motor.		
Jog	Pressure on the footswitch pad will cause the cutting accessory to rotate at a very low speed to position the cutting edge within the cutting window.		

# 18.9 Appendix I: Errors and Notifications

NOTE: Items within [brackets] in the following table are variables. For assistance, contact Stryker.

CODE	TITLE	CORRECTIVE ACTION		
00000005	Motor Actuation Error	The console only allows two motors to operate simultaneously.		
0000006	Motor Actuation Error	Connected motors cannot operate simultaneously.		
0000007	Motor Actuation Error	[Motor] has multiple active inputs. Only the first input detected is used. If the motor is inactive, release all inputs and try again.		
00001000 00001001	Motor Functional Error	[Motor] or cord connected to Port [port] requires service. Report error code to Stryker. See Section 1.3 Contact Information to contact Stryker.		
00001002	Console Functional Error	Report error code to Stryker. See Section 1.3 Contact Information to contact Stryker.		
00001003	Motor Actuation Error	Reset [motor] actuation. Release the motor button, trigger, or handswitch lever to reset. If the error persists, report error code to Stryker. See Section 1.3 Contact Information to contact Stryker.		
00001004	Motor Compatibility Error	Motor connected to Port [port] is not supported. See Section 6 For Use With.		
00001005	Motor/Console Functional Error	Error detected with [motor] connected on Port [port]. Remove [motor] from Port [port]; use a different motor. If the error persists, report error code to Stryker. See Section 1.3 Contact Information to contact Stryker.		
00001007	Motor Functional Error	Error detected with [motor] connected to Port [port]. Remove [motor] from Port [port]. If the error is resolved, return [motor] and cord to Stryker. If the error persists, report error code to Stryker. See Section 1.3 Contact Information to contact Stryker.		
00001008	Motor Temperature Error	[Motor] connected to Port [port] has reached an elevated operating temperature. Allow handpiece to cool before restarting.		
00001009	Motor Temperature Error	[Motor] or cord connected to Port [port] requires service. Report error code to Stryker. See Section 1.3 Contact Information to contact Stryker.		
0000100A	Motor Service Requirement	[Motor] requires service. Return handpiece to Stryker for service. See Section 1.3 Contact Information to contact Stryker.		
0000100B	Motor Stall Error	Excessive load detected on Port [port]. Report error code to Stryker. See Section 1.3 Contact Information to contact Stryker.		
0000100E	Cutter Speed Notification	Ensure [motor] speed does not exceed specified attachment limitations. Failure to do so may result in user and/or patient injury.		
00002000	Footswitch	Footswitch connected to port [port] requires service. Report error code to Stryker. See		
00002001	Functional Error  Console Functional Error	Section 1.3 Contact Information to contact Stryker.  Report error code to Stryker. See Section 1.3 Contact Information to contact Stryker.		
00002003	Footswitch Actuation Error	Reset Footswitch [port] actuation. Release the footswitch button or pedal to reset the actuation. If the error persists, report error code to Stryker. See Section 1.3 Contact Information to contact Stryker.		
00002004	Footswitch Compatibility Error	Footswitch connected to Port [port] is not supported. See Section 6 For Use With.		

25 www.stryker.com Date Released: <unreleased>

CODE	TITLE	CORRECTIVE ACTION		
00002005	Footswitch/	Error detected with footswitch on Port [port]. Remove the footswitch from Port [port]; use		
	Console	a different footswitch. If the error persists, report error code to Stryker. See Section 1.3		
	Functional Error	Contact Information to contact Stryker.		
00002006	Footswitch	Footswitch connected to port [port] requires service. Report error code to Stryker. See		
	Functional Error	Section 1.3 Contact Information to contact Stryker.		
00002007	CORE Q	Footswitch connected to port [port] requires service to enable haptic features. Confirm the		
	Footswitch	error to continue using the footswitch without haptic or Q Guidance System compatibility.		
	Functional Error	See Section 1.3 Contact Information to contact Stryker.		
00002008	CORE Q	Footswitch connected to port [port] requires service to enable haptic features. Confirm the		
	Footswitch	error to continue using the footswitch without haptic or Q Guidance System compatibility.		
	Functional Error	See Section 1.3 Contact Information to contact Stryker.		
00002009	CORE Q	Footswitch connected to port [port] requires service to enable haptic features. Confirm the		
	Footswitch	error to continue using the footswitch without haptic or Q Guidance System compatibility.		
	Functional Error	See Section 1.3 Contact Information to contact Stryker.		
00003001	Console	Reset console. If the error persists, report error code to Stryker. See Section 1.3 Contact		
	Functional Error	Information to contact Stryker.		
00003002	Console	Irrigation pump is nonfunctional. Reset console. If the error persists, report error code to		
	Functional Error	Stryker. See Section 1.3 Contact Information to contact Stryker.		
00003003	Console	RFID is nonfunctional. Reset console. If the error persists, report error code to Stryker. See		
	Functional Error	Section 1.3 Contact Information to contact Stryker.		
00003004	Console	Reset console. If the error persists, report error code to Stryker. See Section 1.3 Contact		
00003005	Functional Error	Information to contact Stryker.		
00003006	Console	Port illumination error occurred. Continue without illumination or report error code to Stryker.		
	Functional Error	See Section 1.3 Contact Information to contact Stryker.		
00003007	Console	Reset console. If the error persists, report error code to Stryker. See Section 1.3 Contact		
00003008	Functional Error	Information to contact Stryker.		
00003009				
0000300A		10° A		
0000300B	14			
0000300C	Motor/Console	Error detected with [motor] on Port [port]. Remove [motor] and cord from Port [port]; use		
	Functional Error	a different motor or cord. If the error persists, report error code to Stryker. See Section 1.3  Contact Information to contact Stryker.		
00000000	0	·		
0000300D	Console Functional Error	Report error code to Stryker. See Section 1.3 Contact Information to contact Stryker.		
0000000	+	Frank Winsting accepted in installed groundly.		
0000300E	Console Functional Error	Ensure irrigation cassette is installed properly.		
00003010	Motor	Use a Stryker approved cutter. If the error persists, report error code to Stryker. See Section		
00003010	Attachment	1.3 Contact Information to contact Stryker.		
	Error	1.5 Contact information to contact Stryker.		
00003011	Irrigation	Use a Stryker approved irrigation cassette. If the error persists, report error code to Stryker.		
00003011	Cassette Error	See Section 1.3 Contact Information to contact Stryker.		
	Cassette Life	dee dection i.d contact information to contact on year.		
00003012	Console	Report error code to Stryker. See Section 1.3 Contact Information to contact Stryker.		
00003012	Functional Error	Theport offer code to difficor. God decitor 1.0 defined information to contact difficor.		
00003014	Console	Error with audio function. Reset console. If the error persists, report error code to Stryker.		
00000014	Functional Error			
00003015	Console	·		
UUUUUU 13	LOUISUIG	Power supply over temperature. This may result from excessive use of motor duty cycle.		

CODE	TITLE	CORRECTIVE ACTION		
00003016 Console		Power supply temperature sensor error. Report error code to Stryker. See Section 1.3		
	Functional Error	Contact Information to contact Stryker.		
00003017	USB Error	Unrecognized USB device connected.		
00003018	Console	RFID is nonfunctional. Reset console. If the error persists, report error code to Stryker. See		
00003019	Functional Error	Section 1.3 Contact Information to contact Stryker.		
00003101	Console Functional Error	Irrigation pump is nonfunctional. Report error code to Stryker. See Section 1.3 Contact Information to contact Stryker.		
00003102	Console Functional Error	RFID is nonfunctional. Report error code to Stryker. See Section 1.3 Contact Information to contact Stryker.		
00003103	Console	Report error code to Stryker. See Section 1.3 Contact Information to contact Stryker.		
00003104	Functional Error			
00003105	Console Functional Error	Reset console. If the error persists, report error code to Stryker. See Section 1.3 Contact Information to contact Stryker.		
00003106	Console Functional Error	Report error code to Stryker. See Section 1.3 Contact Information to contact Stryker.		
00003107	Console Functional Error	Reset console. If the error persists, report error code to Stryker. See Section 1.3 Contact Information to contact Stryker.		
00003108	Console	Report error code to Stryker. See Section 1.3 Contact Information to contact Stryker.		
00003109	Functional Error			
0000310A				
0000310B				
00004001	Console	Reset console. If the error persists, report error code to Stryker. See Section 1.3 Contact		
00004002	Functional Error	Information to contact Stryker.		
00004003				
00004004				
00004005	Motor/Console Functional Error	Disconnect all motors and reset the console. If the error is resolved, return the motors and cords to Stryker. If the error persists, report error code to Stryker. See <i>Section 1.3 Contact Information</i> to contact Stryker.		
00004006	Console Functional Error	Report error code to Stryker. See Section 1.3 Contact Information to contact Stryker.		
00004007	Motor/Console	Disconnect all motors and reset the console. If the error is resolved, return the motors and		
00004008	Functional Error	cords to Stryker. If the error persists, report error code to Stryker. See Section 1.3 Contact Information to contact Stryker.		
00004009	Console	Report error code to Stryker. See Section 1.3 Contact Information to contact Stryker.		
0000400A	Functional Error			
0000400B				
0000400C				
00004101				
00004102				
00004103				
00004104				
00004105				
00005001	Q Guidance	Q Guidance System timed out. Check the Ethernet connection to the Q Guidance System.		
	System	Press Confirm to try and reconnect.		
	1			
	Connection			

CODE	TITLE	CORRECTIVE ACTION			
00005002	Q Guidance System Connection Error	to the Q Guidance System and restart the CORE 2 Console.			
00005003	Q Guidance System Connection Error	Q Guidance System unexpectedly disconnected. Check the Ethernet connection to the Q Guidance System. Press Confirm to try and reconnect.			
00005004	Q Guidance System Compatibility Error	The version of software on the CORE 2 Console is incompatible with the current Q Guidance System. Report error code to Stryker. See the <i>Contact Information</i> section of the Instructions For Use provided with the equipment to contact Stryker.			
00005005	Q Guidance System Functional Error	Q Guidance System experienced an unexpected error. Check the Ethernet connection to the Q Guidance System and restart the CORE 2 Console.			
Compatibility Error  O0005005  Q Guidance System  Q Guidance System experienced an unexpected error. Check the Ethernet connection to the Context of the Con		Guidance System.			

# 18.10 Appendix J: Specifications

Model:	CORE 2 Console		
REF:	REF 5400-052-000		
Dimensions:			
Width:	13.0 inch [330.2 mm]		
Height:	5.4 inch [137.2 mm]		
Depth:	17.4 inch [442.0 mm]		
Weight:	17.3 lb [7.8 kg]		
Material:	In accordance with the European REACH regulation and other environmental regulatory requirements, components within the product contain the following substances:		
	Diboron Trioxide, CAS No. 1303-86-2 Lead Monoxide (Oxide), CAS No. 1317-36-8 Lead Titanium Trioxide, CAS No. 12060-00-3		
Equipment Type:	Class 1 Type BF Applied Part		
Power Supply:	Input voltage: 100-240 V    50/60 Hz, 6-3 A  Motor port output voltage: 40 V ===  Footswitch port output voltage: 5 V ===		
Fuse Type, Rating, and Breaking Capacity:	2 x 6.3 A, 250 VAC, 5 x 20 mm, (F) Fast-Acting, (L) Low Breaking Capacity 63 A at 250 VAC, IEC 60127		
Enclosure (Ingress) Protection:	IPX0		
Ground Type:	Protective Earth (ground); when connected to facility power		
Mode of Operation:	Continuous operation with intermittent loading		
Duty Cycle:	See the duty cycle times defined in the Instructions For Use supplied with the motor and/or accessories.		

Document Number: 5400-052-700EN

ΕN 5400-052-700-EN Rev-AH

#### **Product Safety Certification:**



CSA Group certification mark for United States and Canada. These products were tested and meet medical electrical equipment certification requirements, including compliance with applicable 60601 series standards. For additional information, contact Stryker.



The Regulatory Compliance Mark (RCM) is a visible indication of a product's compliance with all applicable ACMA regulatory arrangements, including all technical and record-keeping requirements.

#### Four (4) Channel RFID

Module:

Frequency of Operation: 13.56 MHz

> RF Bandwidth: 13.553 MHz- 13.567 MHz

Modulation: ASK

RF Field Strength: 67.92 dBµV/m at 3 m

**Touch Screen:** 7 inch [177.8 mm] (800 x 480), 24-bit color, wide viewing angle: 170°

Adjustable Volume: 0 dBA to 52 dBA

**Environmental Conditions:** Operation Storage and Transportation Temperature: 10 °C -20 °C **Humidity Limitation: Atmospheric Pressure** Limitation:

#### 18.10.1 Essential Performance

The CORE 2 Console on its own does not have Essential Performance. See the user manual supplied with the Spine Guidance Software (see Section 6 For Use With) for any Essential Performance related to the use of the CORE 2 Console at the medical electrical system level.

# 18.11 Appendix K: Electromagnetic Compatibility

Guidance and manufacturer's declaration - electromagnetic emissions  The CORE 2 Console is intended for use in the electromagnetic environment specified below. The customer or the user of the CORE 2 Console should assure that the console is used in such an environment.			
RF emissions CISPR 11	Group 1	The CORE 2 Console uses RF energy only for the internal function. Therefore, the RF emissions are very low and are not likely to cause any interference in nearby electronic equipment.	
RF emissions CISPR 11	Class A	The CORE 2 Console is suitable for use in all establishments other than domestic, and may used in domestic establishments and those directly connected to the public low-voltage por	
Harmonic emissions IEC 61000-3-2	Class A	supply network that supplies buildings used for domestic purposes, provided the following warning is heeded:	
Voltage fluctuations/ flicker emissions IEC 61000-3-3	Complies	WARNING: The emissions characteristics of this equipment make it suitable for use in industrial areas and hospitals (CISPR 11 class A). If it is used in a residential environment (for which CISPR 11 class B is normally required) this equipment might not offer adequate protection to radio-frequency communication services. The user might need to take mitigation measures, such as shielding, relocating or reorienting the equipment.	

	Guidance and manufacturer's declaration - electromagnetic immunity				
The CORE 2 Console is intended for use in the electromagnetic environment specified below. The customer or the user of the CORE 2 Console should assure that the console is used in such an environment.					
Immunity test	IEC 60601 test level	Compliance level	Electromagnetic environment - guidance		
Electrostatic discharge (ESD) IEC 61000-4-2	±2, ±4, ±6, ±8 kV Contact ±2, ±4, ±8, ±15 kV Air	±2, ±4, ±6, ±8 kV Contact ±2, ±4, ±8, ±15 kV Air	Floors should be wood, concrete or ceramic tile. If floors are covered with synthetic material, the relative humidity should be at least 10%.		
Electrical fast transient/ burst	±2 kV at 100 kHz repetition frequency for power supply lines	±2 kV at 100 kHz repetition frequency for power supply lines	Mains power quality should be that of a typical commercial or hospital environment.		
IEC 61000-4-4	±1 kV at 100 kHz repetition frequency for input/output lines	±1 kV at 100 kHz repetition frequency for input/output lines			
Surge	±0.5, ±1 kV line(s) to line(s)	±1 kV line(s) to line(s)	Mains power quality should be that of a typical		
IEC 61000-4-5	±0.5, ±1, ±2 kV line(s) to earth	±2 kV line(s) to earth	commercial or hospital environment.		
Voltage dips, short interruptions and voltage variations on power supply input lines  IEC 61000-4-11	$ <5\% \ U_{\tau} $ (>95% dip in $U_{\tau}$ ) for 0.5 cycle $ 0\% \ U_{\tau} $ (100% dip in $U_{\tau}$ ) for 0.5 cycle at 0°, 45°, 90°, 135°, 180°, 225°, 270°, and 315° $ 0\% \ U_{\tau} (100\% \ \text{dip in } U_{\tau}) $ for 1 cycle at 0° $ 40\% \ U_{\tau} (60\% \ \text{dip in } U_{\tau}) $ for 5 cycles $ 70\% \ U_{\tau} $ (30% dip in $U_{\tau}$ ) for 25 & 30 cycles at 0° $ <5\% \ U_{\tau} $ (>95% dip in $U_{\tau}$ ) for 5 s $ 0\% \ U_{\tau} $ (100% dip in $U_{\tau}$ ) for 5 s	$ <5\% \ U_{\tau} $ $ (>95\% \ dip \ in \ U_{\tau}) $ $ for 0.5 \ cycle $ $ 0\% \ U_{\tau} $ $ (100\% \ dip \ in \ U_{\tau}) $ $ for 0.5 \ cycle \ at 0^{\circ}, 45^{\circ}, 90^{\circ}, 135^{\circ}, $ $ 180^{\circ}, 225^{\circ}, 270^{\circ}, and 315^{\circ} $ $ 0\% \ U_{\tau} (100\% \ dip \ in \ U_{\tau}) $ $ for 1 \ cycle \ at 0^{\circ} $ $ 40\% \ U_{\tau} (60\% \ dip \ in \ U_{\tau}) $ $ for 5 \ cycles $ $ 70\% \ U_{\tau} $ $ (30\% \ dip \ in \ U_{\tau}) $ $ for 25 \ & 30 \ cycles \ at 0^{\circ} $ $ <5\% \ U_{\tau} $ $ (>95\% \ dip \ in \ U_{\tau}) $ $ for 5 \ s $ $ 0\% \ U_{\tau} $ $ (100\% \ dip \ in \ U_{\tau}) $ $ for 5 \ s $	Mains power quality should be that of a typical commercial or hospital environment. If the user of the CORE 2 Console requires continued operation during power mains interruptions, it is recommended that the CORE 2 Console be powered from an uninterruptible power supply or a battery.		
Power frequency (50/60 Hz) magnetic field IEC 61000-4-8	3 A/m, 30 A/m at 50 and 60 Hz	3 A/m, 30 A/m at 50 and 60 Hz	Power frequency magnetic fields should be at levels characteristic of a typical location in a typical commercial or hospital environment.		

NOTE:  $U_{\tau}$  is the AC mains voltage prior to application of the test level.

Guidance and manufacturer's declaration - electromagnetic immunity				
The CORE 2 Console is intended for use in the electromagnetic environment specified below. The customer or the user of the CORE 2 Console should assure that the console is used in such an environment.				
Immunity test	IEC 60601 test level	Compliance level	Electromagnetic environment - guidance	
Conducted RF IEC 61000-4-6	3 Vrms 150 kHz to 80 MHz outside ISM bands 80% AM at 1 kHz	3 Vrms 150 kHz to 80 MHz outside ISM bands 80% AM at 1 kHz		
	6 Vrms 150 kHz to 80 MHz in ISM bands 80% AM at 1 kHz	6 Vrms 150 kHz to 80 MHz in ISM bands 80% AM at 1 kHz		
Radiated RF IEC 61000-4-3	3 V/m 80 MHz to 2.7 GHz 80% AM at 1 kHz	3 V/m 80 MHz to 2.7 GHz 80% AM at 1 kHz	warning: Portable RF equipment (including peripherals such as antenna cables and external antennas) should be used no closer than 30 cm (12 inches) to any part of the CORE 2 Console including cables specified by the manufacturer.	
	27 V/m 385 MHz Pulse modulation 18 Hz, Maximum power 1.8 W	27 V/m 385 MHz Pulse modulation 18 Hz, Maximum power 1.8 W	Otherwise, degradation of the performance of this equipment could result.	
	28 V/m 450 MHz, FM ± 5 kHz deviation, 1 kHz sine, Maximum power 2 W	28 V/m 450 MHz, FM ± 5 kHz deviation, 1 kHz sine, Maximum power 2 W	Field strengths from fixed RF transmitters, as determined by an electromagnetic site survey <sup>a</sup> should be less than the compliance level in each frequency range <sup>b</sup> .  Interference may occur in the vicinity of equipment marked with the following symbol:	
	9 V/m 710, 745, 780, 5240, 5500, 5785 MHz, Pulse modulation 217 Hz, Maximum power 0.2 W	9 V/m 710, 745, 780, 5240, 5500, 5785 MHz, Pulse modulation 217 Hz, Maximum power 0.2 W	(((c)))	
	28 V/m 810, 870, 930 MHz, Pulse modulation 18 Hz, Maximum power 2 W	28 V/m 810, 870, 930 MHz, Pulse modulation 18 Hz, Maximum power 2 W	(Non-ionizing electromagnetic radiation)	
	28 V/m 1720, 1845, 1970, 2450 MHz, Pulse modulation 217 Hz, Maximum power 2 W	28 V/m 1720, 1845, 1970, 2450 MHz, Pulse modulation 217 Hz, Maximum power 2 W		
Proximity magnetic fields IEC 61000-4-39	65 A/m 134.2 kHz, pulse modulation 2.1 kHz	65 A/m 134.2 kHz, pulse modulation 2.1 kHz		
	7.5 A/m 13.56 MHz, pulse modulation 50 kHz	7.5 A/m 13.56 MHz, pulse modulation 50 kHz		

NOTE 1: At 80 MHz and 800 MHz the higher frequency range applies.

NOTE 2: These guidelines may not apply in all situations. Electromagnetic propagation is affected by absorption and reflection from structures, objects and people.

Printed Date: Apr 29, 2024 18:37:01 GMT

<sup>&</sup>lt;sup>a</sup> Field strengths from fixed transmitters, such as base stations for radio (cellular/cordless) telephones and land mobile radios, amateur radio, AM and FM radio broadcast and TV broadcast cannot be predicted theoretically with accuracy. To assess the electromagnetic environment due to fixed RF transmitters, an electromagnetic site survey should be considered. If the measured field strength in the location in which the CORE 2 Console is used exceeds the applicable RF compliance level above, the CORE 2 Console should be observed to verify normal operation. If abnormal performance is observed, additional measures may be necessary, such as re-orienting or relocating the CORE 2 Console.

<sup>&</sup>lt;sup>b</sup> Over the frequency range 150 kHz to 80 MHz, field strengths should be less than 3 V/m.

# 18.12 Appendix L: Compliance Statements

The CORE 2 Console creates and uses radio frequencies and may cause interference with other medical equipment. If interference occurs, see the information contained within this appendix.

#### 18.12.1 Federal Communications Commission (FCC) & Industry Canada (IC)

Contains 4 Channel RFID Module FCC ID: Q9R-5400052020 or Q9R-5400052000 IC: 4919A-5400052020 or 4919A-5400052000

This device complies with FCC Part 15 and Industry Canada license exempt RSS standard(s). Operation is subject to the following two conditions: (1) this device may not cause interference, and (2) this device must accept any interference, including interference that may cause undesired operation of the device.

Changes or modifications not expressly approved by Stryker Instruments could void your authority to operate the equipment.

### 18.12.2 Hazardous Materials Statement (China Only)

Hazardous Substances						
Part Name	Lead (Pb)	Mercury (Hg)	Cadmium (Cd)	Hexavalent Chromium (Cr (VI))	Polybrominated Biphenyls (PBB)	Polybrominated Diphenyl Ethers (PBDE)
Front Bezel	Х	0	0	0	0	0
Motor Controller PCBA	Х	0	0	0	0	0
Irrigation Pump Controller PCBA	X	0	0	0	0	0
Main Controller PCBA	Х	0	0	0	0	0
IMX53 SOM PCBA	X	0	0	0	0	0
Power Supply	Х	0	0	0	0	0

This table is prepared in accordance with the provisions of SJ/T 11364.

Enterprises may further provide in this box technical explanation for marking "X" based on their actual circumstances.

O: Indicates that said hazardous substance contained in all of the homogeneous materials for this part is below the limit requirement of GB/T 26572.

X: Indicates that said hazardous substance contained in at least one of the homogeneous materials used for this part is above the limit requirement of GB/T 26572.





5400-052-700-DA	5400-052-700-NO
5400-052-700-DE	5400-052-700-PL
5400-052-700-ES	5400-052-700-PT
5400-052-700-FI	5400-052-700-SV
5400-052-700-FR	5400-052-700-TR
5400-052-700-IT	5400-052-700-ZH
5400-052-700-JA	700002939929 (RO)
5400-052-700-KO	700002940095 (RU)
5400-052-700-NL	700003015473 (EL)

ot Release Little City of the Stryker or its affiliated entities own, use, or have applied for the following trademarks or service marks: Bone Mill+, Copilot Q, CORE, ESSx, Formula, Pello, Pi Drive, Q Guidance, RemB, Saber, Sumex, System 6, TPS, TPX, and the Stryker logo. All other trademarks are trademarks of their respective owners or holders.



#### Stryker Instruments

1941 Stryker Way Portage, Michigan 49002 USA (269) 323-7700 (800) 253-3210



Stryker European Operations Limited Anngrove, IDA Business & Technology Park Carrigtwohill, Co Cork T45 HX08 Ireland



Stryker EMEA Supply Chain Services B. Frans Maasweg 2 Venlo 5928 SB, The Netherlands



UK Responsible Person Stryker UK Ltd, Stryker House, Hambridge Road, Newbury, Berkshire, RG14 5AW

Copyright © 2024 Stryker



2024-04 5400-052-700-EN Rev-AH www.stryker.com