

Medtronic MMT-342 Extended Reservoir Instruction Manual

Home » Medtronic » Medtronic MMT-342 Extended Reservoir Instruction Manual



Medtronic

MMT-342 Extended Reservoir Instruction Manual





Extended Reservoir

Contents

- 1 MMT-342 Extended
- Reservoir
- 2 Indications for Use
- **3 Contraindications**
- 4 Documents / Resources
- **5 Related Posts**

MMT-342 Extended Reservoir

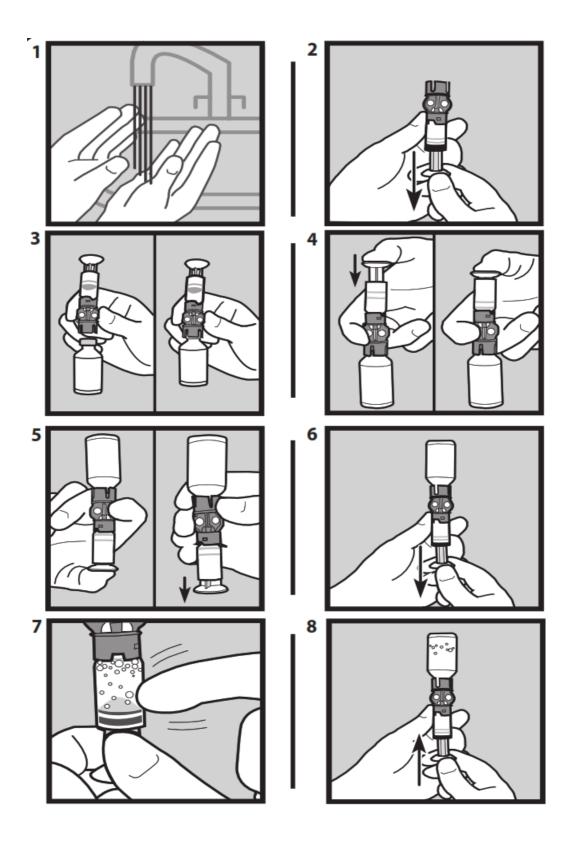

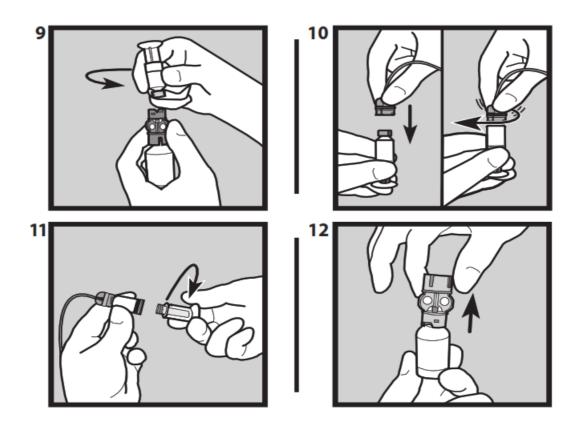

Indications for Use

The Extended Reservoir is indicated for the subcutaneous infusion of insulin from compatible Medtronic insulin pumps and infusion sets. Refer to your Medtronic insulin pump user guide for a list of compatible insulins and infusion sets.

Contraindications

This reservoir is contraindicated for the infusion of blood or blood products.

Warnings

- Do not use with two or three day infusion sets. The reservoir may only be used for up to seven days with use of the Medtronic Extended infusion set. Use of the reservoir with two or three day infusion sets may lead to hyperglycemia or diabetic ketoacidosis.
- Do not use the reservoir for more than seven days. Using the reservoir for more than seven days may result in the delivery of too little insulin, which may cause hyperglycemia.
- Reservoir and transfer guard are sterile, nonpyrogenic, and for single use only.
- Do not clean or resterilize. Reuse of the reservoir may lead to any one of the following: insulin degradation, infection, inaccurate medication delivery, or leaks which may cause damage to the pump.
- Do not use if package has been opened or damaged.
- Dispose of transfer guard safely in sharps container.
- Failure to remove trapped air from reservoir may result in inaccurate delivery of medication.
- If insulin, or any liquid, gets inside the tubing connector, it can temporarily block the vents that allow the pump to properly fill the infusion set. This may result in the delivery of too little or too much insulin, which can cause hyperglycemia or hypoglycemia. If this occurs, start over with a new reservoir and infusion set.
- The pump reservoir should be used for a maximum of seven days, or according to the insulin labeling, whichever duration is shorter.

Precautions

- Read all instructions carefully before using the Extended Reservoir.
- Insulin should be at room temperature before filling reservoir.
- Once reservoir is filled, use promptly. Do not store.
- Check for leaks after changing the reservoir and infusion set.
- Conduct your first setup in the presence of your healthcare professional.

Warranty

Visit http://www.medtronicdiabetes.com/warranty.

© 2022 Medtronic. All rights reserved. Medtronic, Medtronic logo and Further, Together are trademarks of

All other brands are trademarks of a Medtronic company.

Consult instructions for u se	Open here	Recyclable, contains recy cled content	Do not resterilize
LOT Batch code	Caution	$R_{\textit{Only}}_{\textit{Requires prescription i}}$ n the USA	Do not use if package is damaged
Sterilized using ethylene oxide	REF Catalogue number	Single sterile barrier system	Manufacturer
Duration of use (7 d ays)	Do not re-us	MD Medical device	Manufacturing site

Refer to pump and infusion set user guides for installation and filling.

USA: Medtronic Diabetes Global Headquarters 24 Hour HelpLine: +1-800-646-4633 To order supplies: +1-800-843-6687

> **Extended Reservoir** Medtronic **Medtronic MiniMed**

18000 Devonshire Street Northridge, CA 91325 USA 1800 646 4633 +1818 576 5555

www.medtronicdiabetes.com



(01)00763000652128(10)NA



M020459C002 2

Documents / Resources



Medtronic MMT-342 Extended Reservoir [pdf] Instruction Manual MMT-342, MMT-342T, MMT-342 Extended Reservoir, Extended Reservoir, Reservoir

Manuals+,