

# **MEGACOR FASTest PARVO Card Instructions**

Home » MEGACOR » MEGACOR FASTest PARVO Card Instructions



#### **Contents**

- 1 MEGACOR FASTest PARVO Card
- **2 INFORMATION ON THE TEST-KIT** 
  - 2.1 TEST-KIT COMPONENTS
  - 2.2 LIABILITY
- **3 INTRODUCTION**
- **4 INFORMATION ON THE SPECIMEN**
- MATERIAL
- **5 SPECIMEN COLLECTION AND**
- **PREPARATION**
- **6 TEST PROCEDURE** 
  - **6.1 READING OF THE TEST RESULT**
- **7 PRECAUTIONS FOR USERS**
- **8 TEST PRINCIPLE**
- 9 INFORMATION FOR THE INTERPRETATION
- 10 Documents / Resources
  - 10.1 References
- 11 Related Posts




**MEGACOR FASTest PARVO Card** 



# **INFORMATION ON THE TEST-KIT**

# **TEST-KIT COMPONENTS**

• 1 test-kit FASTest® PARVO Card contains:

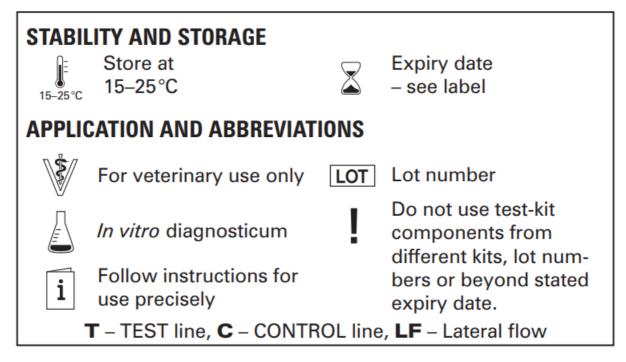

## LIABILITY

• The entire risk due to the performance of this product is assumed by the purchaser. The manufacturer shall not be liable for indirect, special or consequential damages of any kind resulting from the use of this product.

## **ACCURACY**

• Sensitivity 96.0 %

- Specificity 99.9 %
- (Comparison Method: Electron microscopy, ELISA)

## INTRODUCTION

- The Canine Parvovirus (CPV) was fi rst described in 1978 as cause of diarrhoea in dogs. At fi rst the virus was detected in North America, but it spread quickly world-wide.
- The Canine Parvovirus (CPV), the Feline Panleukopenia Vi-rus (FPV) and the Mink Enteritis Virus (MEV) show structural similarities. Puppies are infected through an oronasal path at an early age. The virus is excreted by infected animals via feces and remains infectious in the environment up to one year. Thereby, kennels can be permanently contaminated. The clinical symptoms of Parvovirus enteritis are severe diarrhoea, vomiting, anorexia, dehydration and panleuko-penia.
- Fecal samples can be used for the detection of the parvovirus specific antigens CPV-1, CPV-2, CPV-2a, CPV-2b und CPV-2c.
- The use of the FASTest® PARVO Card enables the veterinarian to quickly confi rm an aetiological diagnosis of a CPV infection, to start the therapy immediately and to initiate the required quarantine procedures.

#### INFORMATION ON THE SPECIMEN MATERIAL


- Due to the normally inhomogeneous or nest-like dissemination of antigens in the feces, the specimen material has to be mixed up homogeneously (spatula, vortex-mixer) before sampling.
- For the test, the required amount of feces as described in issue 4b / Specimen collection and preparation, is needed. The amount depends on the consistency of the sample. Use the attached spi-ral feces collection stick.
- Non-cooled (15–25 °C), the sample should be tested within 4 hours! At 2–8 °C, the sample can be stored up to 4 days, perma-nently at minimum –20 °C.
- Keep in mind that the sample material, as well as all used test-kit components, should have reached room temperature at the time of application.
- Endogeneous and exogeneous interfering substances of the sample (e. g. proteases, mucosa components, blood, but also viscosity, pH-value as well as grass and cat litter) can cause in-terferences (matrix effects) that can infl uence the target meas-urement. These can lead to an impaired LF and / or unspecifi c reactions on T and C.

#### SPECIMEN COLLECTION AND PREPARATION

- a. Open the sample tube with the buffer diluent.
- **b.** Introduce the spiral feces collection stick (cs) several times at various points into the well-homogenized feces. Pull it out and introduce the feces sticking on the cs (0.2 g) into the sample tube (fi g.1)
- **NOTE:** In case of watery feces, introduce the cs into the feces and then immediately into the sample tube. Mix well with the buffer. Repeat this step three times in a row!
- c. Close the sample tube tightly and shake it gently until the sample has been dissolved homogeneously into the buffer diluent (fi g.2).

#### **TEST PROCEDURE**

- 1. Remove the test cassette from its foil pouch shortly before use. Place it on a flat surface.
- 2. Shake the sample tube again to dissolve the specimen homogeneously. Then break the tip of the sample tube (opposite side of the blue screw cap) manually.
- 3. Hold the sample tube vertically (blue screw tap pointing upwards) and discard the fi first two drops. Then add three drops of the sample-buffer mixture into the round a simple window of the test cassette (fi g.3).

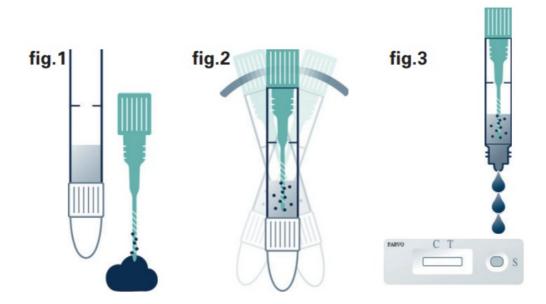

#### **READING OF THE TEST RESULT**

• Read the test result 5 minutes after the three drops have been dropped into the round sample window.



# POSITIVE TEST RESULT (fig.4)

• A pink-purple TEST line of any intensity (varying from weak to strongly intensive) and a pink-purple CONTROL line ap-pear.

# **NEGATIVE TEST RESULT (fig.5)**

• Only a pink-purple CONTROL line appears. This line indi-cates, irrespective of its intensity, that the test has been per-formed properly.


## **INVALID TEST RESULT**

• No CONTROL line visible. The test should be repeated using a new test cassette.

# fig.4 POSITIVE TEST RESULT

# fig.5 NEGATIVE TEST RESULT





## PRECAUTIONS FOR USERS

- The guidelines for working in medical laboratories must be observed. It is recommended to wear disposable
  gloves and other personal protective equipment (protec-tive clothing, possibly a face mask). Wash and
  disinfect hands after completing the test.
- Label sample material and associated sample tube to en-sure a precise assignment.
- Use a new sample tube and a new test cassette for each sample.
- The buffer diluent contains low concentrations of toxic sodium azide as a preservative, therefore avoid skin / eye contact and / or ingestion.
- The sample material must be seen as potentially infectious and disposed of accordingly, together with the used test-kit components.

### **TEST PRINCIPLE**

- The FASTest® PARVO Card is based on latest rapid immu-nochromatographic technique.
- Positive feces samples contain Parvovirus antigens CPV-2a, 2b, 2c and its subtypes 2c(a) and 2c(b). These
  antigens will react in the conjugate pad area with mobile monoclonal anti-Parvovirus antibodies (anti-Pv mAbs),
  which are bound to gold particles. Migrating ("lateral fl ow", LF) along the nitrocellulose membrane, these
  specific antigen-antibody complexes are bound by fixed anti-Pv mAbs producing a pink-purple TEST line (T).
- These anti-Pv mAbs guarantee a high level of specificity for the aetiologic detection of Parvovirus. The intensity or width of the test line depends on the concentration of Parvovirus antigens in the tested sample.
- A correct test procedure will be indicated by a second, pink-purple CONTROL line (C).

## INFORMATION FOR THE INTERPRETATION

- The interpretation of the test result should always be based on anamnestic and clinical data as well as the therapy and prophylaxis possibilities.
- Any non-described colour or contour variation of T and C within the indicated incubation time or after more than 10 minutes (e. g. greyish, shadow-like lines) has to be considered as unspecific reaction and therefore as nega-tive test result.
- Tcan vary both in intensity and width. Therefore, any pink-purple line appearing within the required incubation time is to be interpreted as a positive test result.
- Clinical healthy animals with or without dectectable contact to Parvovirus shedders or to deseased animals can shed Parvovirus and therefore react positive in the FASTest® PARVO Card. That's why, as a matter of principle, the Parvovirus antigen status of an animal before vaccination should be tested with FASTest® PARVO Card.

- Vaccination with modifi ed-live high titre CPV-2 vaccine may result in shedding of Parvovirus for a period of 3 to 14 days post vaccination. The FASTest® PARVO Card can become positive due to the fact of a recent Parvovirus vaccination.
- Because of intermittent antigen shedding, during incuba-tion time (4–6, max. 9 days) or early phase of Parvovirus infection or with ongoing diarrhoea, a single negative test result should be confirmed by testing a serial feces sample (individual testing of at least three consecutive feces samples).
- Supplied Exclusively To The UK Veterinary Market By
- Vetlab Supplies Ltd
- · Visit Our Website
- www.vetlabsupplies.co.uk
- Telephone: 01798 874567
- email us: info@vetlabsupplies.co.uk
- · Manufacturer:
- 6912 Hörbranz AUSTRIA <u>www.megacor.com</u>

## **Documents / Resources**



MEGACOR FASTest PARVO Card [pdf] Instructions

**FASTest PARVO Card** 

# References

- OMEGACOR Diagnostik GmbH Veterinary in vitro diagnostics
- Wholesale Vet Supplies & Products for Practices & Labs | Vet Supplies Online UK

Manuals+,