



# NATIONAL INSTRUMENTS USB-6229 Multifunction DAQ Device User Guide

[Home](#) » [NATIONAL INSTRUMENTS](#) » NATIONAL INSTRUMENTS USB-6229 Multifunction DAQ Device User Guide



## READ ME FIRST NI-DAQmx™ and DAQ Device Installation Guide

Install your software before installing new hardware.

### Contents

- [1 Install Application Software](#)
- [2 Unpack and Install the Devices, Accessories, and Cables](#)
- [3 Accessories](#)
- [4 Troubleshooting](#)
- [5 Documents / Resources](#)
  - [5.1 References](#)
- [6 Related Posts](#)

## Install Application Software

Install NI application software, such as NI LabVIEW, or another application development environment (ADE), such as ANSI C or Visual Basic .NET. Refer to the NI-DAQmx Readme on the software media for supported application software and ADE versions.

Back up any applications before upgrading software or modifying the application.

### Install NI-DAQmx

Install NI-DAQmx driver software before installing new hardware devices so Windows can detect them.

1. Insert the software media. If the NI-DAQmx installer does not open automatically, select Start»Run. Enter

x:\autorun.exe, where x is the drive letter. Complete the instructions.

2. Register your NI hardware online at [ni.com/register](http://ni.com/register) when prompted.
3. The last dialog box opens with the following options.
  - Restart Later to install more NI software or documentation. If you are using a MXI-3 link from a PC to control a PXI chassis, exit and install the MXI-3 software, available at [ni.com/downloads](http://ni.com/downloads), before using the DAQ device.
  - Shut Down or Restart if you are ready to install your device.
  - Restart if you are using a system running the LabVIEW Real-Time Module.

Download NI-DAQmx to the target using MAX. Refer to the MAX Remote Systems Help by selecting Help»Help Topics»Remote Systems in MAX.

If you have problems installing your software, go to [ni.com/support/daqmx](http://ni.com/support/daqmx).

## Unpack and Install the Devices, Accessories, and Cables

Remove the packaging and inspect the device. Contact NI if the device is damaged. Do not install a damaged device.

If you have more than one DAQ device to install, install them all now using the procedure for your device type. If your system includes SCXI modules to connect to DAQ devices, first install the DAQ components.



**Caution** The device is static sensitive. Always properly ground yourself and the equipment when handling or connecting the device.

For safety and compliance information, refer to the device documentation, available at [ni.com/manuals](http://ni.com/manuals) or on the NI-DAQmx software media.



The following symbols may be on your device.



This icon denotes a caution, which advises you of precautions to take to avoid injury, data loss, or a system crash. When this symbol is marked on the device, refer to the Read Me First: Safety and Electromagnetic Compatibility document for precautions to take.



When this symbol is marked on a product, it denotes a warning advising you to take precautions to avoid electrical shock.




When this symbol is marked on a product, it denotes a component that may be hot. Touching this component may result in bodily injury.

### PCI and PCI Express Devices

Complete the following steps to install a PCI and PCI Express device:


1. Power off and unplug the computer.
2. Remove the computer cover and/or the expansion slot cover.
3. Touch any metal part of the computer to discharge any static electricity.

Figure 1. Installing a PCI/PCI Express Device

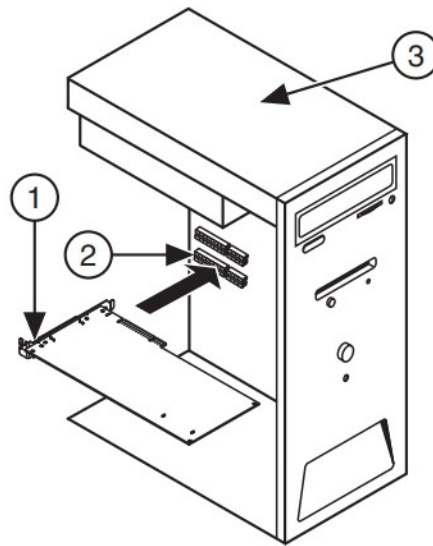

1. PCI/PCI Express DAQ Device
2. PCI/PCI Express System Slot
3. PC with PCI/PCI Express Slot
4. Insert the device into the applicable PCI/PCI Express system slot. Gently rock the device into place. Do not force the device into place. Per the PCI standard, NI PCI DAQ devices with the Universal PCI connector are supported in PCI-compliant buses, including PCI-X. You cannot install PCI Express devices in PCI slots and vice versa. PCI Express devices support up-plugging into a PCI Express slot of higher lane width. For guidelines, refer to [ni.com/pciexpress](http://ni.com/pciexpress).
5. Secure the device mounting bracket to the computer back panel rail.
6. (Optional) On NI M and X Series PCI Express devices, such as the NI PCIe-625x/635x, connect the PC and the device disk drive power connectors. Refer to the device user manual for when to use the disk drive power connector. Use a disk drive power connector that is not in the same power chain as the hard drive.

Figure 2. Attaching Disk Drive Power to the PCI Express Device

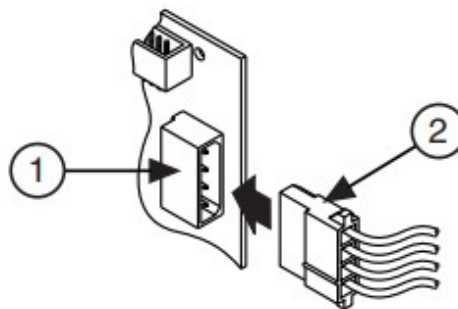

1. Device Disk Drive Power Connector
  2. PC Disk Drive Power Connector
- Connecting or disconnecting the disk drive power connector can affect the analog performance of your device. To compensate for this, NI recommends that you self-calibrate the PCI Express DAQ device in MAX after connecting or disconnecting the disk drive power connector; refer to the DAQ Getting Started Guide available online at [ni.com/manuals](http://ni.com/manuals).
7. Replace the computer cover, if applicable.
  8. Plug in and power on your computer.

### PXI and PXI Express Devices

Complete the following steps to install a PXI and PXI Express device:


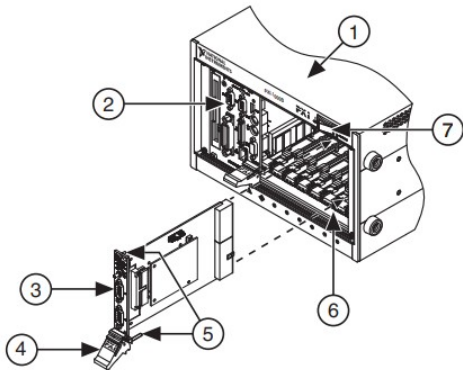
1. Power off and unplug the PXI/PXI Express chassis. Refer to your chassis manual to install or configure the chassis.
-  **Caution** Refer to the Read Me First: Safety and Electromagnetic Compatibility with your PXI/PXI Express chassis or device before removing covers or connecting or disconnecting signal wires.


Figure 3. Installing a PXI/PXI Express Device in the Chassis



1. PXI/PXI Express Chassis	5. Front-Panel Mounting Screws
2. PXI/PXI Express System Controller	6. Module Guides
3. PXI/PXI Express Module	7. Power Switch
4. Injector/Ejector Handle	

2. Identify a supported PXI/PXI Express slot in the chassis. Some devices have PXI/PXI Express slot requirements; for information, refer to the device documentation.

Figure 4. Symbols for PXI Express/PXI Express Hybrid/PXI Slots

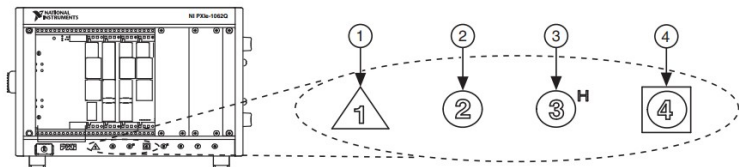

1. PXI Express System Controller Slot	3. PXI Express Hybrid Peripheral Slot
2. PXI Express Peripheral Slot	4. PXI Express System Timing Slot

If you are using a PXI Express chassis, you can place PXI devices in the PXI slots. If a PXI device is hybrid slot compatible, you can use the PXI Express Hybrid slots. PXI Express devices can be placed only in PXI Express slots and PXI Express Hybrid slots. Refer to the chassis documentation for details.

3. Remove the filler panel of an unused PXI/PXI Express slot.
4. Touch any metal part of the chassis to discharge static electricity.
5. Ensure that the PXI/PXI Express module injector/ejector handle is not latched and swings freely.
6. Place the PXI/PXI Express module edges into the module guides at the top and bottom of the chassis.
7. Slide the device into the PXI/PXI Express slot to the rear of the chassis.
8. When you begin to feel resistance, pull up on the injector/ejector handle to latch the device.
9. Secure the device front panel to the chassis using the front-panel mounting screws.
10. Plug in and power on your PXI/PXI Express chassis.

## Windows Device Recognition

Windows versions earlier than Windows Vista recognize newly installed devices when the computer restarts. Vista installs device software automatically. If the Found New Hardware wizard opens, install the software automatically is recommended for each device.

### NI Device Monitor

After Windows detects newly installed NI devices, NI Device Monitor runs automatically at startup.



Make sure the NI Device Monitor icon, shown at left, is visible in the taskbar notification area. Otherwise, the NI Device Monitor does not open. To turn the NI Device Monitor on, unplug your device, restart NI Device Monitor, and plug in your device. Launch NI Device Monitor from the Start menu, (Windows 8) from NI Launcher, or (Windows 10) from the All Apps menu.

The NI Device Monitor prompts you to select from the following options. These options may vary, depending on the devices and software installed on your system.

- Begin an application with this device—Launches LabVIEW. Choose this option if you have already configured your device in MAX.
- Configure and test this device—Opens MAX.
- Test this device—Launches MAX test panels for your device.
- Launch Instruments & Apps for this device—Launches NI ELVISmx Instrument Launcher. This option only appears if your device supports NI ELVISmx.
- Do nothing—Recognizes your device but does not launch an application.

The following features are available by clicking the NI Device Monitor icon and then clicking the Settings icon at the top right corner of the panel:

- Run at startup—Runs NI Device Monitor at system startup (default).
- Prevent all notifications—Prevents future notifications for any device.
- Reset Default Actions—Clears all actions set by the Always Do This option and restores factory default settings.
- Exit—Turns off NI Device Monitor. To turn on NI Device Monitor, launch NI Device Monitor from the Start menu, (Windows 8) from NI Launcher, or (Windows 10) from the All Apps menu.

## Accessories

Install accessories and/or terminal blocks according to the instructions in their installation guides. For SCXI and SCC signal conditioning systems, continue with the instructions in the DAQ Getting Started Guide.

## Troubleshooting

If you have problems installing your software, go to [ni.com/support/daqmx](http://ni.com/support/daqmx). For hardware troubleshooting, go to [ni.com/support](http://ni.com/support) and enter your device name, or go to [ni.com/kb](http://ni.com/kb).

If you need to return your National Instruments hardware for repair or device calibration, go to [ni.com/info](http://ni.com/info) and enter rdsenn to start the Return Merchandise Authorization (RMA) process. Go to [ni.com/info](http://ni.com/info) and enter rddq8x for a complete listing of the NI-DAQmx documents and their locations.

### Next Step

To confirm your device is working properly and start your application, refer to the DAQ Getting Started Guide available online at [ni.com/manuals](http://ni.com/manuals). Additional resources are online at [ni.com/gettingstarted](http://ni.com/gettingstarted).

You can find device terminal/pinout locations in MAX, the NI-DAQmx Help, or the device documentation. In MAX, right-click the device name under Devices and Interfaces, and select Device Pinouts.

Refer to the NI Trademarks and Logo Guidelines at [ni.com/trademarks](http://ni.com/trademarks) for more information on National Instruments trademarks. Other product and company names mentioned herein are trademarks or trade names of their respective companies. For patents covering National Instruments products/technology, refer to the appropriate location: Help»Patents in your software, the patents.txt file on your media, or the National Instruments Patents Notice at [ni.com/patents](http://ni.com/patents). You can find information about end-user license agreements (EULAs) and third-party legal notices in the readme file for your NI product. Refer to the Export Compliance Information at

[ni.com/legal/export-compliance](http://ni.com/legal/export-compliance) for the National Instruments global trade compliance policy and how to obtain relevant HTS codes, ECCNs, and other import/export data. NI MAKES NO EXPRESS OR IMPLIED WARRANTIES AS TO THE ACCURACY OF THE INFORMATION CONTAINED HEREIN AND SHALL NOT BE LIABLE FOR ANY ERRORS. U.S. Government **Customers:** The data contained in this manual was developed at private expense and is subject to the applicable limited rights and restricted data rights as set forth in FAR 52.227-14, DFAR 252.227-7014, and DFAR 252.227-7015. © 2003–2016 National Instruments. All rights reserved.

### COMPREHENSIVE SERVICES

We offer competitive repair and calibration services, as well as easily accessible documentation and free downloadable resources.

### SELL YOUR SURPLUS

We buy new, used, decommissioned, and surplus parts from every NI series.

We work out the best solution to suit your individual needs.

Sell For Cash Get Credit Receive a Trade in deal

OBSOLETE NI HARDWARE IN STOCK & READY TO SHIP

We stock New, New Surplus, Refurbished, and Reconditioned NI Hardware.

Bridging the gap between the manufacturer and your legacy test system.



1-800-915-6216 tS CC








[www.apexwaves.com](http://www.apexwaves.com)



[sales@apexwaves.com](mailto:sales@apexwaves.com)

All trademarks brand and brands and brand names are the property of thier respective owners

## Documents / Resources

	<a href="#">NATIONAL INSTRUMENTS USB-6229 Multifunction DAQ Device</a> [pdf] User Guide USB-6229 Multifunction DAQ Device, USB-6229, Multifunction DAQ Device, DAQ Device, Device
	<a href="#">NATIONAL INSTRUMENTS USB-6229 Multifunction DAQ Device</a> [pdf] User Manual USB-6229 Multifunction DAQ Device, USB-6229, Multifunction DAQ Device, DAQ Device, Device
	<a href="#">NATIONAL INSTRUMENTS USB-6229 Multifunction DAQ Device</a> [pdf] Owner's Manual USB-6229 Multifunction DAQ Device, USB-6229, Multifunction DAQ Device, DAQ Device, Device
	<a href="#">NATIONAL INSTRUMENTS USB-6229 Multifunction DAQ Device</a> [pdf] Owner's Manual USB-6229 Multifunction DAQ Device, USB-6229, Multifunction DAQ Device, DAQ Device, Device
	<a href="#">NATIONAL INSTRUMENTS USB-6229 Multifunction DAQ Device</a> [pdf] Owner's Manual USB-6229 Multifunction DAQ Device, USB-6229, Multifunction DAQ Device, DAQ Device, Device

## References

- [!\[\]\(fd4127b9e2af37bd6ea0fa06afa8e6d8\_img.jpg\) Test and Measurement Systems, a part of Emerson - NI](#)
- [!\[\]\(3278d6283d12f18012b5aa7d40747611\_img.jpg\) Test and Measurement Systems, a part of Emerson - NI](#)
- [!\[\]\(bb96b32142ec45f72f12316beae3ef61\_img.jpg\) Calibration Services - NI](#)
- [!\[\]\(a75d0d7d1ac0ea815a0c027a77b137d5\_img.jpg\) Contact Us - NI](#)
- [!\[\]\(adab168ecea4e2ae40993afba3fcd26e\_img.jpg\) Software and Driver Downloads - NI](#)
- [!\[\]\(e95ea1a0e297340f96c3d715d76d8c23\_img.jpg\) Example Programs - NI Community](#)
- [!\[\]\(0e0cdd76cf8fb3c858658faf72d7f324\_img.jpg\) NI Learning Center - NI](#)
- [!\[\]\(c7bdebfc2a52eab4f6683b0c1c0c28d2\_img.jpg\) Using Info Codes - NI](#)
- [!\[\]\(8a5c092736ceaf7cfeed23b17ea5e6ff\_img.jpg\) Search Results - NI](#)
- [!\[\]\(dd896e8effa212be4a7431ac3e5bf510\_img.jpg\) Legal Information - NI](#)
- [!\[\]\(1136f3a14b3ba5842784adf33e611db1\_img.jpg\) Legal Information - NI](#)
- [!\[\]\(d536ae100fbef949d5488b8fe23458f5\_img.jpg\) Trade Compliance - NI](#)
- [!\[\]\(ca07eb06779edef206c13bdfc2c41b40\_img.jpg\) Product Documentation - NI](#)
- [!\[\]\(7e7914364faa22e4d6649c877c7e723a\_img.jpg\) Contact Us - NI](#)
- [!\[\]\(8ca478e471a5a40f192eb324324796da\_img.jpg\) National Instruments Patents - NI](#)
- [!\[\]\(1ef1c1e934c0d3468708b1b65c673a8e\_img.jpg\) Shop - NI](#)
- [!\[\]\(2feef24d2b62f527f17ec4a26c99892b\_img.jpg\) Log In - National Instruments](#)
- [!\[\]\(62fbabcb8f920179a05cac5e6f77b9ec\_img.jpg\) Shop - NI](#)
- [!\[\]\(ea93f456ce60033911637cde1e339ebc\_img.jpg\) NI Services - NI](#)
- [!\[\]\(5ee090fbd54350d5f2535fbbb0cd8843\_img.jpg\) Support - NI](#)
- [!\[\]\(4dd804f7f115c0312bcea2f969779146\_img.jpg\) Support - NI](#)
- [!\[\]\(0917fa5071e46a535e4715939ddc0471\_img.jpg\) NI-DAQ™mx Download - NI](#)
- [!\[\]\(27fec434af9954d953dfa4171448e1b3\_img.jpg\) Shop - NI](#)
- [!\[\]\(d145641c384340f63dd70fecc7aabb25\_img.jpg\) NI Trademarks and Logo Guidelines - NI](#)
- [!\[\]\(243bbedc054f34725b139b217207eb1a\_img.jpg\) Education Services - NI](#)
- [!\[\]\(f3c6d79887bd9f21070de580cbc98211\_img.jpg\) Support - NI](#)
- [!\[\]\(2d1ece5ae055d1ae0a9970ac957b3b56\_img.jpg\) Example Programs - NI Community](#)
- [!\[\]\(5b120c922ef28e4fc683ca8b94422cdb\_img.jpg\) NI Learning Center - NI](#)
- [!\[\]\(3ecc71fc952378d9f4ffcad55785a56c\_img.jpg\) Using Info Codes - NI](#)
- [!\[\]\(b72ce2783b5377c43149ef95e1a2e921\_img.jpg\) Search Results - NI](#)
- [!\[\]\(411232913beeb58fd0033db165ed1b36\_img.jpg\) Product Documentation - NI](#)
- [!\[\]\(e83c8c58bd2fde02f1aaa2a40b47a814\_img.jpg\) Contact Us - NI](#)
- [!\[\]\(0c02fd0d294a73ffdb4e0a069fbf4bfa\_img.jpg\) Log In - National Instruments](#)
- [!\[\]\(eb1dbccbedb5ea0b264d2e100bde2403\_img.jpg\) NI Services - NI](#)
- [!\[\]\(a026f29e1ac3218f0e4f926eafc73d32\_img.jpg\) Support - NI](#)
- [User Manual](#)

[Manuals+](#), [Privacy Policy](#)

This website is an independent publication and is neither affiliated with nor endorsed by any of the trademark owners. The "Bluetooth®" word mark and logos are registered trademarks owned by Bluetooth SIG, Inc. The "Wi-Fi®" word mark and logos are registered trademarks owned by the Wi-Fi Alliance. Any use of these marks on this website does not imply any affiliation with or endorsement.