



PCE INSTRUMENTS PCE-423N Hot Wire Anemometer User Manual

[Home](#) » [PCE Instruments](#) » PCE INSTRUMENTS PCE-423N Hot Wire Anemometer User Manual 



User Manual
PCE-423N Heat Wire Anemometer



User manuals in various languages



<http://www.pce-instruments.com>

Contents

- 1 Safety notes
- 2 Specifications
- 3 Delivery scope
- 4 Device description
- 5 Switching the meter on and off
- 6 Measurement preparation
- 7 Measuring mode
- 8 Settings
- 9 Contact
- 10 Disposal
- 11 Documents / Resources
 - 11.1 References

Safety notes

Please read this manual carefully and completely before you use the device for the first time. The device may only be used by qualified personnel and repaired by PCE Instruments personnel. Damage or injuries caused by non-observance of the manual are excluded from our liability and not covered by our warranty.

- The device must only be used as described in this instruction manual. If used otherwise, this can cause dangerous situations for the user and damage to the meter.
- The instrument may only be used if the environmental conditions (temperature, relative humidity, ...) are within the ranges stated in the technical specifications. Do not expose the device to extreme temperatures, direct sunlight, extreme humidity or moisture.
- Do not expose the device to shocks or strong vibrations.
- The case should only be opened by qualified PCE Instruments personnel.
- Never use the instrument when your hands are wet.
- You must not make any technical changes to the device.
- The appliance should only be cleaned with a damp cloth. Use only pH-neutral cleaner, no abrasives or solvents.
- The device must only be used with accessories from PCE Instruments or equivalent.
- Before each use, inspect the case for visible damage. If any damage is visible, do not use the device.
- Do not use the instrument in explosive atmospheres.
- The measurement range as stated in the specifications must not be exceeded under any circumstances.
- Non-observance of the safety notes can cause damage to the device and injuries to the user.

- Do not touch the hot wire.

We do not assume liability for printing errors or any other mistakes in this manual.

We expressly point to our general guarantee terms which can be found in our general terms of business.


Specifications

Velocity	
Measurement range	0.00 ... 30.00 m/s 0.0 ... 5905.5 ft/min
Resolution	0.01 m/s 0.1 ft/min
Accuracy* the higher value applies	± 0.10 m/s or ± 5 % of rdg. at 0 ... 5 m/s ± 0.30 m/s or ± 5 % of rdg. at 5 ... 30 m/s ± 19.6 ft/min or ± 5 % of rdg. at 0 ... 984.2 ft/min ± 59.0 ft/min or ± 5 % of rdg. at 984.2 ... 5905.5 ft/min
Flow rate	
Measurement range	0.0 ... 339120.0 m ³ /h 0.0 ... 99598.0 CFM
Resolution	0.1 m ³ /h 0.1 CFM
Temperature	
Measurement range	0 ... 50 °C 32 ... 122 °F
Resolution	0.1 °C 0.1 °F
Accuracy*	± 1 °C ± 1.8 °F
Further specification	
Telescopic probe length	210 ... 426 mm / 8.2 ... 16.7"
Telescopic probe diameter	12 mm / 0.47"
Memory space	10,000 measuring points
File format	CSV
Interface	micro USB
Bracket	3/8" tripod bracket
Display	2" LCD, 176 x 220 pixels
Measurement rate	1 Hz
Power supply (rechargeable battery)	internal rechargeable 1000 mAh battery
Power supply (external)	5 V DC, 1 A
Operating conditions	0 ... 50 °C (32 ... 122 °F), <85 % RH, non-condensing
Storage conditions	-10 ... 60 °C (14 ... 140 °F), <85 % RH, non-condensing
Dimensions (without telescopic probe)	145 x 50 x 35 mm / 5.7 x 1.9 x 1.3"
Weight	156 g / 0.34 lbs

Delivery scope


1 x hot wire anemometer PCE-423N
1 x micro USB cable

Device description

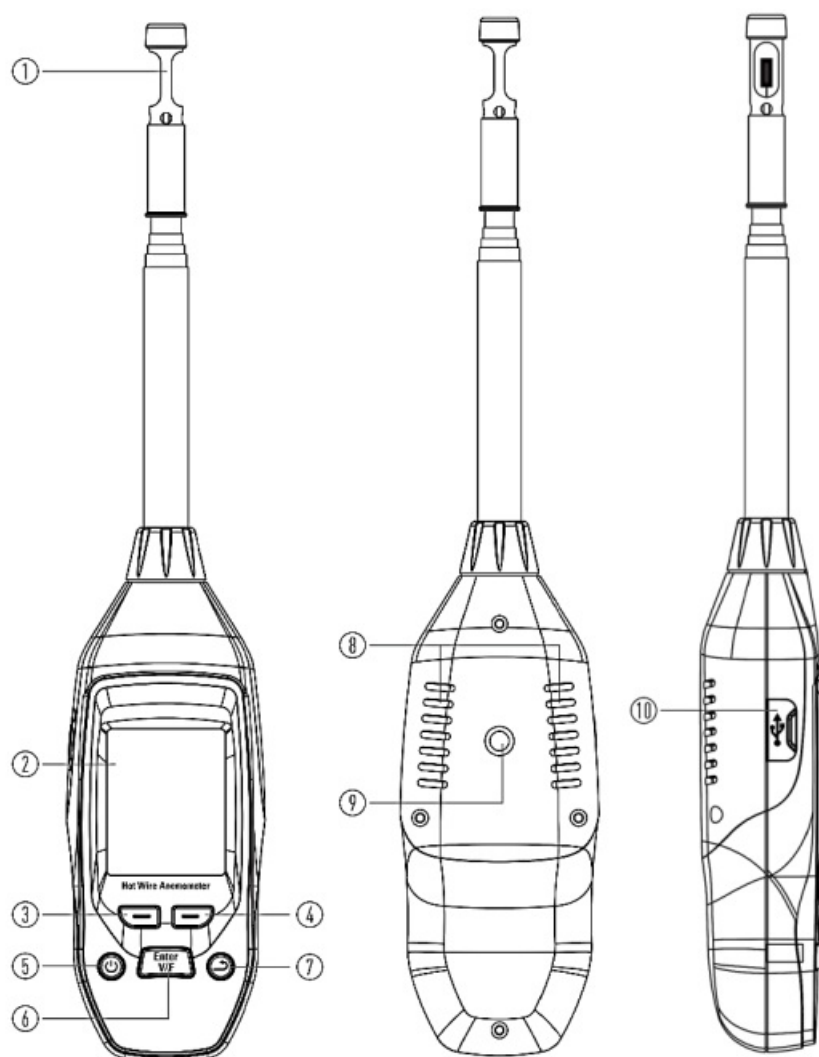

No.	Meaning / function
1	flow sensor, temperature sensor
2	display
3	left function key
4	right function key
5	on/off key
6	Enter-V/F key, toggle key (velocity. flow rate)
7	back key
8	air slits
9	tripod bracket
10	micro USB connector

Switching the meter on and off

To switch the meter on or off, press and hold the  key.

Measurement preparation


Before making a measurement, slide the probe guard down. Switch on the device. Point the opening of the sensor in the direction of the flow to be measured. When you have finished your measurement, push the guard back up so that the sensor system is not damaged.

Measuring mode



7.1 Main display

After the meter has been switched on, the velocity measurement is carried out immediately. At the same time, the current temperature is measured and displayed. To select between the velocity and the flow rate measurement, press and release the enter-V/F key once. The “V” on the display stands for velocity and the “F” for flow. The flow rate depends on the velocity and the set area. You can set the area under 8.2 Flow rate setting to set the area.

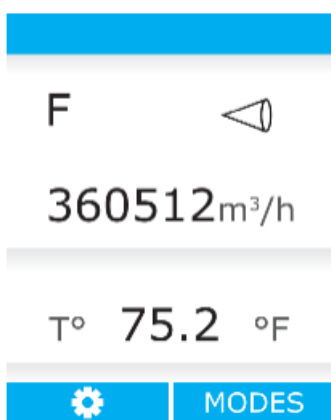Note: Saving individual measured values is not possible in normal measuring mode:






7.2 Average measurement (time-dependent)


To display the average, press the right function key in measuring mode to select **MODES**. The display now shows **AVG** for the average reading (time-dependent) and . Now press the left function key to select **AVG**. The current velocity, the average, the highest and the lowest measured value are displayed here. Press the left function key to save the displayed values **SAVE**. Press the right function key to start or pause the current average measurement . To repeat the average measurement, go to normal measurement mode with the back key and start the average measurement again.




7.3 Average measurement (different points)

To determine the average of different measuring points, press the right function key **MODES** in measuring mode.

Press the right function key again to select . To save the displayed values, now press the left function key . The values are saved once per keystroke. To include the current measuring point in the average measurement and select the next one, press the right function key . To repeat the average measurement, go back to normal measuring mode with the back key and start the average measurement again.

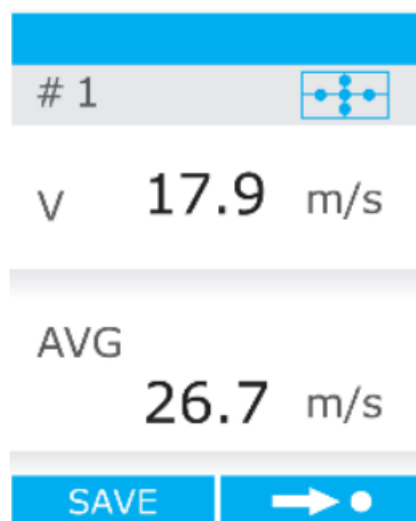

Settings

To make settings, press the left function key  in measuring mode. Use the function keys to select between the individual functions displayed. At the same time, you can change selected parameters with the function keys. To open a setting, press the enter-V/F key. Press the back key to go back one level. Press the enter-V/F key to confirm your entry.



Setting	Meaning
Unit	Set the unit
Area / Funnel	Enter the dimensions for the flow rate
Auto-off	Set the automatic power off
History	Read memory
Brightness	Show brightness of the display
Date / Time	Set date and time
Calibration	Calibrate flow

8.1 Set unit

To set the unit for the flow and the temperature, go to the Settings menu and to the Unit menu item. Here, you can select between the temperature or the flow rate. Then you can change the unit.

Function	Units
Flow rate	m/s, m ³ /h / ft/min, CFM
Temperature	°C, °F


8.2 Flow rate setting

To specify the dimensions for the flow rate, go to the settings and select the menu item “Area/Funnel”. Here, you can specify four different dimensions for square as well as round areas. In addition, a cylindrical area can be specified. The last selected area is adopted in measuring mode.



8.3 Automatic power off


Via the automatic power off function, the meter can be set to switch itself off after the set time. The following setting options are available here: “NONE” (function deactivated), 2 minutes, 10 minutes, 1 hour.

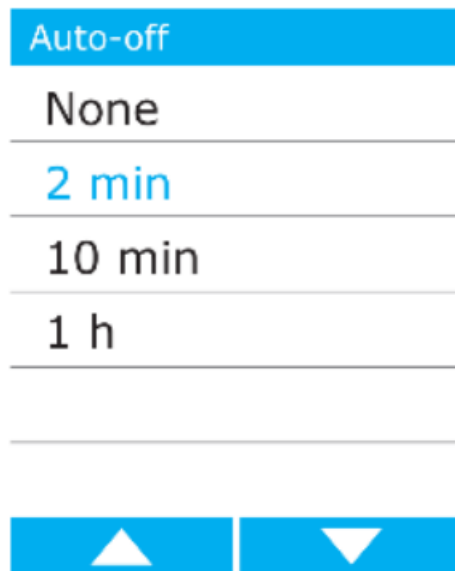

8.4 View saved data

To view the saved data, go to the settings and select the item “History”. All saved measurement data can be viewed there. It is not possible to delete or edit the data on the meter itself.

Note: If no data has been saved, this item cannot be opened.

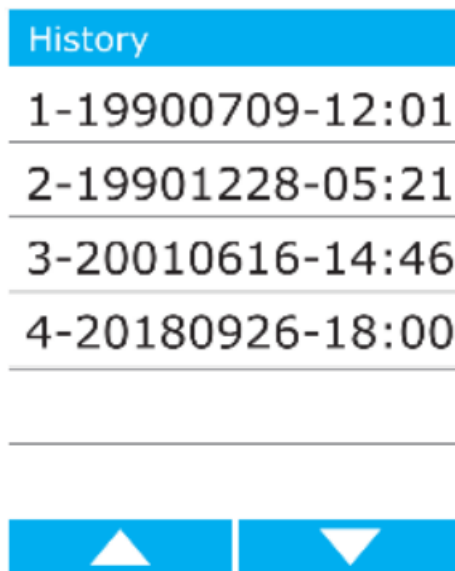


8.4.1 Transfer data to the computer

To transfer the measurement data to a computer, the meter must first be switched off. Now connect the meter to a computer which recognises it as a mass data storage device. The data can now be found in CSV data format.

8.5 Display brightness

To adjust the display brightness, go to the settings and open the item “Brightness”. You can now use the function keys to adjust the brightness of the display.

Brightness

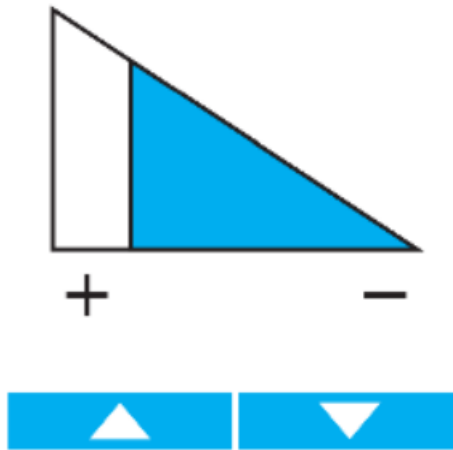

8.6 Date and time

To set the date and time, go to the settings and open the menu item "Data/Time Setup". Here, the date and time can be set in the format YYYY/MM/DD. You can also choose between English and German style here. Use the function keys to change the parameters as desired. Use the enter-V/F key to accept the value and jump to the next item at the same time.

Data & Time

2018/08/13


12H AM

10:47



8.7 Calibration

To calibrate the flow rate, go to the "Calibration" item in the settings. Here the displayed measured value can be set using a factor ("Gain"). The default value is 1.00. The coefficient range is between 0.5 and 2.

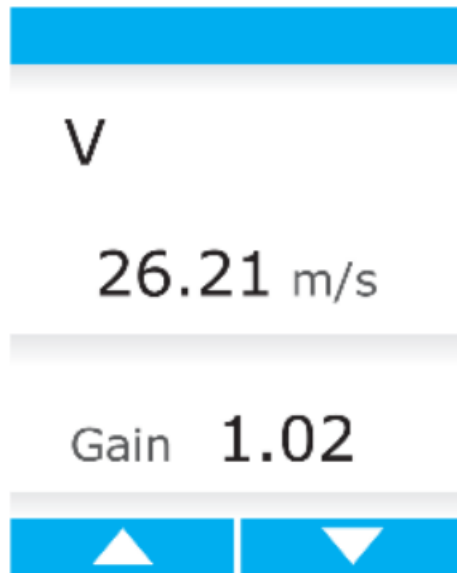

Contact

If you have any questions, suggestions or technical problems, please do not hesitate to contact us. You will find the relevant contact information at the end of this user manual.

Disposal


For the disposal of batteries in the EU, the 2006/66/EC directive of the European Parliament applies. Due to the contained pollutants, batteries must not be disposed of as household waste.

They must be given to collection points designed for that purpose.

In order to comply with the EU directive 2012/19/EU we take our devices back. We either re-use them or give them to a recycling company which disposes of the devices in line with law.

For countries outside the EU, batteries and devices should be disposed of in accordance with your local waste regulations.

If you have any questions, please contact PCE Instruments.

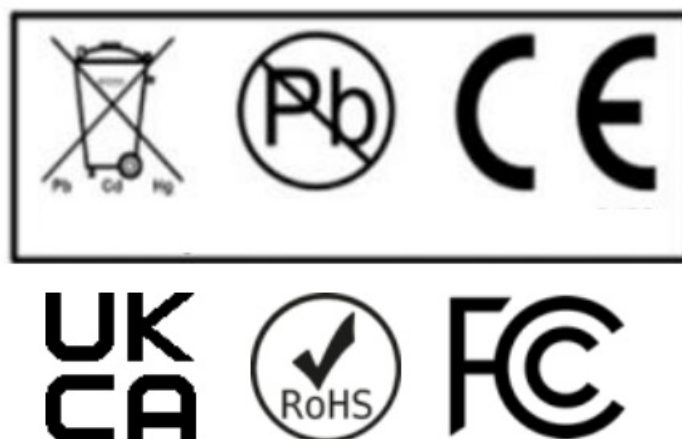


PCE Instruments contact information

<p>Germany PCE Deutschland GmbH Im Langel 26 D-59872 Meschede Deutschland Tel.: +49 (0) 2903 976 99 0 Fax: +49 (0) 2903 976 99 29 info@pce-instruments.com www.pce-instruments.com/deutsch</p>	<p>France PCE Instruments France EURL 23, rue de Strasbourg 67250 Soultz-Sous-Forets France Téléphone: +33 (0) 972 3537 17 Numéro de fax: +33 (0) 972 3537 18 info@pce-france.fr www.pce-instruments.com/french</p>	<p>Spain PCE Ibérica S.L. Calle Mayor, 53 02500 Tobarra (Albacete) España Tel. : +34 967 543 548 Fax: +34 967 543 542 info@pce-iberica.es www.pce-instruments.com/espanol</p>
<p>United Kingdom PCE Instruments UK Ltd Unit 11 Southpoint Business Park Ensign Way, Southampton Hampshire United Kingdom, SO31 4RF Tel: +44 (0) 2380 98703 0 Fax: +44 (0) 2380 98703 9 info@pce-instruments.co.uk www.pce-instruments.com/english</p>	<p>Italy PCE Italia s.r.l. Via Pesciatina 878 / B-Interno 6 55010 Loc. Gragnano Capannori (Lucca) Italia Telefono: +39 0583 975 114 Fax: +39 0583 974 824 info@pce-italia.it www.pce-instruments.com/italiano</p>	<p>Turkey PCE Teknik Cihazları Ltd.Şti. Halkalı Merkez Mah. Pehlivan Sok. No.6/C 34303 Küçükçekmece – İstanbul Türkiye Tel: 0212 471 11 47 Faks: 0212 705 53 93 info@pce-cihazlari.com.tr www.pce-instruments.com/turkish</p>
<p>The Netherlands PCE Brookhuis B.V. Institutenweg 15 7521 PH Enschede Nederland Telefoon: +31 (0)53 737 01 92 info@pcebenelux.nl www.pce-instruments.com/dutch</p>	<p>United States of America PCE Americas Inc. 1201 Jupiter Park Drive, Suite 8 Jupiter / Palm Beach 33458 FL USA Tel: +1 (561) 320-9162 Fax: +1 (561) 320-9176 info@pce-americas.com www.pce-instruments.com/us</p>	<p>Denmark PCE Instruments Denmark ApS Birk Centerpark 40 7400 Herning Denmark Tel.: +45 70 30 53 08 kontakt@pce-instruments.com www.pce-instruments.com/dansk</p>

© PCE Instruments

Documents / Resources

	<p>PCE INSTRUMENTS PCE-423N Hot Wire Anemometer [pdf] User Manual PCE-423N Hot Wire Anemometer, PCE-423N, Hot Wire Anemometer, Wire Anemometer</p>
---	--

References

- [France.fr : Actualités, destinations et infos du tourisme en France](#)

- [!\[\]\(83eb2aa26b610eb6a9dca7cf4702d681_img.jpg\) iberica.es](http://iberica.es)
- [!\[\]\(94dfacbf937cdd7da4837a6fcd8fc785_img.jpg\) Make an offer on the domain instruments.co.uk - Domains.co.uk](https://domains.co.uk)
- [!\[\]\(dae8c3c5fa7c80febd6526a5e8a853bf_img.jpg\) Computer Instruments | Home](#)
- [!\[\]\(8f38ab9775d1331a4e1fd6648d0a83f1_img.jpg\) Discover Italy: Official Tourism Website - Italia.it](http://italia.it)
- [!\[\]\(5e48b3241d711ef916255d822ab3415f_img.jpg\) Industrial Measurement Products and Solutions | PCE Instruments](#)
- [!\[\]\(c4c3604751fde0df44855086d7798e30_img.jpg\) PCE Instruments Denmark ApS | PCE Instruments](#)
- [!\[\]\(a16ee0329f478adb49fd7876490e96fe_img.jpg\) PCE Deutschland GmbH Prüfgeräte vom Hersteller | PCE Instruments](#)
- [!\[\]\(a8a494e883c31c6f4a74584cc935a790_img.jpg\) PCE Brookhuis B.V. | PCE Instruments](#)
- [!\[\]\(8a50a875cd94cd57f6a7348a4d34b45f_img.jpg\) PCE Americas Inc. : Test Instruments | PCE Instruments](#)
- [!\[\]\(7ddc0498d10972f0f157498fccf65370_img.jpg\) PCE Iberica S.L. Instrumentación | PCE Instruments](#)
- [!\[\]\(1481f3a2b8d8d64dbbf1eb2242b57620_img.jpg\) PCE Instruments France | PCE Instruments](#)
- [!\[\]\(1d12b5523dd7503f9f6b056602d4b0bb_img.jpg\) PCE Italia s.r.l. / Strumenti di Misura | PCE Instruments](#)
- [!\[\]\(a3cf9896eece75d50b7dee194989c9bc_img.jpg\) PCE Teknik Cihazlar Paz. Tic. Ltd.Şti. | PCE Instruments](#)
- [!\[\]\(26147612c3694ee09d020cac0faae7d9_img.jpg\) PCE Americas Inc. : Test Instruments | PCE Instruments](#)
- [!\[\]\(46af714d66844046465576855b12c56a_img.jpg\) Industrial Measurement Products and Solutions | PCE Instruments](#)
- [User Manual](#)

Manuals+