

PCE Instruments PCE-AC 2000 CO2 Analyser User Manual

[Home](#) » [PCE Instruments](#) » PCE Instruments PCE-AC 2000 CO2 Analyser User Manual 

PCE Instruments PCE-AC 2000 CO2 Analyser User Manual



Contents

- [1 Safety notes](#)
- [2 Device description](#)
- [3 Technical specifications](#)
- [4 Operation](#)
- [5 Warranty](#)
- [6 Disposal](#)
- [7 PCE Instruments contact information](#)
- [8 Documents / Resources](#)
 - [8.1 References](#)
- [9 Related Posts](#)

Safety notes

Please read this manual carefully and completely before you use the device for the first time. The device may only be used by qualified personnel and repaired by PCE Instruments personnel. Damage or injuries caused by non-observance of the manual are excluded from our liability and not covered by our warranty.

- The device must only be used as described in this instruction manual. If used otherwise, this can cause dangerous situations for the user and damage to the meter.
- The instrument may only be used if the environmental conditions (temperature, relative humidity, ...) are within the ranges stated in the technical specifications. Do not expose the device to extreme temperatures, direct sunlight, extreme humidity or moisture.
- Do not expose the device to shocks or strong vibrations.
- The case should only be opened by qualified PCE Instruments personnel.
- Never use the instrument when your hands are wet.
- You must not make any technical changes to the device.
- The appliance should only be cleaned with a damp cloth. Use only pH-neutral cleaner, no abrasives or solvents.
- The device must only be used with accessories from PCE Instruments or equivalent.
- Before each use, inspect the case for visible damage. If any damage is visible, do not use the device.
- Do not use the instrument in explosive atmospheres.
- The measurement range as stated in the specifications must not be exceeded under any circumstances.
- Non-observance of the safety notes can cause damage to the device and injuries to the user

We do not assume liability for printing errors or any other mistakes in this manual.

We expressly point to our general guarantee terms which can be found in our general terms of business.

If you have any questions please contact PCE Instruments. The contact details can be found at the end of this manual.

Device description

Front side / CO2 traffic light

CO2 good / green:

0 ... 599 ppm


CO2 OK / yellow:

600 ... 1199 ppm

CO2 poor / red:

1200 ... 9999 ppm

Rear side

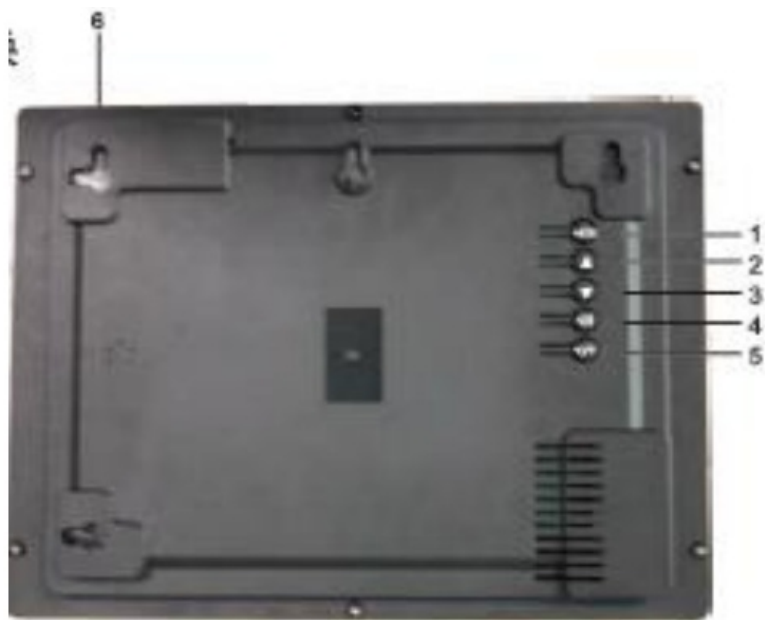

1. Mode key
2. Up key
3. Down key
4. Alarm key
5. °C / °F key
6. Socket for power supply

Technical specifications

CO2	
Measurement range	0 ... 9999 ppm
Accuracy	±70 ppm ±5 % of rdg.
Resolution	1 ppm
Temperature	
Measurement range	-10 ... 100 °C
Resolution	0.1 °C
Accuracy	±1.5 °C
Relative humidity	
Measurement range	0... 99.9 % RH
Resolution	0.1 % RH
Accuracy	±3 %
General	
Traffic light function	green: 0 ... 599 ppm yellow: 600 ... 1199 ppm red: 1200 ... 9999 ppm
Alarm	adjustable, audible
Repeatability	<±0.5 %
Response time	10 s
Operating conditions	0 ... 50 °C, 0 ... 90 % RH, non-condensing
Storage conditions	-30 ... 70 °C, 0 ... 90 % RH, non-condensing
Power supply	via mains adaptor 9 VDC, 350 mA
Dimensions	388 x 288 x 43 mm
Weight	approx. 2420 g

Operation

Power on CO2 analyser

As soon as you connect the mains adapter to the CO2 analyser via the plug socket, the analyser will power on. The initialization time is 7 seconds. The meter displays a countdown. After the time has elapsed, the unit is ready for operation.

Switch unit

Press the °C/°F key to switch the unit for the temperature between °C and °F.

Set alarm

Press the mode key to set the alarm. Use the arrow keys to adjust the alarm value up or down. Once the desired value has been set, press the mode key to save the setting.

Note: An alarm value of 1200 ppm is set at the factory.

Warranty

You can read our warranty terms in our General Business Terms which you can find here: <https://www.pce-instruments.com/english/terms>.

Disposal

For the disposal of batteries in the EU, the 2006/66/EC directive of the European Parliament applies. Due to the contained pollutants, batteries must not be disposed of as household waste.

They must be given to collection points designed for that purpose.

In order to comply with the EU directive 2012/19/EU we take our devices back. We either re-use them or give them to a recycling company which disposes of the devices in line with law.

For countries outside the EU, batteries and devices should be disposed of in accordance with your local waste regulations.

If you have any questions, please contact PCE Instruments.



PCE Instruments contact information

Germany

PCE Deutschland GmbH Im Langel 4
D-59872 Meschede
Deutschland
Tel.: +49 (0) 2903 976 99 0
Fax: +49 (0) 2903 976 99 29
info@pce-instruments.com
<http://www.pce-instruments.com/deutsch>

United Kingdom

PCE Instruments UK Ltd Unit 11 Southpoint Business Park Ensign Way, Southampton Hampshire United Kingdom, S031 4RF
Tel: +44 (0) 2380 98703 0
Fax: +44 (0) 2380 98703 9
info@pce-instruments.co.uk
www.pce-instruments.com/english

The Netherlands

PCE Brookhuis B.V. Institutenweg 15 7521 PH Enschede Nederland

Telefoon: +31 (0)53 737 01 92
info@pcebenelux.nl
www.pce-instruments.com/dutch

United States of America

PCE Americas Inc. 1201 Jupiter Park Drive, Suite 8 Jupiter / Palm Beach 33458 FL USA
Tel: +1 (561) 320-9162
Fax: +1 (561) 320-9176
info@pce-americas.com
www.pce-instruments.com/us

France

PCE Instruments France EURL 23, rue de Strasbourg 67250 Soultz-Sous-Forets France Telephone: +33 (0) 972 3537 17 Numero de fax: +33 (0) 972 3537 18 info@pce-france.fr www.pce-instruments.com/french

Italy

PCE Italia s.r.l. Via Pesciatina 878 / B-Interno 6 55010 Loc. Gragnano Capannori (Lucca) Italia
Telefono: +39 0583 975 114
Fax: +39 0583 974 824
info@pce-italia.it
www.pce-instruments.com/italiano

China

PCE (Beijing) Technology Co., Limited 1519 Room, 6 Building Zhong Ang Times Plaza No. 9 Mentougou Road, Tou Gou District 102300 Beijing, China
Tel: +86 (10) 8893 9660
info@pce-instruments.cn
www.pce-instruments.cn

Spain

PCE Iberica S.L. Calle Mayor, 53 02500 Tobarra (Albacete) Espana Tel. : +34 967 543 548
Fax: +34 967 543 542
info@pce-iberica.es
www.pce-instruments.com/espanol


Turkey

PCE Teknik Cihazlan Ltd. ?ti. Halkali Merkez Mah. Pehlivan Sok. No.6/C 34303 Kliglikgekmece – Istanbul TOrkiye
Tel: 0212 471 11 47
Faks: 0212 705 53 93
info@pce-cihazlari.com.tr
www.pce-instruments.com/turkish

Hong Kong

PCE Instruments HK Ltd. Unit J, 21/F., COS Centre 56 Tsun Yip Street Kwun Tong Kowloon, Hong Kong
Tel: +852-301-84912
jyi@pce-instruments.com
www.pce-instruments.cn

Documents / Resources



[PCE Instruments PCE-AC 2000 CO2 Analyser](#) [pdf] User Manual
PCE-AC 2000 CO2 Analyser, PCE-AC 2000, CO2 Analyser

References

- [France.fr : Actualités, destinations et infos du tourisme en France](#)
- [iberica.es](#)
- [instruments.cn](#)
- [Make an offer on the domain instruments.co.uk - Domains.co.uk](#)
- [Computer Instruments | Home](#)
- [Discover Italy: Official Tourism Website - Italia.it](#)
- [PCEi¼^âCE—äº-ï¼%ç\\$'æŠ€æœ%é™â...-â](#)
- [Industrial Measurement Products and Solutions | PCE Instruments](#)
- [PCE Deutschland GmbH Prüfgeräte vom Hersteller | PCE Instruments](#)
- [PCE Brookhuis B.V. | PCE Instruments](#)
- [PCE Americas Inc. : Test Instruments | PCE Instruments](#)
- [PCE Iberica S.L. Instrumentación | PCE Instruments](#)
- [PCE Instruments France | PCE Instruments](#)
- [PCE Italia s.r.l. / Strumenti di Misura | PCE Instruments](#)
- [PCE Teknik Cihazlar Paz. Tic. Ltd.Şti. | PCE Instruments](#)
- [PCE Americas Inc. : Test Instruments | PCE Instruments](#)
- [PCE Americas Inc. : Test Instruments | PCE Instruments](#)