

# **PHILIPS APPLE IOS Bluetooth Pairing Instruction Manual**

Home » Philips » PHILIPS APPLE IOS Bluetooth Pairing Instruction Manual



### **EXISTING ACCOUNTS APPLE IOS**

Bluetooth Pairing Guide for the Philips DreamMapper mobile app

This guide is for patients with an Apple IOS device who have an existing DreamMapper account.

Please ensure you are next to your sleep apnea machine, that it is plugged in and that the blower is not running.

In June 2021, after discovering a potential health risk related to the foam in certain CPAP, BiPAP and Mechanical Ventilator devices, Philips issued a voluntary Field Safety Notice (outside U.S.) / voluntary recall notification (U.S. only). As part of our remediation process, patients whose affected device is not equipped with a wireless modem must transmit their device settings following the steps outlined below. Once this operation is complete, we will be able to set the proper prescription on your replacement device.

Instructions: Bluetooth Pairing Guide for Existing DreamMapper Accounts


#### **Contents**

- 1 App Setup for Existing DreamMapper Accounts
- 2 DreamStation Setup
- 3 Turn on Bluetooth
- **4 Bluetooth Setup**
- 5 Bluetooth Pairing
- **6 Data Transfer**
- 7 Completion
- 8 Documents / Resources
  - 8.1 References
- 9 Related Posts


### **App Setup for Existing DreamMapper Accounts**

To ensure the proper prescription on your replacement device, please verify that the email address you are using for DreamMapper matches either the email address you used to register your device with for the Voluntary Device Recall OR matches the email address we recently contacted you about the recall.

To check your email address on the DreamMapper app:

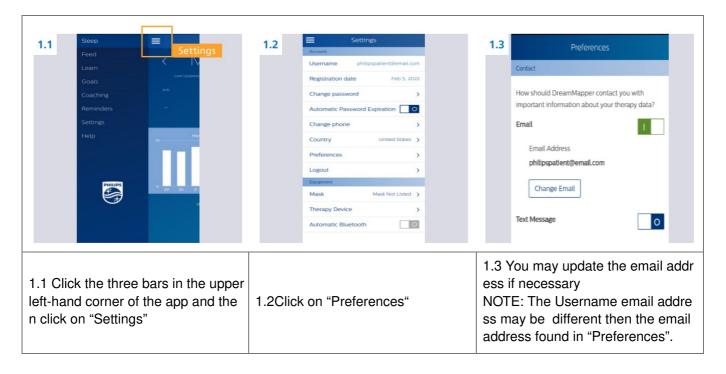


## **DreamStation Setup**

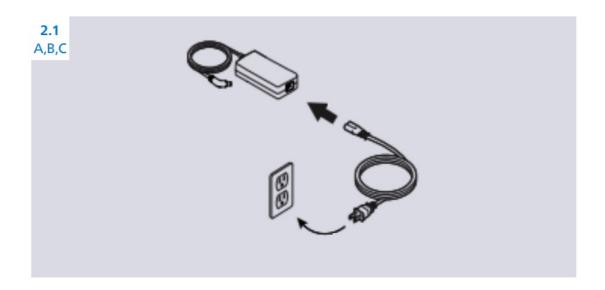

### 2.1 Supply AC Power to the DreamStation machine


Complete the following steps to operate the device using AC power:

- A. Plug the socket end of the AC power cord (included) into the power supply (also included).
- B. Plug the pronged end of the AC power cord into an electrical outlet that is not controlled by a wall switch
- C. Plug the power supply cord's connector Into the power inlet on the side of the device

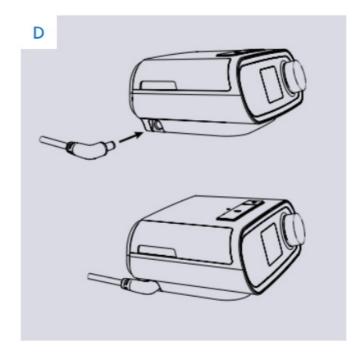


D. Verify that the plug at the si de of the device, at the power supply, and at the electrical outlet are fully Inserted. This will help to ensure that a secure reliable electrical connection has been made.


Note: If the following Check Power icon appears on the screen. Please repeat seep 4.

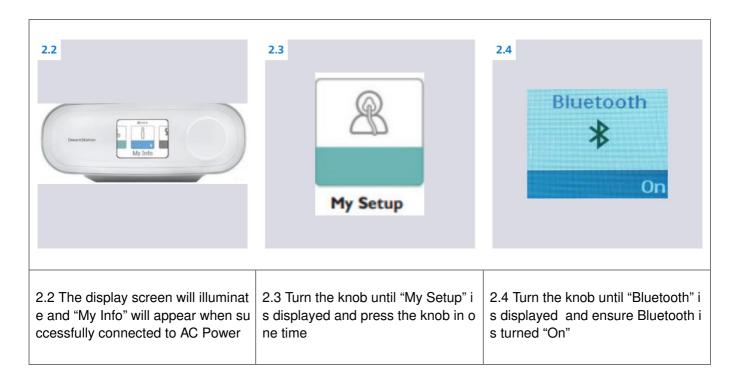


## **Turn on Bluetooth**

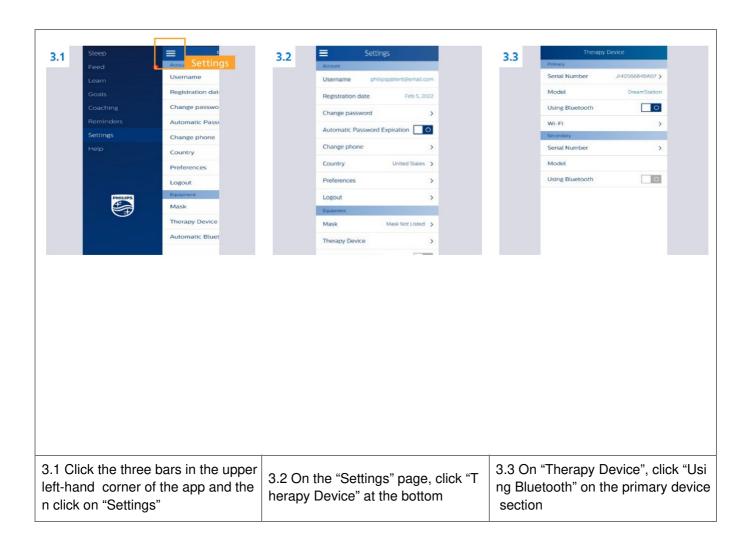

# **Bluetooth Setup**

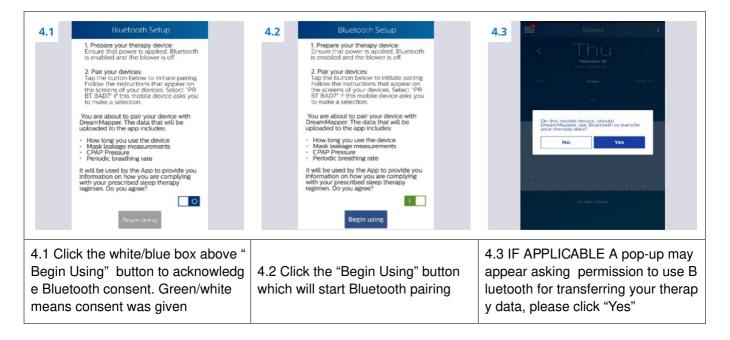


**Instructions:** Bluetooth Pairing Guide for Existing DreamMapper Accounts **Turn on Bluetooth Continued** 

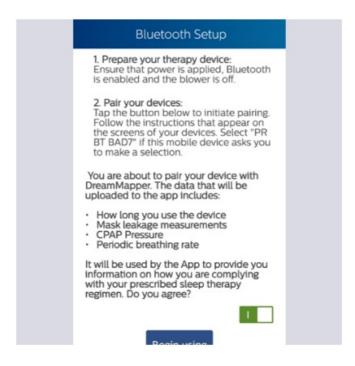


4.4 IF APPLICABLE After clicking "Yes" in step 3, click the "Begin Using" button again for Bluetooth Pairing

# **Bluetooth Pairing**







5.1 A pairing request will appear on your mobile device, asking you to enter a 6-digit code

5.2 On the display screen of your sl eep machine, you will see the word "Pair" and the word "No" in the low er left-hand corner 5.3 Turn the knob on your sleep ma chine which will change the "No" to "Yes" and press the knob in one tim e, a 6-digit code will appear




5.4 Type the 6-digit code into your Apple mobile device and then select "Pair"

## **Data Transfer**



- 6.1 IF APPLICABLE Click "Yes" to acknowledge data sharing which is necessary to capture your machine s therapy settings
- 6.2 You will return to the "Therapy Device" screen. The "Using Bluetoo th" box on the primary device shoul d now be green/ white
- 6.3 Go back one screen to the main "Settings" screen, click the three b ars in the upper left-hand corner a nd select "Sleep"

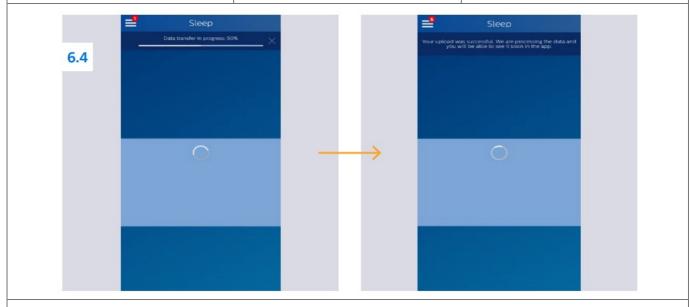

6.4 Once the transfer reaches 100% and you receive a message that the upload was successful, you are done!

## Completion

7.1 Thank you for completing the above steps! We will now be able to set the proper prescription for your replacement sleep machine.

Complete DreamMapper instructions for use can be found in the application under Help-FAQ tab. You may also contact DreamMapper Support at 844-240-1649.

For more information regarding the voluntary recall process, please visit: <a href="mailto:phillips.com/src-recall-process">phillips.com/src-recall-process</a>





## **Documents / Resources**



<u>PHILIPS APPLE IOS Bluetooth Pairing</u> [pdf] Instruction Manual APPLE IOS Bluetooth Pairing, Bluetooth Pairing, IOS Bluetooth Pairing, APPLE Bluetooth Pairing

### References

- O Understanding the recall process | Philips Healthcare
- Philips United States | Philips

Manuals+,