



ResMed AirCurve 10 VAuto Auto-Adjusting Bilevel Device User Guide

[Home](#) » [ResMed](#) » ResMed AirCurve 10 VAuto Auto-Adjusting Bilevel Device User Guide 

ResMed AirCurve 10 VAuto Auto-Adjusting Bilevel Device User Guide



Welcome

The AirCurve™ 10 VAuto, AirCurve 10 S and AirCurve 10 ST are bilevel positive airway pressure devices.

 **WARNING**

 **CAUTION**

In the US, Federal law restricts this device to sale by or on the order of a physician.

Contents

- [1 Indications for use](#)
- [2 Setup](#)
- [3 My Options](#)
- [4 Cleaning](#)
 - [4.1 Reassembling](#)
- [5 Traveling](#)
- [6 Troubleshooting](#)
- [7 General troubleshooting](#)
- [8 Device messages](#)
- [9 General warnings and cautions](#)
- [10 Technical specifications](#)
- [11 Symbols](#)
- [12 Product](#)
- [13 Documents / Resources](#)
 - [13.1 References](#)
- [14 Related Posts](#)

Indications for use

AirCurve 10 VAuto

The AirCurve 10 VAuto device is indicated for the treatment of obstructive sleep apnea (OSA) in patients weighing more than 66 lb (30 kg). It is intended for home and hospital use. The humidifier is intended for single patient use in the home environment and re-use in a hospital/institutional environment.

AirCurve 10 S

The AirCurve 10 S device is indicated for the treatment of obstructive sleep apnea (OSA) in patients weighing more than 66 lb (30 kg). It is intended for home and hospital use. The humidifier is intended for single patient use in the home environment and re-use in a hospital/institutional environment.

AirCurve 10 ST

The AirCurve 10 ST device is indicated for the treatment of obstructive sleep apnea (OSA) in patients weighing more than 66 lb (30 kg). It is intended for home and hospital use. The humidifier is intended for single patient use in the home environment and re-use in a hospital/institutional environment.

Contraindications

Positive airway pressure therapy may be contraindicated in some patients with the following preexisting conditions:

- severe bullous lung disease
pneumothorax or pneumomediastinum
- pathologically low blood pressure, particularly if associated with intravascular volume depletion
- dehydration
- cerebrospinal fluid leak, recent cranial surgery, or trauma.

Adverse effects

You should report unusual chest pain, severe headache, or increased breathlessness to your prescribing physician. An acute upper respiratory tract infection may require temporary discontinuation of treatment.

The following side effects may arise during the course of therapy with the device:

- drying of the nose, mouth, or throat
- nosebleed
- bloating
- ear or sinus discomfort
- eye irritation
- skin rashes.

At a glance

The AirCurve 10 includes the following:

- Device with HumidAir™ integrated humidifier
- Water tub
- Air tubing
- Power supply unit
- Travel bag
- SD card (already inserted).

Contact your care provider for a range of accessories available for use with the device including:

- Air tubing (heated and non-heated): ClimateLineAir™, SlimLine™, Standard
- Water tub: Standard water tub, cleanable water tub (can be disinfected)
- Filter: Hypoallergenic filter, standard filter
- Air10™ DC/DC converter
- SD card reader
- Air10 oximeter adapter
- Air10 USB adapter.

About your device



2. Air filter cover
3. Power inlet
4. Serial number and device number
5. Water tub
6. Screen
7. Adapter cover
8. SD card cover

About the control panel



Start/Stop button

Press to start/stop therapy.

Press and hold for three seconds to enter power save mode.



Dial

Turn to navigate the menu and press to select an option.









Turn to adjust a selected option and press to save your change.




Home button

Press to return to the Home screen.

Different icons may be displayed on the screen at different times including:

-  Ramp Time
-  Humidity
-  Humidifier warming
-  Humidifier cooling
-  Wireless signal strength (green)
-  Wireless transfer not enabled (gray)
-  No wireless connection
-  Airplane Mode

Setup

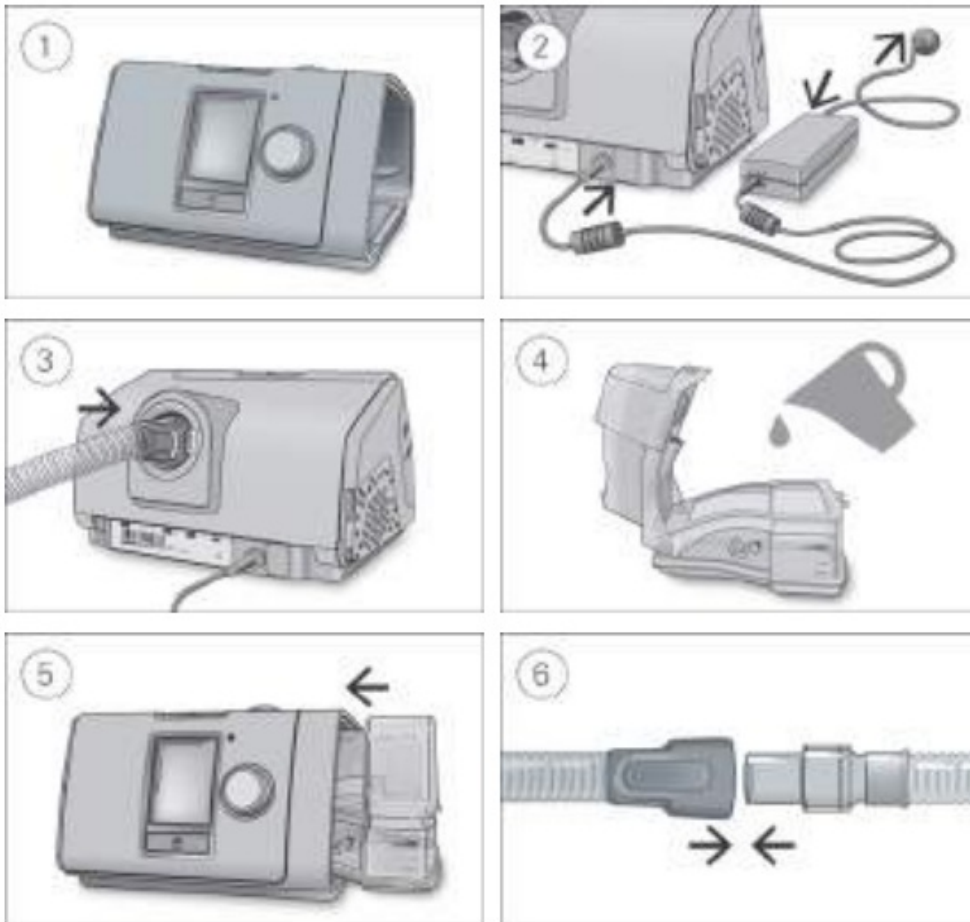

CAUTION

Do not overfill the water tub as water may enter the device and air tubing.

1. Place the device on a stable level surface.
2. Plug the power connector into the rear of the device. Connect one end of the power cord into the power supply unit and the other end into the power outlet.
3. Connect the air tubing firmly to the air outlet located on the rear of the device.
4. Open the water tub and fill it with distilled water up to the maximum water level mark. Do not fill the water tub with hot water.
5. Close the water tub and insert it into the side of the device.
6. Connect the free end of the air tubing firmly onto the assembled mask.
See the mask user guide for detailed information.
Recommended masks are available on www.resmed.com.

Starting therapy

1. Fit your mask.
2. Press Start/Stop or breathe normally if SmartStart is enabled.

You will know that therapy is on when the Sleep Report screen is displayed.



The pressure bar shows the inspiratory and expiratory pressures in green.

The green bar will expand and contract as you breathe in and out.

The screen will go black automatically after a short period of time. You can press Home or the dial to turn it back on. If power is interrupted during therapy, the device will automatically restart therapy when power is restored.

The AirCurve 10 device has a light sensor that adjusts the screen brightness based on the light in the room.

Stopping therapy

1. Remove your mask.
2. Press Start/Stop or if SmartStart is enabled, therapy will stop automatically after a few seconds.

The Sleep Report now gives you a summary of your therapy session.



Usage hours—Indicates the number of hours of therapy you received last session.

Mask Seal—Indicates how well your mask sealed:



Good mask seal.



Needs adjusting, see Mask Fit.

Humidifier—Indicates if your humidifier is working properly:



Humidifier working.



Humidifier might be faulty, contact your care provider.

If set by your care provider, you will also see:

Events per hour—Indicates the number of apneas and hypopneas experienced per hour.

More Info—Turn the dial to scroll down to view more detailed usage data.

Power save mode

- Your AirCurve 10 device records your therapy data. In order to allow it to transmit the data to your care provider, you should not unplug the device. However, you can put it into power save mode to save electricity.

To enter power save mode:

- Press and hold Start/Stop for three seconds.
The screen goes black.


To exit power save mode:

- Press Start/Stop once.
The Home screen is displayed.

My Options

Your AirCurve 10 device has been set up for your needs by your care provider, but you may find you want to make small adjustments to make your therapy more comfortable.

Highlight My Options and press the dial to see your current settings. From here, you can personalize your options.

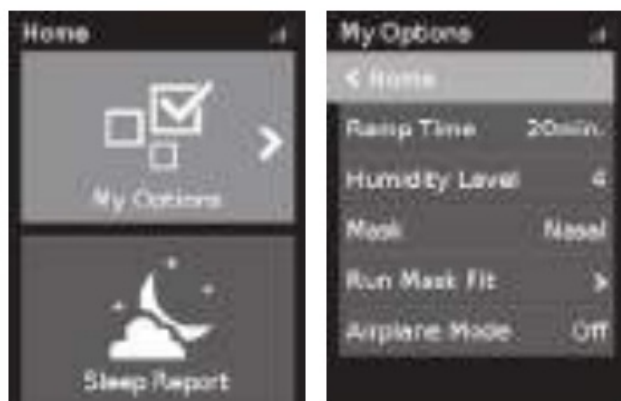


Ramp Time

Designed to make the beginning of therapy more comfortable, Ramp Time is the period during which the pressure increases from a low start pressure to the prescribed treatment pressure.

You can set your Ramp Time to Off or between 5 to 45 minutes.

To adjust Ramp Time:

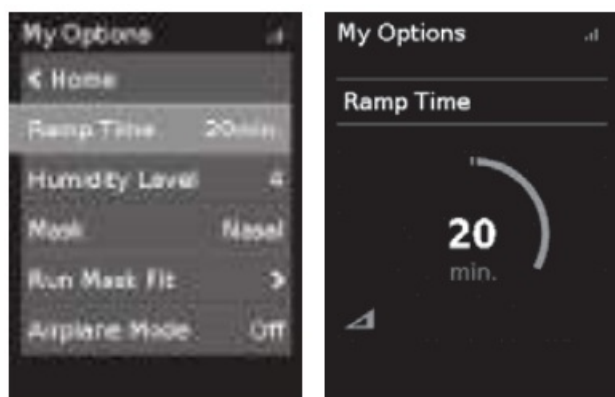


1. In My Options, turn the dial to highlight Ramp Time and then press the dial.
2. Turn the dial to adjust the ramp time to your preferred setting and press the dial to save the change.

Humidity Level

The humidifier moistens the air and is designed to make therapy more comfortable. If you are getting a dry nose or mouth, turn up the humidity. If you are getting any moisture in your mask, turn down the humidity. You can set the Humidity Level to Off or between 1 and 8, where 1 is the lowest humidity setting and 8 is the highest humidity setting.

To adjust the Humidity Level:

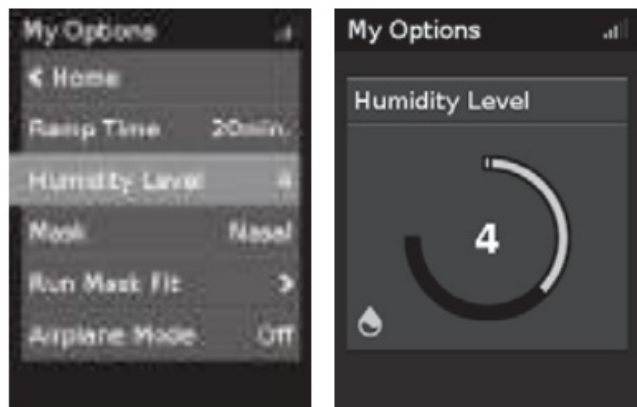

1. In My Options, turn the dial to highlight Humidity Level and then press the dial.
2. Turn the dial to adjust the humidity level and press the dial to save the change.

If you continue to get a dry nose or mouth, or moisture in your mask, consider using ClimateLineAir heated air tubing. ClimateLineAir together with Climate Control delivers more comfortable therapy.

Mask Fit

Mask Fit is designed to help you assess and identify possible air leaks around your mask.

To check Mask Fit:



1. Fit the mask as described in the mask user guide.
2. In My Options, turn the dial to highlight Run Mask Fit and then press the dial.
The device starts blowing air.
3. Adjust the mask, mask cushion and headgear until you get a Good result.

To stop Mask Fit, press the dial or Start/Stop. If you are unable to get a good mask seal, talk to your care provider.

More options

Your care provider may have given you access to personalize a few more options.

Leak Alert: When Leak Alert is enabled, the device beeps if the mask leaks too much air or if you remove the

mask during therapy.

SmartStart: When SmartStart is enabled, therapy starts automatically when you breathe into your mask. When you remove your mask, it stops automatically after few seconds.




Mask: This option shows your mask type setting. If you use more than one type of mask, adjust this setting when switching between masks.

Run Warmup: This option allows you to pre-heat the water before starting therapy, so that the air is not cold or dry at the beginning of therapy.

Caring for your device

It is important that you regularly clean your AirCurve 10 device to make sure you receive optimal therapy. The following sections will help you with disassembling, cleaning, checking and reassembling your device.

Disassembling

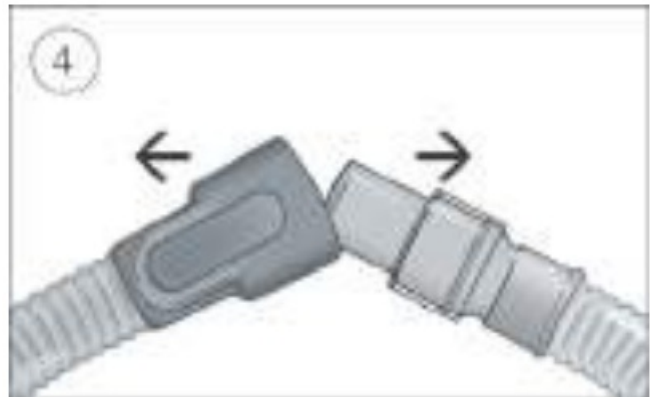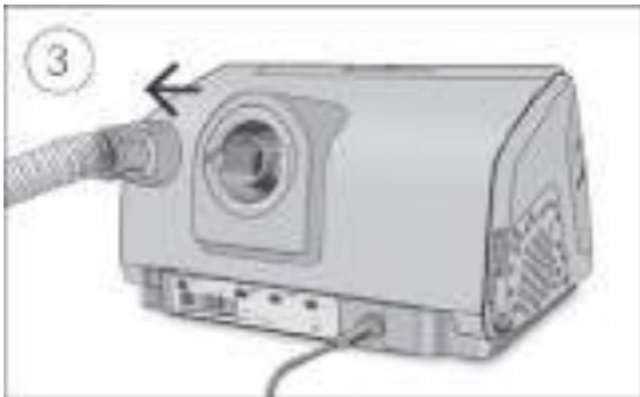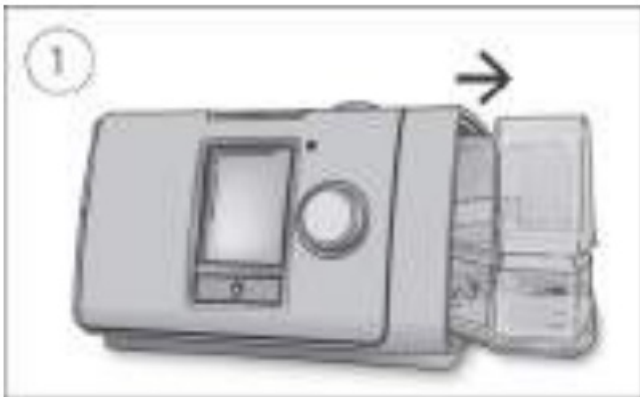

1. Hold the water tub at the top and bottom, press it gently and pull it away from the device.
2. Open the water tub and discard any remaining water.
3. Hold the cuff of the air tubing and gently pull it away from the device.
4. Hold both the cuff of the air tubing and the swivel of the mask, then gently pull apart.

Cleaning

You should clean the device weekly as described. Refer to the mask user guide for detailed instructions on cleaning your mask.

1. Wash the water tub and air tubing in warm water using mild detergent. Do not wash in a dishwasher or washing machine.
2. Rinse the water tub and air tubing thoroughly and allow to dry out of direct sunlight and/or heat.
3. Wipe the exterior of the device with a dry cloth.

Checking

You should regularly check the water tub, air tubing and the air filter for any damage.

1. Check the water tub:

- Replace it if it is leaking or has become cracked, cloudy or pitted.
 - Replace it if the seal is cracked or torn.
 - Remove any white powder deposits using a solution of one part household vinegar to 10 parts water.
2. Check the air tubing and replace it if there are any holes, tears or cracks.
 3. Check the air filter and replace it at least every six months. Replace it more often if there are any holes or blockages by dirt or dust.

To replace the air filter:



1. Open the air filter cover and remove the old air filter. The air filter is not washable or reusable.
2. Place a new air filter onto the air filter cover and then close it. Make sure the air filter is fitted at all times to prevent water and dust from entering the device.

Reassembling


When the water tub and air tubing are dry, you can reassemble the parts.

1. Connect the air tubing firmly to the air outlet located on the rear of the device.
2. Open the water tub and fill it with distilled room temperature water up to the maximum water level mark.
3. Close the water tub and insert it into the side of the device.
4. Connect the free end of the air tubing firmly onto the assembled mask.

Therapy data

Your AirCurve 10 device records your therapy data for you and your care provider so they can view and make changes to your therapy if required. The data is recorded and then transferred to your care provider wirelessly or via an SD card.

Wireless

Your AirCurve 10 device is equipped with cellular communication. This allows your therapy data to be wirelessly transmitted to your care provider to enhance the quality of your treatment. It also allows therapy settings to be updated in a more timely manner or your device software to be upgraded. The Wireless signal strength icon  displayed at the top right of your screen indicates the signal strength.

The data is usually transmitted after therapy has stopped. In order to make sure that your data is transferred, leave your device connected to the power outlet at all times and make sure that it is not in Airplane Mode.

Notes:


- Therapy data might not be transmitted if you use it outside of the country or region of purchase.
- Devices with cellular communication might not be available in all regions.

SD card

An alternative way for your therapy data to be transferred to your care provider is via the SD card. Your care provider may ask you to send the SD card by mail or to bring it in. When instructed by your care provider, remove the SD card.

Do not remove the SD card from the device when the SD light is flashing.

To remove the SD card:

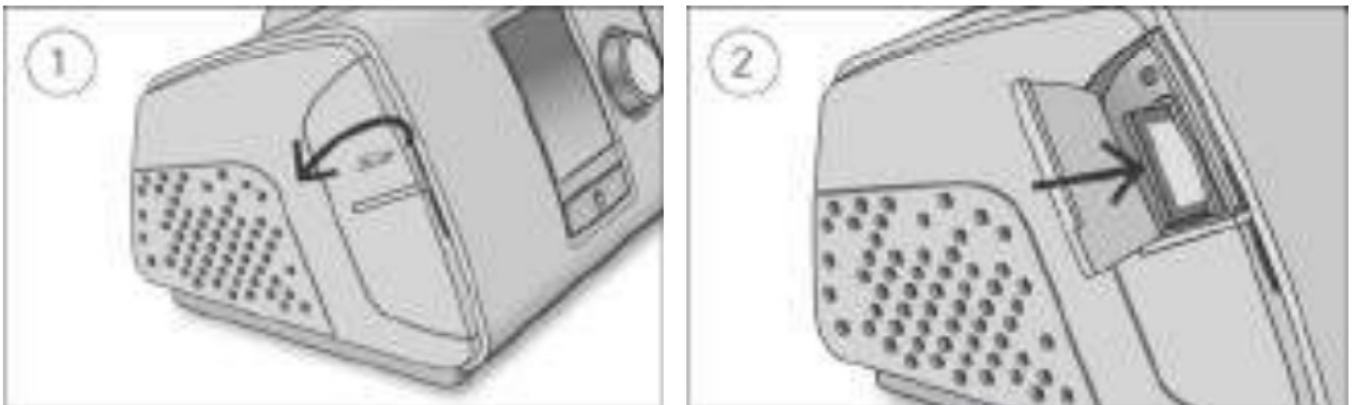

1. Open the SD card cover.
2. Push in the SD card to release it. Remove the SD card from the device. Place the SD card in the protective folder and send it back to your care provider.

For more information on the SD card refer to the SD card protective folder provided with your device

Note: The SD card should not be used for any other purpose.

Traveling

You can take your AirCurve 10 device with you wherever you go. Just keep the following in mind:

- Use the travel bag provided to prevent damage to the device.

- Empty the water tub and pack it separately in the travel bag.
- Make sure you have the appropriate power cord for the region you are traveling to. For information on purchasing, contact your care provider.
- If you are using an external battery, you should turn off the humidifier in order to maximize the life of your battery. Do this by turning the Humidity Level to Off.

Traveling by plane

Your AirCurve 10 device may be taken on board as carry-on luggage. Medical devices do not count toward your carry-on luggage limit.


You can use your AirCurve 10 device on a plane as it meets the Federal Aviation Administration (FAA) requirements. Air travel compliance letters can be downloaded and printed from www.resmed.com

When using the device on a plane:

- Make sure the water tub is completely empty and inserted into your device. The device will not work without the water tub inserted.
- Turn on Airplane **Mode**

To turn on Airplane **Mode**:



1. In My Options, turn the dial to highlight Airplane Mode  and then press the dial.
2. Turn the dial to select On and then press the dial to save the change. The Airplane Mode icon is displayed at the top right of the screen.



CAUTION

Do not use the device with water in the water tub on a plane due to the risk of inhalation of water during turbulence.



Troubleshooting

If you have any problems, have a look at the following troubleshooting topics. If you are not able to fix the problem, contact your care provider or ResMed. Do not try to open the device.

General troubleshooting

Problem/possible cause	Solution
Air is leaking from around my mask Mask may be fitted incorrectly.	Make sure your mask is fitted correctly. See your mask user guide for fitting instructions or use the Mask Fit function to check your mask fit and seal.
I am getting a dry or blocked nose Humidity level may be set too low.	Adjust the Humidity Level. If you have Climate Line Air heated air tubing, see the Climate Line Air user guide
I am getting droplets of water on my nose, in the mask and air tubing Humidity level may be set too high.	Increase the Humidity Level. You may need a chin strap to keep your mouth closed or a full face mask.
Air pressure in my mask seems too high (it feels like I am getting too much air) Ramp may be turned on	Use the Ramp Time option.
Air pressure in my mask seems too low (it feels like I am not getting enough air) Ramp may be in progress.	Wait for air pressure to build up or turn Ramp Time off.
My screen is black Backlight on the screen may have turned off. It turns off automatically after a short period of time. Power may not be connected.	Press Home or the dial to turn it back on Connect the power supply and make sure the plug is fully inserted.
I have stopped therapy, but the device is still blowing air Device is cooling down	Device blows a small amount of air in order to avoid condensation in the air tubing. It will stop automatically after 20 minutes
My water tub is leaking Water tub may not be assembled correctly Water tub may be damaged or cracked.	Check for damage and reassemble the water tub correctly. Contact your care provider for a replacement.
My therapy data has not been sent to my care provider Wireless coverage may be poor.	Make sure that the device is placed where there is coverage (ie, on your bedside table, not in a drawer or on the floor). The Wireless signal strength icon  indicates good coverage when all bars are displayed, and poor coverage when fewer bars are displayed.
The No wireless connection icon  is displayed on the top right of the screen. No wireless network available	Make sure that the device is placed where there is coverage (ie, on your bedside table, not in a drawer or on the floor). If instructed to do so, send the SD card to your care provider. The SD card also contains your therapy data.
Device may be in Airplane Mode.	Turn off Airplane Mode, see Traveling by plane
Data transfer is not enabled for your device.	Contact your care provider to enable the data transfer service.
My screen and buttons are flashing Software upgrade is in progress.	Software upgrade takes approximately 10 minutes to complete.

Device messages

Device message/possible cause	Solution
High leak detected, check your water tub, tub seal or side cover Water tub may not be inserted properly. Water tub seal may not be inserted properly.	Make sure the water tub is correctly inserted. Open the water tub and make sure that the seal is correctly inserted.
High leak detected, connect your tubing Air tubing may not be connected properly.	Make sure the air tubing is firmly connected at both ends
Mask may be fitted incorrectly.	Make sure your mask is fitted correctly. See your mask user guide for fitting instructions or use the Mask Fit function to check your mask fit and seal.
Tubing blocked, check your tubing Air tubing may be blocked.	Check the air tubing and remove any blockages. Press the dial to clear the message and then press Start/Stop to restart the device.
SD card error, remove your card and press Start to begin therapy SD card may not be inserted correctly.	Remove and reinsert the SD card.
Read only card, please remove, unlock and re-insert SD card SD card switch may be in the lock (read-only) position	Move the switch on the SD Card from the lock position  to the unlock  position and then re-insert it.
System fault, refer to user guide, Error 004 Device may have been left in a hot environment Air filter may be blocked. Air tubing may be blocked. There may be water in the air tubing.	Allow to cool before re-use. Disconnect the power supply and then reconnect it to restart the device. Check the air filter and replace it if there are any blockages. Disconnect the power supply and then reconnect it to restart the device. Check the air tubing and remove any blockages. Press the dial to clear the message and then press Start/Stop to restart the device. Empty the water from the air tubing. Disconnect the power supply and then reconnect it to restart the device
All other error messages, for example, System fault, refer to user guide, Error 0XX An unrecoverable error has occurred on the device.	Contact your care provider. Do not open the device.

Reassembling parts


Some parts of your device are designed to easily come off in order to avoid damage to the parts or the device. You can easily reassemble them as described below.

To insert the water tub seal:



1. Place the seal into the lid.
2. Press down along all edges of the seal until it is firmly in place.

To reassemble the water tub lid:

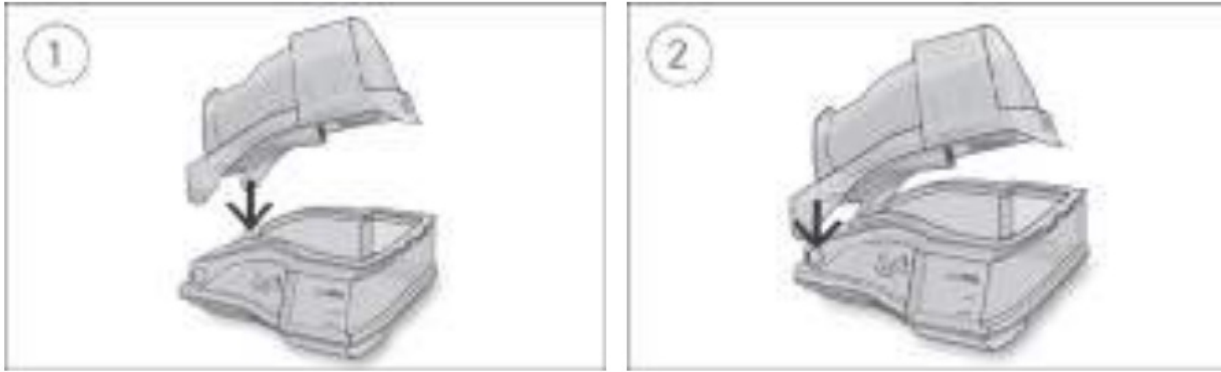

1. Insert one side of the lid into the pivot hole of the base.
2. Slide the other side down the ridge until it clicks into place.

General warnings and cautions



WARNING

- Make sure that you arrange the air tubing so that it will not twist around the head or neck.
- Make sure the power cord and plug are in good condition and the equipment is not damaged.
- Keep the power cord away from hot surfaces.
- If you notice any unexplained changes in the performance of the device, if it is making unusual sounds, if the device or the power supply are dropped or mishandled, or if the enclosure is broken, discontinue use and contact your care provider or your ResMed Service Center.
- Do not open or modify the device. There are no user serviceable parts inside. Repairs and servicing should only be performed by an authorized ResMed service agent.
- Beware of electrocution. Do not immerse the device, power supply or power cord in water. If liquids are spilled into or onto the device, unplug the device and let the parts dry. Always unplug the device before cleaning and make sure that all parts are dry before plugging it back in.
- Supplemental oxygen must not be used while smoking or in the presence of an open flame.
- Always make sure that the device is turned on and airflow generated before the oxygen supply is turned on. Always turn the oxygen supply off before the device is turned off, so that unused oxygen does not accumulate within the device enclosure and create a risk of fire.
- Do not perform any maintenance tasks while the device is in operation.
- The device should not be used adjacent to or stacked with other equipment. If adjacent or stacked use is necessary, the device should be observed to verify normal operation in the configuration in which it will be used.
- The use of accessories other than those specified for the device is not recommended. They may result in increased emissions or decreased immunity of the device.



CAUTION

- Use only ResMed parts and accessories with the device. Non-ResMed parts may reduce the effectiveness of the treatment and/or damage the device.
- Use only vented masks recommended by ResMed or by the prescribing doctor with this device. Fitting the

mask without the device blowing air can result in rebreathing of exhaled air. Make sure that the mask vent holes are kept clear and unblocked to maintain the flow of the fresh air into the mask.

- Be careful not to place the device where it can be bumped or where someone is likely to trip over the power cord.
- Blocking the air tubing and/or air inlet of the device while in operation could lead to overheating of the device.
- Keep the area around the device dry, clean and clear of anything (eg, clothes or bedding) that could block the air inlet or cover the power supply unit.
- Do not place the device on its side as water might get into the device.
- Incorrect system setup may result in incorrect mask pressure reading. Ensure the system is correctly set up.
- Do not use bleach, chlorine, alcohol, or aromatic-based solutions, moisturizing or antibacterial soaps or scented oils to clean the device, the water tub or air tubing. These solutions may cause damage or affect the humidifier performance and reduce the life of the products.
- If you use the humidifier, always place the device on a level surface lower than your head to prevent the mask and air tubing from filling with water.
- Leave the water tub to cool for ten minutes before handling to allow the water to cool and to make sure that the water tub is not too hot to touch.
- Make sure that the water tub is empty before transporting the device.

Technical specifications

90W power supply unit

AC input range: 100–240V, 50–60Hz 1.0–1.5A, Class II
115V, 400Hz 1.5A, Class II (nominal for aircraft use)

DC output: 24V 3.75A

Typical power consumption: 53W (57VA)

Peak power consumption: 104W (108VA)

Environmental conditions

Operating temperature: +41°F to +95°F (+5°C to +35°C)

Note: The air flow for breathing produced by this therapy device can be higher than the temperature of the room.

Under extreme ambient temperature conditions

(104°F/40°C) the device remains safe.

Operating humidity: 10 to 95% relative humidity, non-condensing

Operating altitude: Sea level to 8,500' (2,591 m); air pressure range 1013 hPa to 738 hPa

Storage and transport temperature: -4°F to +140°F (-20°C to +60°C)

Storage and transport humidity: 5 to 95% relative humidity, non-condensing

Electromagnetic compatibility

The AirCurve 10 complies with all applicable electromagnetic compatibility requirements (EMC) according to IEC60601-1-

2:2007, for residential, commercial and light industry environments. It is recommended that mobile communication devices

are kept at least 1 m away from the device.

Information regarding the electromagnetic emissions and immunity of this ResMed device can be found on www.resmed.com, on the Products page under Service and Support.

IEC 60601-1:2005 classification

Class II (double insulation), Type BF, Ingress protection IP22.
Sensors

Pressure sensor: Internally located at device outlet, analog gauge pressure

type, -5 to +45 cm H₂O

Flow sensor: Internally located at device inlet, digital mass flow type, -70 to +180 L/min

Maximum single fault steady pressure

Device will shut down in the presence of a single fault if the steady state pressure exceeds: 30 cm H₂O for more than 6 sec or 40 cm H₂O for more than 1 sec.

Sound

Pressure level measured according to ISO 17510-1:2007 (CPAP mode):

SlimLine: 26.6 dBA with uncertainty of 2 dBA

Standard: 26.6 dBA with uncertainty of 2 dBA

Power level measured according to ISO 17510-1:2007 (CPAP mode):

SlimLine: 34.6 dBA with uncertainty of 2 dBA

Standard: 34.6 dBA with uncertainty of 2 dBA

Declared dual-number noise emission values in accordance with ISO 4871:1996.

Physical – device and water tub

Dimensions (H x W x D): 4.57" x 10.04" x 5.91"

(116 mm x 255 mm x 150 mm)

Air outlet (complies with ISO 5356-1:2004): 22 mm

Weight (device and standard water tub): 44 oz (1248 g)

Weight (device and cleanable water tub): 44 oz (1248 g)

Housing construction: Flame retardant engineering thermoplastic

Water capacity: To maximum fill line 380 mL

Standard water tub – material: Injection molded plastic, stainless steel and silicone seal

Cleanable water tub – material: Injection molded plastic, stainless steel and silicone seal

Temperature

Maximum heater plate: 154°F (68°C)

Cut-out: 165°F (74°C)

Maximum gas temperature: 106°F (41°C)

Air filter

Standard: Material: Polyester non woven fiber

Average arrestance: >75% for ~7 micron dust

Hypoallergenic: Material: Acrylic and polypropylene fibers in a polypropylene carrier

Efficiency: >98% for ~7-8 micron dust; >80% for ~0.5 micron dust

Aircraft use

ResMed confirms that device meets the Federal Aviation Administration (FAA) requirements (RTCA/DO-160, section 21,

category M) for all phases of air travel.

Wireless module

Technology used: CDMA (USA and Canada only)

2G GSM (all regions except USA and Canada)

FCC ID: 2ACHL-AIR10CD

The AirCurve 10 device complies with FCC Rules.

The AirCurve 10 device should be used at a minimum distance of 0.8" (2 cm) from the body during operation.

Additional

information regarding the FCC Rules for this device can be found on www.ResMed.com/ProductSupport.

Operating pressure range


VAuto, S, ST, T: 3 to 25 cm H₂O

CPAP: 4 to 20 cm H₂O

Supplemental oxygen

Maximum flow: 15 L/min (S, ST, T, CPAP), 4 L/min (VAuto)

Pneumatic flow path

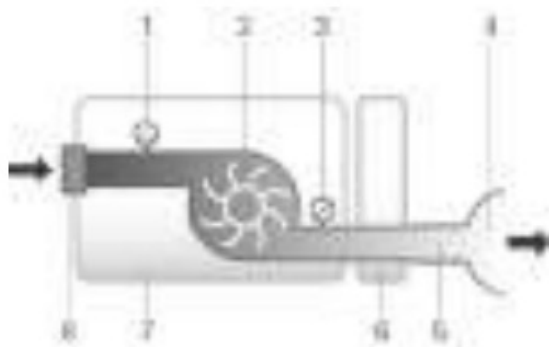

1. Flow sensor
2. Blower
3. Pressure sensor
4. Mask
5. Air tubing
6. Water tub
7. Device
8. Inlet filter

Design life

Device, power supply unit: 5 years

Cleanable water tub: 2.5 years

Standard water tub, air tubing: 6 months

General

The patient is an intended operator.

Humidifier performance

The following settings have been tested at 71.6°F (22°C) ambient temperature:

Mask Pressure

cm H₂O

RH output % Nominal system output AH1

, BTPS2

Setting 4 Setting 8 Setting 4 Setting 8

3 85 100 6 >10

4 85 100 6 >10

10 85 100 6 >10

20 85 90 6 >10

25 85 90 6 >10

1 AH – Absolute Humidity in mg/L

2 BTPS – Body Temperature Pressure Saturated

Air tubing

Air tubing Material Length Inner diameter

ClimateLineAir Flexible plastic and electrical components 6'6" (2 m) 0.6" (15 mm)

SlimLine Flexible plastic 6' (1.8 m) 0.6" (15 mm)

Standard Flexible plastic 6'6" (2 m) 0.75" (19 mm)

Heated air tubing temperature cut-out: 106°F (41°C)

Notes

- The manufacturer reserves the right to change these specifications without notice.
- The electrical connector end of the heated air tubing is only compatible with the air outlet at the device end and should not be fitted to the mask.
- Do not use electrically conductive or antistatic air tubing.
- The temperature and relative humidity settings displayed are not measured values.

Displayed values

Value Range Display resolution

Pressure sensor at air outlet:

Mask pressure 3–25 cm H₂O 0.1 cm H₂O

Flow derived values:

Leak 0–120 L/min 1 L/min

Tidal volume 0–4000 mL 1 mL

Respiratory rate 0–50 bpm 1 bpm

Minute ventilation 0–30 L/min 0.1 L/min

Ti 0.1–4.0 sec 0.1 sec

I:E ratio 1:100–2:1 0.1

Value Accuracy¹

Pressure measurement¹

Mask pressure²

±[0.5 cm H₂O + 4% of measured value] Flow and flow derived values¹

Flow ±6 L/min or 10% of reading, whichever is greater, at 0 to 150 L/min positive flow

Leak²

±12 L/min or 20% of reading, whichever is greater, 0 to 60 L/min

Tidal volume^{2,3} ± 20%

Respiratory rate^{2,3} ± 1.0 bpm

Minute ventilation^{2,3} ± 20%

¹ Results are expressed at ATPD (Ambient Temperature and Pressure, Dry).

² Accuracy may be reduced by the presence of leaks, supplemental oxygen, tidal volumes <100 mL or minute ventilation <3 L/min.

³ Measurement accuracy verified as per ISO 10651-1:2004 for Home Care Ventilatory Support Devices (Figure 101 and Table 101) using nominal ResMed mask vent flows.

Pressure accuracy

Maximum static pressure variation at 10 cm H₂O according to ISO 17510-1:2007

Standard air tubing SlimLine air tubing

Without humidification ± 0.5 cm H₂O ± 0.5 cm H₂O

With humidification ± 0.5 cm H₂O ± 0.5 cm H₂O

Maximum dynamic pressure variation according to ISO 17510-1:2007

Device without humidification and Standard air tubing / Device with humidification and Standard air tubing

Pressure (cm H₂O) 10 BPM 15 BPM 20 BPM

4 0.5 / 0.5 0.5 / 0.5 0.8 / 0.8

8 0.5 / 0.5 0.5 / 0.5 0.8 / 0.8

12 0.5 / 0.5 0.5 / 0.5 0.8 / 0.8

16 0.5 / 0.5 0.5 / 0.5 0.8 / 0.8

20 0.5 / 0.5 0.5 / 0.5 0.8 / 0.8

25 0.3 / 0.3 0.5 / 0.4 0.7 / 0.7

Device without humidification and SlimLine air tubing / Device with humidification and SlimLine air tubing

Pressure (cm H₂O) 10 BPM 15 BPM 20 BPM

4 0.5 / 0.5 0.5 / 0.5 0.8 / 0.8

8 0.5 / 0.5 0.5 / 0.5 0.8 / 0.8

12 0.5 / 0.5 0.5 / 0.5 0.8 / 0.8




16 0.5 / 0.5 0.5 / 0.5 0.8 / 0.8





20 0.5 / 0.5 0.5 / 0.5 0.8 / 0.8





25 0.4 / 0.3 0.6 / 0.5 0.8 / 0.8





Symbols




The following symbols may appear on the product or packaging.





 Read instructions before use.  Indicates a warning or caution.  Follow instructions before use.




 Manufacturer.  European Authorized Representative.  Batch code.  REF

Catalog number.  Serial number.  Device number.  On / Off.  Device weight. IP22
Protected against finger sized objects and against dripping water when tilted up to 15 degrees from specified

orientation.  Direct current.  Type BF applied part.  Class II equipment.  Humidity

limitation.  Temperature limitation.  Non-ionising radiation.  China pollution control logo 1.

 China pollution control logo 2.  Prescription only (In the US, Federal law restricts these devices to sale by or on the order of a physician).  Maximum water level.  Use distilled water only.

 Operating altitude.  Atmospheric pressure limitation.  Complies with RTCA DO-160 section 21, category M.



Environmental information

This device should be disposed of separately, not as unsorted municipal waste. To dispose of your device, you should use appropriate collection, reuse and recycling systems available in your region. The use of these

collection, reuse and recycling systems is designed to reduce pressure on natural resources and prevent hazardous substances from damaging the environment. If you need information on these disposal systems, please contact your local waste administration. The crossed-bin symbol invites you to use these disposal systems. If you require information on collection and disposal of your ResMed device please contact your ResMed office, local distributor or go to www.resmed.com/environment.

Servicing

The AirCurve 10 device is intended to provide safe and reliable operation when operated in accordance with the instructions provided by ResMed. ResMed recommends that the AirCurve 10 device be inspected and serviced by an authorized ResMed Service Centre if there is any sign of wear or concern with device function. Otherwise, service and inspection of the products generally should not be required during their design life.

Limited warranty

ResMed Ltd (hereafter 'ResMed') warrants that your ResMed product shall be free from defects in material and workmanship from the date of purchase for the period specified below

Product

- Mask systems (including mask frame, cushion, headgear and tubing)—excluding single-use devices
- Accessories—excluding single-use devices
- Flex-type finger pulse sensors
- Humidifier water tubs 90 days
- Batteries for use in ResMed internal and external battery systems 6 months
- Clip-type finger pulse sensors
- CPAP and bilevel device data modules
- Oximeters and CPAP and bilevel device oximeter adapters
- Humidifier cleanable water tubs
- Titration control devices 1 year
- CPAP, bilevel and ventilation devices (including external power supply units)
- Humidifiers
- Battery accessories
- Portable diagnostic/screening device

This warranty is only available to the initial consumer. It is not transferable. If the product fails under conditions of normal use, ResMed will repair or replace, at its option, the defective product or any of its components. This Limited Warranty does not cover: a) any damage caused as a result of improper use, abuse, modification or alteration of the product; b) repairs carried out by any service organization that has not been expressly authorized by ResMed to perform such repairs; and c) any damage or contamination due to cigarette, pipe, cigar or other smoke. Warranty is void on product sold, or resold, outside the region of original purchase.

Warranty claims on defective product must be made by the initial consumer at the point of purchase.

This warranty replaces all other expressed or implied warranties, including any implied warranty of merchantability or fitness for a particular purpose. Some regions or states do not allow limitations on how long an implied warranty lasts, so the above limitation may not apply to you. ResMed shall not be responsible for any incidental or consequential damages claimed to have resulted from the sale, installation or use of any ResMed product. Some regions or states do not allow the exclusion or limitation of incidental or consequential damages, so the above limitation may not apply to you. This warranty gives you specific legal rights, and you may also have other rights which vary from region to region. For further information on your warranty rights, contact your local ResMed dealer or ResMed office.

Further information

If you have any questions or require additional information on how to use the device, contact your care provider.



ResMed Ltd

1 Elizabeth Macarthur Drive
Bella Vista NSW 2153 Australia

DISTRIBUTED BY

ResMed Corp 9001 Spectrum Center Boulevard San Diego CA 92123 USA




ResMed (UK) Ltd 96 Jubilee Ave Milton Park Abingdon Oxfordshire OX14 4RW UK

See www.resmed.com for other ResMed locations worldwide. For patent information, see www.resmed.com/ip. AirCurve, Air10, ClimateLine, HumidAir and SlimLine are trademarks of ResMed Ltd. SlimLine and ClimateLine are registered in U.S. Patent and Trademark Office. SD Logo is a trademark of SD-3C, LLC. © 2014 ResMed Ltd. 378121/1 2014-08



Documents / Resources

	<p>ResMed AirCurve 10 VAUTO Auto-Adjusting Bilevel Device [pdf] User Guide AirCurve 10 VAUTO, AirCurve 10 S, AirCurve 10 ST, AirCurve 10 VAUTO Auto-Adjusting Bilevel Device, Auto-Adjusting Bilevel Device, Bilevel Device</p>
---	---

References

- [Res Sleep apnea and COPD - learn about symptoms and treatment | ResMed](#)
- [Res Environmental policy - ResMed](#)
- [Res Legal disclaimers and intellectual property - ResMed](#)
- [Res ResMed.com/ProductSupport](#)