

# RICE LAKE 920i Programmable HMI Indicator, Controller Installation Guide

Home » RICE LAKE » RICE LAKE 920i Programmable HMI Indicator, Controller Installation Guide 🖫



920i Programmable HMI Indicator, Controller Installation Guide

#### **Contents**

- 1 Panel Mount Enclosure
- Installation
- 2 Installation
- 3 Grounding
- 4 Stripping Cables
- **5 Power Specifications**
- **6 Parts Kit Contents**
- 7 Documents / Resources
  - 7.1 References
- **8 Related Posts**

### **Panel Mount Enclosure Installation**

This document contains drawings, replacement parts lists and instructions for installing panel mount models of 920i indicators.

See the 920i Installation Manual, PN 67887, for general installation, configuration and calibration information.



#### WARNING

The 920i has no on/off switch. Before opening the unit, ensure the power cord is disconnected from the power outlet

Use a wrist strap for grounding and to protect components from electrostatic discharge (ESD) when working inside the indicator enclosure.

This unit uses double pole/neutral fusing which could create an electric shock hazard. Procedures requiring work inside the indicator must be performed by qualified service personnel only.

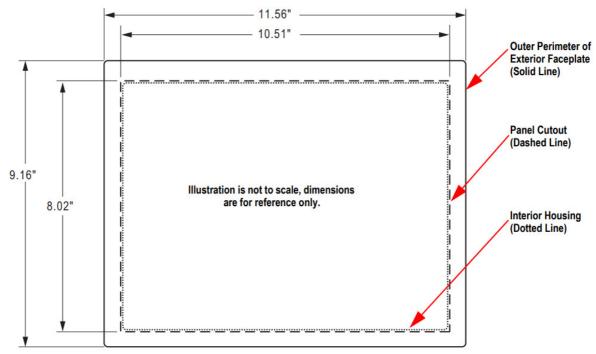


Figure 1. Panel Cutout for Panel Mount Enclosure

#### Installation

Use the dimensions shown in Figure 1 to lay out the panel cutout for the panel mount enclosure. See Figure 2 for enclosure dimensions.

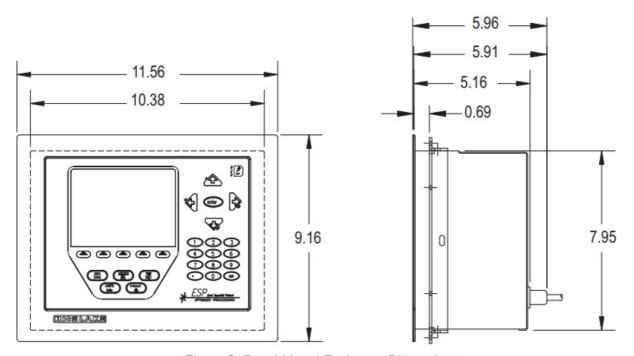


Figure 2. Panel Mount Enclosure Dimensions

# Once the cutout has been prepared:

- 1. Insert the enclosure into the cutout from the front of the panel.
- 2. Install the reinforcing plate on the enclosure from the inside of the panel.
- 3. Install the clinching bracket on the enclosure from inside the panel.
- 4. Secure the bracket to the enclosure using the six 1/4" screws provided in the parts kit (PN 71522).

5. Use the nine 1 1/2" screws (PN 82425) to secure the clinching bracket to the panel door.

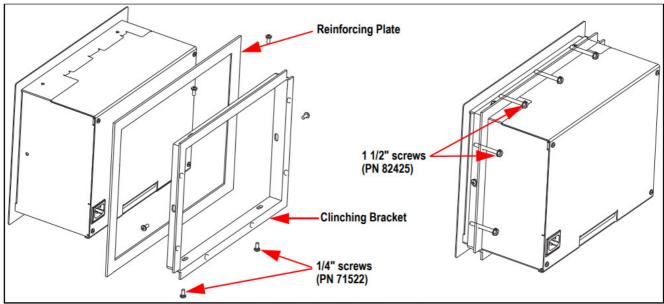


Figure 3. Clinching Bracket Assembly

# 920i Programmable HMI Indicator/Controller Panel Mount Enclosure

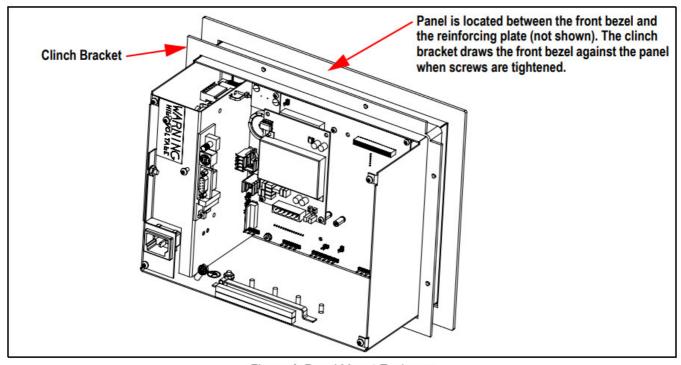


Figure 4. Panel Mount Enclosure

# Grounding

Except for the power cord, all cables routed through the cord grips should be grounded against the indicator enclosure.

- 1. Install the ground clamps on the grounding bar, using the ground clamp screws. Do not tighten the screws at this time.
- 2. Route cables under cabling bar and through the cord grips and the grounding clamps to determine the cable

lengths required to reach the cable connectors.

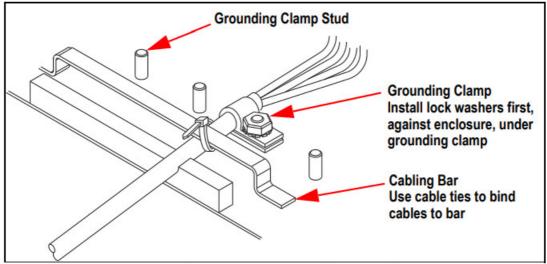


Figure 5. Cable Installation with Grounding Clamp

- 3. Mark the cables to remove insulation and shield. See Stripping Cables on next page.
- 4. Route stripped cables through the cord grips and grounding clamps.
- 5. Ensure the shields contact the grounding clamps and tighten the ground clamp screws.

## **Stripping Cables**

#### **Foil Insulated Cable**

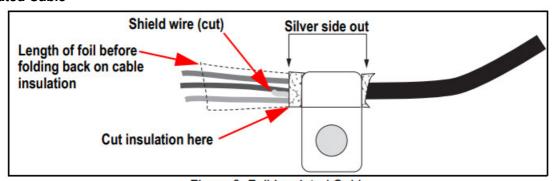


Figure 6. Foil Insulated Cable

- 1. Strip the insulation and foil from the cable 1/2 (15 mm) past the grounding clamp.
- 2. Fold the foil shield back on the cable where the cable passes through the clamp.
- 3. Ensure the silver (conductive) side of the foil is turned outward for contact with the grounding clamp.

# **Braided Shielding**

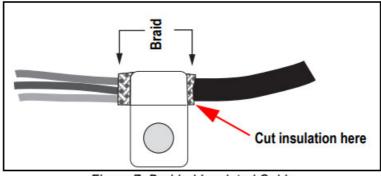


Figure 7. Braided Insulated Cable

- 1. Strip the insulation and braided shield from a point just past the grounding clamp.
- 2. Strip another 1/2 (15 mm) of the insulation to expose the braid where the cable passes through the clamp.

### **Load Cell Cables**

Cut the shield wire just past the grounding clamp. Shield wire function is provided by contact between the cable shield and the grounding clamp.

# **Power Specifications**

Line Voltages	115 or 230 VAC
Frequency	50 or 60 Hz
Maximum Power	65W on secondary
Consumption	Primary power consumption:100W TRMS Constant current:1.5 A TRMS (115VAC); 1.0 A TRMS (230VAC)
Fusing 115 VAC and 230 VAC North Americ an	2 x 3.15A TR5 sub-miniature fuses Wickmann Time-Lag 19374 Series UL Listed, CSA Certified and Approved
230 VAC European	2 x 3.15A TR5 sub-miniature fuses Wickmann Time-Lag 19372 Series UL Recognized, Semko and VDE Approved

See the 920i installation manual for additional specifications.

#### **Parts Kit Contents**


Table 1-1 lists the parts kit contents for the panel mount version of the 920i.

Part No.	Description	Qty
14626	Kep nuts, 8-32NC	5
54206	Machine screws, 6-32 x 3/8	2
15133	Lock washers, No. 8, Type A	5
71522	Machine screws, 8-32NC x 1/4	6
82425	Machine screws, 10-32NF x 1-1/2	9
15631	Cable ties	4
53075	Cable shield ground clamps	5
42350	Capacity label	1
71095	Clinching bracket	1
15887	6-position screw terminal for load cell connection	1
70599	6-position screw terminals for J2 and J10	2
71126	4-position screw terminal for J9 and optional keyboard connection	2
71125	3-position screw terminal for J11	1



© Rice Lake Weighing Systems Specifications subject to change without notice.
230 W. Coleman St. Rice Lake,
WI 54868 USA
U.S. 800-472-6703 Canada/Mexico 800-321-6703
International 715-234-9171
Europe +31 (0)26 472 1319

#### **Documents / Resources**

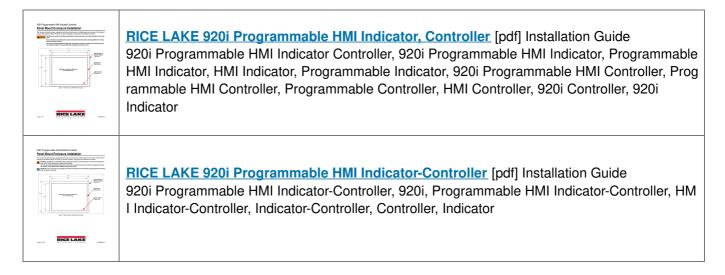

#### References

- Rice Lake Weighing Systems
- Rice Lake Weighing Systems

Manuals+,