



sauermann SI-CA 130 Versatile Analyzer with Touch Screen Display User Guide

[Home](#) » [sauermann](#) » sauermann SI-CA 130 Versatile Analyzer with Touch Screen Display User Guide 

sauermann SI-CA 130 Versatile Analyzer with Touch Screen Display User Guide



Contents

- 1 SAFETY INSTRUCTIONS
- 2 Before Using the Flue Gas Analyzer
- 3 Analyzers description
- 4 Operating temperature, protection of the instruments and information about storage
- 5 First start-up
- 6 ON / OFF
- 7 Stop / Restart the Pump
- 8 Combustion Analysis, Saving & Printing
- 9 Software & Apps
- 10 Customer service portal
- 11 Documents / Resources
- 12 Related Posts

SAFETY INSTRUCTIONS

- These operating instructions describe the basic handling of the device.
- Please refer to the operating instructions available at www.sauermanngroup.com for safe use of the product and detailed information.
- Do not give this device to a child.
- The magnets in the back of the instrument can damage credit cards, hard drives, mechanical watches, pacemakers, defibrillators and other devices proven sensitive to magnetic fields. It is recommended to keep the instrument at a distance of at least 25 cm (10") away from any of these devices.
- These gas analyzers are designed to measure flue gases exhausting from combustion equipment. They are not designed for continuous operations and/or use as a control/alarm system

The Si-CA 130 and Si-CA 230 analyzers are touchscreen devices with just the on/off button:



Before Using the Flue Gas Analyzer

WARNING!

- Be sure all connections are tight to assure accurate sampling.
- When conducting measurements, the water trap/filter assembly MUST be in a VERTICAL position.

Water trap OK



Water trap NOT OK



Analyzers description

1. Min-DIN connection for CO and CO₂ probe
2. Thermocouple connection for air temperature
3. Thermocouple connection for flue gas temperature
4. P- connection
5. P+ connection
6. Gas connection
7. USB connection



Operating temperature, protection of the instruments and information about storage

- **Operating temperature:** from -5 to 45 °C (23 to 113 °F)
- **Protection:** IP42


If the instrument is stored outside the operating temperature (for example in a van, a warehouse,...) please let the analyzer acclimate to room temperature for at least 15 minutes before starting and operating the analyzer.

If the ambient temperature is lower than 10 °C (50 °F), the analyzer should be acclimated to ambient temperature before performing measurements.

First start-up



DO NOT insert the gas probe in the flue/chimney/stack.


Keep  pressed for 3 seconds to turn on the analyzer.



- Tap “Start”.



- Select your country then tap “Next”.

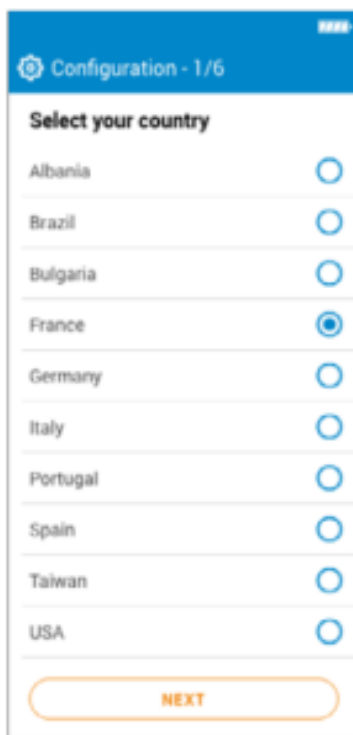

- Select your language then tap “Next”.

Configuration - 2/6

Select your language

English	<input checked="" type="radio"/>
French	<input type="radio"/>
Spanish	<input type="radio"/>
Italian	<input type="radio"/>
German	<input type="radio"/>
Portuguese	<input type="radio"/>
Dutch	<input type="radio"/>
Chinese	<input type="radio"/>

NEXT

- Set the date then tap “Next”.

Configuration - 3/6

Set your date

DAY	MONTH	YEAR
01	03	2020

Month - Day - Year ☐

Day - Month - Year ☒

NEXT

- Set the time then tap “Next”.

Configuration - 4/6

Set your time

10	:	35
----	---	----


24 hours ☐

AM ☐


PM ☒

NEXT

- Set your time zone then tap “Next”.

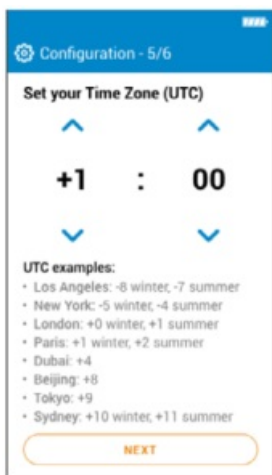

- Select if you want your pump turned ON or OFF after Auto-Zero then tap “Save”.

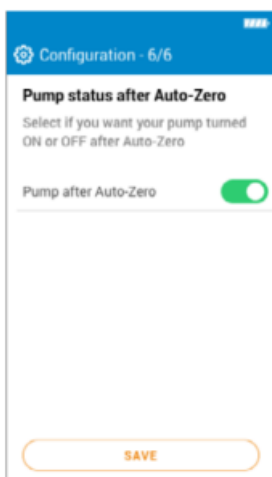

- Autozero is in progress.



- The probe can be inserted in the chimney.

10:35 - 10/12/2021

Gas analysis

NATURAL GAS

O2	4.23 %
CO	140 ppm
Eff.	82.9 %
CO2	500 ppm
T-gas	374 °F
T-air	79.3 °F
Excess air	21.4 %
NO	16.2 ppm

Icons: Waveform, Save, Print, Share

The analyzer displays the measurements.




ON / OFF



During autozero DO NOT insert the gas probe in the chimney.



Keep  pressed for 3 seconds to turn on the analyzer. Once the autozero is finished, insert the gas probe in the chimney and gas measurements are displayed.


10:35 - 10/12/2021

Gas analysis

NATURAL GAS

O2	4.23 %
CO	140 ppm
Eff.	82.9 %
CO2	500 ppm
T-gas	374 °F
T-air	79.3 °F
Excess air	21.4 %
NO	16.2 ppm

Icons: Waveform, Save, Print, Share

Keep  pressed for 3 seconds to turn off the analyzer. Before powering off, disconnect hoses from the analyzer and empty and dry the water trap.

Stop / Restart the Pump

It is possible to turn off the pump during a gas analysis.



Tap . Pump is off and values are on hold.



Tap . Pump is on and measurements re-start.


Combustion Analysis, Saving & Printing




Before proceeding with the combustion analysis, remember to set the proper fuel.



- Tap “Settings”.

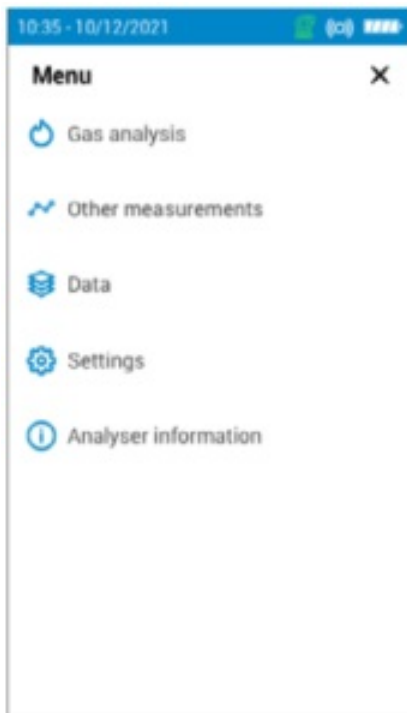


- Tap “Analysis”.

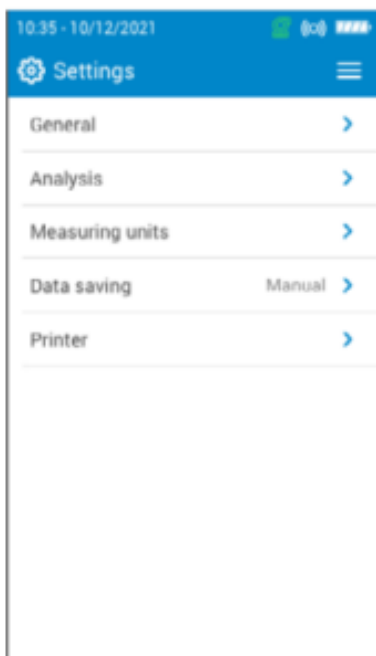


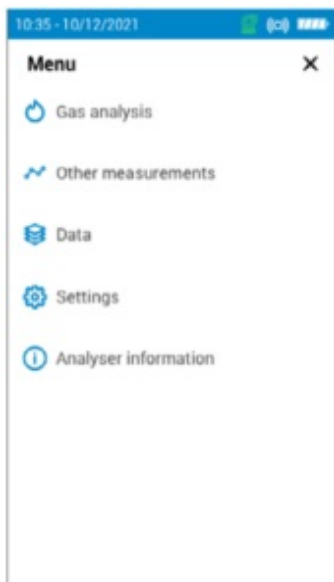
- Tap “Fuels”.




- Tap the required fuel.

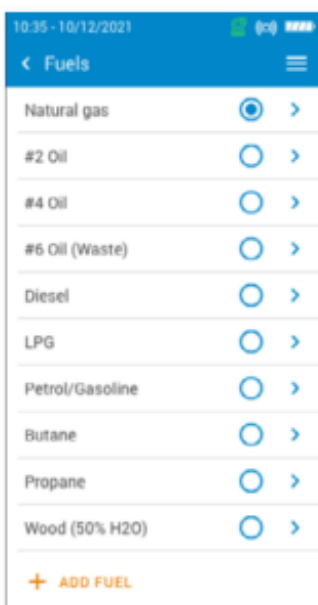


- Once the required fuel is selected, tap  then tap “Gas analysis”.



- Measurements of the gas analysis are displayed.

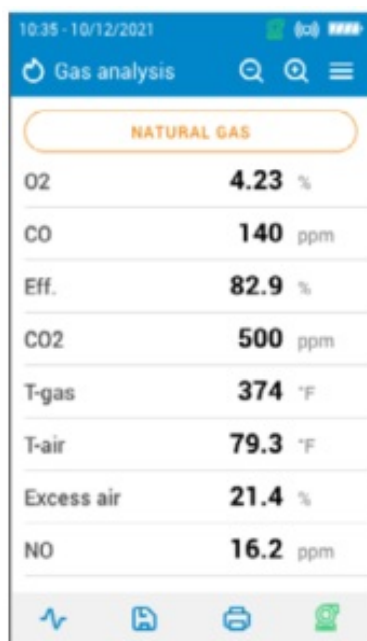

You can also quickly access the fuel selection menu via the fuel shown at the top of the combustion gas analysis screen

- To view the different measured parameters, just scroll the screen.
- To save combustion data, first tap on the Save icon  then select or create a folder and tap on Save. The Sauermann Combustion mobile phone app and/or PC software can also be used to save data.
- To prints the results, use the Wireless Printer available as option

Software & Apps

Download the Sauermann Combustion App



Download the Sauermann Combustion Software



Download the full manual



Monitoring Configuration Emissions Measurement on Boilers, Engines & other Applications

- Si-CA 030



- Si-CA 130



- Si-CA 230



- Wireless Printer



- Wireless connection




- PC and mobile Apps



Customer service portal

Use our Customer service portal to contact us <https://sauermann-en.custhelp.com>

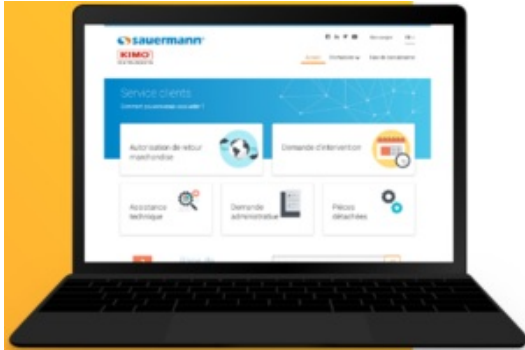

WWW.SAUERMANNGROUP.COM



Documents / Resources



[sauermann SI-CA 130 Versatile Analyzer with Touch Screen Display](#) [pdf] User Guide
SI-CA 130, SI-CA 230, SI-CA 130 Versatile Analyzer with Touch Screen Display, Versatile Analyzer with Touch Screen Display, Touch Screen Display