



SMART CAREGIVER 433-RB Remote Reset Button Instruction Manual

[Home](#) » [Smart Caregiver](#) » SMART CAREGIVER 433-RB Remote Reset Button Instruction Manual 

Contents

- [1 SMART CAREGIVER 433-RB Remote Reset Button](#)
- [2 Product Information](#)
- [3 Product Usage Instructions](#)
- [4 Quick Start Instructions](#)
- [5 Battery LED Indicators](#)
- [6 Important Information](#)
- [7 Limited Warranty](#)
- [8 FCC Caution](#)
- [9 Documents / Resources](#)



SMART CAREGIVER 433-RB Remote Reset Button



Product Information

The Smart Caregiver 433-RB Reset Button is a device designed for fall prevention and caregiver assistance. It works in conjunction with the 433-CMU Economy Central Monitor and the 433-EC Caregiver Pager. Please note that the 433-RB is not waterproof or water-resistant, and prolonged exposure to moisture is not recommended.

Product Usage Instructions

1. Open the reset button by removing it from the slot on the bottom (refer to Figure 1).
2. Install one 12V/23A battery inside the reset button (refer to Figure 2).
3. Attach the lanyard by placing the loop at the bottom of the lanyard over the pin at the top of the reset button (refer to Figure 3). While holding the lanyard in place, snap the reset button back together.
4. Mount the reset button using the screws or double-sided tape provided.
5. To test, press the reset button. The red light at the top of the reset button should illuminate.

The red light indicates that the device is activated, while a fading red light indicates a low battery. The 433-RB works with the 433-CMU and 433-EC devices.

Contact Information:

For further assistance or inquiries, please contact Smart Caregiver at:

- **Phone:** (800) 650-3637
- **Website:** www.smartcaregiver.com.

Quick Start Instructions

1. Use a flat head screwdriver to pop reset button open from slot on bottom. (See Figure 1)
2. Install one 12V/23A Battery (See Figure 2)
3. **Attach Lanyard**
Place loop in bottom of lanyard over pin at the top of the reset button. (See Figure 3) While holding lanyard in place, snap reset button back together.
4. **Mounting**

Reset button may be mounted using the screws or double sided tape provided.

5. Test


Press reset button. Red light at the top of reset button should illuminate.



(Figure 1)



(Figure 2)

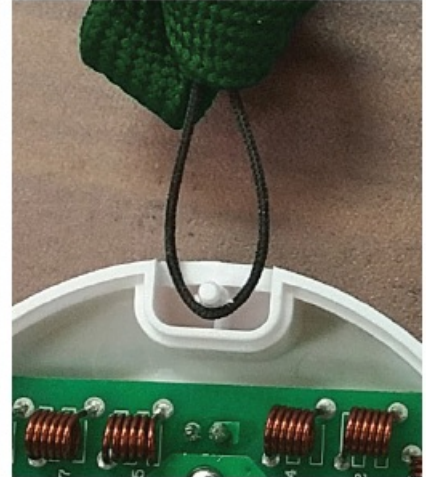

(Figure 3)

Battery LED Indicators



Red = Activated
When Fades = Low Battery

Works with 433-CMU and 433-EC

Not waterproof or water resistant.

- Exposure to moisture for long periods of time is not recommended.

Important Information

Smart Caregiver 433-RB Reset Button

Please be aware that the 433-RB will reset an alarming 433-CMU Economy Central Monitor that has been triggered by one or more devices. For example, if a 433-CMU (and 433-PGD pager, if in use) has been triggered by a sensor pad and a motion sensor simultaneously, its display will show both devices have been triggered (by number). Caregivers may reset the Economy Central Monitor with a 433-RB, but it will reset the alert and clear from memory all currently active alerts.

If multiple active alerts have been reset by the 433-RB, caregivers may still see which devices triggered recent alerts by pressing "REVIEW" button on the 433-PGD Caregiver Pager.



433-RB
Reset Button



433-CMU Central Monitor



433-PGD Caregiver Pager

IMPORTANT INFORMATION:

Cordless and Wireless Systems rely on wireless technology which is subject to physical and environmental considerations. Please be aware that the transmitter will not be 100% accurate if it is out of range at any time. It is the end-user's responsibility to make sure that the product is used correctly and within range of each other. Cordless and wireless systems and devices are intended as an adjunct to good caregiving practices and are not a substitute for proper staffing and patient management practices. We recommend that all caregivers receive periodic training in the operation of these systems and that the devices are tested daily. It is important to read and follow the directions.

Read the instructions and Legal Disclaimer.

The Smart Caregiver Corporation devices are designed to be installed by the end user. As such, it is the entire responsibility of the buyer to insure that the system is properly installed and tested. Further, the system is not designed to replace good caregiving practices including, but not limited to:

- Direct patient supervision
- Adequate training for staff personnel for fall prevention and elopement
- Testing of the system before each use

WARNING:

The manufacturer does not claim that this device will stop elopement and/or stop falls. This device is designed to augment caregivers' comprehensive resident mobility management program. Failure to comply with the warning may result in injury or death. This device is not suitable for all individuals. Other devices may be required. This device is not a substitute for visual monitoring by a caregiver. Where permissible, it is the seller's intent to limit any liability for special, consequential or incidental economic damages to refund of the purchase price or replacement of the goods. Seller disclaims any liability for compensatory or other damages arising out of the use of the goods.

Limited Warranty

Seller warrants that the goods sold will be free from defects of workmanship and manufacturing, for a warranty period from the date of sale. Other than this limited warranty, seller makes no express or implied warranties. Except for this limited warranty. No express or implied warranties are given and no affirmation of seller, by words or action will constitute a warranty. The goods being purchased are being sold on a "with all faults" basis. The entire risk as to the quality and performance of the goods is with the buyer. Should the goods prove defective following their purchase, the buyer, and not the manufacturer, distributor or retailer, assumes the entire cost of all necessary installation, servicing or repairs.

FCC Caution

Any Changes or modifications not expressly approved by the party responsible for compliance could void the user's authority to operate the equipment.

This device complies with part 15 of the FCC Rules. Operation is subject to the following two conditions:

1. This device may not cause harmful interference, and
2. This device must accept any interference received, including interference that may cause undesired operation.

IMPORTANT NOTE:

Note:

This equipment has been tested and found to comply with the limits for a Class B digital device, pursuant to part 15 of the FCC Rules. These limits are designed to provide reasonable protection against harmful interference in a residential installation. This equipment generates, uses and can radiate radio frequency energy and, if not installed and used in accordance with the instructions, may cause harmful interference to radio communications. However, there is no guarantee that interference will not occur in a particular installation. If this equipment does cause harmful interference to radio or television reception, which can be determined by turning the equipment off and on, the user is encouraged to try to correct the interference by one or more of the following measures:

- Reorient or relocate the receiving antenna.
- Increase the separation between the equipment and receiver.
- Connect the equipment into an outlet on a circuit different from that to which the receiver is connected.
- Consult the dealer or an experienced radio/TV technician for help.


FCC Radiation Exposure Statement:

This equipment complies with FCC radiation exposure limits set forth for an uncontrolled environment.

Fall Prevention by Smart Caregiver

(800) 650-3637 | www.smartcaregiver.com.

Documents / Resources

	<p>SMART CAREGIVER 433-RB Remote Reset Button [pdf] Instruction Manual 433-RB, 2AUNU433-RB, 2AUNU433RB, 433-RB Remote Reset Button, Remote Reset Button, Reset Button, Button</p>
--	--