

# Spectronix Eye-BERT Gen 2 Programming Software User Guide

Home » Spectronix » Spectronix Eye-BERT Gen 2 Programming Software User Guide 🖫



Eye-BERT Gen2
Software Programming Guide

## **Contents**

- 1 Overview:
- 2 USB Interface:
- 3 Optional Ethernet Interface:
- 4 Updating the Firmware:
- 5 Commands:
- 6 Documents / Resources
  - **6.1 References**

### Overview:

The Eye-BERT Gen2 allows remote control and monitoring via USB or optional Ethernet connection. Once a connection is made to the Eye-BERT using one of these interfaces, all command and control is the same regardless of which interface is used.

#### **USB Interface:**

In order for Windows to recognize the Eye-BERT Gen2 USB port the USB driver must first be installed, after which the Eye-BERT Gen2 appears as an additional COM port on the computer.

Currently Windows XP, Vista, 7, and 8 are supported. Windows 7 requires the extra step listed below; Windows 8 requires additional steps which can be found in the following application note:


http://www.spectronixinc.com/Downloads/Installing%20Under%20Windows%208.pdf

- 1. Copy the file "cdc NTXPV764.inf" from the supplied CD to the hard drive.
- 2. Plug the Eye-BERT Gen2 into a free USB port. When the hardware installation wizard asks for the driver location, browse to the "cdc NTXPVista.inf" file on the hard drive.
- 3. After the driver has been installed right click "my computer" and select "properties". In the properties window select the "hardware" tab. Click on "device manager" and expand the "Ports (COM & LPT)" item. Locate the "Spectronix, Inc." entry and note the assigned COM number, (ie "COM4"). This is the COM port that the software will use to communicate with the Eye-BERT Gen2.

Note, on some operating systems such as Window 7, manual USB driver installation may be necessary. If the hardware installation wizard fails, go to "My Computer" > "Properties" > "Hardware" > "Device Manager", and find the "Spectronix" or "SERIAL DEMO" entry under "Other Devices" and select "Update Driver". At this point you will be able to browse to the location of the driver.


## **Optional Ethernet Interface:**

The Eye-BERT Gen2 communicates using TCP/IP on port number 2101 and is shipped with a default IP address of 192.168.1.160. Connection to this port is illustrated below using HyperTerminal, TeraTerm, and RealTerm.

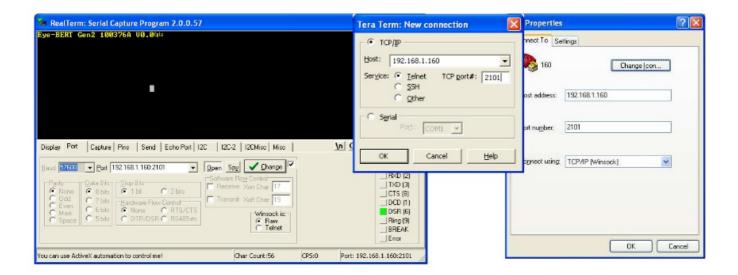

#### Changing the IP Address

The Digi Device Discovery utility allows the user to retrieve and change the Eye-BERT IP address. The installation program "40002265\_G.exe" can be found on the Spectronix or Digi web sites. After installing the utility, disable Windows Firewall and any other virus or firewall programs and start the program. The program will report the IP and MAC addresses of all compatible devices on the network. Right click on the device and select "Configure Network Settings" to change the network settings.

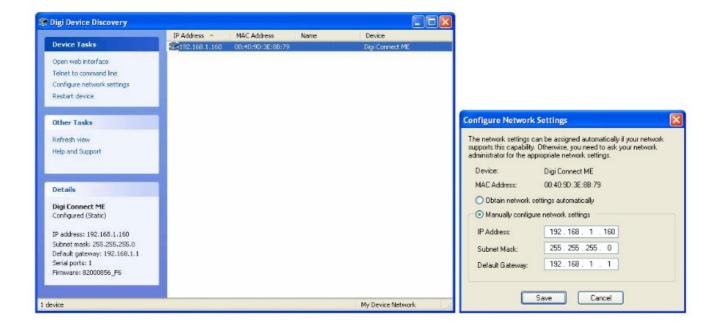

## **Updating the Firmware:**

It is possible for the user to update the Eye-BERT Gen2 firmware over the USB (V 1.10 and above) or Ethernet port (if supplied) using the Spectronix Bootloader application which can be found on the included CD or downloaded from the Spectronix web site. With the unit powered off press and hold the power button, the LED will blink rapidly and after several seconds it will turn solid. With the OEM version (no LCD) press and hold the power button while connecting the power source. Release the button and follow the bootloader user's manual for instructions on loading the firmware.

#### Commands:

The Eye-BERT Gen2 uses ASCII data to communicate with a host computer; the tables below list the individual commands, parameters, and responses from the Eye-BERT Gen2.

#### Notes:

- 1. All communication is initiated by the host.
- 2. Commands are not case sensitive.
- 3. A space or equal sign should be inserted between the command and any parameters.
- 4. All commands should be terminated with a <CR> <LF>.
- 5. Responses from the Eye-BERT Gen2 are terminated with <CR> <LF> <0x00>.

Get Unit Information	
Command:	Parameters:
"?"	(none)
Response:	Parameters:
Unit name	Eye-BERT Gen2 100376A
Firmware Rev	V0.6
Termination	CR/LF <0x00>
Notes:	

Set the data rate	
Command:	Parameters:
"SetRate"	"#######" (Bit Rate in Kbps)
Response:	Parameters:
(none)	
Notes:	Sets to the closest standard bit rate  Example: "setrate=150000000" for 155.52Mbps.

Set the pattern (generator and detector)	
Command:	Parameters:
"SetPat"	"7" (PRBS 2 <sup>7</sup> -1) "3" (PRBS 2 <sup>31</sup> -1) "x" (K28.5 pattern) "y" (K28.7 pattern) "m" (mixed frequency pattern) "I" (loopback, repeater mode) New in Version 1.7
Response:	Parameters:
(none)	
Notes:	Example: "setpat=7"

Selects the input source	
Command:	Parameters:
"SetInput"	"O" (optical SFP) "E" (electrical SMA)
Response:	Parameters:

(none)	
Notes:	Example: "setinput=E"

Selects the input poliarity	
Command:	Parameters:
"SetInPol"	"+" (noninverted) "-" (inverted)
Response:	Parameters:
(none)	
Notes:	Example: "SetInPol +". The input polarity applies to both the SFP and SMA input s.

Controls the SFP Out	put
Command:	Parameters:
"SetSFP"	"0" (output off) "1" (output on) "+" (output not inverted) "-" (output inverted)
Response:	Parameters:
(none)	
Notes:	Example: "SFP=1" turns on the SFP output
Controls the SMA Ou	tput
Command:	Parameters:
"SetSMA"	"0" (output off) "1" (output on) "+" (output not inverted) "-" (output inverted)
Response:	Parameters:
(none)	
Notes:	Example: "SMA=0" turns off the electrical output
Set the wavelength (V 1.7 and above)	
Command:	Parameters:
"SetWL"	"####.##" (Wavelength in nm)
Response:	Parameters:
(none)	· a.amotoro.

Reset error counters, BER, and test timers	
Command:	Parameters:
"Reset"	(none)
Response:	Parameters:
(none)	
Notes:	

Example: "setwl=1550.12"

Notes:

Read the status and settings		
Command:	Parameters:	
"Stat"	(none)	
Response:	Parameters:	
Command Echo	STAT:	
SFP Tx power (dBm) and pol arity	-2.3+ Power (dBm) followed by polarity	
SFP Tx wavelength (nm)	1310.00	
SFP temperature (°C)	42	
SMA output and polarity	+" = not inverted, "-" = inverted, "x"= disabled	
Bit rate (bps)	250000000	
Pattern	3 (per "setpat" command)	
Termination	CR/LF <0x00>	
Notes:	All parameters are separated by "," and the message is terminated with CR/LF Example:  STAT: -2.3+, 1310.00, 42, -, 2500000000, 3	

Read the measurements	
Command:	Parameters:
"meas"	(none)

Response:	Parameters:
Command Echo	MEAS:
BERT Input	E "O"= optical SFP, "E"= electrical SMA
SFP Rx power (dBm)	-21.2
SMA Rx amplitude (%)	64
Lock Status	Lock "Lock" or "LOL"
Error count	2.354e04
Bit count	1.522e10
BER	1.547e-06
Test Time (seconds)	864
Termination	CR/LF <0x00>
Notes:	All parameters are separated by "," and the message is terminated with CR/LF Example:  MEAS: E, -21.2, 64, Lock, 2.354e04, 1.522e10, 1.547e-06, 864

Prints Transceiver Register Information and Values	
Command:	Parameters:
"PrintSFP"	
Response:	Parameters:
SFP information	(ASCII text formatted information about the SFP including: Vendor, Model, Serial Number, Power Levels, and data from both the ID and Diagnostic registers)
Notes:	SFP Vendor: OPNEXT, INC. Part Number: TRS2001EN-0065 SN: L12E15424 Date Code 07-06-12 Diagnostics: Internal Calibration Media: 50um, 80 m Wavelength: 850.00 nm Speed Range: 10300.00 Mbps to 10300.00 Mbps  Temperature: 31 C Rx Power: -40.0 dBm Tx Power: -2.6 dBm  SFP Information Registers:

	60	00	00	00	00	00	00	00	00	00	00	00	00	00	00	00	00
	70	00	00	00	00	00	00	00	00	00	00	00	00	00	00	00	00
	80	00	00	00	00	00	00	00	00	00	00	00	00	00	00	00	00
	90	00	00	00	00	00	00	00	00	00	00	00	00	00	00	00	00
	a0	00	00	00	00	00	00	00	00	00	00	00	00	00	00	00	00
	b0	00	00	00	00	00	00	00	00	00	00	00	00	00	00	00	00
	c0	00	00	00	00	00	00	00	00	00	00	00	00	00	00	00	00
	d0	00	00	00	00	00	00	00	00	00	00	00	00	00	00	00	00
	e0	00	00	00	00	00	00	00	00	00	00	00	00	00	00	00	00
	f0	00	00	00	00	00	00	00	00	00	00	00	00	00	00	00	00
	SFP	Dia	igno	sit	c F	Regi	ist∈	ers	:								
		00	01	02	03	04	05	06	07	80	09	0 a	0b	0с	0d	0e	0f
	+																
	00	55	00	f6	00	-	00		-				-	-	8с	79	18
	10		4c				58	02		37	2d		7b		d1	05	
	20	37		00	fb		d0	01	8e			00	00	00	00	00	
	30	00	00	00	00	00	00	00		00	00	00	00		00	00	
	40	00	00	00	00	3f	80	00		00	00	00	00	01	00		00
	50	01	00	00	00	01	00	00		01	00	00		00	00	00	
	60	21	00	80	76		_	15	74	00	00	00	00	00	00		00
	70	00	40	00	00	00	40	00	00	41	54	53	31	00	00	00	
	80	00	00	00	00	00	00	00	00	00	00	00	00	00	00	00	
	90	0.0	00	00	00	00	00	00	00	00	00	00	00	00	00		00
	a0	00	00	00	00	00	00	00	00	00	00	00	00	00	00		00
	b0	0.0	00	00	00	00	00	00	00	00	00	00	00	00	00	00	00
	c0	0.0	00	00	00	00	00	00		00	00	00	00	00	00		00
	d0	0.0	00	00	00	00	00	00	-	00	00	00	00	00	00	00	00
	e0	0.0	00	00	-	00	00		00			00		00		0.0	
	f0						00	00	00	ff	ff	ff	ff	ff	ff	ff	ff
Termination	CR	/LI	<	0x	00:	>											

Read SFP Register				
Command:	Parameters:			
"RdSFP"	"t" "#" "t" : register type – either "I" for information or "D" for diagnostic, "#": register number in hex Example: "RdSFP I 0x44" Reads the first byte of the serial number from the information register at address 0x44			
Response:	Parameters:			
Register type, register number, value	Example: "a0:44 = 35" (information register (0xA0), register number (0x44), value (5 ASCII)			
Termination	CR/LF <0x00>			
Notes:	The physical address of the information register is 0xA0 and the physical addres s of the diagnostic register is 0xA2. All values passed in and returned are in hex, preceding "0x" is optional. Input parameters should be separated by a space. No te, not all SFP vendors support reading and writing all locations. See SFF-8472 f or more information.			

Write SFP Register, then respond with read back value				
Command:	Parameters:			
"WrSFP"	"t" "#" "v" "t" : register type – either "I" for information or "D" for diagnostic, "#": register number in hex, "v": value to be written in			

	hex. Example: "WrSFP D 0x80 0x55" Writes 0x55 to the first byte of the user w ritable EEPROM area at register at address 0x80.
Response:	Parameters:
Register type, register number, value	Example: "a2:80 = 55" (diagnostic register (0xA2), register number (0x80), value read back (0x55)
Termination	CR/LF <0x00>
Notes:	The physical address of the information register is 0xA0 and the physical addres s of the diagnostic register is 0xA2. All values passed in and returned are in hex, preceding "0x" is optional. Input parameters should be separated by a space. No te, not all SFP vendors support reading and writing all locations. See SFF-8472 f or more information.

Pulse SFP Optical Output (V 0.6 and above)				
Command:	Parameters:			
"Pulse"	"PW" "Per" "PW": is the pulse width in uS and "Per" is the period in uS. The valid range for PW is 1 to 65000uS (6.5mS) and the valid range for Per is 1 to 1,000,000 (1 second).  Example: "Pulse 10 1000"  Produces a 10uS pulse with a 1mS period.			
Response:	Parameters:			
none				
Notes:	The pulse command modulates the optical output signal by controlling the trans mit enable pin on the SFP, therefore the optical output signal will be switched bet ween the current rate/pattern and no light. To approximate a CW signal it is recommended to set the BERT to 11.3Gb, PRBS31. The modulation will continue unt il any input is received on either the Ethernet or USB ports. The turn on / off time of the laser in the SFP will affect the minimum pulse width of the actual optical output; this will vary with SFP model and manufacturer.			

## www.spectronixinc.com

Eye-BERT Gen2 Software Programming Guide V 1.12

## **Documents / Resources**



<u>Spectronix Eye-BERT Gen 2 Programming Software</u> [pdf] User Guide Eye-BERT Gen 2 Programming Software, Eye-BERT Gen 2, Programming Software

# References

- <u>Overview Spectronix</u>
- User Manual

#### Manuals+, Privacy Policy

This website is an independent publication and is neither affiliated with nor endorsed by any of the trademark owners. The "Bluetooth®" word mark and logos are registered trademarks owned by Bluetooth SIG, Inc. The "Wi-Fi®" word mark and logos are registered trademarks owned by the Wi-Fi Alliance. Any use of these marks on this website does not imply any affiliation with or endorsement.