




---

[Home](#) » [Sper Scientific Instruments](#) » **Sper Scientific Instruments 870007 Inline Dissolved Oxygen Analyzer User Manual** 

## Contents [ [hide](#) ]

- [1 Sper Scientific Instruments 870007 Inline Dissolved Oxygen Analyzer](#)
- [2 Introduction](#)
- [3 Installation and Wiring](#)
- [4 Operation Interface](#)
- [5 Measurement interface](#)
- [6 Appendix](#)
- [7 FAQ](#)
- [8 Documents / Resources](#)
  - [8.1 References](#)

# Sper Scientific

**Sper Scientific Instruments 870007 Inline Dissolved Oxygen Analyzer**



## Introduction

Industrial Inline Dissolved Oxygen Analyzer offers excellent functionality, stable performance, easy operation, low power consumption along with the highest safety and reliability.

The dissolved oxygen analyzer can be widely used in industrial application such as thermal power generation, chemical industry, metallurgy, environmental protection, pharmaceutical, biochemical, food and tap water.

## Technical Features

1. Extremely quickly and precision dissolved oxygen sensor.
2. It is suitable for harsh application and maintenance-free.
3. Provides two ways of 4-20mA output for dissolved oxygen and temperature.
4. With data recording function, user easy to check history data and history curve.


## Technical Specifications

Specifications	Details
Name	Inline Dissolved Oxygen Analyzer


Shell	ABS plastic
Power Supply	90V ~ 260V AC 50/60Hz
Power Consumption	4W
Output	Two 4-20mA output tunnels, RS485
Relay	5A/250V AC      5A/30V DC
Size	144mm×144mm×104mm
Weight	0.9kg
Protocol	Modbus RTU
Range	0.00 mg/L ~20.00 mg/L 0.00 % ~200.00 % -10.0 °C ~100.0 °C
Accuracy	±1%FS ±0.5°C
Waterproof Level	IP65
Storage Environment	-40°C~70°C 0%~95%RH (non-condensing)
Working Environment	-20°C~50°C 0%~95%RH (non-condensing)

## Installation and Wiring


### SIZE

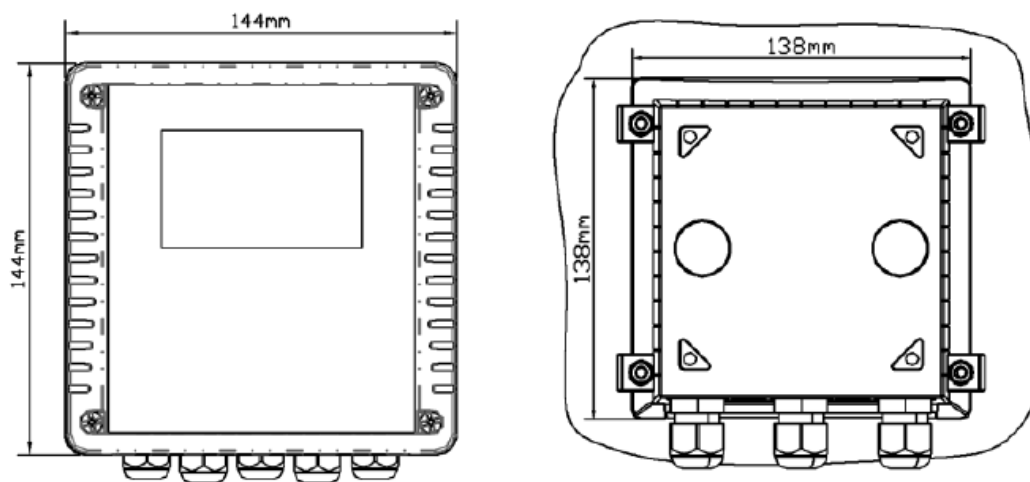

## Installation

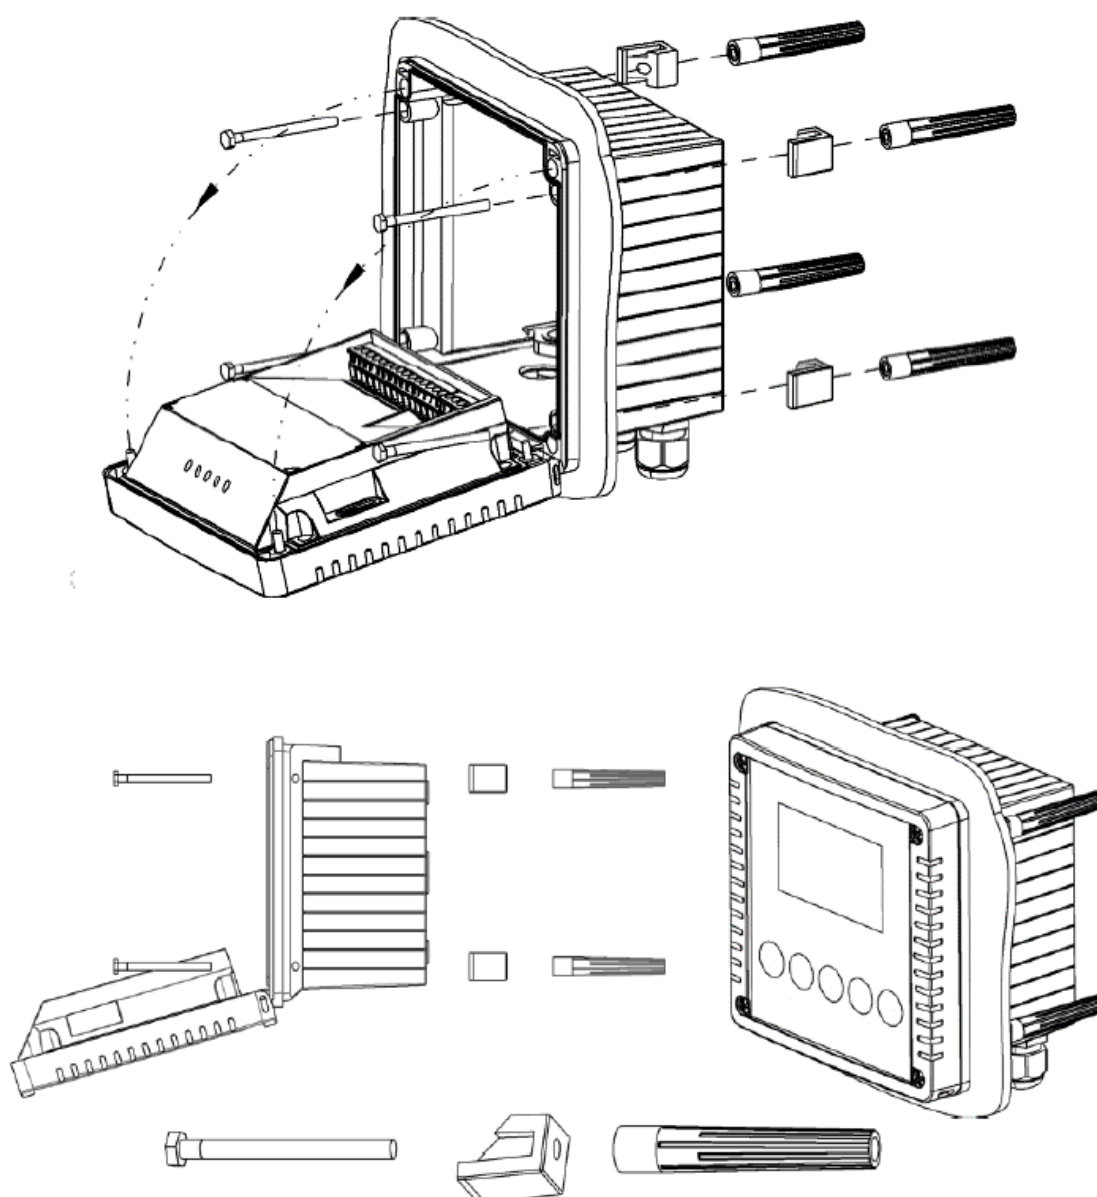


## Wiring

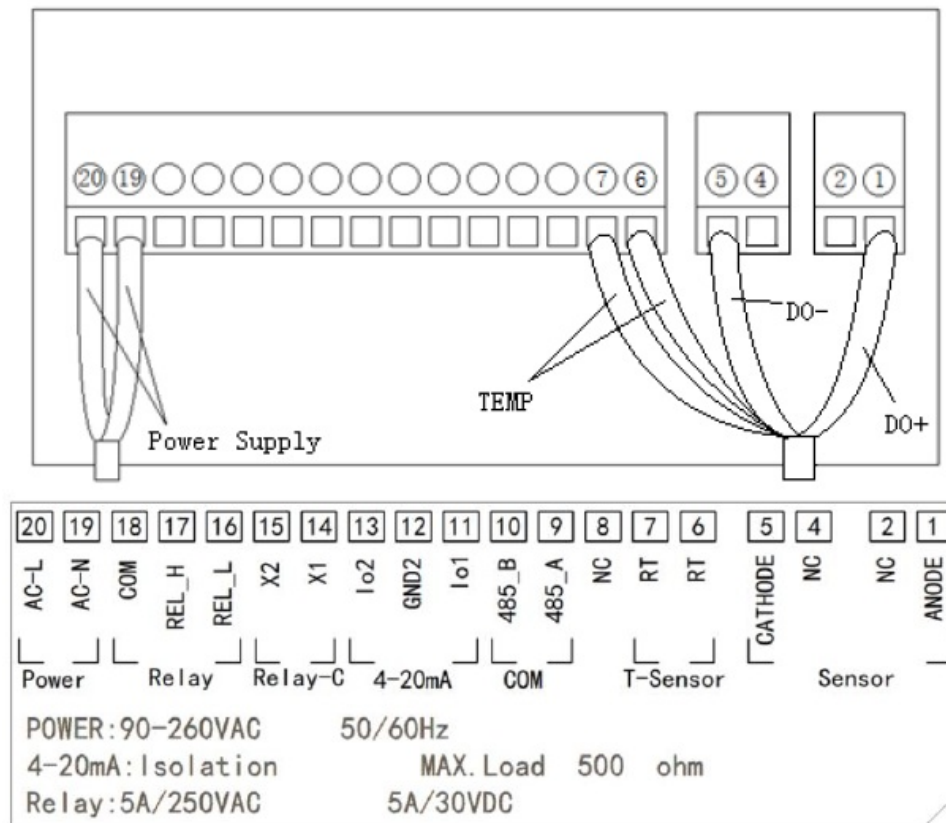

## Operation Interface

There are 2 modules in the main panel of the dissolved oxygen measuring instrument, LED LCD display module and button module. Users can set and adjust the parameters of the instrument through the 5 buttons on the panel.

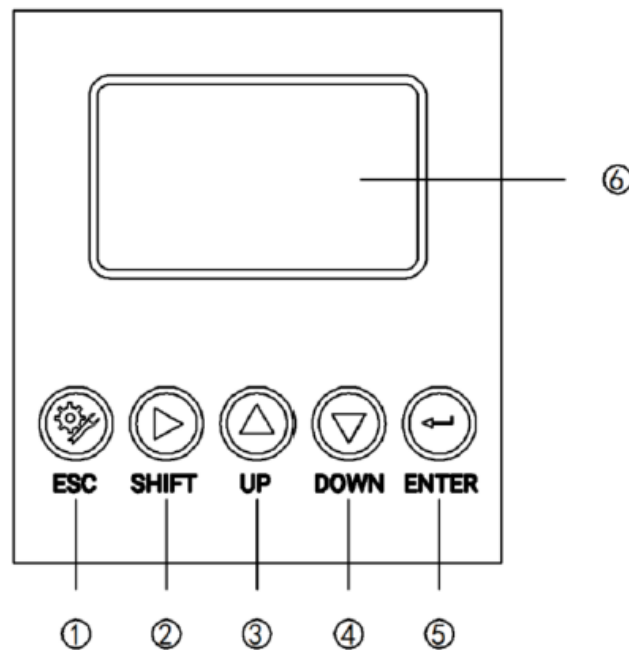


Picture 1 Operation Interface

1. Set/Exit button
2. Select/Shift button
3. Up button
4. Down button
5. Confirm button
6. LED screen

## Measurement interface

Enter the main measurement interface after the start-up animation.

When the instrument is working normally, the LED display shows the following content.

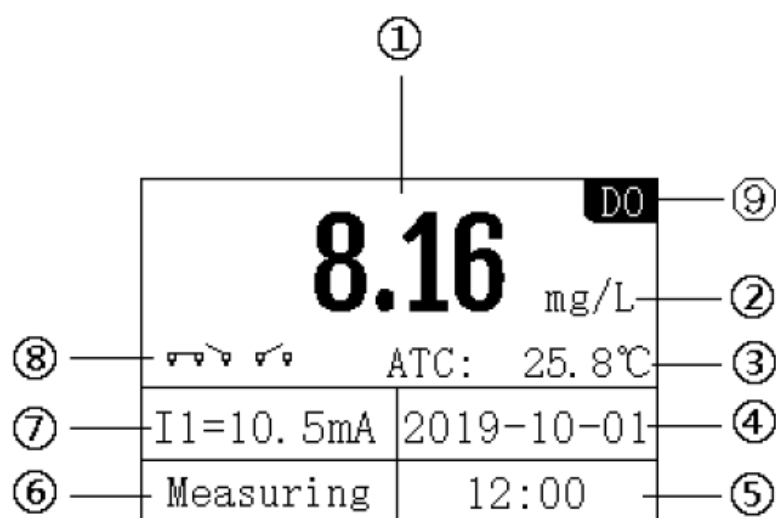


Picture 2 Main interface

1. Measurement value
2. Unit
3. Temperature
4. Real-time date
5. Real time
6. Measurement status
7. 4-20mA corresponding value of dissolved oxygen
8. Relay status
9. Mode

## Setting


- Press “Set/Exit Button” to enter the password input interface.

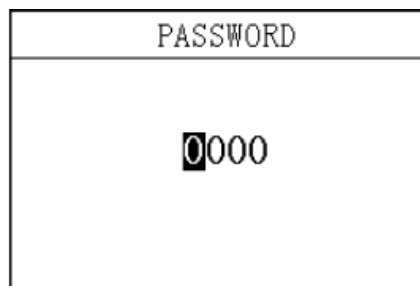

Picture 3 Password

### Enter settings:

Enter the password “3700” to enter the setup menu.

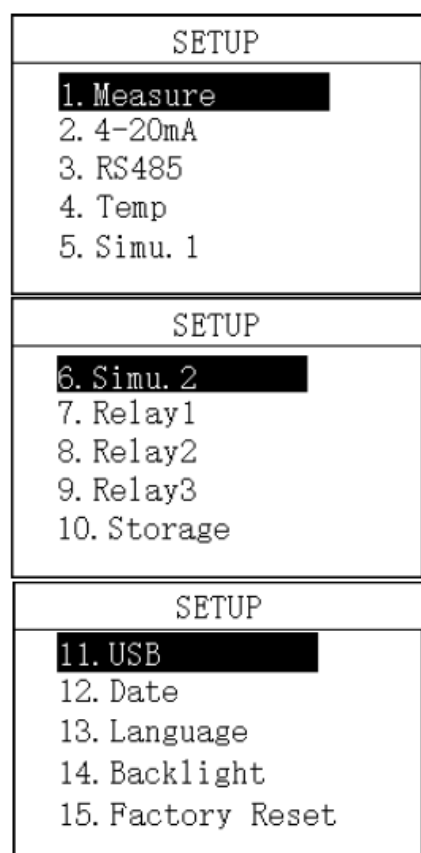

Picture 4 Setting Menu

### Unit

In this menu, users can change the measurement method.

Measure
Mode : ► % mg/L ppm ug/L ppb

**Picture 3.1 Unit**

## 20mA

In this menu, users can change the corresponding value of 4-20mA and set the corresponding effective range.

4-20mA
4mA : 00.00 mg/L
20mA : 20.00 mg/L
4mA : +000 °C
20mA : +100 °C

**Picture 3.2 4-20mA**

## ModbusRTU communication

In this menu, users can change the communication address and rate.

Modbus RTU
Address : 003
B. R. : 4800 bps ►9600 bps 19200 bps

**Picture 3.3 ModbusRTU communication**



## Temperature

In this menu, users can set the temperature offset and manually set the temperature.

Temp
Sensor : ▶ Pt1000 NTC10k
MTC : +025.0°C

**Picture 3.4 Temperature**

## Simulation

In this menu, users can simulate the 4-20mA current output. The current output can be verified by simulating the measurement of the IO1 (measured value) and IO2 (temperature) ports. The release relay is closed. The relay is simulated and verified.

Simulation1
Current1: 04.00mA
Current2: 04.00mA
Relay1: ON ▶ OFF

**Picture 3.5.1 Simulation1**

Simulation2
Relay2 : ON ▶ OFF
Relay3 : ON ▶ OFF

**Picture 3.5.2 Simulation2**

Relay1
Func. : ON ▶ OFF
High : 10.00 mg/L
Hyst : 1.00 mg/L
Delay : 030 S

**Picture 3.6 Relay1**

## Relay1

In this menu, users can switch the relay 1 function, set the parameter alarm upper limit value, alarm return difference value, and alarm delay time.

Relay2	
Func. :	ON ▶ OFF
Low :	03.00 mg/L
Hyst :	1.00 mg/L
Delay :	030 S

**Picture 3.7 Relay2**

## Relay2

In this menu, users can switch the relay 2 function, set the parameter alarm lower limit value, alarm return difference value, and alarm delay time.

Relay3	
Func. :	ON ▶ OFF
Period :	001.0h
Clean :	010s

**Picture 3.8 Relay3**

## Relay3

In this menu, users can set the relay 3 function, set the cleaning time and cleaning cycle.

Storage	
Switch :	ON ▶ OFF
Clear :	YES ▶ NO
Interval :	005 min

**Picture 3.9 Storage**

## Storage

In this menu, users can set the storage function (default off), clear storage memory and recording interval.

Date
Y - M - D : 2019-10-01
H : M : S : 12:00:00

**Picture 3.10 Date&Time**

### **Date&Time**

In this menu, users can change date and time according to different time zone.

Language
Language : ▶ 简体中文
English

**Picture 3.11 Language**

### **Language**


Users can choose English or Chinese according to need.

Backlight
Func. : ▶ ON
Delay 30S
Bright : 3
Contrast : 2

**Picture 3.12 Backlight**

## Backlight


In this menu, users can change the backlight mode of the LCD screen. The backlight can be always on or delayed off (the default is delayed off), the backlight brightness can be changed (brightness level 1-5, brightness increases), and the contrast can be changed.

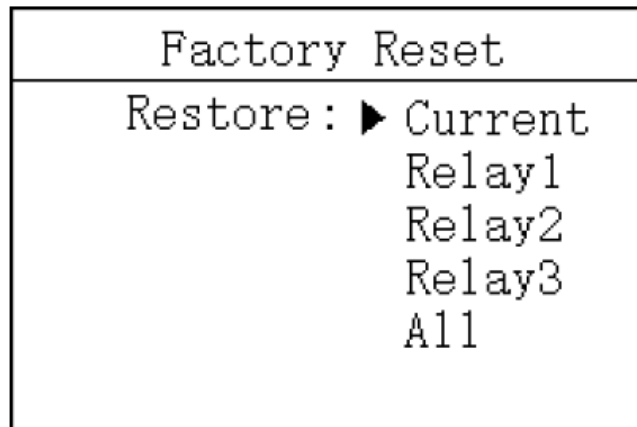

**Picture 3.13 Factory data reset**

## Factory data reset


In this menu, users can restore the current output and relay to the factory parameters.

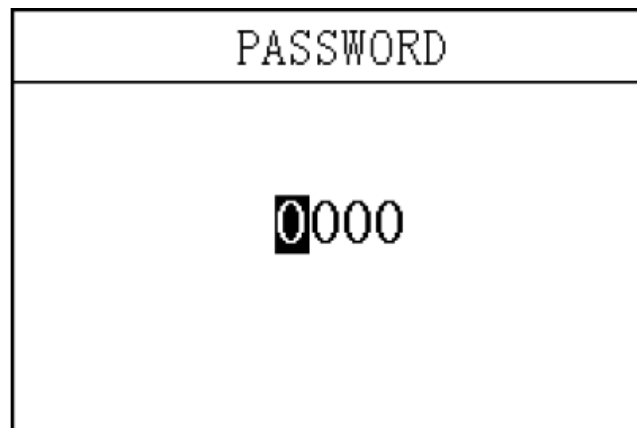

**Picture 5 Password**

## Calibration


Press "ESC" to enter the password input interface.

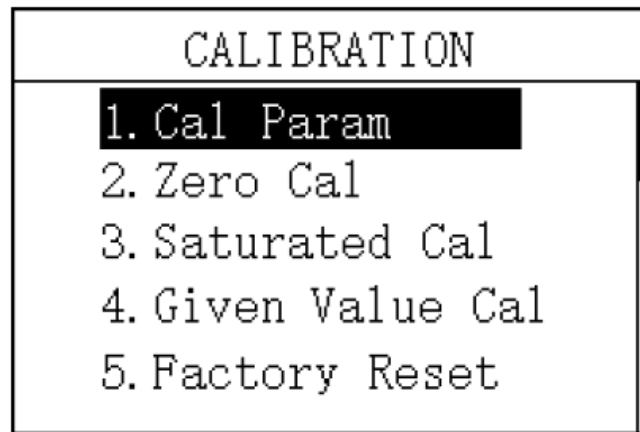

**Picture 6 Calibration menu**

#### **Enter calibration menu:**

Enter the password "3900" to enter the calibration menu.

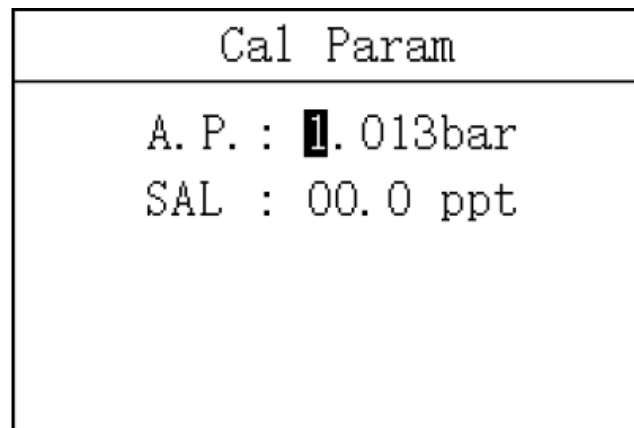

**Picture 4.1 Parameter Calibration**

#### **Parameter Calibration**

In this menu, users can manually change the parameters of atmospheric pressure and salinity.

Zero Cal
<div>2.1 nA</div> <div>25.7 °C</div>
Please Press Enter
Zero Cal
<div>0.9 nA</div> <div>25.7 °C</div>
Cal Success

**Picture 4.2 Zero Calibration**

### Zero Calibration

In this menu, users shall put the electrode into anaerobic water. When the value comes stable, press 'Enter' button.

Saturated Cal
<div>70.0 nA</div> <div>25.7 °C</div>
Please Press Enter
Saturated Cal
<div>68.2 nA</div> <div>25.7 °C</div>
Cal Success

**Picture 4.3 Saturated Calibration**

### Saturated Calibration

In this menu, users shall put the electrode into air. When the value comes stable, press 'Enter' button.

Given Value Cal	
16.28 ppb	<b>1</b> 000 ppb (≤1000)
Press Enter	

**Picture 4.4 Given Value Calibration**

### Given Value Calibration

Put the electrode in the measuring liquid of known concentration, set it to the ppb value of the solution of known concentration, and press the confirm key.

Factory Reset ▶ YES NO
------------------------------

**Picture 4.5 Factory data reset**

### Factory data reset

In this menu, users can restore the calibration parameters to the factory parameters.

PASSWORD
<b>0</b> 000

**Picture 7 Password**

### History Data Display

Press “ESC” to enter the password input interface.

Record	1/1000
2020-01-09 12:48:28	6.00 mg/L
2020-01-09 12:43:28	6.00 mg/L
2020-01-09 12:38:28	6.00 mg/L
2020-01-09 12:33:28	6.00 mg/L

**Picture 8 History**

### Enter History Data Display:


- Enter the password “1300” to enter the History Data Display.
- Press the up and down keys to switch the display. It can store up to 1000 records and overwrite automatically if reach maximum.

PASSWORD
0000

**Picture 9 Password**

### Waveform Display

Press “ESC” to enter the password input interface.

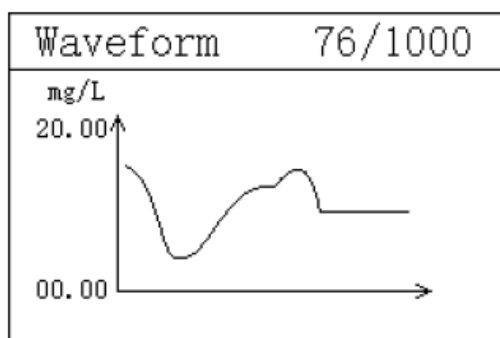

**Picture 10 Waveform Display**

### Enter Waveform Display:

Enter the password “1400” to enter the Waveform Display. Press the up and down keys to switch the display.

## Appendix



## Communication protocol

### Communication parameters:

- Baudrate:4800, 9600, 19200(9600default)
- Serial data format: 8N1(8 data bits, No parity, 1 stop bit) Function code: 03
- Device address: Dissolved oxygen analyzer defaults to 3

### Register definition:

Register address(Dec)	Definition	R/W	Remarks
0	Temp	R	×0.1°C sint16
1	DO	R	×0.01mg/L uint16
2	nA	R	×0.01nA uint16
3	Saturation	R	×0.1% uint16
8	RTU Addresses	R/W	Modbus communication address DO defaults 3.
9	Baudrate	R/W	4800 9600 19200 9600 as default

### Examples of communication formats:

#### Data reading instruction

Addr. + Func. + Register start address + Number of Registers read + CRC check code (Hex) e.g. Tx:03 03 00 01 00 01 D4 28

Address	Func.	Register start address	Number of Registers read	CRC check code
03	03	0001	0001	D428

### Data return instruction:

Address + Func. + Data length + Data + CRC check code (Hex) e.g. Rx:03 03 02 00 DF 80 1C

Address	Func.	Data length	DO value	CRC check code
---------	-------	-------------	----------	----------------

03	03	02	00DF	801C
----	----	----	------	------

**DF**  
 HEX DF  
 DEC 223

- The hexadecimal number DF is converted to decimal by a calculator (programmer mode) to obtain the value 223.
- The actual value contains 2 decimal places, then the actual value is  $223 \times 0.01 = 2.23$

### Electrode parameter table of Online Dissolved Oxygen Analyzer

Type	DOG-209FA
DO Range	0.00mg/L~20.00mg/L
Temperature Range	0.0°C~60.0°C
Accuracy	3% $\pm$ 0.5°C

Withstand pressure	0.06MPa
Waterproof level	IP68/NEMA6P
Polarization time	60min
Deviation	± 0.1mg/L

Sper Scientific Instruments [www.sperdirect.com](http://www.sperdirect.com)

## FAQ


- **Q: What are the industries where the dissolved oxygen analyzer can be used?**

A: The analyzer can be used in thermal power generation, chemical industry, metallurgy, environmental protection, pharmaceutical, biochemical, food, and tap water industries.

- **Q: Is the dissolved oxygen sensor suitable for harsh environments?**

A: Yes, the dissolved oxygen sensor is suitable for harsh applications and is maintenance-free.

## Documents / Resources

 <p>870007 Inline Dissolved Oxygen Analyzer User Manual</p> <p>Sper Scientific Instruments</p>	<p><a href="#">Sper Scientific Instruments 870007 Inline Dissolved Oxygen Analyzer [pdf]</a></p> <p>] User Manual</p> <p>870007 Inline Dissolved Oxygen Analyzer, 870007, Inline Dissolved Oxygen Analyzer, Dissolved Oxygen Analyzer, Oxygen Analyzer</p>
---	--

## References

- [User Manual](#)

# Leave a comment

Your email address will not be published. Required fields are marked \*

Comment \*

Name

Email

Website

☐ Save my name, email, and website in this browser for the next time I comment.

**Post Comment**

**Search:**

e.g. whirlpool wrf535swhz

**Search**

[Manuals+](#) | [Upload](#) | [Deep Search](#) | [Privacy Policy](#) | [@manuals.plus](#) | [YouTube](#)

This website is an independent publication and is neither affiliated with nor endorsed by any of the trademark owners. The "Bluetooth®" word mark and logos are registered trademarks owned by Bluetooth SIG, Inc. The "Wi-Fi®" word mark and logos are registered trademarks owned by the Wi-Fi Alliance. Any use of these marks on this website does not imply any affiliation with or endorsement.